



Declaration Ref No: DC21-0035

## CE Declaration of Conformity

According to Annex III of the IVD Directive 98/79/EC

We,

### Atlas Medical

Head office: Ludwig-Erhard-Ring 3  
Blankenfelde-Mahlow, Germany.  
Tel: +49 - 33708 – 3550 30  
Email: [info@atlas-medical.com](mailto:info@atlas-medical.com)

Middle East Site: Sahab Free Zone Area, P. O. Box 212555, Amman, Jordan.

Tel.: +962 6 4026468  
Fax: +962 6 4022588  
Email: [info@atlas-medical.com](mailto:info@atlas-medical.com)

Declare our responsibility that the following product:

### See Attached list

- Comply with all essential requirements (AnnexI) of the IVD Directive 98/79/EC. This compliance has been properly documented and covers the items listed in Annex I of the IVD Directive.
- This product is produced under Atlas quality system (ISO13485:2016) issued by GMED:  
**Certificate N°:** 36655 rev 1  
**Expiry Date:** October 8<sup>th</sup>.2023
- Comply with the essential requirements of following standards (EN 18113-1, -2,-4:2011, EN ISO 15223:2016 , EN ISO 23640:2015, EN ISO 14971:2019, ISO 2859/1:1999, EN ISO 13612:2002, EN ISO 13641:2002.

And  
Intended for In-Vitro Professional use only.

### Manufacturer

Atlas Medical

Ludwig-Erhard-Ring 3

Blankenfelde-Mahlow , Germany.



Atlas Medical	Issue date	Date of review	Management approval	MRXDO10F.10 08.02.2011
	March.2021	09.03.2021		



## CE Declaration of Conformity

According to Annex III of the IVD Directive 98/79/EC

Product Description
8.00.02.0.0100 : ASO Latex Kit, 100 Tests (4ml Latex, 2x1.0ml controls).
8.00.00.0.0100: CRP Latex Kit, 100 Tests (4 ml Latex, 2x1.0 ml Controls)
8.00.04.0.0100: RF Latex Kit, 100 Tests (4ml Latex, 2x1.0ml controls)
8.00.17.0.0100: D-Dimer Latex Kit, 100 Tests
8.00.13.0.0300 : Streptococcus Latex Kit, 6 Groups, 6x50 Tests (5x1.5ml Latex (A,B,C,G,F), 1x3ml Latex(D), 1x1.0ml Positive Control, 1x2ml Extraction Reagent E, 1x1.5ml Extraction Reagent 1, 1x1.5ml Extraction Reagent 2, 2x2.5ml Extraction Reagent 3, Stirring Sticks, Glass Slide).
8.00.18.3.0500 : RPR Syphilis (Coarse Grain) Kit, 500 Tests (10 ml latex, 2x1ml control) Without card,stirring sticks.
8.00.18.3.1000 RPR Carbon Antigen (Coarse Grain) Kit, 1000 Tests (Reagent only).



**CE Declaration of Conformity**

We,  
**Atlas Medical GmbH**  
 Head office: Ludwig-Erhard-Ring 3  
 15827 Blankenfelde-Mahlow Germany  
 Tel: +49(0)33708355030  
 Email: info@atlas-site.com

Middle East Site: : Sahab Industrial Zone Area, King Abdullah II Industrial City  
 Amman 11512, Jordan  
 Tel.: +962 6 4026468  
 Fax: +962 6 4022588  
 Email: [info@atlas-medical.com](mailto:info@atlas-medical.com)

Declare our responsibility that the following product:

**Blood Grouping Reagents:**  
**(Anti-A Monoclonal Reagent, Anti-B Monoclonal Reagent , Anti-AB Monoclonal Reagent and**  
**Anti-D IgG/IgG blend Reagent)**  
**see the attached list of variants**  
**That are classified as Annex II, list A**

Is produced under Atlas quality system (ISO13485: 2016) supported by GMED certificate and  
 complies with the essential requirements of

**In Vitro Diagnostic Medical Devices Directive 98/79/EC**

And

EN ISO 18113-1, -2 :2011, EN ISO 15223:2016  
 EN ISO 14971:2019, EN ISO 23640 :2015 , ISO 2859 :2017,  
 EN 13612:2002, EN 13641:2002 , EN 13975:2003,  
 EN ISO 13485:2016, EN 62366-1:2020

And

Intended for In-Vitro Professional use only.

**Conformity Assessment Route:**

Annex IV.3 –Approval full Quality Assurance System.  
 Annex IV.4-EC Design Examination (of the product)


**Notified Body:**


G-MED	<b>CE</b>	0459
-------	-----------	------

GMED, Laboratoire national de métrologie et d'essais  
 1 rue Gaston Boissier 75015 Paris  
 Tél. : 01 40 43 37 00 , TVA:FR 28 839 022 522


**EC Certificates No.:**

- CE Certificate of Approval full Quality Assurance System: 33540 rev4.
- CE Certificate Of EC Design Examination: 33544 rev3.

Atlas Medical GmbH	Start of CE Marking	Date of expiry	Name & Position	Signature	MRXDO10F.11 21.10.2013
	09 <sup>th</sup> october 2017	26 <sup>th</sup> May 2025	Amani Al-hababbeh (RA Manager)		



Product Code	Product Name	GMDN Code
8.02.00.0.0010	Anti-A Monoclonal Reagent (Titer: 1/512), 10ml/vial, 1 vial/Carton Box	52532
8.02.00.1.0100	Anti-A Monoclonal Reagent (Titer: 1/512), 10ml/vial, 10 vials / Plastic Pack	52532
8.02.00.1.0180	Anti-A Monoclonal Reagent (Titer: 1/512), 10ml/vial, 18 vials / Carton Box	52532
8.02.01.0.0010	Anti-B Monoclonal Reagent (Titer: 1/512), 10ml/vial, / Carton Box	52538
8.02.01.1.0100	Anti-B Monoclonal Reagent (Titer: 1/512), 10ml/vial, 10 vials / Plastic Pack	52538
8.02.01.1.0180	Anti-B Monoclonal Reagent (Titer: 1/512), 10ml/vial, 18 vials / Carton Box	52538
8.02.02.0.0010	Anti-AB Monoclonal Reagent (Titer: 1/512), 10ml/vial, 1 vial/ Carton Box	46442
8.02.02.1.0100	Anti-AB Monoclonal Reagent (Titer: 1/512), 10ml/vial, 10 vials/Plastic Pack	46442
8.02.02.1.0180	Anti-AB Monoclonal Reagent (Titer: 1/512), 10ml/vial, 18 vials/Carton Box	46442
8.02.03.0.0010	Anti-D IgG/IgM Blend Reagent (Titer: 1/128), 10ml/vial, 1 vial/ Carton Box	52647
8.02.03.1.0100	Anti-D IgG/IgM Blend Reagent (Titer: 1/128), 10ml/vial, 10 vials / Plastic Pack	52647
8.02.03.1.0180	Anti-D IgG/IgM Blend Reagent (Titer: 1/128), 10ml/vial, 18 vials / Carton Box	52647
8.02.04.0.0010	Anti-A Monoclonal Reagent (Titer: 1/256), 10ml/vial, 1 Vial/Carton Box	52532
8.02.04.0.0100	Anti-A Monoclonal Reagent (Titer: 1/256), 10ml/vial, 10 vials / Plastic Pack	52532
8.02.05.0.0010	Anti-B Monoclonal Reagent (Titer: 1/256), 10ml/vial, 1vial/Carton Box	52538
8.02.05.0.0100	Anti-B Monoclonal Reagent (Titer: 1/256), 10ml/vial, 10 vials /Plastic Pack	52538
8.02.05.6.0030	ABO Set (Anti-A (1/256), Anti-B (1/256), Anti-D (1/64)),3x10ml / plastic Pack	45308
8.02.05.7.0020	ABO Set: Anti-A (1/256), Anti-B (1/256), 2x10ml /Plastic Pack	52695
8.02.06.0.0010	Anti-AB Monoclonal Reagent (Titer: 1/256), 10ml/vial, 1vial/Carton Box	46442
8.02.06.1.0100	Anti-AB Monoclonal Reagent (Titer: 1/256), 10ml/vial,10 vials /Plastic Pack	46442
8.02.06.1.0180	Anti-AB Monoclonal Reagent (Titer: 1/256), 10ml/vial,18 vials / Carton Box	45308
8.02.07.0.0010	Anti-D IgG/IgM Blend Reagent (Titer: 1/64), 10ml/vial, 1Vial/ Carton Box	52647
8.02.07.1.0100	Anti-D IgG/IgM Blend Reagent (Titer: 1/64), 10ml/vial, 10 vials / Plastic Pack	52647

Atlas Medical GmbH	Start of CE Marking	Date of expiry	Name & Position	Signature,	MRXDO10F.11 21.10.2013
	09 <sup>th</sup> october 2017	26 <sup>th</sup> May 2025	Amani Al-hababbeh (RA Manager)		

8.02.47.0.0030	ABO Set (Anti-A (1/512), Anti-B (1/512), Anti-D (1/128)), 3x10ml/Plastic Pack	45308
8.02.47.1.0030	ABO Set (Anti-A (1/256), Anti-B (1/256), Anti-D (1/64)), 3x10ml /Carton Box.	45308
8.02.47.3.0030	ABO Set (Anti-A (1/256), Anti-B (1/256), Anti-D (1/64)), 3x10ml /Plastic Pack	45308
8.02.47.5.0030	ABO Set (Anti-A (1/256), Anti-B (1/256), Anti-D (1/128)), 3x10ml/Plastic Pack	45308
8.02.49.0.0040	ABO Set (Anti-A (1/256), Anti-B (1/256), Anti-AB (1/256), Anti-D (1/64)), 4x10ml/Carton Box	45308
8.02.49.2.0040	ABO Set (Anti-A (1/256), Anti-B (1/256), Anti-AB (1/256), Anti-D (1/128)), 4 x 10ml, 4 vials/Plastic Pack	45308
8.02.53.0.0040	ABO Set (Anti-A (1/512), Anti-B (1/512), Anti-AB (1/512) Anti-D (1/128)), 4x10ml/Plastic Pack	45308
8.02.53.1.0040	ABO Set (Anti-A (1/512), Anti-B (1/512), Anti-AB (1/512) Anti-D (1/128)), 4x10ml, 4vials/Plastic Pack	45308
8.02.70.0.0010	Anti-A monoclonal reagent , Titer (1/1024), 10 ml/vial, 1Vial/ Carton Box	52532
8.02.71.0.0010	Anti-B Monoclonal reagent (Titer: 1/1024) , 10 ml/vial ,1Vial/ Carton Box	52538
8.02.72.0.0010	Anti-AB Monoclonal reagent (Titer: 1/1024) , 10 ml/vial , 1Vial/ Carton Box	45308
8.02.85.0.0010	Anti-D IgG/IgM Blend Reagent , Titer 1/256, 10ml/vial, 1Vial/ Carton Box	52647



Atlas Medical GmbH	Start of CE Marking	Date of expiry	Name & Position	Signature	MRXDO10F.11
	09 <sup>th</sup> october 2017	26 <sup>th</sup> May 2025	Amani Al-hababbeh (RA Manager)		21.10.2013

**GMED certifie que le système de management de la qualité développé par**

*GMED certifies that the quality management system developed by*

**ATLAS MEDICAL GmbH**  
**Ludwig-Erhard-Ring 3**  
**15827 Blankenfelde-Mahlow GERMANY**

**pour les activités**  
*for the activities*

**Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic in vitro .**

*Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices.*

**réalisées sur le(s) site(s) de**  
*performed on the location(s) of*

**Voir addendum**

*See addendum*

**est conforme aux exigences des normes internationales**  
*complies with the requirements of the international standards*

**ISO 13485: 2016**

**Début de validité / Effective date October 9th, 2020 (included)**

**Valable jusqu'au / Expiry date : October 8th, 2023 (included)**

**Etabli le / Issued on : October 8th, 2020**



GMED N° 36655-1

Ce certificat est délivré selon les règles de certification GMED / This certificate is issued according to the rules of GMED certification

Renouvelle le certificat 36655-0



**On behalf of the President**  
**Béatrice LYS**  
Technical Director

**Ce certificat couvre les activités et les sites suivants :**  
*This certificate covers the following activities and sites:***French version :**

Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic *in vitro* à usage professionnel et/ ou d'autodiagnostic, dans les domaines du groupage sanguin, de la microbiologie, de la biochimie, de la toxicologie, de l'oncologie, de la cardiologie, de l'histologie, de l'endocrinologie et des maladies infectieuses, dans les techniques d'Agglutination/ ELISA/ Tests rapides/ Colorimétrie/ Disques antibiotiques.

**English version:**

*Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices for professional use and/or for self-testing, in the field of Immunohematology, Microbiology, Biochemistry, Toxicology, Oncology, Cardiology, Histology, Endocrinology Biosensors and Infectious diseases, in techniques of Agglutination/ ELISA/ Rapid tests/ Colorimetry/Antibiotic disks.*

**ATLAS MEDICAL GmbH**  
**Ludwig-Erhard-Ring 3**  
**15827 Blankenfelde-Mahlow**  
**GERMANY**

French version:

**Siège social, responsable de la mise sur le marché**

English version:

*Headquarter, legal manufacturer*

\*\*\*\*\*  
**Sahab Industrial Zone Area**  
**King Abdullah II Industrial City**  
**Amman 11512**  
**JORDAN**

French version:

**Conception, fabrication et contrôle final**

English version:

*Design, manufacture and final control*

\*\*\*\*\*  
**William James House**  
**Cowley Road,**  
**Cambridge, CB OWX**  
**United Kingdom**

French version:

**Contact réglementaire**

English version:

*Regulatory Administration*

\*\*\*\*\*  
**3 sites / 3 sites**

DocuSigned by:



**On behalf of the President**  
**Béatrice LYS**  
**Technical Director**



Date: 05/Jan/2023

## **STATEMENT**

We, Atlas Medical having a registered office at Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow, Berlin, Germany assign SRL Sanmedico having a registered office at A. Corobceanu Street 7A, apt.9, Chisinau MD-2012, Moldova, as authorized representative in correspondence with the conditions of directive 98/79/EEC.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

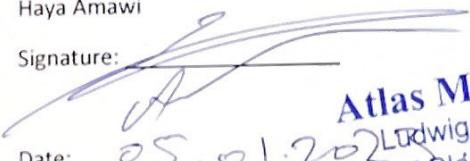
On Behalf of Manufacturer:

General Manager

Haya Amawi

Signature:

Date:

  
Atlas Medical GmbH  
Ludwig - Erhard Ring 3  
15827 Blánkenfelde - Mahlow  
Tel. (0049) 33708 - 355030

**Atlas Medical:** Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow, Berlin, Germany,  
Tel:+4933708355030

**Regulatory Office:** William James House, Cowley Rd, Cambridge, CB4 0WX, United Kingdom  
Tel: +44 (0) 1223 858 910

**Middle East Site:** P.O Box 204, King Abdullah II Industrial Estate, Amman, 11512, Jordan  
Tel: +962 6 4026468

## Blood Grouping Reagents:

### Anti-A Monoclonal Reagent, Anti-B Monoclonal Reagent, Anti-AB Monoclonal Reagent, Anti-D IgG/IgM blend Reagent, & Their variants SLIDE AND TUBE TESTS

**IVD** For In-Vitro and professional use only

2°C  8°C Store at 2- 8°C

#### INTENDED USE

The blood grouping reagents are used to detect the presence or absence of A, B or Rhesus Antigens on the surface of human red blood cells based on hemagglutination using slide or tube test techniques in whole blood samples or anticoagulant blood samples collected in EDTA , citrate or heparin tubes.

#### INTRODUCTION & PRINCIPLES

Blood grouping reagents are prepared from In-Vitro culture supernatants of hybridized immunoglobulin-secreting mouse cell lines. The reagents are diluted with phosphate buffer containing sodium chloride, EDTA and bovine albumin to give reagents that are optimized for use in tube and slide procedures. **Anti-A monoclonal reagent is colored with acid blue (patent blue) dye, Anti-B monoclonal reagent is colored with acid yellow (tartrazine) dye, and Anti-AB monoclonal reagent is not colored.** The test procedure is based on hemagglutination principle, where red cells possessing the antigen agglutinate in the presence of the corresponding antibody indicating that the result is positive. The test is considered negative when no agglutination appears.

Anti-D IgG/IgM blend reagent is prepared from carefully blended human monoclonal IgM and IgG. Anti-D IgG/IgM blend reagent is suitable for slide and tube test procedures. The reagent will directly agglutinate Rh D positive cells, including majority of variants (but not D<sup>vI</sup>) and a high proportion of weak D (Du) phenotypes. The reagent will agglutinate category D<sup>vI</sup> and low grade weak D (D<sup>u</sup>) phenotypes by the indirect anti-globulin techniques.

Anti-D IgG/IgM blend reagent is diluted with a sodium chloride solution, sodium phosphate solution and bovine albumin (sodium caprylate free). Anti-D IgG/IgM blend reagent is not colored. The procedure is based on hemagglutination principle, where red cells' possessing the antigen agglutinates in the presence of the corresponding antibody in the reagent indicating that the result is positive. The test is considered negative when no agglutination appears.

#### MATERIALS

##### MATERIALS PROVIDED

###### Blood Grouping Reagents:

- Anti-A monoclonal reagent (10 ml/vial), Clone: (9113D10).
- Anti-B monoclonal reagent (10 ml/vial), Clone: (9621A8).
- Anti-AB monoclonal reagent (10ml/vial), Clone: (152D12+9113D10).
- Anti-D IgG/IgM Blend reagent (10 ml/vial), Clone: (P3X61 + P3X21223B10 + P3X290 + P3X35).

##### MATERIALS NEEDED BUT NOT PROVIDED

- Plastic test tube or glass.
- Isotonic saline solution (% 0.9) NaCl.
- Applicator sticks.
- Centrifuge (100-1200 (g) for tube test).
- Timer.
- Incubator
- Anti-Human Globulin Reagent (can be ordered from Atlas Medical).
- White or transparent glass slide.

#### PRECAUTIONS

- The reagents are intended for in vitro diagnostic use only.
- The test is for well trained professional healthy user not for lay user.
- These reagents are derived from animal and human sources, thus, appropriate care must be taken in the use and disposal of these reagents, as there are no known test methods that can guarantee absence of infectious agents.
- Do not use reagents if it is turbid or contain particles as this may indicate reagent deterioration or contamination.
- Protective clothing should be worn when handling the reagents.
- **The reagents contain (0.1-0.2%) Sodium Azide and 0.02% sodium arsenite which is toxic and can be absorbed through the skin. When drained, the drains should be thoroughly flushed with water.**
- The reagents should be used as supplied and in accordance to the procedure mentioned below. Don't use beyond expiration date.
- Avoid cross contamination of reagents or specimens.
- Visible signs of microbial growth in any reagent may indicate degradation and the use of such reagent should be discontinued.

- Don't use these reagents if the label is not available or damaged.
- Do not use dark glass slide.
- Don't use the kit if damaged or the glass vials are broken or leaking and discard the contents immediately.
- Test materials and samples should be discarded properly in a biohazard container.
- Wash hands and the test table top with water and soap once the testing is done.
- Haemolysed blood sample should not be used for testing.
- The test should be performed at room temperature in a well lit area with very good visibility.
- Failure to follow the procedure in this package insert may give false results or safety hazard.
- Close the vial tightly after each test.
- The reagent is considered toxic, so don't drink or eat beside it.
- If spillage of reagent occurs clean with disinfectant (disinfectant used could be irritant so handle with care).

#### STORAGE CONDITIONS

- The reagents should be stored refrigerated between 2 - 8°C.
- Never Freeze or expose to elevated temperature.
- The reagent is stable until the expiry date stated on the product label. Do not use the reagents past the expiry date.

#### REAGENT PREPARATION

- The reagents are intended for use as supplied, no prior preparation or dilution of the reagent is required.
- All reagents should be brought to room temperature before use.

#### SPECIMEN COLLECTION AND PREPARATION

- Blood collected with or without anticoagulant (EDTA, Heparin or Citrate) can be used for Antigen typing.
- Note:** Blood collected without anticoagulant should be tested immediately.
- The specimens should be tested as soon as possible after collection. If testing is delayed, the specimens should be stored at 2- 8 °C. Sample must be retained to room temperature prior to analysis. (Testing should be carried out within five days of collections).
- Insure that there is no sign of hemolysis.
- At the time of the test, centrifuge the blood sample at 1200 RCF for 3 minutes.
- Blood collection is to be done with great care.

#### PROCEDURES

##### A. DIRECT TUBE METHOD AT ROOM TEMPERATURE

1. Prepare a 5% suspension of red blood cells in isotonic solution.
2. Using the vial dropper, transfer a drop (40±10µl) of each reagent into a separate and appropriately marked tube.
3. Add 50 µl of red blood cell suspension prepared in step 1.
4. Shake to homogenize the mixture, then centrifuge at 500g for 1 minute.
5. Gently shake the tube in such a way to detach the cell pellet and macroscopically observe for any possible agglutination.
6. Read the reaction immediately.
7. For Anti-D tube, if the reaction is weak or negative, shake the tubes and incubate at 37°C for 15 minutes.
8. Wash the red blood cells twice with isotonic saline solution (NaCl 0.9%) and discard the last washing liquid.
9. Add one drop (50µl) of the AHG reagent into the tube. Mix and centrifuge at 120g for 1 minute.
10. Gently shake the tube in such a way to detach the cell pellet and macroscopically observe for any possible agglutination.
11. Read the reaction immediately.

##### B. ANTIGLOBULIN INDIRECT METHOD for ANTI-D

1. After immediately centrifuging and reading as above, if the reaction is weak or negative, shake the tubes and incubate at 37°C for 15 minutes.
2. Wash the red blood cells twice with isotonic saline solution (NaCl 0.9%) and discard the last washing liquid.
3. Add one drop (40 µl ± 10 µl) of ANTI-HUMAN GLOBULIN to the tube. Mix and centrifuge at 120 (g) for 1 minute.
4. Gently shake the tube in such a way to detach the cell pellet and macroscopically observe for any possible agglutination.
5. Read the reaction immediately.

##### C. DIRECT SLIDE METHOD AT ROOM TEMPERATURE

1. Bring reagents and samples to room temperature (18-25°C).
2. Using the wax pen divide the slide into appropriate numbers of divisions.
3. Using the provided dropper, place one drop (40 µl ± 10 µl) of each reagent onto its correspondent division on the slide.
4. Add 25µl of the precipitated cells next to each drop of reagents.
5. Mix the reagent and the cells using a clean stirring stick over an area with a diameter of approximately 20-40mm.
6. Incubate the slide at room temperature (18-25°C) without stirring for 30 seconds.
7. Hold the slide and gently rock the slide for 3 minutes and observe macroscopically for any agglutination.
8. Read the reaction immediately.

## READING THE RESULT

**POSITIVE:** If Agglutination appears.

**NEGATIVE:** If no agglutination is observed.

Use the below table to determine the blood group:

Result of each reaction					ABO Group
Anti-A monoclonal reagent	Anti-B monoclonal reagent	Anti-AB monoclonal reagent	Anti-D IgG/IgM blend reagent		
+	-	+	+	A+	
+	-	+	-	A-	
-	+	+	+	B+	
-	+	+	-	B-	
+	+	+	+	AB+	
+	+	+	-	AB-	
-	-	-	+	O+	
-	-	-	-	O-	

## STABILITY OF THE REACTIONS

- ABO Blood Grouping Tube tests should be read immediately following centrifugation.
- Slide tests should be interpreted within three minutes to avoid the possibility that a negative result may be incorrectly interpreted as positive due to drying of reagents.
- Delay in reading and interpreting results may result in weekly positive or falsely negative reactions. Slide tests should be interpreted at the end of the three minutes.

## PROCEDURE LIMITATION

- False positive/ negative results may occur due to:
  - Contamination from test materials.
  - Improper storage, cells concentration, incubation time or temperature.
  - Improper or excessive centrifugation.
  - Deviation from the recommended technique.
  - Blood samples of weak A or B subgroups may give rise to false negative results or weak reactions when tested using slide test method. It is advisable to re-test weak subgroups using tube test method.
- Weaker reactions may be observed with stored blood than with fresh blood.
- ABO antigens are not fully developed at birth, weaker reactions may therefore occur with cord or neonatal red cells.
- ABO blood grouping interpretation on individuals greater than 6 months old should be confirmed by testing serum or plasma of the individual against group A and group B red cells (reverse grouping). If the results obtained with the serum do not correlate with the red cell test, further investigation is required.
- Return the kit to the agent if it does not function properly.
- Anti-D IgG/IgM blend Reagent tests conducted on particular weak-D phenotypes, while satisfactory, cannot ensure recognition of all weak variants, due to the variability of antigen patterns.

## DIAGNOSTIC PERFORMANCE CHARACTERISTICS

The following tables compare the results in slide and tube techniques of 3 lots of Atlas Medical reagents and the results of a CE marked device.

Slide Technique					
Group A					
Positive with anti-A monoclonal reagent and anti-AB monoclonal reagent					
Negative with anti-B and Negative control	CE marked device	Lot A	Lot B	Lot C	Compliance
232	232	232	232	232	100%
Tube Technique					
Group A					
Positive with anti-A monoclonal reagent and anti-AB monoclonal reagent					
Negative with anti-B and Negative control	CE marked device	Lot A	Lot B	Lot C	Compliance
212	212	212	212	212	100%
Slide Technique					
Group B					
Positive with anti-B monoclonal reagent and anti-AB monoclonal reagent					
Negative with anti-A and Negative control	CE marked device	Lot A	Lot B	Lot C	Compliance

CE marked device	Lot A	Lot B	Lot C	Compliance
Tube Technique				
Group B				
Positive with anti-B monoclonal reagent and anti-AB monoclonal reagent				
Negative with anti-A and Negative control				
CE marked device	Lot A	Lot B	Lot C	Compliance
61	61	61	61	100%

CE marked device	Lot A	Lot B	Lot C	Compliance
Slide Technique				
Group O				
Negative with anti-A monoclonal reagent, Anti-B monoclonal reagent and anti-AB monoclonal reagent				
Negative with Negative control				
CE marked device	Lot A	Lot B	Lot C	Compliance
241	241	241	241	100%
Tube Technique				
Group O				
Negative with anti-A monoclonal reagent, Anti-B monoclonal reagent and anti-AB monoclonal reagent				
Negative with Negative control				
CE marked device	Lot A	Lot B	Lot C	Compliance
243	243	243	243	100%

CE marked device	Lot A	Lot B	Lot C	Compliance
Slide Technique				
Group AB				
Positive with anti-A monoclonal reagent, Anti-B monoclonal reagent and anti-AB monoclonal reagent				
Negative with Negative control				
CE marked device	Lot A	Lot B	Lot C	Compliance
33	33	33	33	100%
Tube Technique				
Group AB				
Positive with anti-A monoclonal reagent, Anti-B monoclonal reagent and anti-AB monoclonal reagent				
Negative with Negative control				
CE marked device	Lot A	Lot B	Lot C	Compliance
24	24	24	24	100%

No inversion in diagnosis has been shown: from a qualitative point of view we have observed 100% compliance in direct group testing in slide and tube techniques for determination of A, B, AB and O groups for the three lots of Atlas Medical.

## QUALITY CONTROL

The reactivity of all blood grouping reagents should be confirmed by testing known positive and negative red blood cells on each day of use. To confirm the specificity and sensitivity, Blood grouping reagents should be tested with antigen-positive and antigen-negative red blood cells.

## REFERENCES

- BCSH Blood Transfusion Task Force. Guidelines for microplate techniques in liquid-phase blood grouping and antibody screening. Clin. Lab. Haem 1990; 12, 437-460.
- Issitt P. D. Applied Blood Group Serology, 3rd ed. Miami: Montgomery Scientific, 1985.
- Kholer G., Milstein C. Continuous culture of fused cells secreting antibody of predefined specificity, 256, 495-497, 1975
- Messeter L. et. al. Mouse monoclonal antibodies with anti-A, anti-B and anti-A,B specificities, some superior to human polyclonal ABO reagents, Vox Sang 46, 185-194, 1984
- Race R.R. and Sanger R. Blood groups in man, 6th ed., Oxford: Blackwell Scientific, 1975.
- Voak D. ET. al., Monoclonal anti-A and anti-B development as cost effective reagents. Med. Lab. Sci 39, 109-122. 1982.

7. Standards for Blood Banks and Transfusion Service. 11th Ed.,  
Washington D.C., AABB 1984:25.  
8. Widmann F.K.ed Technical Manual, 9th Ed., Washington D.C.: AABB  
1985:9.



**Atlas Medical GmbH**  
**Ludwig-Erhard-Ring 3**  
**15827 Blankenfelde-Mahlow**  
**Germany**  
**Tel: +49 - 33708 – 3550 30**  
**Email: [Info@atlas-medical.com](mailto:Info@atlas-medical.com)**  
**Website: [www.atlas-medical.com](http://www.atlas-medical.com)**

PPI861A01  
Rev.L (19.02.2022)

**CE 0459**

**LIST OF VARIENTS:**

Product Code	Product Name
8.02.00.0.0010	Anti-A Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 1 vial/Carton Box
8.02.00.1.0100	Anti-A Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 10 vials / Plastic Pack
8.02.00.1.0180	Anti-A Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 18 vials / Carton Box
8.02.01.0.0010	Anti-B Monoclonal Reagent (Titer: 1 /512), 10ml/vial, / Carton Box
8.02.01.1.0100	Anti-B Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 10 vials / Plastic Pack
8.02.01.1.0180	Anti-B Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 18 vials / Carton Box
8.02.02.0.0010	Anti-AB Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 1 vial/ Carton Box
8.02.02.1.0100	Anti-AB Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 10 vials/Plastic Pack
8.02.02.1.0180	Anti-AB Monoclonal Reagent (Titer: 1 /512), 10ml/vial, 18 vials/Carton Box
8.02.03.0.0010	Anti-D IgG/IgM Blend Reagent (Titer: 1 /128), 10ml/vial, 1 vial/ Carton Box
8.02.03.1.0100	Anti-D IgG/IgM Blend Reagent (Titer: 1 /128), 10ml/vial, 10 vials / Plastic Pack
8.02.03.1.0180	Anti-D IgG/IgM Blend Reagent (Titer: 1 /128), 10ml/vial, 18 vials / Carton Box
8.02.04.0.0010	Anti-A Monoclonal Reagent (Titer: 1 /256), 10ml/vial, 1 Vial/Carton Box
8.02.04.0.0100	Anti-A Monoclonal Reagent (Titer: 1 /256), 10ml/vial, 10 vials / Plastic Pack
8.02.05.0.0010	Anti-B Monoclonal Reagent (Titer: 1 /256), 10ml/vial, 1vial/Carton Box
8.02.05.0.0100	Anti-B Monoclonal Reagent (Titer: 1 /256), 10ml/vial, 10 vials /Plastic Pack
8.02.05.6.0030	ABO Set (Anti-A (1/256), Anti-B (1/256), Anti-D (1/64)),3x10ml / plastic Pack
8.02.05.7.0020	ABO Set: Anti-A (1/256), Anti-B (1/256), 2x10ml /Plastic Pack
8.02.06.0.0010	Anti-AB Monoclonal Reagent (Titer: 1 /256), 10ml/vial, 1vial/Carton Box
8.02.06.1.0100	Anti-AB Monoclonal Reagent (Titer: 1 /256), 10ml/vial,10 vials /Plastic Pack
8.02.06.1.0180	Anti-AB Monoclonal Reagent (Titer: 1 /256), 10ml/vial,18 vials / Carton Box
8.02.07.0.0010	Anti-D IgG/IgM Blend Reagent (Titer: 1 /64), 10ml/vial, 1Vial/ Carton Box
8.02.07.1.0100	Anti-D IgG/IgM Blend Reagent (Titer: 1 /64), 10ml/vial, 10 vials / Plastic Pack
8.02.47.0.0030	ABO Set (Anti-A (1 /512), Anti-B (1 /512), Anti-D (1 /128)),3x10ml/Plastic Pack
8.02.47.1.0030	ABO Set (Anti-A (1 /256), Anti-B (1 /256), Anti-D (1 /64)),3x10ml /Carton Box.
8.02.47.3.0030	ABO Set (Anti-A (1 /256), Anti-B (1 /256), Anti-D (1 /64)),3x10ml /Plastic Pack
8.02.47.5.0030	ABO Set (Anti-A (1 /256), Anti-B (1 /256), Anti-D (1 /128)),3x10ml/Plastic Pack
8.02.49.0.0040	ABO Set (Anti-A (1 /256), Anti-B (1 /256), Anti-AB (1 /256), Anti-D (1 /64)),4x10ml/Carton Box
8.02.49.2.0040	ABO Set (Anti-A (1 /256), Anti-B (1 /256), Anti-AB (1 /256), Anti-D (1 /128)), 4 x 10ml, 4 vials/Plastic Pack
8.02.53.0.0040	ABO Set (Anti-A (1 /512), Anti-B (1 /512), Anti-AB (1 /512) Anti-D (1 /128)), 4x10ml/Plastic Pack
8.02.53.1.0040	ABO Set (Anti-A (1 /512), Anti-B (1 /512), Anti-AB (1 /512) Anti-D (1 /128)), 4x10ml, 4vials/Plastic Pack
8.02.70.0.0010	Anti-A monoclonal reagent , Titer (1/1024), 10 ml/vial, 1Vial/ Carton Box
8.02.71.0.0010	Anti-B Monoclonal reagent (Titer: 1 /1024) , 10 ml/vial ,1Vial/ Carton Box
8.02.72.0.0010	Anti-AB Monoclonal reagent (Titer: 1 /1024) , 10 ml/vial , 1Vial/ Carton Box
8.02.85.0.0010	Anti-D IgG/IgM Blend reagent ( Titer 1 /256),10ml/vial, 1Vial/ Carton Box

<b>REF</b>	Catalogue Number		Temperature limit
<b>IVD</b>	In Vitro diagnostic medical device		Caution
	Contains sufficient for <n> tests and Relative size		Consult instructions for use (IFU)
<b>LOT</b>	Batch code		Manufacturer
	Fragile, handle with care		Use-by date
	Manufacturer fax number		Do not use if package is damaged
	Manufacturer telephone number		Date of Manufacture
	Keep away from sunlight		Keep dry

## ANTISTREPTOLYSIN-O (ASO) LATEX SLIDE TEST

For the qualitative and quantitative measurement of antibodies to Antistreptolysin-O in human serum.

**IVD** For in -vitro diagnostic and professional use only



### INTENDED USE

ATLAS ANTISTREPTOLYSIN-O (ASO) latex slide Test is used for the qualitative and quantitative measurement of antibodies to Antistreptolysin-O in human serum.

### INTRODUCTION

The group A  $\beta$ -hemolytic streptococci produces various toxins that can act as antigens. One of these exotoxins streptolysin-O, was discovered by Todd in 1932.

A person infected with group A  $\beta$ -hemolytic streptococci produces specific antibodies against these exotoxins, one of which is antistreptolysin-O. The quantity of this antibody in a patient's serum will establish the degree of infection due to the  $\beta$ -hemolytic streptococcal.

The usual procedure for the determination of the antistreptolysin titer is based on the inhibitory effect that the patient's serum produces on the hemolytic power of a pre-titrated and reduced streptolysin-O. However, the antigen-antibody reaction occurs independently of the hemolytic activity of streptolysin-O. This property enables the establishment of a qualitative and quantitative test for the determination of the antistreptolysin-O by agglutination of latex particles on slide.

### PRINCIPLE

ASO test method is based on an immunologic reaction between streptococcal exotoxins bound to biologically inert latex particles and streptococcal antibodies in the test sample. Visible agglutination occurs when increased antibody level, are present in the test specimen.

### MATERIALS

#### MATERIALS PROVIDED

- ASO Latex Reagent: Latex particles coated with streptolysin O, pH, 8.2. Preservative
- ASO Positive Control(Red cap): Human serum with an ASO concentration > 200 IU/mL.Preservative
- ASO Negative Control (Blue cap) Animal serum. Preservative
- Reaction Slide.
- Stirring Sticks.

#### MATERIALS REQUIRED BUT NOT PROVIDED

- Timer.
- Test Tubes 12x75mm.
- Test Tube Rack.
- Serological pipettes.
- High intensity light.
- Saline Solution, 0.9% NaCl.

#### PRECAUTIONS

- All reagents contain 0.1% (w/v) sodium azide as a preservative. Store all reagents at 2-8°C. **DO NOT FREEZE.**
- Reagents containing sodium azide may be combined with copper and lead plumbing to form highly explosive metal azides. Dispose of reagents by flushing with large amounts of water to prevent azide build-up.
- For In Vitro diagnostic use.
- Positive and negative controls prepared using human serum found negative for hepatitis B surface antigen (HBsAg) and HIV-III by FDA required test; however, handle controls as if potentially infectious.

#### REAGENT STORAGE AND STABILITY

- Reagents are stable until specified expiry date on bottle label when stored refrigerated (2-8°C).
- **DO NOT FREEZE.**
- The ASO Latex Reagent, once shaken must be uniform without visible clumping. When stored refrigerated, a slight sedimentation may occur and should be considered normal.
- Do not use the latex reagent or controls if they become contaminated.

#### SPECIMEN COLLECTION AND STORAGE

- Use fresh serum collected by centrifuging clotted blood.
- If the test cannot be carried out on the same day, store the specimen for 7 days at 2-8°C and for 3 months at -20°C.

- For longer periods the sample must be frozen.
- As in all serological tests, hemolytic or contaminated serum must not be used.
- **DO NOT USE PLASMA.**

#### PROCEDURE

##### Qualitative method

1. Allow the reagents and samples to reach room temperature. The sensitivity of the test may be reduced at low temperatures.
2. Place 50  $\mu$ L of the sample and one drop of each Positive and Negative controls into separate circles on the slide test.
3. Mix the ASO-latex reagent vigorously or on a vortex mixer before using and add one drop (50  $\mu$ L) next to the sample to be tested.
4. Mix the drops with a stirrer, spreading them over the entire surface of the circle. Use different stirrers for each sample.
5. Place the slide on a mechanical rotator at 80-100 r.p.m. for 2 minutes. False positive results could appear if the test is read later than two minutes.

##### Semi-quantitative method

1. Make serial two fold dilutions of the sample in 9 g/L saline solution.
2. Proceed for each dilution as in the qualitative method.

#### QUALITY CONTROL

Positive and Negative Controls should be included in each test batch.

Acceptable performance is indicated when a uniform milky suspension with no agglutination is observed with the ASO Negative Control and agglutination with large aggregates is observed with the ASO Positive Control.

#### RESULTS

##### A.QUALITATIVE TEST:

A negative reaction is indicated by a uniform milky suspension with no agglutination as observed with the ASO Negative Control.

A positive reaction is indicated by any observable agglutination in the reaction mixture. The specimen reaction should be compared to the ASO Negative Control (Fig. 1).

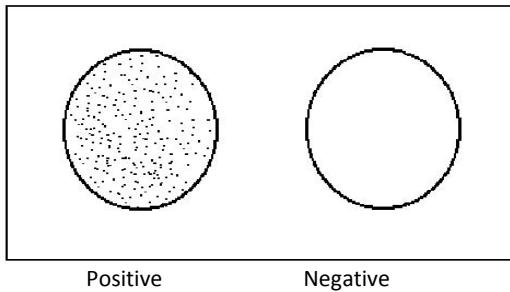


Figure 1

#### B. QUANTITATIVE TEST

A positive reaction is indicated by any observable agglutination in the reaction mixture. Record the last dilution showing a positive reaction. Concentration of ASO can be determined by multiplying the last positive dilution factor of the sample with the concentration of the positive control (200 IU/ml).

The titer of the serum is the reciprocal of the highest dilution which exhibits a positive reaction.

IU/ml of sample = conc. of positive control (200) x specimen titer

<u>DILUTION</u>	<u>IU/ml</u>
1:1	200
1:2	400
1:4	800
1:8	1600
Etc.	

#### REFERENCE VALUES

Up to 200 IU/mL(adults) and 100 IU/mL (children < 5 years old)<sup>6</sup>. Each laboratory should establish its own reference range.

#### PERFORMANCE CHARACTERISTICS

##### Analytical sensitivity:

200 ( $\pm 50$ ) IU/ml.

##### PROZONE EFFECT

No prozone effect was detected up to 1500IU/ml.

##### SENSITIVITY

98%.

##### SPECIFICITY

97%.

#### NON INTERFERING SUBSTANCES:

- Hemoglobin (10g/dl)
  - Bilirubin(20mg/dl)
  - Lipemia(10g/dl)
- Other substances may interfere

#### REFERENCES

1. Haffejee . Quarterly Journal of Medicine 1992. New series 84; 305: 641-658.
2. Ahmed Samir et al. Pediatric Annals 1992; 21: 835-842.
3. Spaun J et al. Bull Wld Hlth Org 1961; 24: 271-279.
4. The association of Clinical Pathologists 1961. Broadsheet 34.
5. Picard B et al. La Presse Medicale 1983; 23: 2-6.
6. Klein GC. Applied Microbiology 1971; 21: 999-1001.
7. Young DS. Effects of drugs on clinical laboratory test, 4th ed. AACC Press, 1995.

#### ATLAS Medical

William James House,  
Cowley Road, Cambridge, CB4 4WX, UK  
Tel: ++44 (0) 1223 858 910  
Fax: ++44 (0) 1223 858 524

#### PPI003A01

Rev H (09.09.2017)

<b>REF</b>	Catalogue Number		Store at
<b>IVD</b>	For In-Vitro Diagnostic use		Caution
	Number of tests in the pack		Read product insert before use
<b>LOT</b>	Lot (batch) number		Manufacturer
	Fragile, handle with care		Expiry date
	Manufacturer fax number		Do not use if package is damaged
	Manufacturer telephone		

#### INTERFERENCES

## ATLAS RHEUMATOID FACTOR (RF) LATEX KIT

latex slide test for the qualitative and semi-quantitative measurement of RF in human serum.

**IVD** For In-Vitro diagnostic and professional use only

2°C  8°C  
Store at 2-8°C

### INTENDED USE

A latex slide test for the qualitative and semi-quantitative measurement of RF in human serum.

### INTRODUCTION

Rheumatoid factors (RF) are antibodies directed against antigenic sites in the Fc fragment of human and animal IgG . Their frequent occurrence in rheumatoid arthritis makes them useful for diagnosis and monitoring of the disease.

One method used for rheumatoid factor detection is based on the ability of rheumatoid arthritis sera to agglutinate sensitized sheep red cells, as observed by Waaler and Rose. A more sensitive reagent consisting of biologically inert latex beads coated with human gamma globulin was later described by Singer and Plotz. The RF kit is based on the principle of the latex agglutination assay of Singer and Plotz .The major advantage of this method is rapid performance (2 minute reaction time) and lack of heterophile antibody interference.

### PRINCIPLE

The RF reagent is based on an immunological reaction between human IgG bound to biologically inert latex particles and rheumatoid factors in the test specimen. When serum containing rheumatoid factors is mixed with the latex reagent, visible agglutination occurs.

### MATERIALS

#### MATERIALS PROVIDED

- RF Latex Reagent: Latex particles coated with human gamma-globulin, pH, 8,2. Preservative. Contains N, N-dimethylformamide .
- RF Positive Control Serum: Human serum with a RF concentration > 30 IU/mL.Preservative.

- RF Negative Control Serum:Animal serum.
- Preservative.
- Reaction Slide
- Stirring sticks

#### MATERIALS REQUIRED BUT NOT PROVIDED

- Timer
- Test Tubes (for dilution)
- Serological pipettes (for sample addition and for dilution)
- Rotator (optional)
- Glycine Buffer (20x): add one part to nineteen parts of distilled water before use.

#### PRECAUTIONS

- All reagents contain 0.1 % ( w/v) sodium azide as a preservative.
- Reagents containing sodium azide may be combined with copper and lead plumbing to form highly explosive metal azides. Dispose of reagents by flushing with large amounts of water to prevent azide buildup.
- For In Vitro diagnostic use.
- Positive and negative controls prepared using human serum found negative for hepatitis B surface antigen (HBsAg) by FDA required test; however, handle controls as if potentially infectious.
- Accuracy of the test depends on the drop size of the latex reagent (40µl). Use only the dropper supplied with latex and hold it perpendicularly when dispensing.
- Use a clean pipette tip and stirring stick for each specimen, and glass slides should be thoroughly rinsed with water and wiped with lint-free tissue after each use.
- Check reactivity of the reagent using the controls provided.

#### STORAGE AND STABILITY

- Reagents are stable until specified expiry date on bottle label when stored refrigerated (2-8°C).
- Do not freeze.
- The RF latex reagent, once shaken must be uniform without visible clumping. When stored refrigerated, a slight sedimentation may occur and should be considered normal.
- Do not use the latex reagent or controls if they become contaminated.

#### SPECIMEN COLLECTION AND STORAGE

- Use fresh serum collected by centrifuging clotted blood.
- If the test cannot be carried out on the same day, store the specimen for 7 days at 2-8°C and for 3 months at -20°C.
- As in all serological tests, hemolytic or contaminated serum must not be used.
- Do not use PLASMA.

#### PROCEDURE

##### Qualitative method

1. Allow the reagents and samples to reach room temperature. The sensitivity of the test may be reduced at low temperatures.
2. Place 50 µL of the sample and one drop of each Positive and Negative controls into separate circles on the slide test.
3. Mix the RF-latex reagent vigorously or on a vortex mixer before using and add one drop (50 µL) next to the sample to be tested.
4. Mix the drops with a stirrer, spreading them over the entire surface of the circle. Use different stirrers for each sample.
5. Place the slide on a mechanical rotator at 80-100 r.p.m. for 2 minutes. False positive results could appear if the test is read later than two minutes.

##### Semi-quantitative method

1. Make serial two fold dilutions of the sample in 9 g/L saline solution.
2. Proceed for each dilution as in the qualitative method.

#### READING AND INTERPRETATION

Examine macroscopically the presence or absence of visible agglutination immediately after removing the slide from the rotator. The presence of agglutination indicates a RF concentration equal or greater than 8 IU/mL (Note 1).

The titer, in the semi-quantitative method, is defined as the highest dilution showing a positive result.

#### CALCULATIONS

The approximate RF concentration in the patient sample is calculated as follows:

$$8 \times \text{RF Titer} = \text{IU/mL}$$

## INTERFERENCES

### NON INTERFERING SUBSTANCES:

- Hemoglobin (10g/dl)
- Bilirubin(20mg/dl)
- Lipemia(10g/dl)

Other substances may interfere.

## QUALITY CONTROL

1. RF Positive and Negative Control should be included in each test batch.
2. Acceptable performance is indicated when a uniform milky suspension with no agglutination is observed with the RF Negative Control and agglutination with large aggregates is observed with the RF Positive Control.

## PERFORMANCE CHARACTERISTICS

### Analytical sensitivity

8(6-16) IU/ml, under the described assay conditions.

### PROZONE EFFECT

No prozone effect was detected up to 1500 IU/ml.

### DIAGNOSTIC SENSITIVITY

100%.

### DIAGNOSTIC SPECIFICITY

100%.

The diagnostic sensitivity and specificity have been obtained using 118 samples compared with the same method of a computer.

## LIMITATIONS

- Reaction time is critical. If reaction time exceeds 2 minutes, drying of the reaction mixture may cause false positive result.
- Freezing the RF Latex Reagent will result in spontaneous agglutination.
- Intensity of agglutination is not necessarily indicative of relative RF concentration; therefore, screening reactions should not be graded.
- Increased levels of RF may be found in some diseases other than rheumatoid arthritis such as infectious mononucleosis, sarcodosis, lupus erythematosus, Sjogren's syndrome.
- Certain patients with rheumatoid arthritis will not have the RF present in their serum.

- The incidence of false positive results is about 3-5 %.Individuals suffering from infectious mononucleosis, hepatitis, syphilis as well as elderly people may give positive results.
- Diagnosis should not be solely based on the results of latex method but also should be complemented with a Waaler Rose test along with the clinical examination.

## REFERENCE VALUES

Up to 8 IU/mL. Each laboratory should establish its own reference range.

## NOTES

1. Results obtained with a latex method do not compare with those obtained with Waaler Rose test. Differences in the results between methods do not reflect differences in the ability to detect rheumatoid factors.

## REFERENCES

1. Robert W Dorner et al. Clinica Chimica Acta 1987; 167: 1 – 21.
2. Frederick Wolfe et al. Arthritis and Rheumatism 1991; 34: 951- 960.
3. Robert H Shmerling et al. The American Journal of Medicine 1991; 91: 528 –534.
4. Adalbert F. Schubart et al. The New England Journal of Medicine 1959; 261: 363 – 368.
5. Charles M. Plotz 1956; American Journal of Medicine; 21:893 – 896.
6. Young DS. Effects of drugs on clinical laboratory test, 4th ed. AACC Press, 1995.

## ATLAS MEDICAL

William James House Cowley Road,

Cambridge, CB4 0WX, UK.

Tel: +44 (0) 1223 858 910

Fax: +44 (0) 1223 858 524

PPI008A01, Rev H (17.06.2017)

REF	Catalogue Number		Store at
IVD	For In-Vitro Diagnostic use	⚠	Caution
Σ	Number of tests in the pack	📖	Read product insert before use
LOT	Lot (batch) number	💻	Manufacturer
glass	Fragile, handle with care	✉	Expiry date
fax	Manufacturer fax number	🚫	Do not use if package is damaged
phone	Manufacturer telephone number		



ФЕДЕРАЛЬНАЯ СЛУЖБА ПО НАДЗОРУ В СФЕРЕ ЗДРАВООХРАНЕНИЯ  
(РОСЗДРАВНАДЗОР)

## РЕГИСТРАЦИОННОЕ УДОСТОВЕРЕНИЕ НА МЕДИЦИНСКОЕ ИЗДЕЛИЕ

от 07 мая 2019 года № РЗН 2019/8352

На медицинское изделие

Индикаторы химические для контроля процесса паровой и воздушной стерилизации по ТУ 20.59.52-001-35927791-2017

Настоящее регистрационное удостоверение выдано

Общество с ограниченной ответственностью "Научно-Производственное Объединение "Маркер" (ООО "НПО "Маркер"), Россия,  
117292, Москва, ул. Профсоюзная, д. 26/44

Производитель

Общество с ограниченной ответственностью "Научно-Производственное Объединение "Маркер" (ООО "НПО "Маркер"), Россия,  
117292, Москва, ул. Профсоюзная, д. 26/44

Место производства медицинского изделия

ООО «НПО Маркер», Россия, 300013, г. Тула, Привокзальный р-н,  
ул. Болдина, д. 98а, лит. Е

Номер регистрационного досье № РД-25642/72833 от 30.01.2019

Класс потенциального риска применения медицинского изделия I

Код Общероссийского классификатора продукции по видам экономической деятельности 32.50.50.000

Настоящее регистрационное удостоверение имеет приложение на 2 листах

приказом Росздравнадзора от 07 мая 2019 года № 3413  
допущено к обращению на территории Российской Федерации.

Врио руководителя Федеральной службы  
по надзору в сфере здравоохранения

Д.В. Пархоменко

0039607

**ПРИЛОЖЕНИЕ**  
**К РЕГИСТРАЦИОННОМУ УДОСТОВЕРЕНИЮ**  
**НА МЕДИЦИНСКОЕ ИЗДЕЛИЕ**

от 07 мая 2019 года

№ РЗН 2019/8352

Лист 1

На медицинское изделие

**Индикаторы химические для контроля процесса паровой и воздушной стерилизации по ТУ 20.59.52-001-35927791-2017, в вариантах исполнения:**

1. Индикаторы химические для контроля процесса паровой и воздушной стерилизации, в составе:

1.1. Интегрирующий индикатор «Маркер», 5 класс для контроля процесса паровой и воздушной стерилизации.

1.2. Многопараметрический индикатор «ХимТест», 4 класс для контроля параметров паровой стерилизации для режимов: 121 °C /20 мин, 126 °C /10 мин, 134 °C /5 мин.

1.3. Многопараметрический индикатор «ХимТест», 4 класс для контроля параметров воздушной стерилизации для режимов: 160 °C /150 мин, 180 °C /60 мин, 200 °C /30 мин.

1.4. Имитирующий индикатор «Маркер-Прион», 6 класс для контроля параметров паровой стерилизации для режима: 134 °C /18 мин.

2. Индикаторы химические для контроля процесса паровой и воздушной стерилизации лекарственных средств, в составе:

2.1. Многопараметрический индикатор «Маркер-Фарм», 4 класс для контроля параметров паровой и воздушной стерилизации для режимов: 100 °C /30 мин, 110 °C /20 мин, 120 °C /15 мин, 180 °C /30 мин.

2.2. Многопараметрический индикатор «ХимТест-Фарм-1», 4 класс для контроля параметров паровой стерилизации для режимов: 100 °C /15 мин, 110 °C /10 мин, 120 °C /8 мин.

2.3. Многопараметрический индикатор «ХимТест-Фарм-2», 4 класс для контроля параметров паровой стерилизации для режимов: 110 °C /15 мин, 120 °C /12 мин.

2.4. Многопараметрический индикатор «ХимТест-Фарм-3», 4 класс для контроля параметров паровой стерилизации для режимов: 100 °C /30 мин, 110 °C /20 мин, 120 °C /15 мин.

2.5. Многопараметрический индикатор «ХимТест-Фарм-4», 4 класс для контроля параметров паровой стерилизации для режимов: 112 °C /20 мин, 121 °C /15 мин.

2.6. Многопараметрический индикатор «ХимТест-Фарм-5», 4 класс для контроля параметров паровой стерилизации для режимов: 140 °C /30 мин, 121 °C /20 мин.

2.7. Многопараметрический индикатор «ХимТест-Фарм-6», 4 класс для контроля параметров паровой стерилизации для режима: 120 °C /30 мин.

2.8. Многопараметрический индикатор «ХимТест-Фарм-7», 4 класс для контроля

Врио руководителя Федеральной службы  
по надзору в сфере здравоохранения

Д.В. Пархоменко

00555896

ФЕДЕРАЛЬНАЯ СЛУЖБА ПО НАДЗОРУ В СФЕРЕ ЗДРАВООХРАНЕНИЯ  
(РОСЗДРАВНАДЗОР)

**ПРИЛОЖЕНИЕ  
К РЕГИСТРАЦИОННОМУ УДОСТОВЕРЕНИЮ  
НА МЕДИЦИНСКОЕ ИЗДЕЛИЕ**

от 07 мая 2019 года

№ РЗН 2019/8352

Лист 2

параметров воздушной стерилизации для режима: 180 °C /30 мин.

2.9. Многопеременный индикатор «ХимТест-Фарм-8», 4 класс для контроля параметров воздушной стерилизации для режима: 180 °C /45 мин.

3. Индикаторы химические для контроля процесса стерилизации (парового обеззараживания) медицинских отходов, в составе:

3.1. Многопеременный индикатор «ХимТест-О-1», для контроля параметров парового обеззараживания для режимов: 120 °C /90 мин, 126 °C /60 мин, 132 °C /45 мин, 134 °C /27 мин.

3.2. Многопеременный индикатор «ХимТест-О-2», для контроля параметров парового обеззараживания для режимов: 120 °C /120 мин, 126 °C /90 мин, 132 °C /60 мин, 134 °C /35 мин.

3.3. Многопеременный индикатор «ХимТест-О-3», для контроля параметров парового обеззараживания для режимов: 132 °C /90 мин, 134 °C /60 мин.

№

Врио руководителя Федеральной службы  
по надзору в сфере здравоохранения



Д.В. Пархоменко

0055897

**ООО «Научно-Производственное Объединение Маркер»**

ИНН: 7728890217

КПП: 772801001

ОГРН: 5147746104182

117292, г. Москва, ул. Профсоюзная, д. 26/44

тел.: +7 (495) 178-02-08; e-mail: info@nptmarker.ru

**Индикаторы химические для контроля процесса паровой и воздушной стерилизации  
ТУ 20.59.52-001-35927791-2017**

**ПАСПОРТ**

03.03.2020

*Индикаторы химические для контроля процесса паровой и воздушной стерилизации:*

многопеременный индикатор «ХимТест», 4 класс для контроля параметров воздушной стерилизации для режимов: 160 °C /150 мин, 180 °C /60 мин, 200 °C /30 мин;

Партия № 2503/2

Дата изготовления: март 2020 г.

Годен до: март 2025 г.

Вид исполнения: листы с индикаторами

**Результаты приемосдаточных испытаний**

Наименование испытаний (проверок)	№№ пунктов ТУ (технических требований)	Результат испытаний
Проверка соответствия комплекту документации	1.1.1	соответствует
Проверка исполнений, общего внешнего вида, конструкции, формы, материалов, основных размеров, массы	1.2.1-1.2.3	соответствует
Проверка условий достижения конечного состояния	1.2.4, 1.2.5	соответствует
Проверка условий не достижения конечного состояния	1.2.6	соответствует
Проверка комплектности, маркировки и упаковки	1.3, 1.4, 1.5	соответствует

Генеральный директор ООО «НПО Маркер»

И.П. Антонова



**ООО «Научно-Производственное Объединение Маркер»**

ИНН: 7728890217

КПП: 772801001

ОГРН: 5147746104182

117292, г. Москва, ул. Профсоюзная, д. 26/44

тел.: +7 (495) 178-02-08; e-mail: info@promarker.ru

**Индикаторы химические для контроля процесса паровой и воздушной стерилизации  
ТУ 20.59.52-001-35927791-2017**

**ПАСПОРТ**

03.03.2020

*Индикаторы химические для контроля процесса паровой и воздушной стерилизации:*

многопеременный индикатор «ХимТест», 4 класс для контроля параметров паровой стерилизации для режимов: 120 °С /45 мин, 126 °С /30 мин, 132 °С /20 мин;

Партия № 2503/2

Дата изготовления: март 2020 г.

Годен до: март 2025г.

Вид исполнения: листы с индикаторами

**Результаты приемосдаточных испытаний**

Наименование испытаний (проверок)	№№ пунктов ТУ (технических требований)	Результат испытаний
Проверка соответствия комплекту документации	1.1.1	соответствует
Проверка исполнений, общего внешнего вида, конструкции, формы, материалов, основных размеров, массы	1.2.1-1.2.3	соответствует
Проверка условий достижения конечного состояния	1.2.4, 1.2.5	соответствует
Проверка условий не достижения конечного состояния	1.2.6	соответствует
Проверка комплектности, маркировки и упаковки	1.3, 1.4, 1.5	соответствует

Генеральный директор ООО «НПО Маркер»

И.П. Антонова



**ООО «Научно-Производственное Объединение Маркер»**

ИНН: 7728890217

КПП: 772801001

ОГРН: 5147746104182

117292. г. Москва, ул. Профсоюзная, д. 26/44

тел.: +7 (495) 178-02-08; e-mail: info@promarker.ru

**Индикаторы химические для контроля процесса паровой и воздушной стерилизации  
ТУ 20.59.52-001-35927791-2017**

**ПАСПОРТ**

03.03.2020

*Индикаторы химические для контроля процесса паровой и воздушной стерилизации:  
многопараметрический индикатор «ХимТест», 4 класс для контроля параметров паровой  
стерилизации для режимов: 121 °C /20 мин, 126 °C /10 мин, 134 °C /5 мин;*

Партия № 2503/2

Дата изготовления: март 2020 г.

Годен до: март 2025г.

Вид исполнения: листы с индикаторами

**Результаты приемосдаточных испытаний**

Наименование испытаний (проверок)	№№ пунктов ТУ (технических требований)	Результат испытаний
Проверка соответствия комплекту документации	1.1.1	соответствует
Проверка исполнений, общего внешнего вида, конструкции, формы, материалов, основных размеров, массы	1.2.1-1.2.3	соответствует
Проверка условий достижения конечного состояния	1.2.4, 1.2.5	соответствует
Проверка условий не достижения конечного состояния	1.2.6	соответствует
Проверка комплектности, маркировки и упаковки	1.3, 1.4, 1.5	соответствует

Генеральный директор ООО «НПО Маркер»

И.П. Антонова



**ООО «Научно-Производственное Объединение Маркер»**

ИНН: 7728890217

КПП: 772801001

ОГРН: 5147746104182

117292, г. Москва, ул. Профсоюзная, д. 26/44

тел.: +7 (495) 178-02-08; e-mail: info@promarker.ru

**Индикаторы химические для контроля процесса паровой и воздушной стерилизации  
ТУ 20.59.52-001-35927791-2017**

**ПАСПОРТ**

03.03.2020

*Индикаторы химические для контроля процесса паровой и воздушной стерилизации:*

многопеременный индикатор «ХимТест-Фарм-4», 4 класс для контроля параметров паровой стерилизации для режимов: 112 °C /20 мин, 121 °C /15 мин;

Партия № 2503/2

Дата изготовления: март 2020 г.

Годен до: март 2025 г.

Вид исполнения: листы с индикаторами

**Результаты приемосдаточных испытаний**

Наименование испытаний (проверок)	№№ пунктов ТУ (технических требований)	Результат испытаний
Проверка соответствия комплекту документации	1.1.1	соответствует
Проверка исполнений, общего внешнего вида, конструкции, формы, материалов, основных размеров, массы	1.2.1-1.2.3	соответствует
Проверка условий достижения конечного состояния	1.2.4, 1.2.5	соответствует
Проверка условий не достижения конечного состояния	1.2.6	соответствует
Проверка комплектности, маркировки и упаковки	1.3, 1.4, 1.5	соответствует

Генеральный директор ООО «НПО Маркер»

И.П. Антонова

