

STATEMENT

We, ACON Laboratories, Inc., having a registered office at *5850 Oberlin Drive #340, San Diego, CA 92121* authorize SRL Sanmedico having a registered office at *A. Corobceanu street 7A, apt. 9, Chisinău, MD-2012, Moldova*

to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

Date: March 18, 2024

Signature:



Qiyi Xie, Md, MPH
V.P. of Regulatory & Clinical Affairs
ACON Laboratories, Inc.



Certificate

No. Q5 104507 0001 Rev. 03

Holder of Certificate: **ACON Laboratories, Inc.**
5850 Oberlin Drive, #340
San Diego CA 92121
USA

Certification Mark:



Scope of Certificate: **Design and Development, Manufacture and distribution of In Vitro Diagnostic Test Kits and Reagents for the Determination of Infectious Diseases, Clinical Chemistry, Drugs of Abuse, Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose Monitoring System, Lancing Devices and Lancets**

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: www.tuvsud.com/ps-cert?q=cert:Q5 104507 0001 Rev. 03

Report No.: SH22743A01

Valid from: 2022-09-15
Valid until: 2025-09-06

Date, 2022-09-15

Christoph Dicks
Head of Certification/Notified Body

Certificate

No. Q5 104507 0001 Rev. 03

Applied Standard(s):

EN ISO 13485:2016
Medical devices - Quality management systems -
Requirements for regulatory purposes
(ISO 13485:2016)
DIN EN ISO 13485:2016

Facility(ies):

ACON Laboratories, Inc.
5850 Oberlin Drive, #340, San Diego CA 92121, USA

Address holder for registration only

ACON Laboratories, Inc.
10125 Mesa Rim Road, San Diego CA 92121, USA

Manufacture and distribution of
In Vitro Diagnostic Test Kits and Reagents for the Determination of
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose
Monitoring System, Lancing Devices and Lancets

ACON Laboratories, Inc.
6865 Flanders Dr., Suite B, San Diego CA 92121, USA

Storage of
In Vitro Diagnostic Test Kits and Reagents for the Determination of
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose
Monitoring System, Lancing Devices and Lancets

AZURE Institute, Inc.
10125 Mesa Rim Road, San Diego CA 92121, USA

Design and Development of
In Vitro Diagnostic Test Kits and Reagents for the Determination of
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose
Monitoring System, Lancing Devices and Lancets

Acon Laboratories Inc.
Guerrero Negro 9942 Parque Industrial Pacifico IV, 22644
Tijuana B.C. CP, MEXICO

Manufacture of
blood glucose test strips, antigen rapid test and IgG/IgM antibody
rapid test for infectious disease.



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-245.10.07



Product Service

EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)
(List A and B and devices for self-testing)

No. V1 104507 0003 Rev. 06

Manufacturer:

ACON Laboratories, Inc.

5850 Oberlin Drive, #340
San Diego CA 92121
USA

**Product Category(ies): Blood glucose measuring systems for self testing
and self-testing devices for clinical chemistry,
hematology and pregnancy and ovulation**

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for design, manufacture and final inspection of the respective devices / device families in accordance with IVDD Annex IV. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of List A devices an additional Annex IV (4) certificate is mandatory. All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:V1 104507 0003 Rev. 06](http://www.tuvsud.com/ps-cert?q=cert:V1_104507_0003_Rev.06)

Report no.:

SH22743EXT01

Valid from:

2022-05-04

Valid until:

2025-05-26

Date,

2022-05-04

Christoph Dicks
Head of Certification/Notified Body



EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)
(List A and B and devices for self-testing)

No. V1 104507 0003 Rev. 06

Model(s):

On Call Plus Blood Glucose Monitoring System,
On Call Plus Blood Glucose Test Strips,
On Call EZ II Blood Glucose Monitoring System,
On Call Advanced Blood Glucose Monitoring System,
On Call Advanced Blood Glucose Test Strips,
On Call Chosen Blood Glucose Test Strips,
On Call Vivid Blood Glucose Monitoring System (OGM-101),
On Call Vivid Blood Glucose Test Strips (OGS-101),
On Call Sharp Blood Glucose Monitoring System (OGM-121),
On Call Sharp Blood Glucose Test Strips (OGS-121)
On Call Plus II Blood Glucose Monitoring System (OGM-171),
On Call Plus II Blood Glucose Test Strips (OGS-171),
On Call Extra Blood Glucose Monitoring System (OGM-191),
On Call Extra Blood Glucose Test Strips (OGS-191),
On Call GK Dual Blood Glucose & Ketone Monitoring System (OGM-161),
On Call Blood Ketone Test Strips (OGS-161),
Urinalysis Reagent Strips (Urine),
UTI Urinary Tract Infection Test Strips,
Cholesterol Monitoring System (CCM-111),
CHOL Total Cholesterol Test Devices (CCS-111),
TRIG Triglycerides Test Devices (CCS-112),
HDL High Density Lipoprotein Test Devices (CCS-113),
3-1 Lipid Panel Test Devices (CCS-114),
Cholesterol CTRL Control Devices,
Cholesterol Monitoring System (CCM-101),
CHOL Total Cholesterol Test Strips (CCS-101),
PT/INR Monitoring System (CCM-151),
PT/INR Test Strips (CCS-151),
Hemoglobin Testing System (CCM-141),
Hemoglobin Test Strips (CCS-141),
hCG Pregnancy Rapid Test Cassette (Urine),
Pregnancy Rapid Test Midstream,
On Call Extra Mobile Blood Glucose Monitoring System (OGM-281),
On Call Sure Blood Glucose Monitoring System (OGM-211),
On Call Sure Sync Blood Glucose Monitoring System (OGM-212),
On Call Sure Blood Glucose Test Strips (OGS-211),
GIMA Blood Glucose Monitoring System,
GIMA Bluetooth Blood Glucose Monitoring System,
GIMA Blood Glucose Test Strips,
On Call GU Dual Blood Glucose & Uric Acid Monitoring



EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)
(List A and B and devices for self-testing)

No. V1 104507 0003 Rev. 06

System (OGM-201),
On Call Blood Uric Acid Test Strips (OGS-201),
LH Ovulation Rapid Test Cassette (Urine),
Ovulation Rapid Test Midstream,
Ovulation & Pregnancy Test Combo Pack,
On Call Extra Voice Blood Glucose Monitoring System
(OGM-291),
Early Detection Pregnancy Test,
Digital Pregnancy Test,
Go-Keto Blood Glucose & Ketone Monitoring System (OGM-
161),
Go-Keto Blood Ketone Test Strips (OGS-161),
Go-Keto Blood Glucose Test Strips,
On Call Extra GM Blood Glucose Monitoring System(OGM-
191),
On Call Extra GM Blood Glucose Test Strips (OGS-191),
On Call Plus GM Blood Glucose Monitoring System,
On Call Plus GM Blood Glucose Test Strips,
Go-Keto Urinalysis Reagent Strips

Facility(ies):

ACON Laboratories, Inc.
5850 Oberlin Drive, #340, San Diego CA 92121, USA

ACON Laboratories, Inc.
10125 Mesa Rim Road, San Diego CA 92121, USA

AZURE Institute, Inc.
10125 Mesa Rim Road, San Diego CA 92121, USA

Acon Laboratories Inc.
Guerrero Negro 9942 Parque Industrial Pacifico IV, 22644 Tijuana
B.C. CP, MEXICO

Declaration of Conformity

ACON Laboratories, Incorporated
5850 Oberlin Drive #340
San Diego, CA 92121, USA

**We, the manufacturer, declare under our sole responsibility that the
in vitro diagnostic device:**

Mission[®] Urinalysis Reagent Strips (U031-XX1)

classified as Others in the directive 98/79/EC,

**meets all the provisions of the directive 98/79/EC on *in vitro* diagnostic
medical devices which apply to it**

**The self-declaration is according to Annex III
(excluding Section 6) of the Directive.**

Authorized Representative:
Medical Device Safety Service GmbH
Schiffgraben 41
30175 Hannover, Germany

Signed this 11 day of February, 2020
in San Diego, CA USA



Qiyi Xie, MD, MPH
Senior Staff, Regulatory Affairs & Clinical Affairs
Acon Laboratories, Inc.



Mission® Urinalysis Reagent Strips and Urine Analyzers

Obtain reliable and cost-effective results with *Mission®* Urinalysis Reagent Strips and Urine Analyzers!

- *Accurate*
- *Reliable*
- *Convenient*



Global Diagnostics for Local Markets™

Urinalysis Reagent Strips

Simple and Accurate


- Analytical sensitivity better than or comparable to market leaders
- High quality color chart ensures accurate visual reading

Flexible


- Compatible for visual and analyzer reading
- More than 30 different combinations available

Multiple Packaging Options and Long Shelf Life


- Canister Packaging
 - Available in 25, 50, 100 and 150 strips per kit
 - 2 year shelf life for unopened canisters which offers cost savings and convenience for high volume testing
 - 3 month shelf life for strips in opened canisters
- Pouch Packaging *New!*
 - Single-strip Pouch
 - Individually packaged strips with 1, 3, 6 and 20 strips and 1 color chart per kit for OTC or low volume testing
 - Unique packaging maintains 2 year shelf life for all strips in the kit compared to 3 months for remaining strips in an opened canister
 - Multi-strip Pouch
 - Canister Refill Kits with 25 strips/pouch uniquely packaged to save cost for low volume testing and extended shelf life by using the canister for refills



Step 1: Immerse strip into urine



Step 2: Remove excess urine

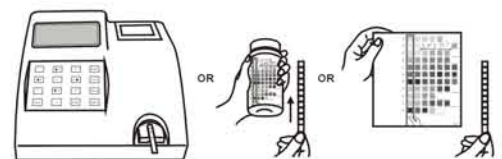

Step 3: Obtain results by analyzer or visual reading

Catalog No.	No. of Parameters	Type of Strip [♦]		Strips per Canister [◊]	Pouch Packaging [▲]	Reading Method			Analyzer-Read Strips: Standard (S) or Additional (A)	Parameters												
		For Visual Reading	For Analyzer Reading (U120/U500)			Visual	U120	U500		ASC	GLU	BIL	KET	SG	BLO	pH	PRO	URO	NIT	LEU	ALB	CRE
U031-131	13	13C	NA	100 [■]	✓	✓	NA	NA	A	*	*	*	*	*	*	*	*	*	*	*	*	*
U031-111	11	11A		100	✓	✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*		
U031-101	10	10U		100	✓	✓	✓	✓	S		*	*	*	*	*	*	*	*	*	*		
		10A				✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*			
		10C				✓	✓	✓	S		*	*	*	*	*	*	*	*	*	*	*	
U031-091	9	9U		100	✓	✓	✓	✓	S		*	*	*	*	*	*	*	*	*			
U031-081	8	8U		100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*			
		8N				✓	✓	✓	S		*	*	*	*	*	*	*	*	*			
		8S				✓	✓	✓	A		*	*	*	*	*	*	*	*	*			
U031-071	7	7N		100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*			
U031-061	6	6N	6NE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*			
		6U	6UE			✓	✓	✓			*	*	*	*	*	*	*	*				
U031-051	5	5B	5BE	100	✓	✓	✓		A		*	*	*	*	*	*	*	*	*			
		5N	5NE			✓	✓	✓			*	*	*	*	*	*	*	*				
		5S	5SE			✓	✓				*	*	*	*	*	*	*	*				
		5U	5UE			✓	✓				*	*	*	*	*	*	*	*				
U031-041	4	4S	4SE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*			
		4B	4BE			✓	✓				*	*	*	*	*	*	*	*				
		4K	4KE			✓	✓	✓			*	*	*	*	*	*	*	*				
		4G	4GE			✓	✓				*	*	*	*	*	*	*	*				
		4N	4NE			✓	✓	✓			*	*	*	*	*	*	*	*				
		4P	4PE			✓	✓	✓			*	*	*	*	*	*	*	*				
U031-031	3	3P	3PE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*			
		3K	3KE			✓	✓	✓			*	*	*	*	*	*	*	*				
		3G	3GE			✓	✓	✓			*	*	*	*	*	*	*	*				
		3N	3NE			✓	✓	✓			*	*	*	*	*	*	*	*				
U031-021	2	2G	2GE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*			
		2K	2KE			✓	✓	✓			*	*	*	*	*	*	*	*				
		2N	2NE			✓	✓	✓			*	*	*	*	*	*	*	*				
		2B	2BE			✓	✓	✓			*	*	*	*	*	*	*	*				
		2U	2UE			✓	✓	✓			*	*	*	*	*	*	*	*				
		2S	2SE			✓	✓	✓			*	*	*	*	*	*	*	*				
		2C	2CE	100 [■]	✓	✓	✓		*	*	*	*	*	*	*	*	*	*				
U031-011	1	1B	1BE	100	✓	✓	✓		A		*	*	*	*	*	*	*	*	*			
		1P	1PE			✓	✓	✓			*	*	*	*	*	*	*	*				
		1G	1GE			✓	✓	✓			*	*	*	*	*	*	*	*				
		1K	1KE			✓	✓	✓			*	*	*	*	*	*	*	*				
		1R	1RE			✓	✓	✓			*	*	*	*	*	*	*	*				

♦ Type of Strip:
Visual Strip Size
1-6 Parameters: 5 mm x 80 mm; 7-11 Parameters: 5 mm x 108 mm;
12-13 Parameters: 5 mm x 121 mm
U120/U500 Strip Size
1-11 Parameters: 5 mm x 108 mm;
"E" means extended strip length for 1-6 Parameters

◊ Also available in canisters of 25, 50 and 150 strips
■ Not available in canisters of 150 strips
▲ Single-strip Pouch available in 1, 3, 6 and 20 strip kit
Canister Refill Kit, with 25 strips per pouch or canister, available in 3-pouch and 1- canister kit, or 4-pouch kit

CE Marked for sale in the European Community
Cleared for US 510(k)



U120 Urine Analyzer



Accurate

- Up to 120 tests/hour in Continuous Test Option
- Capable of reading 1 strip at a time in Single Test Option
- Test modes include Routine, STAT and QC
- Automatic calibration for accurate results and easy operation

Reliable

- Can read up to 4 Strip combinations with 8, 9, 10, 11 parameters, additional strips with 1-11 parameters available upon request
- Minimal training required

Convenient Operation

- Saves and recalls the last 2,000 results automatically
- Audible beep signals operator to dip strips in urine
- Can print up to 3 copies per test for convenient reviewing and easy record keeping
- Option to print results on sticker paper for quick and simple record management

Easy Data Management

- Includes RS232C port for easy data transfer to an external computer or LIS
- Optional Barcode Reader to record patient ID

Unique Lockout Functions *new!*

- Strip Lockout
 - Prevents using strips of another brand on the U120 Urine Analyzer
 - Requires barcode reader scan or manual entry of the canister code
- User Lockout
 - Eliminates unapproved users from testing
 - Up to 10 lab operators can perform testing, but only the lab administrator can change analyzer settings
- QC Lockout
 - Prevents testing without passing QC
 - QC tests can be performed once every 8 hours, day, week or month
 - Analyzer will alert when to run QC test
 - If QC tests fail, analyzer will switch to STAT mode and list "E" at the end of each test number

Specifications

Feature	Specifications
Analyzer Type	Manual
Methodology	Reflectance Photometry
Detection	Photosensitive Diode
Throughput	Single Test Option: 60 tests/hour Continuous Test Option: 120 tests/hour
Test Modes	Routine, STAT and QC
Lockout Functions	Strip Lockout: Available Upon Request; User/QC Lockout: Included with option to turn ON/OFF
Memory	Last 2,000 results
Strip Incubation Time	1 Minute
Wavelength of Monochromatic LED	525 nm and 635 nm
Standard Strips	8, 9, 10, 11 Parameters (5 mm x 108 mm)
Additional Strips Available	1-11 Parameters (5 mm x 108 mm); see URS Parameters
Total Combinations Per Analyzer	4 Combinations
Analyzer Ports	Standard RS232C Port for Barcode Reader or Data Transfer USB Port for Data Transfer 25 Pin Parallel Port for External Printer
Capabilities	Internal Thermal Printer (included) RS232C Barcode Reader (optional) Optional External Printer (not included) USB or RS232C Data Transfer Cable (optional)
Major Readable Barcodes	Code 128, Code 39, Codabar (NW-7), Interleaved 25, UPC-A, UPC-E, EAN 8, EAN 13
Calibration	Automatic
Available Languages on the Screen	English and additional language(s)
Operating Conditions	0-40°C (32-104°F); ≤ 85% RH
Storage Conditions	-5-50°C (23-122°F); ≤ 90% RH
Power Source	100-240 VAC, 50-60 Hz
Dimensions (L x W x H)	27.2 cm x 26.9 cm x 14.6 cm (10.7" x 10.6" x 5.7")
Display Dimensions (L x W)	10.8 cm x 5.7 cm (4.2" x 2.2")
Weight	2.6 kg (5.7 lbs)

Ordering Information

Product Name	Catalog No.	Components		Kit Box Dimensions (L x W x H) & Weight	Carton Dimensions (L x W x H) & Weight	Number of Kits/Carton
U120 Urine Analyzer	U111-101 [†]	1 Urine Analyzer 1 Strip holder 2 Printer Paper Rolls	2 Fuses (2.0A) 1 Power Cord 1 Quick Start Guide 1 Instruction Manual	42.0 cm x 41.5 cm x 31 cm; 5.0 kg 16.4" x 16.2" x 12.1"; 176.4 oz		1
U120 Urine Analyzer with Barcode Reader	U111-111 [†]	1 Urine Analyzer 1 Strip holder 2 Printer Paper Rolls 1 Barcode Reader (RS232C)	2 Fuses (2.0A) 1 Power Cord 1 Serial Splitter Cable (RS232C) 1 Quick Start Guide 1 Instruction Manual	44.5 cm x 44.5 cm x 40.0 cm; 5.5 kg 17.5" x 17.5" x 15.7"; 194 oz		1
Barcode Reader	U221-111 [†]	1 Barcode Reader (RS232C)	1 Serial Splitter Cable (RS232C)	23.6 cm x 10.8 cm x 7.8 cm; 0.482 kg 9.3" x 4.3" x 3.1"; 17.0 oz	63.0 cm x 37.0 cm x 30.0 cm; 12.0 kg 24.8" x 14.6" x 11.8"; 423.3 oz	22
Printer Paper Rolls	U121-101	4 Printer Paper Rolls	Thermal Paper (0.06 m x 20 m): 200 results/roll Sticker Paper (0.06 m x 9 m): 100 results/roll	12.0 cm x 12.0 cm x 6.5 cm; 0.36 kg 4.7" x 4.7" x 2.6"; 12.7 oz	63.0 cm x 37.0 cm x 30.0 cm; 19.4 kg 24.8" x 14.6" x 11.8"; 684.3 oz	50
U120 Data Transfer Kit	U221-131 [†]	1 Data Transfer Cable (RS232C)	1 Package Insert	12.0 cm x 12.0 cm x 6.5 cm; 0.4 kg 4.7" x 4.7" x 2.6"; 14.1 oz	63.0 cm x 37.0 cm x 30.0 cm; 21.4 kg 24.8" x 14.6" x 11.8"; 684.3 oz; 754.9 oz	8

U500 Urine Analyzer



Accurate and Efficient

- Up to 500 tests/hour for medium/large volume sample testing
- Professional accuracy equivalent to market leader
- Automatic strip detection and alignment for better efficiency
- Test modes include Routine, STAT and QC

Easy to Operate

- Large touch screen LCD offers simple menu navigation
- Uniquely designed strip platform/waste tray unit for easy one-step cleaning

Convenient

- Automatic calibration and waste disposal reduce hands-on time
- Can read strips with 8, 9, 10, 11 parameters, additional strips with 1-11 parameters available upon request
- Strip selection of up to 4 combinations for analyzer reading
- Stores up to 2,000 records and automatically flags abnormal results
- Capable of printing results on sticker paper for quick and easy record management

Data Management Capability

- Includes RS232C port for easy data transfer to an external computer or LIS
- Optional Barcode Reader to record patient ID

Unique Lockout Functions Coming Soon!

- Strip Lockout
 - Prevents using strips of another brand on the U500 Urine Analyzer
 - Requires barcode reader scan or manual entry of the canister code
- User Lockout
 - Eliminates unapproved users from testing
 - Up to 10 lab operators can perform testing, but only the lab administrator can change analyzer settings
- QC Lockout
 - Prevents testing without passing QC
 - QC tests can be performed once every 8 hours, day, week or month
 - Analyzer will alert when to run QC test
 - If QC tests fail, analyzer will switch to STAT mode and list "E" at the end of each test number

Specifications

Feature	Specifications
Analyzer Type	Semi-Automatic
Methodology	Reflectance Photometry
Detection	Photosensitive Diode
Throughput	500 tests/hour (Measuring cycle: 7 seconds/test)
Test Modes	Routine, STAT and QC
Lockout Functions	Strip Lockout: Available Upon Request; User/QC Lockout: Included with option to turn ON/OFF
Memory	Last 2,000 Records
Strip Incubation Time	1 Minute
Wavelength	525 and 635 nm
Standard Strips	8, 9, 10, 11 Parameters (5 mm x 108 mm)
Additional Strips Available	1-11 Parameters (5 mm x 108 mm); see URS Parameters
Total Combinations Per Analyzer	4 Combinations
Waste Disposal Capacity	Up to 150 Strips
Analyzer Ports	Standard RS232C Port for Barcode Reader or Data Transfer 25 Pin Parallel Port for External Printer
Capabilities	Internal Thermal Printer (included) RS232C Barcode Reader (optional) Optional External Printer (not included) RS232C Data Transfer Cable (optional)
Major Readable Barcodes	Code 128, Code 39, Codabar (NW-7), Interleaved 25, UPC-A, UPC-E, EAN 8, EAN 13
Calibration	Automatic
Available Languages on the Screen	English and additional language(s)
Operating Conditions	0-40°C (32-104°F); ≤85% RH
Storage Conditions	-5-50°C (23-122°F); ≤90% RH
Power Source	100-240 VAC, 50-60 Hz
Dimensions (L x W x H)	36.6 cm x 28.3 cm x 19.5 cm (14.4" x 11.1" x 7.7")
Display Dimensions (L x W)	11.5 cm x 9.0 cm (4.5" x 3.5")
Weight	4.0 kg (8.8 lbs)

Ordering Information

Product Name	Catalog No.	Components	Kit Box Dimensions (L x W x H) & Weight	Carton Dimensions (L x W x H) & Weight	Number of Kits/Carton
U500 Urine Analyzer	U211-101 [✓]	1 Urine Analyzer 1 Strip Platform/Waste Tray 2 Printer Paper Rolls	2 Fuses (2.0A) 1 Power Cord 1 Instruction Manual	51.0 cm x 42.0 cm x 38.5 cm; 7 kg 20.1" x 16.5" x 15.2"; 246.9 oz	1
U500 Urine Analyzer with Barcode Reader	U211-111 [✓]	1 Urine Analyzer 1 Strip Platform/Waste Tray 2 Printer Paper Rolls 1 Barcode Reader (RS232C)	2 Fuses (2.0A) 1 Power Cord 1 Serial Splitter Cable (RS232C) 1 Instruction Manual	55.0 cm x 55.0 cm x 55.0 cm; 9.2 kg 21.7" x 21.7" x 21.7"; 324.5 oz	1
Barcode Reader	U221-111 ^{✓†}	1 Barcode Reader (RS232C)	1 Serial Splitter Cable (RS232C)	23.6 cm x 10.8 cm x 7.8 cm; 0.482 kg 9.3" x 4.3" x 3.1"; 17.0 oz	22
Printer Paper Rolls	U121-101	4 Printer Paper Rolls	Thermal Paper (0.06 m x 20 m): 200 results/roll Sticker Paper (0.06 m x 9 m): 100 results/roll	12.0 cm x 12.0 cm x 6.5 cm; 0.360 kg 4.7" x 4.7" x 2.6"; 12.7 oz	50
U500 Data Transfer Kit	U221-131 [✓]	1 Data Transfer Cable (RS232C)	1 Package Insert	12.0 cm x 12.0 cm x 6.5 cm; 0.40 kg 4.7" x 4.7" x 2.6"; 14.1 oz	8

We also offer other rapid diagnostic and medical products:

Blood Glucose Monitoring Systems, Immunoassay EIA/ELISA and more.

✓ CE Marked for sale in the European Community **CE**
† Cleared for US 510(k)



ACON Laboratories, Inc., 10125 Mesa Rim Road, San Diego, CA 92121, U.S.A. • Tel: 1-858-875-8000 • Fax: 1-858-200-0729 • E-mail: info@aconlabs.com
Please visit our website for details: www.aconlabs.com

Mission® Urinalysis Reagent Strips (Urine)

Package Insert

REF U031-011	REF U031-051	REF U031-091	English
REF U031-021	REF U031-061	REF U031-101	
REF U031-031	REF U031-071	REF U031-111	
REF U031-041	REF U031-081		

For rapid detection of multiple analytes in human urine.

For *in vitro* diagnostic use only.

INTENDED USE

The Urinalysis Reagent Strips (Urine) are firm plastic strips onto which several separate reagent areas are affixed. The test is for the qualitative and semi-quantitative detection of one or more of the following analytes in urine: Ascorbic acid, Glucose, Bilirubin, Ketone (Acetoacetic acid), Specific Gravity, Blood, pH, Protein, Urobilinogen, Nitrite and Leukocytes.

SUMMARY

Urine undergoes many changes during states of disease or body dysfunction before blood composition is altered to a significant extent. Urinalysis is a useful procedure as an indicator of health or disease, and as such, is a part of routine health screening. The Urinalysis Reagent Strips (Urine) can be used in general evaluation of health, and aids in the diagnosis and monitoring of metabolic or systemic diseases that affect kidney function, endocrine disorders and diseases or disorders of the urinary tract.^{1,2}

PRINCIPLE AND EXPECTED VALUES

Ascorbic acid: This test involves decolorization of Tillmann's reagent. The presence of ascorbic acid causes the color of the test field to change from blue-green to orange. Patients with adequate diet may excrete 2-10 mg/dL daily. After ingesting large amounts of ascorbic acid, levels can be around 200 mg/dL.

Glucose: This test is based on the enzymatic reaction that occurs between glucose oxidase, peroxidase and chromogen. Glucose is first oxidized to produce gluconic acid and hydrogen peroxide in the presence of glucose oxidase. The hydrogen peroxide reacts with potassium iodide chromogen in the presence of peroxidase. The extent to which the chromogen is oxidized determines the color which is produced, ranging from green to brown. Glucose should not be detected in normal urine. Small amounts of glucose may be excreted by the kidney.³ Glucose concentrations as low as 100 mg/dL may be considered abnormal if results are consistent.

Bilirubin: This test is based on azo-coupling reaction of bilirubin with diazotized dichloroaniline in a strongly acidic medium. Varying bilirubin levels will produce a pinkish-tan color proportional to its concentration in urine. In normal urine, no bilirubin is detectable by even the most sensitive methods. Even trace amounts of bilirubin require further investigation. Atypical results (colors different from the negative or positive color blocks shown on the color chart) may indicate that bilirubin-derived bile pigments are present in the urine specimen, and are possibly masking the bilirubin reaction.

Ketone: This test is based on ketones reacting with nitroprusside and acetoacetic acid to produce a color change ranging from light pink for negative results to a darker pink or purple color for positive results. Ketones are normally not present in urine. Detectable ketone levels may occur in urine during physiological stress conditions such as fasting, pregnancy and frequent strenuous exercise.⁴⁻⁶ In starvation diets, or in other abnormal carbohydrate metabolism situations, ketones appear in the urine in excessively high concentration before serum ketones are elevated.⁷

Specific Gravity: This test is based on the apparent pKa change of certain pretreated polyelectrolytes in relation to ionic concentration. In the presence of an indicator, colors range from deep blue-green in urine of low ionic concentration to green and yellow-green in urine of increasing ionic concentration. Randomly collected urine may vary in specific gravity from 1.003-1.035.⁸ Twenty-four hour urine from healthy adults with normal diets and fluid intake will have a specific gravity of 1.016-1.022.⁹ In cases of severe renal damage, the specific gravity is fixed at 1.010, the value of the glomerular filtrate.

Blood: This test is based on the peroxidase-like activity of hemoglobin which catalyzes the reaction of diisopropylbenzene dihydroperoxide and 3,3',5,5'-tetramethylbenzidine. The resulting color ranges from orange to dark blue. Any green spots or green color development on the reagent area within 60 seconds is significant and the urine specimen should be examined further. Blood is often, but not invariably, found in the urine of menstruating females. The significance of a trace reading varies among patients and clinical judgment is required in these specimens.

pH: This test is based on a double indicator system which gives a broad range of colors covering the entire urinary pH range. Colors range from orange to yellow and green to blue. The expected range for normal urine specimens from newborns is pH 5-7.⁹ The expected range for other normal urine specimens is pH 4.5-8, with an average result of pH 6.⁹

Protein: This reaction is based on the phenomenon known as the "protein error" of pH indicators where an indicator that is highly buffered will change color in the presence of proteins (anions) as the indicator releases hydrogen ions to the protein. At a constant pH, the development of any green color is due to the presence of protein. Colors range from yellow to yellow-green for negative results and green to green-blue for positive results. 1-14 mg/dL of protein may be excreted by a normal kidney.¹⁰ A color matching any block greater than trace indicates significant proteinuria. Clinical judgment is required to evaluate the significance of trace results.

Urobilinogen: This test is based on a modified Ehrlich reaction between p-diethylaminobenzaldehyde and urobilinogen in strongly acidic medium to produce a pink color. Urobilinogen is one of the major compounds produced in heme synthesis and is a normal substance in urine. The expected range for normal urine with this test is 0.2-1.0 mg/dL (3.5-17 µmol/L).⁸ A result of 2.0 mg/dL (35 µmol/L) may be of clinical significance, and the patient specimen should be further evaluated.

Nitrite: This test depends upon the conversion of nitrate to nitrite by the action of Gram negative bacteria in the urine. In an acidic medium, nitrite in the urine reacts with p-arsanilic acid to form a diazonium compound. The diazonium compound in turn couples with 1 N-(1-naphthyl) ethylenediamine to produce a pink color. Nitrite is not detectable in normal urine.⁹ The nitrite area will be positive in some cases of infection, depending on how long the urine specimens were retained in the bladder prior to collection. Retrieval of positive cases with the nitrite test ranges from as low as 40% in cases where little bladder incubation occurred, to as high as approximately 80% in cases where bladder incubation took place for at least 4 hours.

Leukocytes: This test reveals the presence of granulocyte esterases. The esterases cleave a derivatized pyrazole amino acid ester to liberate derivatized hydroxy pyrazole. This pyrazole then reacts with a diazonium salt to produce a beige-pink to purple color. Normal urine specimens generally yield negative results. Trace results may be of questionable clinical significance. When trace results occur, it is recommended to retest using a fresh specimen from the same patient. Repeated trace and positive results are of clinical significance.

REAGENTS AND PERFORMANCE CHARACTERISTICS

Based on the dry weight at the time of impregnation, the concentrations given may vary within manufacturing tolerances. The following table below indicates read times and performance characteristics for each parameter.

Reagent	Read Time	Composition	Description
Ascorbic Acid (ASC)	30 seconds	2,6-dichlorophenolindophenol; buffer and non-reactive ingredients	Detects ascorbic acid as low as 5-10 mg/dL (0.28-0.56 mmol/L).
Glucose (GLU)	30 seconds	glucose oxidase; peroxidase; potassium iodide; buffer; non-reactive ingredients	Detects glucose as low as 50-100 mg/dL (2.5-5 mmol/L).
Bilirubin (BIL)	30 seconds	2, 4-dichloroaniline diazonium salt; buffer and non-reactive ingredients	Detects bilirubin as low as 0.4-1.0 mg/dL (6.8-17 µmol/L).
Ketone (KET)	40 seconds	sodium nitroprusside; buffer	Detects acetoacetic acid as low as 2.5-5 mg/dL (0.25-0.5 mmol/L).
Specific Gravity (SG)	45 seconds	bromthymol blue indicator; buffer and non-reactive ingredients; poly (methyl vinyl ether/maleic anhydride); sodium hydroxide	Determines urine specific gravity between 1.000 and 1.030. Results correlate with values obtained by refractive index method within ± 0.005.
Blood (BLO)	60 seconds	3,3',5,5'-tetramethylbenzidine (TMB); diisopropylbenzene dihydroperoxide; buffer and non-reactive ingredients	Detects free hemoglobin as low as 0.018-0.060 mg/dL or 5-10 Ery/µL in urine specimens with ascorbic acid content of < 50 mg/dL.
pH	60 seconds	methyl red sodium salt; bromthymol blue; non-reactive ingredients	Permits the quantitative differentiation of pH values within the range of 5-9.
Protein (PRO)	60 seconds	tetrabromophenol blue; buffer and non-reactive ingredients	Detects albumin as low as 7.5-15 mg/dL (0.075-0.15 g/L).
Urobilinogen (URO)	60 seconds	p-diethylaminobenzaldehyde; buffer and non-reactive ingredients	Detects urobilinogen as low as 0.2-1.0 mg/dL (3.5-17 µmol/L).
Nitrite (NIT)	60 seconds	p-arsanilic acid; N-(1-naphthyl) ethylenediamine; non-reactive ingredients	Detects sodium nitrite as low as 0.05-0.1 mg/dL in urine with a low specific gravity and less than 30 mg/dL ascorbic acid.
Leukocytes (LEU)	120 seconds	derivatized pyrrole amino acid ester; diazonium salt; buffer; non-reactive ingredients	Detects leukocytes as low as 9-15 white blood cells Leu/µL in clinical urine.

The performance characteristics of the Urinalysis Reagent Strips (Urine) have been determined in both laboratory and clinical tests. Parameters of importance to the user are sensitivity, specificity, accuracy and precision. Generally, this test has been developed to be specific for the parameters to be measured with the exceptions of the interferences listed. Please refer to the Limitations section in this package insert.

Interpretation of visual results is dependent on several factors: the variability of color perception, the presence or absence of inhibitory factors, and the lighting conditions when the strip is read. Each color block on the chart corresponds to a range of analyte concentrations.

PRECAUTIONS

- For *in vitro* diagnostic use only. Do not use after the expiration date.
- The strip should remain in the closed canister until use.
- Do not touch the reagent areas of the strip.
- Discard any discolored strips that may have deteriorated.
- All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.
- The used strip should be discarded according to local regulations after testing.

STORAGE AND STABILITY

Store as packaged in the closed canister either at room temperature or refrigerated (2-30°C). Keep out of direct sunlight. The strip is stable through the expiration date printed on the canister label. Do not remove the desiccant. Remove only enough strips for immediate use. Replace cap immediately and tightly. **DO NOT FREEZE.** Do not use beyond the expiration date.

Note: Once the canister has been opened, the remaining strips are stable for up to 3 months. Stability may be reduced in high humidity conditions.

SPECIMEN COLLECTION AND PREPARATION

A urine specimen must be collected in a clean and dry container and tested as soon as possible. Do not centrifuge. The use of urine preservatives is not recommended. If testing cannot be done within an hour after voiding, refrigerate the specimen immediately and let it return to room temperature before testing.

Prolonged storage of unpreserved urine at room temperature may result in microbial proliferation with resultant changes in pH. A shift to alkaline pH may cause false positive results with the protein test area. Urine containing glucose may decrease in pH as organisms metabolize the glucose.

Contamination of the urine specimen with skin cleansers containing chlorhexidine may affect protein (and to a lesser extent, specific gravity and bilirubin) test results.

MATERIALS

Materials Provided

- Strips
- Package insert

Materials Required But Not Provided


- Specimen collection container
- Timer

DIRECTIONS FOR USE

Allow the strip, urine specimen, and/or controls to reach room temperature (15-30°C) prior to testing.

- Remove the strip from the closed canister and use it as soon as possible. Immediately close the canister tightly after removing the required number of strip(s). Completely immerse the reagent areas of the strip in fresh, well-mixed urine and immediately remove the strip to avoid dissolving the reagents. See illustration 1 below.
- While removing the strip from the urine, run the edge of the strip against the rim of the urine container to remove excess urine. Hold the strip in a horizontal position and bring the edge of the strip into contact with an absorbent material (e.g. a paper towel) to avoid mixing chemicals from adjacent reagent areas and/or soiling hands with urine. See illustration 2 below.
- Compare the reagent areas to the corresponding color blocks on the canister label at the specified times. Hold the strip close to the color blocks and match carefully. See illustration 3 below.

Note: Results may be read up to 2 minutes after the specified times.

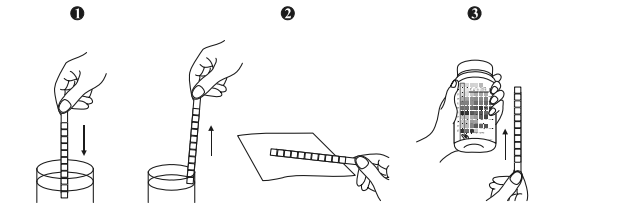

INTERPRETATION OF RESULTS

Results are obtained by direct comparison of the color blocks printed on the canister label. The color blocks represent nominal values; actual values will vary close to the nominal values. In the event of unexpected or questionable results, the following steps are recommended: confirm that the strips have been tested within the expiration date printed on the canister label, compare results with known positive and negative controls and repeat the test using a new strip. If the problem persists, discontinue using the strip immediately and contact your local distributor.

QUALITY CONTROL

For best results, performance of reagent strips should be confirmed by testing known positive and negative specimens/controls whenever a new test is performed, or whenever a new canister is first opened. Each laboratory should establish its own goals for adequate standards of performance.

LIMITATIONS

Note: The Urinalysis Reagent Strips (Urine) may be affected by substances that cause abnormal urine color such as drugs containing azo dyes (e.g. Pyridium®. Azo Gantrisin®, Azo Gantanol®), nitrofurantoin (Microdantin®, Furadantin®), and riboflavin.⁸ The color development on the test pad may be masked or a color reaction may be produced that could be interpreted as false results.

Ascorbic acid: No interference is known.

Glucose: The reagent area does not react with lactose, galactose, fructose or other metabolic substances, nor with reducing metabolites of drugs (e.g. salicylates and nalidixic acid). Sensitivity may be decreased in specimens with high specific gravity (>1.025) and with ascorbic acid concentrations of ≥ 25 mg/dL. High ketone levels ≥ 100 mg/dL may cause false negative results for specimens containing a small amount of glucose (50-100 mg/dL).

Bilirubin: Bilirubin is absent in normal urine, so any positive result, including a trace positive, indicates an underlying pathological condition and requires further investigation. Reactions may occur with urine containing large doses of chlorpromazine or rifampin that might be mistaken for positive bilirubin.⁹ The presence of bilirubin-derived bile pigments may mask the bilirubin reaction. This phenomenon is characterized by color development on the test patch that does not correlate with the colors on the color chart. Large concentrations of ascorbic acid may decrease sensitivity.

Ketone: The test does not react with acetone or β-hydroxybutyrate.⁸ Urine specimens of high pigment, and other substances containing sulfindryl groups may occasionally give reactions up to and including trace (±).

Specific Gravity: Ketoacidosis or protein higher than 300 mg/dL may cause elevated results. Results are not affected by non-ionic urine components such as glucose. If the urine has a pH of 7 or greater, add 0.005 to the specific gravity reading indicated on the color chart.

Blood: A uniform blue color indicates the presence of myoglobin, hemoglobin or hemolyzed erythrocytes.⁸ Scattered or compacted blue spots indicate intact erythrocytes. To enhance accuracy, separate color scales are provided for hemoglobin and for erythrocytes. Positive results with this test are often seen with urine from menstruating females. It has been reported that urine of high pH reduces sensitivity, while moderate to

high concentration of ascorbic acid may inhibit color formation. Microbial peroxidase, associated with urinary tract infection, may cause a false positive reaction. The test is slightly more sensitive to free hemoglobin and myoglobin than to intact erythrocytes.

pH: If the procedure is not followed and excess urine remains on the strip, a phenomenon known as "runover" may occur, in which the acid buffer from the protein reagent will run onto the pH area, causing the pH result to appear artificially low. pH readings are not affected by variations in urinary buffer concentration.

Protein: Any green color indicates the presence of protein in the urine. This test is highly sensitive for albumin, and less sensitive to hemoglobin, globulin and mucoprotein.⁸ A negative result does not rule out the presence of these other proteins. False positive results may be obtained with highly buffered or alkaline urine. Contamination of urine specimens with quaternary ammonium compounds or skin cleansers containing chlorhexidine may produce false positive results.⁸ The urine specimens with high specific gravity may give false negative results.

Urobilinogen: All results lower than 1 mg/dL urobilinogen should be interpreted as normal. A negative result does not at any time preclude the absence of urobilinogen. The reagent area may react with interfering substances known to react with Ehrlich's reagent, such as p-aminosalicylic acid and sulfonamides.⁹ False negative results may be obtained if formalin is present. The test cannot be used to detect porphobilinogen.

Nitrite: The test is specific for nitrite and will not react with any other substance normally excreted in urine. Any degree of uniform pink to red color should be interpreted as a positive result, suggesting the presence of nitrite. Color intensity is not proportional to the number of bacteria present in the urine specimen. Pink spots or pink edges should not be interpreted as a positive result. Comparing the reacted reagent area on a white background may aid in the detection of low nitrite levels, which might otherwise be missed. Ascorbic acid above 30 mg/dL may cause false negatives in urine containing less than 0.05 mg/dL nitrite ions. The sensitivity of this test is reduced for urine specimens with highly buffered alkaline urine or with high specific gravity. A negative result does not at any time preclude the possibility of bacteruria. Negative results may occur in urinary tract infections from organisms that do not contain reductase to convert nitrate to nitrite; when urine has not been retained in the bladder for a sufficient length of time (at least 4 hours) for reduction of nitrate to nitrite to occur; when receiving antibiotic therapy or when dietary nitrate is absent.

Leukocytes: The result should be read between 60-120 seconds to allow for complete color development. The intensity of the color that develops is proportional to the number of leukocytes present in the urine specimen. High specific gravity or elevated glucose concentrations (≥ 2,000 mg/dL) may cause test results to be artificially low. The presence of cephalixin, cephalothin, or high concentrations of oxalic acid may also cause test results to be artificially low. Tetracycline may cause decreased reactivity, and high levels of the drug may cause a false negative reaction. High urinary protein may diminish the intensity of the reaction color. This test will not react with erythrocytes or bacteria common in urine.⁸

BIBLIOGRAPHY

- Free AH, Free HM. *Urinalysis, Critical Discipline of Clinical Science*. CRC Crit. Rev. Clin. Lab. Sci. 3(4): 481-531, 1972.
- Yoder J, Adams EC, Free, AH. *Simultaneous Screening for Urinary Occult Blood, Protein, Glucose, and pH*. Amer. J. Med Tech. 31:285, 1965.
- Shchersten B, Fritz H. *Subnormal Levels of Glucose in Urine*. JAMA 201:129-132, 1967.
- McGarry JD, Lilly. Lecture, 1978: New Perspectives in the Regulation of Ketogenesis. Diabetes 28: 517-523 May, 1978.
- Williamson DH. *Physiological Ketoses, or Why Ketone Bodies?* Postgrad. Med. J. (June Suppl.): 372-375, 1971.
- Paterson P, et al. *Maternal and Fetal Ketone Concentrations in Plasma and Urine*. Lancet: 862-865; April 22, 1967.
- Fraser J, et al. *Studies with a Simplified Nitroprusside Test for Ketone Bodies in Urine, Serum, Plasma and Milk*. Clin. Chem. Acta II: 372-378, 1965.
- Henry JB, et al. Clinical Diagnosis and Management by Laboratory Methods, 20th Ed. Philadelphia. Saunders. 371-372, 375, 379, 382, 385, 2001.
- Tietz NW. Clinical Guide to Laboratory Tests. W.B. Saunders Company. 1976.
- Burtis CA, Ashwood ER. Tietz Textbook of Clinical Chemistry 2nd Ed. 2205, 1994.

Index of Symbols			
	Consult instructions for use		Tests per kit
	For <i>in vitro</i> diagnostic use only		Use by
	Store between 2-30°C		Lot Number
	Authorized Representative		Catalog #

**ACON Laboratories, Inc.**
10125 Mesa Rim Road,
San Diego, CA 92121, USA

**MDSS GmbH**
Schiffgraben 41
30175 Hannover, Germany



Contract No:Co2403079

Date:09/03/2024

Letter of Authorization

Manufacturer: Atlas Medical GmbH
Ludwig-Erhard-Ring 3,
15827Blankenfelde-Mahlow, Germany
Tel: +49 33 70 83 55 030
Email: amug@atlas-medical.com

Regulatory Office: William James House, Cowley Road, Cambridge, CB4 0WX, UK
Tel: +44 1223 858 910
Fax: +44 1223 858 524
Email: info@atlas-site.co.uk

Middle East Site: Sahab Free Zone Area
P. O. Box 204, Amman 11512, Jordan.
Tel.: +962 6 4026468
Fax: +962 6 4022588
Email: info@atlas-medical.com

Agent: San Medico
Republic of Moldova, city Chisina
+37368228890

Atlas Medical, hereby appoint the above mentioned agent to import, register and distribute Atlas Medical Products in Maldova

Appointment Conditions:

1. This appointment is valid for 3 year from the above mentioned date.
2. Either Party can cancel this appointment by giving the other party a 60 day notice.

On behalf of the Manufacturer
General Manager
Haya Amawi



Atlas Medical: Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow, Germany. Tel: +49 33 70 83 55 030
Regulatory Office: William James House, Cowley Road, Cambridge, CB4 0WX, UK. Tel: +44 1223 858 910
Middle East Site : King Abdullah the Second Industrial Estate, Street 19, Sahab Free Zone Area, P.O. Box: 204, Amman 11512, Jordan

GMED certifie que le système de management de la qualité développé par
GMED certifies that the quality management system developed by

ATLAS MEDICAL GmbH
Ludwig-Erhard-Ring 3
15827 Blankenfelde-Mahlow GERMANY

pour les activités
for the activities

Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic in vitro .

Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices.

réalisées sur le(s) site(s) de
performed on the location(s) of

Voir addendum

See addendum

est conforme aux exigences des normes internationales
complies with the requirements of the international standards

ISO 13485: 2016

Début de validité / Effective date October 9th, 2023 (included)

Valable jusqu'au / Expiry date : October 8th, 2026 (included)

Etabli le / Issued on : October 9th, 2023




**CERTIFICATION
DE SYSTEMES
DE MANAGEMENT**
Accréditation n°4-0608
Liste des sites accrédités
et portée disponible sur
www.cofrac.fr

GMED N° 36655-2

Ce certificat est délivré selon les règles de certification GMED / This certificate is issued according to the rules of GMED certification

Renouvelle le certificat 36655-1



On behalf of the President
Béatrice LYS
Technical Director

Ce certificat couvre les activités et les sites suivants :
This certificate covers the following activities and sites:

French version :

Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic *in vitro* à usage professionnel et/ ou d'autodiagnostic, dans les domaines du groupage sanguin, de la microbiologie, de la biochimie, de la toxicologie, de l'oncologie, de la cardiologie, de l'histologie, de l'endocrinologie et des maladies infectieuses, dans les techniques d'Agglutination/ ELISA/ Tests rapides/ Colorimétrie/ Disques antibiotiques.

English version:

Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices for professional use and/or for self-testing, in the field of Immunohematology, Microbiology, Biochemistry, Toxicology, Oncology, Cardiology, Histology, Endocrinology Biosensors and Infectious diseases, in techniques of Agglutination/ ELISA/ Rapid tests/ Colorimetry/Antibiotic disks.

**ATLAS MEDICAL GmbH
Ludwig-Erhard-Ring 3
15827 Blankenfelde-Mahlow
GERMANY**

French version:

Siège social, responsable de la mise sur le marché

English version:

Headquarter, legal manufacturer

**Sahab Industrial Zone Area
King Abdullah II Industrial City
Amman 11512
JORDAN**


French version:

Conception, fabrication et contrôle final

English version:

Design, manufacture and final control

2 sites / 2 sites

DocuSigned by:
Beatrice Lys
FF33BDA98AA04A3...


**On behalf of the President
Béatrice LYS
Technical Director**

CE Declaration of Conformity

Name and address of Manufacturer	Atlas Medical GmbH Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow Germany . Tel: +49(0)33708355030 Email: info@atlas-medical.com
---	--

Atlas Medical GmbH declared our his own responsibility that the following IVD medical devices:

Product Code	Product Name	GMDN code
8.17.003.0300	Atlas Periodic Acid Schiff (PAS) Stain Kit, 3x100ml	43587
8.17.004.0300	Atlas Iron Stain Kit, 3x100ml	43587
8.17.009.1000	Atlas Gram Stain Kit	43733
8.17.010.0750	Atlas ZN (Kinyoun) stain pack , 3x250ml	43587
8.15.144.0250	Atlas ZN Decolouriser, 250 ml /Bottle	43587
8.17.015.0500	Atlas Diff-3 Stain.	43587
8.17.016.1000	Atlas Papanicolau Stain Pack.	43587
8.17.110.0250	Atlas Papanicolau Stain EA35, 250 ml /Bottle.	43587
8.17.111.0250	Atlas Papanicolau Stain EA36, 250 ml /Bottle	43587
8.17.112.0250	Atlas Papanicolau Stain EA65, 250 ml /Bottle.	43587
8.17.114.0250	Atlas Papanicolau Stain EA50, 250 ml /Bottle.	43587
8.17.115.0250	Atlas Papanicolau Stain OG6, 250 ml /Bottle.	43587
8.17.014.1000	Atlas Reticulocytes stain (Methylene Blue) , 1000 ml /Bottle	43587
8.15.037.0250	Atlas Eosin Y (1%) Stain, 250 ml/Bottle	43587
8.15.038.0250	Atlas Eosin Y (5%) Stain, 250 ml/Bottle.	43587
8.15.041.0250	Atlas Field Stain (Solution A), 250ml/Bottle	43587
8.15.042.0250	Atlas Field Stain (Solution B), 250ml/Bottle	43587
8.15.043.0750	Atlas Field Stain Kit 3x250ml (250ml Fixing Reagent , 250ml Eosin Reagent, 250ml Methylene Blue Reagent).	43587
8.15.047.0250	Atlas Giemsa Stain, 250 ml/Bottle.	43587
8.15.059.0250	Atlas Haematoxylin Harris Stain , 250 ml/Bottle	43587
8.15.069.0250	Atlas Leishman Stain , 250 ml/Bottle.	43587
8.15.069.1000	Atlas Leishman Stain , 1000 ml/Bottle.	43587
8.15.074.0250	Atlas Lugol's Iodine, 250 ml/Bottle.	43587
8.15.078.0250	Atlas May Grunwald Stain, 250 ml/Bottle.	43587
8.15.105.0250	Atlas New Methylene Blue for Reticulocytes, 250 ml/Bottle.	43587
8.15.143.0250	Atlas Wright's Stain, 250 ml/Bottle.	43587
8.15.146.0100	Atlas Immersion oil, 100 Bottle/Box	43587

Declaration Ref No: DC21-0249

Date: 15.10.2021

Meets the essential requirements of In Vitro Diagnostic Medical Devices Directive 98/79/EC Annex I
And

EN ISO 13485 :2016 , EN 18113-1, -2,:2011, EN ISO 15223:2016
EN ISO 14971:2019, EN ISO 23640:2015, ISO 2859/1:1999,
EN ISO 13612:2002, EN ISO 13641:2002 , EN ISO 62366-1+A1:2020.


IVD Categorization	Directive 98/79, Other IVDs (Non-annex II, non-self-test).
Conformity Assessment Route	Directive 98/79/EC , Annex III.
Name , Address and Identification number of notified body	N/A

Date of issuance:	15. October.2021
Place	Atlas Medical GmbH
Signed by:	Amani AL-Habahbeh 
Position :	Regulatory Affairs Manager

Atlas Medical GmbH
Ludwig - Erhard Ring 3
15827 Blankenfelde - Mahlow
Tel. (0049) 33708 - 355030

GRAM STAIN PACK

IVD For *in-vitro* diagnostic and professional use only



Store at Room Temperature

INTENDED USE

Gram Stain used for differentiate between gram positive and gram-negative bacteria.

INTRODUCTION

Gram staining is used to differentiate bacterial species into two large groups (Gram-positive and Gram-negative) based on the physical properties of their cell walls.

PRINCIPLE

Gram-positive bacteria have a thick mesh-like cell wall made of peptidoglycan (50-90% of cell wall), which stains Blue while gram-negative bacteria have a thinner layer (10% of cell wall), which stains pink. Gram-negative bacteria also have an additional outer membrane which contains lipids, and is separated from the cell wall by the periplasmic space. There are four basic steps of the Gram stain, which include applying a primary stain (crystal violet) to a heat-fixed smear of a bacterial culture, followed by the addition of a trapping agent (Gram's iodine), rapid decolorization with alcohol or acetone, and *counterstaining* with safranin or basic fuchsin.

Crystal violet (CV) dissociates in aqueous solutions into CV⁺ and chloride (Cl⁻) ions. These ions penetrate through the cell wall and cell membrane of both gram-positive and gram-negative cells. The CV⁺ ion interacts with negatively charged components of bacterial cells and stains the cells Blue.

Iodine (I⁻ or I₃⁻) interacts with CV⁺ and forms large complexes of crystal violet and iodine (CV-I) within the inner and outer layers of the cell. Iodine is often referred to as a mordant, but is a trapping agent that prevents the removal of the CV-I complex and therefore color from the cell.

When a decolorizer such as alcohol or acetone is added, it interacts with the lipids of the cell membrane. A gram-negative cell will lose its outer membrane and the lipopolysaccharide layer is left exposed. The

CV-I complexes are washed from the gram-negative cell along with the outer membrane. In contrast, a gram-positive cell becomes dehydrated from an ethanol treatment. The large CV-I complexes become trapped within the gram-positive cell due to the multilayered nature of its peptidoglycan. The decolorization step is critical and must be timed correctly; the crystal violet stain will be removed from both gram-positive and negative cells if the decolorizing agent is left on too long (a matter of seconds).

After decolorization, the gram-positive cell remains Blue. and the gram-negative cell loses its Blue. color. Counterstain, which is usually positively charged safranin or basic fuchsin, is applied last to give decolorized gram-negative bacteria a pink or red color.

MATERIALS

MATERIALS PROVIDED

- Crystal Violet.
- Gram Iodine.
- Gram Decolouriser.
- Counterstain – Safranin O.

Note: This package insert is also used for individually packed reagent.

Storage and stability

- Store at room temperature.
- Stain Solution is stable up to the printed expiry date.
- Keep the bottles tightly closed to prevent air oxidation.

Precautions

- The reagent may cause eye, skin and respiratory tract irritation; so protective clothing should be worn when handling this reagent.
- The reagent is intended for in vitro diagnostic use only.
- Do not use this reagent if the label is not available or damaged.
- Test materials and samples should be discarded properly in biohazards container.
- This reagent is considered toxic, so do not drink or eat beside it.
- Wash hands and test table top with water and soap once the testing is done.

PROCEDURE

1. immerse the heat fixed smears with Crystal Violet and allow to stain for up to 1 minute.
2. Wash with tap water.
3. Flood the smear with Gram Iodine for 2 minutes.
4. Wash with tap water.
5. Decolorize the smear for few second only.
6. Wash thoroughly with tap water.
7. Counterstain with Safranin O for up to 2 minutes.
8. Wash and allow to dry.
9. Examine under microscope using oil immersion objective

RESULTS

- Gram positive organisms (Blue).
- Gram negative organisms (Red).



ATLAS Medical

Ludwig-Erhard Ring 3

15827 Blankenfelde-Mahlow

Germany


















Tel: +49 - 33708 – 3550 30

Email: Info@atlas-medical.com

Website: www.atlas-medical.com

PPI2112A01

Rev B (08.10.2020)

	Catalogue Number		Temperature limit
	In Vitro diagnostic medical device		Caution
	Contains sufficient for <n> tests and Relative size		Consult instructions for use (IFU)
	Batch code		Manufacturer
	Fragile, handle with care		Use-by date
	Manufacturer fax number		Do not use if package is damaged
	Manufacturer telephone number		Date of Manufacture
	Keep away from sunlight		Keep dry
	Flammable		



浙江东方基因生物制品股份有限公司
Zhejiang Orient Gene Biotech Co.,LTD

STATEMENT

We, Zhejiang Orient Gene Biotech Co., Ltd , having a registered office at 3787#, East Yangguang Avenue, Dipu Street Anji 313300, Huzhou, Zhejiang, China assign SRL SANMEDICO having a registered office at A. Corobceanu street 7A, apt. 9, Chişinău MD-2012, Moldova, as non-exclusive authorized representative for Orient Gene Brand product in correspondence with the conditions of directive 98/79/EEC.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

This Statement letter will be valid from Feb.21th,2023 to Feb.20th, 2024.

Zhejiang Orient Gene Biotech Co., Ltd

General Manager:

Date:2023/2/21



[Handwritten signature in blue ink]

地址：浙江省湖州市安吉县递铺镇阳光大道东段 3787 号
Add: 3787#, East Yangguang Avenue, Dipu Street Anji 313300, Huzhou, Zhejiang, China
电话 Tel:+86-572-5226111 传真 Fax: +86-572-5226222 邮编 P.C.:313300



Certificate

No. Q5 092305 0001 Rev. 01

Holder of Certificate: **Zhejiang Orient Gene Biotech Co., Ltd.**
3787#, East Yangguang Avenue, Dipu Street Anji
313300 Huzhou, Zhejiang
PEOPLE'S REPUBLIC OF CHINA

Certification Mark:



Scope of Certificate: **Design and Development, Production and Distribution of In Vitro Diagnostic Reagent and Instrument for the Detection of Drugs of Abuse, Fertility, Infectious Diseases, Oncology, Biochemistry, Cardiac Diseases, Allergic Disease based on Rapid Test, PCR and Liquid Biochip Method.**

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: www.tuvsud.com/ps-cert?q=cert:Q5 092305 0001 Rev. 01

Report No.: SH2198802

Valid from: 2022-04-11

Valid until: 2024-03-16

Date, 2022-04-11

Christoph Dicks

Head of Certification/Notified Body

Certificate

No. Q5 092305 0001 Rev. 01

Applied Standard(s):

EN ISO 13485:2016
Medical devices - Quality management systems -
Requirements for regulatory purposes
(ISO 13485:2016)
DIN EN ISO 13485:2016

Facility(ies):

Zhejiang Orient Gene Biotech Co., Ltd.
3787#, East Yangguang Avenue, Dipu Street Anji, 313300
Huzhou, Zhejiang, PEOPLE'S REPUBLIC OF CHINA

See Scope of Certificate



浙江东方基因生物制品股份有限公司
Zhejiang Orient Gene Biotech Co., LTD



CE-DOC-OG038
Version 2.0

EC Declaration of Conformity

In accordance with Directive 98/79/EC

Legal Manufacturer: *Zhejiang Orient Gene Biotech Co., Ltd*

Legal Manufacturer Address: *3787#, East Yangguang Avenue, Dipu Street,
Anji 313300, Huzhou, Zhejiang, China*

Declares, that the products
Product Name and Model(s)

Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma)	GDTRO-402a
Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma)	GDTRO-402b

Classification: *Other*
Conformity assessment route: *Annex III (EC DECLARATION OF CONFORMITY)*

We, the Manufacturer, herewith declare with sole responsibility that our product/s mentioned above meet/s the provisions of the Directive 98/79/EC of the European Parliament and of the Council on In-Vitro Diagnostic Medical Devices.

We hereby explicitly appoint

EC Representative's Name: *Shanghai International Holding Corp. GmbH (Europe)*

EC Representative's Address: *Eiffestrasse 80, 20537 Hamburg, Germany*

to act as our European Authorized Representative as defined in the aforementioned Directive.

I, the undersigned, hereby declare that the medical devices specified above conform with the directive 98/79/EC on in vitro diagnostic medical devices and pertinent essential requirements

Date Signed: August 11, 2020

Name of authorized signatory: *Joyce Pang*
Position held in the company: *Vice-President*

Toxicology Urine Test



Product Description	Format	Cut-off Value	Qualification
Acetaminophen (ACE) Test	Strip/Cassette/Dip Card/Cup	5000 ng/mL	CE
Amphetamine (AMP) Test	Strip/Cassette/Dip Card/Cup	2000/1000/500/300/250 ng/mL	CE 510(k)
Barbiturates (BAR) Test	Strip/Cassette/Dip Card/Cup	2000/600/300/200 ng/mL	CE 510(k)
Benzodiazepines (BZO) Test	Strip/Cassette/Dip Card/Cup	600/400/300/200/100 ng/mL	CE 510(k)
Buprenorphine (BUP) Test	Strip/Cassette/Dip Card/Cup	10/5 ng/mL	CE 510(k)
Caffeine (CAF) Test	Strip/Cassette/Dip Card/Cup	6000 ng/mL	/
Carisoprodol (SOMA) Test	Strip/Cassette/Dip Card/Cup	1000 ng/mL	CE
Clonazepam (CLO) Test	Strip/Cassette/Dip Card/Cup	500/100 ng/mL	CE
Cocaine (COC) Test	Strip/Cassette/Dip Card/Cup	600/300/150/100 ng/mL	CE 510(k)
Codeine (COD) Test	Strip/Cassette/Dip Card/Cup	2000 ng/mL	CE
Cotinine (COT) Test	Strip/Cassette/Dip Card/Cup	400/300/200/100/50 ng/mL	CE
Ecstasy (MDMA) Test	Strip/Cassette/Dip Card/Cup	2000/1000/500/300/250/150 ng/mL	CE 510(k)
Ethyl Glucuronide (EtG) Test	Strip/Cassette/Dip Card/Cup	500/300ng/mL	CE
Fentanyl (FEN) Test	Strip/Cassette/Dip Card/Cup	300/200/100/50 ng/mL	CE
Norfentanyl (FEN) Test	Strip/Cassette/Dip Card/Cup	200/50/20/10/5 ng/mL	CE
Gabapentin (GAB) Test	Strip/Cassette/Dip Card/Cup	3750/2000/1000 ng/mL	CE
Hydrocodone (HCD) Test	Strip/Cassette/Dip Card/Cup	300/10 ng/mL	CE
Hydromorphone (HMO) Test	Strip/Cassette/Dip Card/Cup	300 ng/mL	CE
Ketamine (KET) Test	Strip/Cassette/Dip Card/Cup	3000/2000/1000/500/100 ng/mL	CE
Kratom (KRA) Test	Strip/Cassette/Dip Card/Cup	250/150/100 ng/mL	CE
Lysergic acid diethylamide (LSD) Test	Strip/Cassette/Dip Card/Cup	20 ng/mL	CE
Marijuana (THC) Test	Strip/Cassette/Dip Card/Cup	600/300/200/150/100/50/40/25/20/18/15 ng/mL	CE 510(k)
Methadone Metabolite (EDDP) Test	Strip/Cassette/Dip Card/Cup	300/100 ng/mL	CE 510(k)
Methadone (MTD) Test	Strip/Cassette/Dip Card/Cup	1000/600/300/200/50 ng/mL	CE 510(k)
Methamphetamine (MET) Test	Strip/Cassette/Dip Card/Cup	2000/1000/500/300/250 ng/mL	CE 510(k)
Methaqualone (MQL) Test	Strip/Cassette/Dip Card/Cup	300/1000 ng/mL	CE
Methcathinone (MTC) Test	Strip/Cassette/Dip Card/Cup	500/300 ng/mL	CE
3,4-Methylenedioxypropylvalerone (MDPV) Test	Strip/Cassette/Dip Card/Cup	1000/500/300 ng/mL	CE
Methylphenidate (MPD) Test	Strip/Cassette/Dip Card/Cup	300 ng/mL	CE
6-Monoacetylmorphine (6-MAM) Test	Strip/Cassette/Dip Card/Cup	20/10 ng/mL	CE
Morphine (MOP) Test	Strip/Cassette/Dip Card/Cup	2000/600/300/150/100 ng/mL	CE 510(k)
Opiate (OPI) Test	Strip/Cassette/Dip Card/Cup	2000/300/100 ng/mL	CE 510(k)
Oxycodone (OXY) Test	Strip/Cassette/Dip Card/Cup	300/100 ng/mL	CE 510(k)
Phencyclidine (PCP) Test	Strip/Cassette/Dip Card/Cup	50/25 ng/mL	CE 510(k)
Pinaca Ab (K3) Test	Strip/Cassette/Dip Card/Cup	10 ng/mL	CE
Pregabalin (PGB) Test	Strip/Cassette/Dip Card/Cup	2000/1000/500 ng/mL	CE
Propoxyphene (PPX) Test	Strip/Cassette/Dip Card/Cup	600/300 ng/mL	CE 510(k)
Synthetic Marijuana (K2) Test	Strip/Cassette/Dip Card/Cup	75/50/25/20/10 ng/mL	CE
Tramadol (TRA) Test	Strip/Cassette/Dip Card/Cup	200/100 ng/mL	CE
Tricyclic Antidepressants (TCA) Test	Strip/Cassette/Dip Card/Cup	1000/300 ng/mL	CE 510(k)
UR-144 Test	Strip/Cassette/Dip Card/Cup	50 ng/mL	CE
Zolpidem (ZOL) Test ^{New}	Strip/Cassette/Dip Card/Cup	50 ng/mL	/
Zopiclone (ZOP) Test ^{New}	Strip/Cassette/Dip Card/Cup	50 ng/mL	/
Alcohol (ALC) Test	Strip/Cassette/Dip Card/Cup	0.04%	CE

Toxicology Saliva Test



Product Description	Format	Cut-off Value	Qualification
7-Aminoclonazepam (ACL) Test ^{New}	Device	100 ng/mL	/
Amphetamine (AMP) Test	Device	50/40 ng/mL	CE
Barbiturates (BAR) Test	Device	300/50/30 ng/mL	CE
Benzodiazepines (BZO) Test	Device	50/20/10 ng/mL	CE
Buprenorphine (BUP) Test	Device	10/5 ng/mL	CE
Carisoprodol (SOMA) Test	Device	300 ng/mL	/
Cocaine (COC) Test	Device	50/20 ng/mL	CE
Codeine (COD) Test	Device	10 ng/mL	CE
Cotinine (COT) Test	Device	50/30/10 ng/mL	CE
Diphenhydramine (DIP) Test ^{New}	Device	150/100 ng/mL	/
Ecstasy (MDMA) Test	Device	60/50 ng/mL	CE
Ethyl Glucuronide (EtG) Test ^{New}	Device	150/100 ng/mL	/
Fentanyl (FEN) Test	Device	10 ng/mL	CE
Hydrocodone (HCD) Test ^{New}	Device	10 ng/mL	/
Hydromorphone (HMO) Test ^{New}	Device	300/150 ng/mL	/
Ketamine (KET) Test	Device	100/50 ng/mL	CE
Lysergic acid diethylamide (LSD) Test	Device	25/10 ng/mL	CE
Marijuana (THC) Test	Device	50/40/30/25/15/12/10/5/4/3 ng/mL	CE
Methadone Metabolite (EDDP) Test	Device	20 ng/mL	CE
Mephedrone (MEP) Test ^{New}	Device	50 ng/mL	/
Methadone (MTD) Test	Device	75/50/30 ng/mL	CE

Methamphetamine (MET) Test	Device	50 ng/mL	CE
Methaqualone (MQL) Test	Device	150/100 ng/mL	CE
Methcathinone (MTC) Test	Device	50 ng/mL	/
3,4-Methylenedioxypropylvalerone (MDPV) Test	Device	200/100/50 ng/mL	CE
Methylphenidate (MPD) Test	Device	50 ng/mL	/
6-Monoacetylmorphine (6-MAM) Test	Device	25/15/10/5/4 ng/mL	CE
Morphine (MOP) Test	Device	15 ng/mL	CE
Opiate (OPI) Test	Device	50/40 ng/mL	CE
Oxycodone (OXY) Test	Device	50/40/20 ng/mL	CE
Phencyclidine (PCP) Test	Device	10 ng/mL	CE
Phenytoln (PHEN) Test ^{New}	Device	150/100 ng/mL	/
Pinaca Ab (K3) Test ^{New}	Device	10 ng/mL	/
Pregabalin (PGB) Test ^{New}	Device	100 ng/mL	/
Propoxyphene (PPX) Test	Device	50/20 ng/mL	CE
Synthetic Marijuana (K2) Test	Device	25/10/5 ng/mL	CE
Tramadol (TRA) Test	Device	100/50 ng/mL	CE
Tricyclic Antidepressants (TCA) Test	Device	100 ng/mL	CE
XLR-11 Test ^{New}	Device	100 ng/mL	/
Zolpidem (ZOL) Test ^{New}	Device	25 ng/mL	/
Zopiclone (ZOP) Test ^{New}	Device	25 ng/mL	/
Alcohol (ALC) Test	Device	0.05/0.02%	CE

Toxicology Hair Test



Product Description	Format	Label	Cut-off Value	Qualification
Amphetamine (AMP) Test	Cassette	Fluorescence	0.5/0.2 ng/mg	CE
		Gold	5 ng/mg	/
Benzodiazepines (BZO) Test	Cassette	Fluorescence	0.2 ng/mg	/
		Gold	1 ng/mg	/
Cocaine (COC) Test	Cassette	Fluorescence	0.5/0.2 ng/mg	CE
		Gold	5/2 ng/mg	CE
Ecstasy (MDMA) Test	Cassette	Fluorescence	0.2 ng/mg	CE
		Gold	5 ng/mg	/
2-Fluorodeschloroketamin (FKE) Test	Cassette	Fluorescence	0.2 ng/mg	/
Ketamine (KET) Test	Cassette	Fluorescence	0.2 ng/mg	CE
		Gold	2/1/0.5 ng/mg	CE
Marijuana (THC) Test	Cassette	Fluorescence	0.05 ng/mg	CE
		Gold	2/1.5 ng/mg	CE
Methamphetamine (MET) Test	Cassette	Fluorescence	0.5/0.2 ng/mg	CE
		Gold	5/2/1 ng/mg	CE
Methcathinone (MTC) Test	Cassette	Fluorescence	0.2 ng/mg	CE
		Fluorescence	0.2 ng/mg	CE
6-Monoacetylmorphine (6-MAM) Test	Cassette	Gold	2 ng/mg	CE
		Fluorescence	0.2 ng/mg	CE
Morphine (MOP) Test	Cassette	Gold	5/2/0.5 ng/mg	CE
		Fluorescence	0.2 ng/mg	CE
Oxycodone (OXY) Test	Cassette	Gold	4 ng/mg	/
		Fluorescence	0.3 ng/mg	CE
Phencyclidine (PCP) Test	Cassette	Gold	1 ng/mg	CE
		Fluorescence	0.2 ng/mg	CE
Pinaca Ab (K3) Test	Cassette	Gold	0.5 ng/mg	/
		Fluorescence	0.2 ng/mg	CE
Synthetic Marijuana (K2) Test	Cassette	Gold	1 ng/mg	/
Tramadol (TRA) Test	Cassette	Fluorescence	0.2 ng/mg	/
UR-144 Test	Cassette	Fluorescence	0.05 ng/mg	/

Infectious Disease



Product Description	Specimen	Catalog No.	Format	Cut-off Value	Kit Size
Adenovirus Antigen Test	Swab	GCADE-502a√	Cassette	/	20 Tests/Kit
Adenovirus Test	Feces	GCADE-602a√	Cassette	/	20 Tests/Kit
Brucella Antibody Test	WB/S/P	GCBRU-402a√	Cassette	/	25 Tests/Kit
Candida albicans Test	Vaginal Secretion	GCCA-502a√	Cassette	10 ⁶ CFU/mL	20 Tests/Kit
Chagas Antibody Test	S/P	GCCHA-302a√	Cassette	/	25 Tests/Kit
	WB/S/P	GCCHA-402a√	Cassette	/	25 Tests/Kit
Clostridium difficile GDH Test	Feces	GCDD(GDH)-602a√	Cassette	2 ng/mL	20 Tests/Kit
Clostridium difficile Toxin A/B Test	Feces	GCDD(Toxin A/B)-602a√	Cassette	Toxin A: 2 ng/mL Toxin B: 2 ng/mL	20 Tests/Kit
Clostridium difficile GDH & Toxin A/B Combo Test	Feces	GCCD-625a√	Cassette	Toxin A: 2 ng/mL Toxin B: 2 ng/mL	20 Tests/Kit
Chikungunya IgM Test	S/P	GCCHK(IgM)-302a√	Cassette	/	25 Tests/Kit
	WB/S/P	GCCHK(IgM)-402a√	Cassette	/	25 Tests/Kit

Chikungunya IgG/IgM Test	WB/S/P	GCCHK(IgG/IgM)-402a	Cassette	/	25 Tests/Kit
Chlamydia Test	Swab/Urine	GCCHL-502a√	Cassette	4.8×10 ³ IFU/mL	20 Tests/Kit
CMV IgG Test	S/P	GCCMV(IgG)-302a	Cassette	/	25 Tests/Kit
	WB/S/P	GCCMV(IgG)-402a	Cassette	/	25 Tests/Kit
	S/P	GCCMV(IgM)-302a	Cassette	/	25 Tests/Kit
CMV IgM Test	WB/S/P	GCCMV(IgM)-402a	Cassette	/	25 Tests/Kit
	S/P	GCCMV(IgG/IgM)-302a	Cassette	/	25 Tests/Kit
CMV IgG/IgM Test	WB/S/P	GCCMV(IgG/IgM)-402a	Cassette	/	25 Tests/Kit
COVID-19 IgM/IgG Test	WB/S/P	GCCOV-402a√	Cassette	/	25 Tests/Kit
COVID-19 Neutralizing Antibody Test	WB/S/P	GCCOV(NAB)-402b√	Cassette	/	25 Tests/Kit
		GCCOV-502a√	Cassette	/	20 Tests/Kit
	Nasopharyngeal Swab	GCCOV-502Ca√	Cassette	/	20 Tests/Kit
		GCCOV-501a√ ^{New}	Strip	/	20 Tests/Kit
	Nasal Swab	GCCOV-502a-NA√	Cassette	/	1/2/3/5/7/10/15/20 Test(s)/Kit
		GCCOV-503a√ ^{NA}	Device	/	1/2/5/10 Tests/Kit
	NA & NP Swab	GCCOV-502a-NN√	Cassette	/	20 Tests/Kit
	Oral Fluid	GCCOV-702a√	Cassette	/	20 Tests/Kit
		GCCOV-502a-Hxx√	Cassette	/	1/2/3/5/7/10/15/20 Test(s)/Kit
COVID-19 Antigen Self-Test	Nasal Swab	GCCOV-502a-HxxOGE√	Cassette	/	1/2/3/5/8/10/15/20/25 Test(s)/Kit
	Oral Fluid	GCCOV-702a-Hxx√ ^{New}	Cassette	/	1/2/3/5/7/10/15/20 Test(s)/Kit
Digital COVID-19 Antigen Test	Nasal Swab	GCCOV-D503a√ ^{New}	Reader	/	1/2/3/5/7/10/15/20 Test(s)/Kit
COVID-19 Antigen & B.1.1.7 Mutant Strain Combo Test	Nasal Swab	GCCOV(B117)-525a√	Cassette	/	20 Tests/Kit
COVID-19/Flu A&B/RSV Antigen Combo Test	Nasal Swab	GCFCR-T525a√ ^{New}	Cassette	/	20 Tests/Kit
SARS-CoV-2 Delta-series Mutant Strain Antigen Test	Nasal Swab	GCCOV(Del)-T502a√	Cassette	/	20 Tests/Kit
SARS-CoV-2 Ag Fluorescence Rapid Test	Nasal Swab	FCCOV-502a√ ^{New}	Cassette	/	20 Tests/Kit
Dengue IgG/IgM Antibody Test	WB/S/P	GCDEN(lab)-402c√	Cassette	/	25 Tests/Kit
Dengue NS 1 Antigen Test	WB/S/P	GCDEN(NS)-402c√	Cassette	/	25 Tests/Kit
Dengue NS1 & IgG/IgM Combo Test	WB/S/P	GCDEN-425a√	Cassette	/	20 Tests/Kit
EV71 IgM Test	S/P	GCEV71(IgM)-302a√	Cassette	/	25 Tests/Kit
	WB/S/P	GCEV71(IgM)-402a√	Cassette	/	25 Tests/Kit
Giardia lamblia Test	Feces	GCGLA-602a√	Cassette	/	20 Tests/Kit
Gonorrhoeae Test	Swab	GCGON-502b	Cassette	1.0E+7	20 Tests/Kit
HAV IgM Test	S/P	GCHAV(IgM)-302Ba√	Cassette	/	25 Tests/Kit
HAV IgG/IgM Test	WB/S/P	GCHAV(IgG/IgM)-402a√	Cassette	/	25 Tests/Kit
HAV AntigenTest	Feces	GCHAV-602a√	Cassette	/	25 Tests/Kit
	S/P	GCH8cb-302a	Cassette	2 NCU	25 Tests/Kit
HBCAb Hepatitis B Core Antibody Test	S/P	GCH8cb-302b	Cassette	8 NCU	25 Tests/Kit
	WB/S/P	GCH8cb-402a	Cassette	2 NCU	25 Tests/Kit
	S/P	GCH8eb-302a	Cassette	2 NCU	25 Tests/Kit
		GCH8eb-302b	Cassette	8 NCU	25 Tests/Kit
	WB/S/P	GCH8eb-402a	Cassette	2 NCU	25 Tests/Kit
	S/P	GCH8eg-302a	Cassette	0.5 NCU	25 Tests/Kit
HBeAg Hepatitis B Envelope Antigen Test	WB/S/P	GCH8eg-402a	Cassette	0.5 NCU	25 Tests/Kit
	S/P	GCH8sb-301a	Strip	30 mIU/mL	50 Tests/Kit
		GCH8sb-302a	Cassette	30 mIU/mL	25 Tests/Kit
		GCH8sb-401a	Strip	30 mIU/mL	50 Tests/Kit
		GCH8sb-402a	Cassette	30 mIU/mL	25 Tests/Kit
		GCH8sb-402b	Cassette	20 mIU/mL	25 Tests/Kit
		GCH8sg-301a	Strip	1 ng/mL	50 Tests/Kit
	S/P	GCH8sg-302a	Cassette	1 ng/mL	25 Tests/Kit
		GCH8sg-401a	Strip	1 ng/mL	50 Tests/Kit
		GCH8sg-402a	Cassette	1 ng/mL	25 Tests/Kit
HBSAg Hepatitis B Surface Antigen Rapid Test	WB/S/P	GCHBC-402a	Cassette	/	25 Tests/Kit
	S/P	GCHBCISY-345a	Cassette	/	20 Tests/Kit
HBSAg/HCV/HIV/Syphilis Combo Test	WB/S/P	GCHBCISY-445a	Cassette	/	20 Tests/Kit
	S/P	GCHBV-355a	Cassette	/	20 Tests/Kit
HBV HBCAb/HBeAb/HBeAg/HBsAb	WB/S/P	GCHBV-455a	Cassette	/	20 Tests/Kit
	S/P	GCHCV-301a	Strip	/	50 Tests/Kit
		GCHCV-302a√	Cassette	/	25 Tests/Kit
		GCHCV-401a	Strip	/	50 Tests/Kit
HCV Hepatitis C Virus Test	WB/S/P	GCHCV-402a√	Cassette	/	25 Tests/Kit
HCV/HIV Combo Test	WB/S/P	GCHCI-402a	Cassette	/	25 Tests/Kit
HEV Hepatitis E Virus IgM Test	S/P	GCHEV-302a√	Cassette	/	25 Tests/Kit
	S/P	GCHIV-301a	Strip	/	50 Tests/Kit
		GCHIV-302a√	Cassette	/	25 Tests/Kit
HIV 1/2 Antibody Test	WB/S/P	GCHIV-401a	Strip	/	50 Tests/Kit
		GCHIV-402a√	Cassette	/	25 Tests/Kit
HIV 1/2 Antibody Tri-line Test	WB/S/P	GCHIV-GT402a	Cassette	/	25 Tests/Kit
	S/P	GCHIV-T302b	Cassette	/	25 Tests/Kit
HIV 1/2/O Antibody Test	WB/S/P	GCHIV-T402a	Cassette	/	25 Tests/Kit
HIV Antigen/Antibody Combo Test	WB/S/P	GCHV(Ag/Ab)-402a	Cassette	/	25 Tests/Kit
	S/P	GCHSV(IgG)-302a√	Cassette	/	25 Tests/Kit
	WB/S/P	GCHSV(IgG)-402a√	Cassette	/	25 Tests/Kit
	S/P	GCHSV(IgM)-302a√	Cassette	/	25 Tests/Kit
HSV IgM Test	WB/S/P	GCHSV(IgM)-402a√	Cassette	/	25 Tests/Kit
	S/P	GCHSV(IgG/IgM)-302a	Cassette	/	25 Tests/Kit
HSV IgG/IgM Test	WB/S/P	GCHSV(IgG/IgM)-402a	Cassette	/	25 Tests/Kit
	S/P	GCHP-301a√	Strip	/	50 Tests/Kit
		GCHP-302a√	Cassette	/	25 Tests/Kit
		GCHP-401a√	Strip	/	50 Tests/Kit
	WB/S/P	GCHP-402a√	Cassette	/	25 Tests/Kit

H. pylori Antigen Test	Feces	GCHP-601a/	Strip	/	25 Tests/Kit	
		GCHP-601Ca/	Strip	/	25 Tests/Kit	
		GCHP-602a/	Cassette	/	20 Tests/Kit	
		GCHP-602Ca/	Cassette	/	20 Tests/Kit	
Influenza A Antigen Test	Nasal/Throat Swabs	GCFLU(A)-501a/	Strip	1.5 x 10 ⁴ TCID ₅₀	25 Tests/Kit	
		GCFLU(A)-502a/	Cassette	1.5 x 10 ⁴ TCID ₅₀	20 Tests/Kit	
Influenza A/B Antigen Test	Nasal/Throat Swabs	GCFLU(A/B)-501a/	Strip	1.5x 10 ⁴ TCID ₅₀ / 1.5 x 10 ⁵ TCID ₅₀	25 Tests/Kit	
		GCFLU(A/B)-502a/	Cassette	1.5x 10 ⁴ TCID ₅₀ / 1.5 x 10 ⁵ TCID ₅₀	20 Tests/Kit	
			GCFLU(A/B)-502Ca/	Cassette	1.5x 10 ⁴ TCID ₅₀ / 1.5 x 10 ⁵ TCID ₅₀	20 Tests/Kit
		Nasopharyngeal Swab	GCFC-525a/	Cassette	/	20 Tests/Kit
Influenza & COVID-19 Antigen Combo Test	NA & NP Swab	GCFC-525a-NN/	Cassette	/	20 Tests/Kit	
		GCFC-525a-NA/	Cassette	/	20 Tests/Kit	
	Nasal Swab	GCFC-7603a/ ^{New}	Cassette	/	1/5/20 Tests/Kit	
		GCFC-7603a/ ^{New}	Device	/	1/2/5/10 Test(s)/Kit	
Flu, COVID-19, RSV & Adeno Antigen Combo Test	Nasopharyngeal Swab	GCFCRA-545a/	Cassette	/	20 Tests/Kit	
	Nasal Swab	GCFCRA-7525a/ ^{New}	Cassette	/	20 Tests/Kit	
Leishmania Antibody Test	S/P	GCKal-301a	Strip	/	50 Tests/Kit	
		GCKal-401a/	Strip	/	50 Tests/Kit	
	WB/S/P	GCKal-402a	Cassette	/	25 Tests/Kit	
		GCKal-7402a/	Cassette	/	25 Tests/Kit	
Malaria Pan Antigen Test	Whole Blood	GMAL(pan)-402a/	Cassette	200 parasites	25 Tests/Kit	
Malaria P.I. Antigen Test	Whole Blood	GMAL(pf)-402a/	Cassette	200 parasites	25 Tests/Kit	
Malaria P.I./Pan Antigen Test	Whole Blood	GMAL(pf/pan)-402a/	Cassette	200 parasites	25 Tests/Kit	
Malaria P.I./P.v. Antigen Test	Whole Blood	GMAL(pf/pv)-402a/	Cassette	200 parasites	25 Tests/Kit	
Malaria P.I./P.v. Antibody Test	S/P	GMAL(pf/pv Ab)-302a/	Cassette	/	25 Tests/Kit	
Monkeypox IgG/IgM Antibody Test	WB/S/P	GMAL(pf/pv Ab)-402a/	Cassette	/	25 Tests/Kit	
Monkeypox Antigen Test	WB/S/P	GCMKP-402a/ ^{New}	Cassette	/	25 Tests/Kit	
	WB/S/P or Throat swab	GCMKP-502a/ ^{New}	Cassette	/	25 Tests/Kit	
Mononucleosis Test	S/P	GCMON-325a/	Cassette	/	25 Tests/Kit	
		GCMON-402a/	Cassette	/	25 Tests/Kit	
	WB/S/P	GCMON-425a/	Cassette	/	25 Tests/Kit	
		GCMMP(lgM)-302a/	Cassette	/	25 Tests/Kit	
M. pneumonia IgM Test	S/P	GCRSV-502a/	Cassette	/	20 Tests/Kit	
Respiratory Syncytial Virus Antigen Test	Swab	GCROA-602a/	Cassette	/	25 Tests/Kit	
Rotavirus Test	Feces	GCROA-602a/	Cassette	/	25 Tests/Kit	
Rotavirus/Adenovirus Test		GCROA/ADE-602a/	Cassette	/	25 Tests/Kit	
Rubella IgG Test	S/P	GCRUB(lgG)-302a	Cassette	/	25 Tests/Kit	
	WB/S/P	GCRUB(lgG)-402a	Cassette	/	25 Tests/Kit	
Rubella IgM Test	S/P	GCRUB(lgM)-302a	Cassette	/	25 Tests/Kit	
	WB/S/P	GCRUB(lgM)-402a	Cassette	/	25 Tests/Kit	
	S/P	GCRUB(lgG/lgM)-302a	Cassette	/	25 Tests/Kit	
Rubella IgG/IgM Test	WB/S/P	GCRUB(lgG/lgM)-402a	Cassette	/	25 Tests/Kit	
		GCRUB(lgG/lgM)-7402a	Cassette	/	25 Tests/Kit	
Strep A Test	Throat Swab	GCSTR-501a/	Strip	/	25 Tests/Kit	
		GCSTR-501Ca/†	Strip	/	25 Tests/Kit	
		GCSTR-502a/	Cassette	/	20 Tests/Kit	
		GCSTR-502Ca/	Cassette	/	20 Tests/Kit	
Syphilis Test	S/P	GCSYP-301a/	Strip	/	50 Tests/Kit	
		GCSYP-302a/	Cassette	/	25 Tests/Kit	
		GCSYP-401a/	Strip	/	50 Tests/Kit	
		GCSYP-402a/	Cassette	/	25 Tests/Kit	
S. typhi Antigen Test	S/P/Feces	GCSAL(ST)-602a/	Cassette	/	20 Tests/Kit	
TOXO IgG Test	S/P	GCTOX(lgG)-302a/	Cassette	/	25 Tests/Kit	
	WB/S/P	GCTOX(lgG)-402a	Cassette	/	25 Tests/Kit	
TOXO IgM Test	S/P	GCTOXO(lgM)-302a/	Cassette	/	25 Tests/Kit	
	WB/S/P	GCTOXO(lgM)-402a	Cassette	/	25 Tests/Kit	
Toxo IgG/IgM Test	S/P	GCTOX-302b	Cassette	/	25 Tests/Kit	
		GCTOX(lgG/lgM)-302a/	Cassette	/	20 Tests/Kit	
ToRCH Toxo/Rubella/CMV/HSV IgG Combo Test	WB/S/P	GCTOX-402b	Cassette	/	25 Tests/Kit	
	S/P	GCTOG-345a	Cassette	/	20 Tests/Kit	
ToRCH Toxo/Rubella/CMV/HSV IgM Combo Test	S/P	GCTOM-345a	Cassette	/	20 Tests/Kit	
Trichomonas vaginalis Test	Vaginal Swab	GCTV-502a/	Cassette	/	20 Tests/Kit	
Tuberculosis IgG/IgM Test	S/P	GCTB-302a/	Cassette	/	25 Tests/Kit	
	WB/S/P	GCTB-402a/	Cassette	/	25 Tests/Kit	
Typhoid IgG/IgM Test	S/P	GCTYP-301a	Strip	/	50 Tests/Kit	
		GCTYP-302a/	Cassette	/	25 Tests/Kit	
V. cholerae O1 Antigen Test	Feces	GCVCH(O1)-602a/	Cassette	/	25 Tests/Kit	
V. cholerae O1/O139 Antigen Test	Feces	GCVCH(O1/O9)-602a/	Cassette	/	25 Tests/Kit	
ZIKA IgM Test	WB/S/P	GCZIK(lgM)-402a	Cassette	/	25 Tests/Kit	
ZIKA IgG Test	WB/S/P	GCZIK(lgG)-402a	Cassette	/	25 Tests/Kit	
ZIKA NS1 Test	WB/S/P	GCZIK(NS1)-402a	Cassette	/	25 Tests/Kit	

Fertility

Product Description	Specimen	Catalog No.	Format	Cut-off Value	Kit Size
hCG Pregnancy Test	Urine	GAHCG-101a/†	Strip	25 mIU/mL	100 Tests/Kit
		GAHCG-101b/	Strip	10 mIU/mL	100 Tests/Kit
		GAHCG-101d/	Strip	20 mIU/mL	100 Tests/Kit
		GAHCG-102a/†	Cassette	25 mIU/mL	25 Tests/Kit
		GAHCG-102b/	Cassette	10 mIU/mL	25 Tests/Kit
		GAHCG-102d/	Cassette	20 mIU/mL	25 Tests/Kit
		GAHCG-103a/†	Midstream	25 mIU/mL	1/2 Test(s)/Kit
		GAHCG-103b/	Midstream	10 mIU/mL	1/2 Test(s)/Kit
		GAHCG-103d/	Midstream	20 mIU/mL	1/2 Test(s)/Kit
		GAHCG-105a	Panel	25 mIU/mL	25 Tests/Kit
	Urine/Serum	GAHCG-201a/	Strip	25 mIU/mL	100 Tests/Kit
		GAHCG-201b/	Strip	10 mIU/mL	100 Tests/Kit
		GAHCG-202a/	Cassette	25 mIU/mL	25 Tests/Kit
		GAHCG-202b/	Cassette	10 mIU/mL	25 Tests/Kit
Digital Pregnancy Test	Urine	GAHCG-D103a/	Midstream	25 mIU/mL	1/2 Test(s)/Kit
LH Ovulation Test	Urine	GALH-101a/	Strip	25 mIU/mL	100 Tests/Kit
		GALH-101b/	Strip	40 mIU/mL	100 Tests/Kit
		GALH-101d	Strip	30 mIU/mL	100 Tests/Kit
		GALH-102a/	Cassette	25 mIU/mL	25 Tests/Kit
		GALH-102b/	Cassette	40 mIU/mL	25 Tests/Kit
		GALH-103a/	Midstream	25 mIU/mL	1/5 Test(s)/Kit
		GALH-103b/	Midstream	40 mIU/mL	1/5 Test(s)/Kit
		GALH-103d	Midstream	30 mIU/mL	1/5 Test(s)/Kit
FSH Menopause Test	Urine	GAFSH-101a/	Strip	25 mIU/mL	100 Tests/Kit
IGFBP-1 PROM Test	Cervical Secretion	GAIGF1-501a/	Strip	25 ng/mL	25 Tests/Kit
		GAIGF1-502a/	Cassette	25 ng/mL	20 Tests/Kit
Male Fertility Test	Semen	GASPE-002a/	Cassette	15M/mL	1 Test/Kit

Cardiac Marker

Product Description	Specimen	Catalog No.	Format	Cut-off Value	Kit Size
CK-MB Test	S/P	GDCKM-302a/	Cassette	5 ng/mL	25 Tests/Kit
CRP C-Reactive Protein Semi-Quantitative Test	WB/S/P	GDCKM-402a/	Cassette	5 ng/mL	25 Tests/Kit
	WB/S/P	GDGRP-402a/	Cassette	1~3~10 mg/L	25 Tests/Kit
D-dimer Test	WB/P	GDGRP-T402b/	Cassette	10~40~80 mg/L	25 Tests/Kit
Myoglobin Test	WB/S/P	GDCCI-402b/	Cassette	500 ng/mL	25 Tests/Kit
Procalcitonin Test	WB/S/P	GDPMYO-402a/	Cassette	50 ng/mL	25 Tests/Kit
Troponin I Test	S/P	GDPC-T402a/	Cassette	0.5~2~10 ng/mL	25 Tests/Kit
		GDTR0-302a/	Cassette	0.5 ng/mL	25 Tests/Kit
		GDTR0-402a/	Cassette	0.5 ng/mL	25 Tests/Kit
		GDTR0-402b/	Cassette	0.5 ng/mL	25 Tests/Kit
Cardiac Myoglobin/CK-MB/CTnl Combo Test	S/P	GDGCA-335a/	Cassette	50/5/0.5 ng/mL	25 Tests/Kit
		GDGCA-435a/	Cassette	50/5/0.5 ng/mL	25 Tests/Kit
	WB/S/P	GDGCA-W435a/	Cassette	50/5/0.5 ng/mL	20 Tests/Kit

Urinalysis

Product Description	Specimen	Format	Cut-off Value	Kit Size
Ascorbate/†	Urine	Strip	0.5-0.6 mmol/L	100 Tests/Canister
Bilirubin/†	Urine	Strip	8.6-17 µmol/L	100 Tests/Canister
Blood/†	Urine	Strip	5-15 Ery/µL	100 Tests/Canister
Ca/	Urine	Strip	2.5 mmol/L	100 Tests/Canister
Creatinine/	Urine	Strip	50 mg/dL	100 Tests/Canister
Glucose/†	Urine	Strip	2.8~5.5 mmol/L	100 Tests/Canister
Ketone/†	Urine	Strip	0.5~1.0 mmol/L	100 Tests/Canister
Leukocytes/†	Urine	Strip	5-15 Leuko/µL	100 Tests/Canister
Micro Albumin/	Urine	Strip	0.08~0.15 mg/dL	100 Tests/Canister
Nitrite/†	Urine	Strip	13~22 µmol/L	100 Tests/Canister
pH/†	Urine	Strip	0.5	100 Tests/Canister
Protein/†	Urine	Strip	0.15~0.3 g/L	100 Tests/Canister
Specific Gravity/†	Urine	Strip	0.005	100 Tests/Canister
Urobilinogen/†	Urine	Strip	3.3-16 µmol/L	100 Tests/Canister
Urinary Tract Infection Test Strip	Urine	Strip	LEU: 10-15 Leuko/µL NIT: 13-22 µmol/L	3 Tests/Kit

Tumor Marker

Product Description	Specimen	Catalog No.	Format	Cut-off Value	Kit Size
AFP Alpha Fetal Protein Test	S/P	GEAFP-301a	Strip	20 ng/mL	50 Tests/Kit
	WB/S/P	GEAFP-302a/	Cassette	20 ng/mL	25 Tests/Kit
CEA Carcinoembryonic Antigen Test	S/P	GEAFP-401a/	Strip	20 ng/mL	50 Tests/Kit
		GEAFP-402a/	Cassette	20 ng/mL	25 Tests/Kit
		GECEA-301a	Strip	5 ng/mL	50 Tests/Kit
		GECEA-302a	Cassette	5 ng/mL	25 Tests/Kit
		GECEA-401a/	Strip	5 ng/mL	50 Tests/Kit
		GECEA-402a/	Cassette	5 ng/mL	25 Tests/Kit
FOB Fecal Occult Blood Test	Feces	GEFOB-601b/†	Strip	50 ng/mL	25 Tests/Kit
		GEFOB-601Cb/	Strip	50 ng/mL	25 Tests/Kit
		GEFOB-601c/	Strip	100 ng/mL	25 Tests/Kit
		GEFOB-601d	Strip	200 ng/mL	25 Tests/Kit
		GEFOB-602b/†	Cassette	50 ng/mL	20 Tests/Kit
		GEFOB-602Cb/	Cassette	50 ng/mL	20 Tests/Kit
		GEFOB-602c/	Cassette	100 ng/mL	20 Tests/Kit
		GEFOB-602d	Cassette	200 ng/mL	20 Tests/Kit
		GEFOB-602h	Cassette	150 ng/mL	20 Tests/Kit
		GEFOB-602j/	Cassette	10 ng/mL	20 Tests/Kit
FOB/Transferrin Combo Test	Feces	GEFOB/TF-602a/	Cassette	50/10 ng/mL	20 Tests/Kit
Nuclear Matrix Protein 22 Test	Urine	GENMP22-102a/ ^{New}	Cassette	10 U/mL	25 Tests/Kit
		GEPSA-301a/	Strip	4 ng/mL	50 Tests/Kit
PSA Prostate Specific Antigen Test	S/P	GEPSA-302a/	Cassette	4 ng/mL	25 Tests/Kit
	WB/S/P	GEPSA-401a/	Strip	4 ng/mL	50 Tests/Kit
PSA Prostate Specific Antigen Semi-Quantitative Test	S/P	GEPSA-402a/	Cassette	4 ng/mL	25 Tests/Kit
	WB/S/P	GEPSA-302b	Cassette	4 ng/mL, 10 ng/mL	25 Tests/Kit
Transferrin Test	Feces	GETF-601a/	Strip	4 ng/mL, 10 ng/mL	25 Tests/Kit
		GETF-602a/	Cassette	10 ng/mL	20 Tests/Kit

Veterinary

Product Description	Specimen	Catalog No.	Format	Label	Cut-off Value	Kit Size
Canine Adenovirus (CAV) Antigen Test	Secretions	GFCAV-502a	Cassette	Gold	/	10 Tests/Kit
Canine Coronavirus (CCV) Antigen Test	Feces	GFCCV-602a	Cassette	Gold	/	10 Tests/Kit
		FFCCV-602a	Cassette	Fluorescence	10 IU	10 Tests/Kit
Canine Coronavirus (CCV) & Parvovirus (CPV) Antigen Combo Test	Feces	GFCCP-T602a	Cassette	Gold	/	10 Tests/Kit
Canine C-Reactive Protein (cCRP) Test	WB/S/P	FFCCR-402a	Cassette	Fluorescence	10 IU	10 Tests/Kit
Canine Distemper Virus (CDV) Antigen Test	Secretions	GFCDV-502a	Cassette	Gold	/	10 Tests/Kit
		FFCDV-502a	Cassette	Fluorescence	10 IU	10 Tests/Kit
Canine Distemper Virus (CDV), Influenza Virus (CIV) & Adenovirus (CAV) Antigen Combo Test	Secretions	GFCDIA-532a	Cassette	Gold	/	10 Tests/Kit
Canine Influenza Virus (CIV) Antigen Test	Secretions	GFClV-502a	Cassette	Gold	/	10 Tests/Kit
Canine Parvovirus (CPV) Antigen Test	Feces	GFPCV-602a	Cassette	Gold	/	10 Tests/Kit
Canine Progesterone (cProg) Test	WB/S/P	FFCPR-402a	Cassette	Fluorescence	10 IU	10 Tests/Kit
Feline Calicivirus (FCV) Antigen Test	Secretions	GFCCV-502a	Cassette	Gold	/	10 Tests/Kit
Feline Coronavirus (FCoV) Antigen Test	Feces	GFCCV-502a	Cassette	Fluorescence	10 IU	10 Tests/Kit
Feline Herpes Virus (FHV) Antigen Test	Secretions	GFFHV-502a	Cassette	Gold	/	10 Tests/Kit
		FFHHV-502a	Cassette	Fluorescence	10 IU	10 Tests/Kit
Feline Parvovirus (FPV) Antigen Test	Feces	GFFPV-602a	Cassette	Gold	/	10 Tests/Kit
Feline Parvovirus (FPV) & Coronavirus (FCoV) Antigen Combo Test	Feces	FFFPV-602a	Cassette	Fluorescence	10 IU	10 Tests/Kit
Feline Serum Amyloid A (fSAA) Test	WB/S/P	FFSAA-402a	Cassette	Gold	/	10 Tests/Kit
Toxoplasma (Toxo) IgG/IgM Test	WB/S/P	GFTOX-402a	Cassette	Fluorescence	5 mg/L	10 Tests/Kit

Non-Infectious Disease

Product Description	Specimen	Catalog No.	Format	Cut-off Value	Kit Size
Micro-Albumin Test	Urine	GIHSA-101a/	Strip	20 µg/mL	100 Tests/Kit
Vaginal pH Test	Vaginal Secretion	GIHSA-102a	Cassette	20 µg/mL	25 Tests/Kit
		VPH-501a ^{New}	Strip	3.8-4.4	100 Tests/Canister

Autoimmunity

Product Description	Specimen	Catalog No.	Format	Kit Size
Rheumatoid Factor IgM Test	S/P	GCRF(IgM)-302a	Cassette	25 Tests/Kit
Total IgE Test	S/P	GCIgE-302a	Cassette	25 Tests/Kit

Instrument

Product Description	Model
Urine Analyzer	Healgen 500/
Urine Analyzer	Healgen 501/
Colloidal Gold Test Reader	OG-D180
Handheld Oral Fluid Drug Test Reader	OG-D200
Multi-Function Colloidal Gold Test Reader	OG-D600
Fluorescence Immunoassay Analyzer	OG-G200
Handheld Fluorescence Immunoassay Analyzer	OG-G300
Mini Immunofluorescence Analyzer	OG-H100/
Veterinary Fluorescence Immunoassay Analyzer	OG-V100

✓CE Marked

†Cleared for US 510(k)

In Specimen column: WB: Whole Blood

S: Serum

P: Plasma



Zhejiang Orient Gene Biotech Co., Ltd was founded in December 2005 and listed on the SEE STAR Market on February 5, 2020 (securities code: 688298). Orient Gene specializes in R&D, production and sales of in vitro diagnostic products, mainly covering infectious diseases (including COVID-19 test series), toxicology, tumor markers, cardiac markers and fertility testing, etc. Through 16 years of technology accumulation and continuous investment in R&D, the Company has independently developed hundreds of products. The company own more than 200 authorized patents, and has obtained more than 500 product medical device certifications at home and abroad. The Company's sales network covers more than 100 countries, products are mainly sold to Europe, America and other developed countries.

Healgen Scientific LLC, a wholly owned subsidiary of Zhejiang Orient Gene Biotech Co., Ltd develops, manufactures and commercializes in vitro diagnostic test systems worldwide. Our product portfolio spans multiple testing categories and analytes to meet various clinical and laboratory needs.

Healgen Scientific Limited Liability Company
Add: 3818 Fuqua Street, Houston, TX77047, USA.
Tel: +1 713-733-8088
Toll free: 866 982 3818
Fax: +1 713-733-8848

E-mail: Healgensales@healgen.us (For South America and North America)
Web: <http://www.healgen.com>

Zhejiang Orient Gene Biotech Co., Ltd
Add: 3787#, East Yangguang Avenue, Dipu Street,
Anji, Huzhou, Zhejiang, China.
P.C.: 313300
Tel: +86-572-5303755/5303756
Fax: +86-572-5226222
E-mail: sales@orientgene.com (For rest of world)
Web: <http://www.orientgene.com>

Rev.08/2022

PRODUCT CATALOG

Enhancing
Global Health



Troponin I

Troponin I Rapid Test Device (Whole Blood/Serum/Plasma) Package Insert

A rapid visual immunoassay for the qualitative presumptive detection of cardiac Troponin I in human whole blood, serum, or plasma specimens.
For professional in vitro diagnostic use only.

INTENDED USE

The Troponin I Rapid Test Device (Whole Blood/Serum/Plasma) is a rapid visual immunoassay for the qualitative presumptive detection of cardiac Troponin I in human whole blood, serum, or plasma specimens. This kit is intended to be used as an aid in the diagnosis of myocardial infarction (MI).

SUMMARY

Cardiac Troponin I (cTnI) is a protein found in cardiac muscle with a molecular weight of 22.5 kDa.¹ Troponin I is part of a three subunit complex comprising of Troponin T and Troponin C. Along with tropomyosin, this structural complex forms the main component that regulates the calcium sensitive ATPase activity of actomyosin in striated skeletal and cardiac muscle.² After cardiac injury occurs, Troponin I is released into the blood 4-6 hours after the onset of pain. The release pattern of cTnI is similar to CK-MB, but while CK-MB levels return to normal after 72 hours, Troponin I remains elevated for 6-10 days, thus providing for a longer window of detection for cardiac injury. The high specificity of cTnI measurements for the identification of myocardial damage has been demonstrated in conditions such as the perioperative period, after marathon runs, and blunt chest trauma.³ cTnI release has also been documented in cardiac conditions other than acute myocardial infarction (AMI) such as unstable angina, congestive heart failure, and ischemic damage due to coronary artery bypass surgery.⁴ Because of its high specificity and sensitivity in the myocardial tissue, Troponin I has recently become the most preferred biomarker for myocardial infarction.⁵

PRINCIPLE

The Troponin I Rapid Test Device (Whole Blood/Serum/Plasma) has been designed to detect cardiac Troponin I through visual interpretation of color development in the strip. The membrane was immobilized with anti-cTnI antibodies on the test region. During the test, the specimen is allowed to react with colored anti-cTnI antibodies colloidal dog conjugates, which were precoated on the sample pad of the test. The mixture then moves on the membrane by a capillary action, and interact with reagents on the membrane. If there were enough cTnI in specimens, a colored band will form at the test region of the membrane.

Presence of this colored band indicates a positive result, while its absence indicates a negative result. Appearance of a colored band at the control region serves as a procedural control. This indicates that proper volume of specimen has been added and membrane wicking has occurred.

PRECAUTIONS

- For professional In Vitro diagnostic use only.
- Warning: the reagents in this kit contain sodium azide which may react with lead or copper plumbing to form potentially explosive metal azides. When disposing of such reagents, always flush with large volumes of water to prevent azide build-up.
- Do not use it if the tube/pouch is damaged or broken.
- Test is for single use only. Do not re-use under any circumstances.
- Handle all specimens as if they contain infectious agents. Observe established standard procedure for proper disposal of specimens
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assayed.
- Humidity and temperature can adversely affect results

STORAGE AND STABILITY

All reagents are ready to use as supplied. Store unused test device unopened at 2°C-30°C. If stored at 2°C-8°C, ensure that the test device is brought to room temperature before opening. The test is not stable out off the expiration date printed on the sealed pouch. Do not freeze the kit or expose the kit over 30°C.

SPECIMEN COLLECTION AND PREPARATION

- The Troponin I Rapid Test Device (Whole Blood/Serum/Plasma) is intended only for use with human whole blood, serum, or plasma specimens.
- Only clear, non-hemolyzed specimens are recommended for use with this test.
- Serum or plasma should be separated with soonest possible opportunity to avoid hemolysis.
- Perform the testing immediately after the specimen collection. Do not leave the specimens at room temperature for prolonged periods. Specimens may be stored at 2-8°C for up to 3 days. For long term storage, specimens should be kept below -20°C.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Avoid repeated freezing and thawing of specimens.

- Pack the specimens in compliance with applicable regulations for transportation of etiological agents, in case they need to be shipped.
- Icteric, lipemic, hemolyzed, heat treated and contaminated sera may cause erroneous results.
- There is a slight possibility that some whole blood specimens with very high viscosity or which have been stored for more than 2 days may not run properly on the test device. Repeat the test with a serum or plasma specimen from the same patient using a new test device.

MATERIALS

Materials Provided

- Test devices
- Buffer

- Disposable Droppers
- Package insert

Materials Required But Not Provided

- Specimen collection containers
- Centrifuge (for plasma only)

- Clock or Timer

DIRECTIONS FOR USE

Allow test device, specimen, buffer and/or controls to equilibrate to room temperature (15-30°C) prior to testing.

- Remove the test from its sealed pouch, and place it on a clean, level surface. Label the device with patient or control identification. To obtain a best result, the assay should be performed within one hour.

- Transfer 2 drops of serum or plasma to the specimen well of the device with a disposable pipette provided in the kit, and then start the timer.

OR


Transfer 3 drops of whole blood specimen to the specimen well of the device with a disposable pipette provided in the kit, then add 1 drop of buffer, and start the timer.

OR

Allow 3 hanging drops of fingerstick whole blood specimen to fall into the center of the specimen well (S) on the device, then add 1 drop of buffer, and start the timer. Avoid trapping air bubbles in the specimen well (S), and do not drop any solution in observation window.

As the test begins to work, you will see color move across the membrane.

- Wait for the colored band(s) to appear. The result should be read at 10 minutes. Do not interpret the result after 20 minutes.

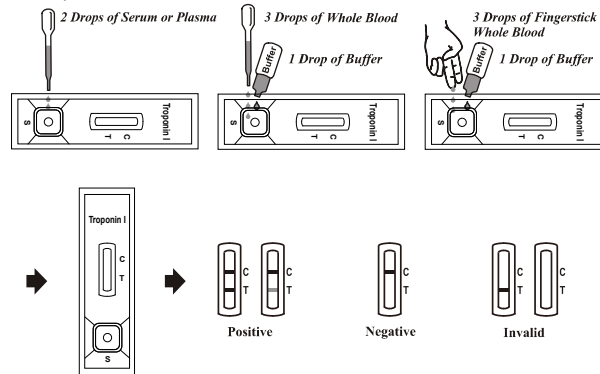

INTERPRETATION OF RESULTS

(Please refer to the illustration above)

POSITIVE: Two colored bands appear on the membrane. One band appears in the control region (C) and another band appears in the test region (T).

NEGATIVE: Only one colored band appears in the control region (C). No apparent colored band appears in the test region (T).

INVALID: Control band fails to appear. Results from any test which has not produced a control band at the specified reading time must be discarded.

Please review the procedure and repeat with a new test. If the problem persists, discontinue using the kit immediately and contact your local distributor.

NOTE:

- The intensity of the color in test region (T) may vary depending on the concentration of aimed substances present in the specimen. Therefore, any shade of color in the test region should be considered positive. Besides, the substances level can not be determined by this qualitative test.
- Insufficient specimen volume, incorrect operation procedure, or performing expired tests are the most likely reasons for control band failure.

QUALITY CONTROL

Internal procedural controls are included in the test. A colored band appearing in the control region (C) is considered an internal positive procedural control. It confirms sufficient specimen volume and correct procedural technique.

External controls are not supplied with this kit. It is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

LIMITATIONS

- The Troponin I Rapid Test Device (Whole Blood/Serum/Plasma) is for professional in vitro diagnostic use, and should be used for the qualitative detection of cardiac Troponin I only. There is no meaning attributed to linen color intensity or width.
- The Troponin I Rapid Test Device (Whole Blood/Serum/Plasma) will only indicate the presence of Troponin I in the specimen and should not be used as the sole criteria for the diagnosis of tuberculosis.
- If the test result is negative and clinical symptoms persist, additional testing using other clinical methods is recommended. The test cannot detect less than 0.5 ng/mL of cTnI in specimens. Thus, a negative result does not at anytime rule out the existence of Troponin I in blood, because the antibodies may be absent or below the minimum detection level of the test.
- Like with all diagnostic tests, a confirmed diagnosis should only be made by a physician after all clinical and laboratory findings have been evaluated.
- Some specimens containing unusually high titers of heterophile antibodies or rheumatoid factor (RF) may affect expected results. Even if the test results are positive, further clinical evaluation should be considered with other clinical information available to the physician.

PERFORMANCE CHARACTERISTICS

Table: Troponin I Rapid Test vs. EIA

Method		Troponin I Rapid Test Device		Total Results
EIA	Results	Positive	Negative	
	Positive	138	2	140
	Negative	1	315	316
Total Results		139	317	456

Relative Sensitivity: 98.6% (94.9%-99.8%)*

Relative Specificity: 99.7% (98.3%-99.9%)*

Overall Agreement: 99.3% (98.1%-99.9%)*

*95% Confidence Interval

BIBLIOGRAPHY

- Adams, et al. Biochemical markers of myocardial injury, Immunoassay Circulation 88: 750-763, 1993.
- Mehegan JP, Tobacman LS. Cooperative interaction between troponin molecules bound to the cardiac thin filament. J.Biol.Chem. 266:966, 1991.
- Adams, et al. Diagnosis of Perioperative myocardial infarction with measurements of cardiac troponin I. N.Eng.J.Med 330:670, 1994.
- Hossein-Nia M, et al. Cardiac troponin I release in heart transplantation. Ann. Thorac. Surg. 61: 227, 1996.
- Alpert JS, et al. Myocardial Infarction Redefined, Joint European Society of Cardiology American College of Cardiology: J. Am. Coll. Cardio., 36(3):959, 2000.