



SHANDONG CHENGWU MEDICAL PRODUCTS FACTORY

Address: Southern end of Quancheng Road, Chengwu County, Heze City, Shandong Province
274200 P.R. China

Tel: +86-15102183521 Web: www.chengwumed.com www.vvzp.com

TECHNICAL DATA SHEET

Blood Collection Needle

The product and vacuum blood tube supporting the use of venous blood specimen collection
Sterile, Non-toxic, pyrogen free, compatible with holders, single use.

Soft-connection:

Safety sheath

Flexible double wings


High quality
stainless needle

Dehp-free pvc tube



| Reference code | Description | Tubinglength | Color |
|----------------|---|----------------|--------|
| CY-127 | Blood Collection Needle 20G x 3/4" (0.90 x 19 mm) | 18cm,25cm,30cm | Yellow |
| CY-128 | Blood Collection Needle 21G x 3/4" (0.80 x 19 mm) | 18cm,25cm,30cm | Green |
| CY-129 | Blood Collection Needle 22G x 3/4" (0.70 x 19 mm) | 18cm,25cm,30cm | Black |
| CY-130 | Blood Collection Needle 23G x 3/4" (0.60 x 19 mm) | 18cm,25cm,30cm | Blue |
| CY-131 | Blood Collection Needle 25G x 3/4" (0.50 x 19 mm) | 18cm,25cm,30cm | Pink |

Hard-connection: Pen Type Blood Collection Needle

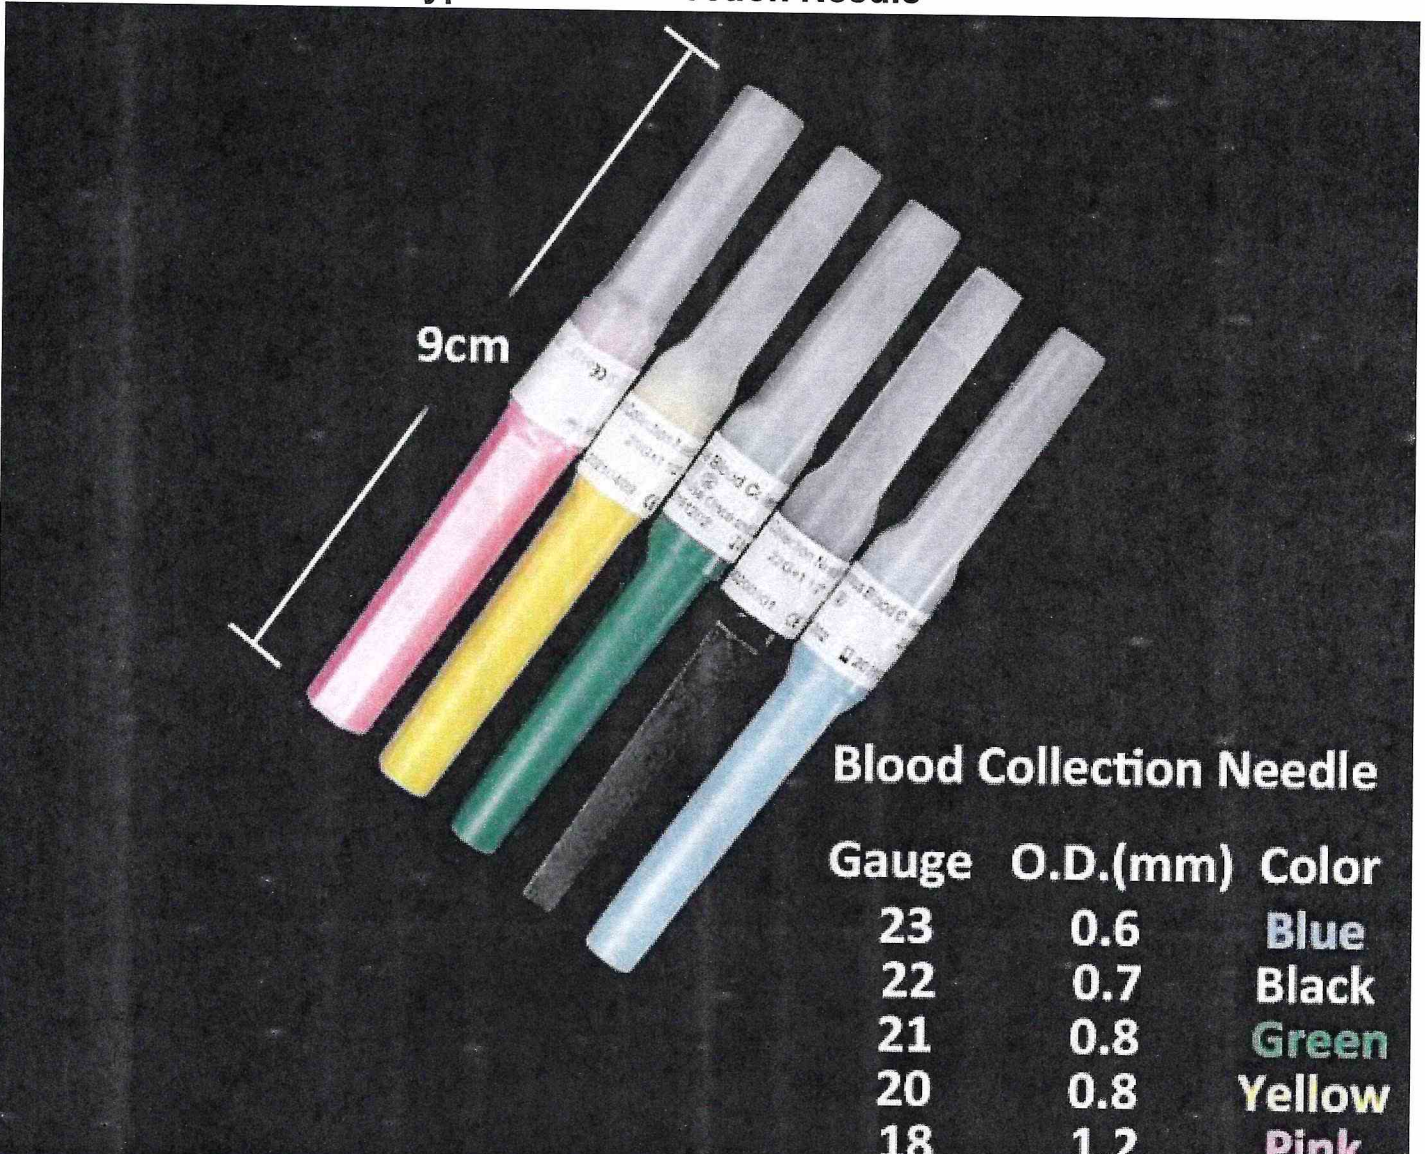

Blood Collection Needle

| Gauge | O.D.(mm) | Color |
|-------|----------|--------|
| 23 | 0.6 | Blue |
| 22 | 0.7 | Black |
| 21 | 0.8 | Green |
| 20 | 0.8 | Yellow |
| 18 | 1.2 | Pink |

| Reference code | Gauge | Tubinglength | Color |
|----------------|-------|--------------|--------|
| CY-116 | 18G | 1 or 1 1/2" | Pink |
| CY-117 | 20G | 1 or 1 1/2" | Yellow |
| CY-118 | 21G | 1 or 1 1/2" | Green |
| CY-119 | 22G | 1 or 1 1/2" | Black |
| CY-120 | 23G | 1 or 1 1/2" | Blue |

FlashBack Blood Collection needle:



| Reference code | Gauge | Tubinglength | Color |
|----------------|-------|--------------|-------|
| CY-113 | 21G | 1 or 1 1/2" | Green |
| CY-114 | 22G | 1 or 1 1/2" | Black |
| CY-115 | 23G | 1 or 1 1/2" | Blue |

Label&remarks

| | | | |
|-------------------|---|--------|---|
| Product name | ✓ | CE | ✓ |
| Quantity (pieces) | ✓ | ⊗ | ✓ |
| LOT | ✓ | ⊗ | ✓ |
| ⌚ | ✓ | ⚙ | ✓ |
| STERILE EO | ✓ | EC REP | ✓ |

Signature and Stamp

Date ... 16th, Aug 2023

