

Table Top Low Speed Centrifuge

Features for BKC-TL4IV:

- * Maintenance-free brushless DC motor.
- * Microprocessor control, LED display.
- * Stainless steel chamber.
- * Rotor recognition system, Automatically electric lid lock, over speed, over temperature, and imbalance protection.



Features for BKC-TL5VII:

- * DC Brushless motor, special damping device make the motor run steady, free maintenance.
- * Display: microprocessor control, LED display of running parameters, 10rpm increments, conversion of RPM/RCF.
- * Function: automatically electric lid lock, over speed, over temperature and imbalance protection, memory flashing function.
- * Alarm: over speed, rotor mounting abnormally.
- * External cold-rolled steel with powder coating, stainless steel centrifugal chamber and lid.

Technical Parameters:

Model	BKC-TL4IV	BKC-TL5VII
Max. Capacity	6*50ml	
Max. Speed	4000rpm	5000rpm
Speed Precision	/	±30rpm
Timing Range	1~60min	0~99min
Noise	≤65dB	<58dB
Consumption	180W	300W
Power Supply	AC110/220V, 50/60Hz	
External Size(W*D*H)mm	395*340*305	330*295*255
Package Size(W*D*H)mm	510*420*330	510*445*445
Net/Gross Weight(kg)	20/22	20/28

Rotor:

BKC-TL4IV					BKC-TL5VII				
Rotor No.	Rotor	Capacity	Speed(rpm)	RCF(xg)	Rotor No.	Rotor	Capacity	Speed(rpm)	RCF(xg)
No.1	Angle Rotor	18*10/7ml	4000	2200	No.1	Angle Rotor	18*10/7ml	5000	4020
No.2		24*10/7ml	4000	2200	No.2		24*10/7ml	5000	4020
No.3		12*15/10ml	4000	2200	No.3		12*15/10ml	5000	4020
No.4		12*20/15ml	4000	2200	No.4		12*20/15ml	5000	4020
No.5		6*50ml	4000	2200	No.5		6*50ml	5000	4020

Table Top Low Speed Refrigerated Centrifuge

Technical Parameters:

Model	BKC-TL5R
Max. Speed	5000rpm
Max. RCF	4390xg
Max. Capacity	4*250ml
Speed Precision	±50rpm
Timing Range	1s~99h59min59s
Temp. Range	-20°C~40°C
Temp. Accuracy	±1°C
Refrigerant	CFC-free refrigerant
Noise	≤65dB
Power Supply	AC110/220V, 50/60Hz
External Size(W*D*H)mm	640*680*380
Package Size(W*D*H)mm	780*800*520
Net Weight(kg)	95
Gross Weight(kg)	120



Features:

- * Maintenance-free brushless DC motor.
- * LED/LCD display.
- * Stainless steel chamber.
- * Automatically electric lid lock, over speed, over temperature, and imbalance protection.

Rotor:

Rotor No.	Rotor	Capacity	Max. Speed(rpm)	Max. RCF(xg)
No.1	Angle Rotor	12*10ml	5000	4390
No.2	Swing Bucket Rotor	4*100ml	5000	4390
		4*2*100ml		
		4*4*10ml		
		4*6*10ml	4000	3500
		4*8*10ml		
		4*4*15ml		
		4*6*15ml		
4*8*15ml	5000	4390		
4*50ml				
4*2*50ml	4000	3500		
No.3	Swing Rotor	4*250ml	4000	3500
		4*8*5ml		
	Adapter	4*8*7ml		
		4*8*10ml		
		4*2*50ml		
No.4	Swing Rotor	4*12*7/5ml	4000	2800
		4*18*7/5ml	4000	2800
No.6	Microplate	4*24*7/5ml	4000	2800
No.7		2*2*48well	4000	2300
No.8		2*2*96well	4000	2300

Constant-Temperature Incubator

Features:

- * Intelligent temperature controller, based on microprocessor with PID parameters controlling function, and LCD display make temperature accurate and reliable.
- * The double door makes the temperature fluctuation small. The toughened-glass inner door is convenient to observe chamber condition without affecting chamber temperature.
- * The working chamber adopts stainless steel and round angle structure, easy to clean.



BJPX-H30



BJPX-H50/80/160/270

Optional Accessories: * Independent temperature protector.

Technical Parameters:

Model	BJPX-H30	BJPX-H50	BJPX-H80	BJPX-H160	BJPX-H270
Capacity	30L	50L	80L	160L	270L
Temp. Range	RT+5~65°C				
Temp. Fluctuation	±0.3°C				
Time Setting	1~9999mins				
Alarm	Over-temperature alarm;audible and visual alarm.				
Shelves	2 pcs/adjustable			3 pcs/adjustable	
Consumption	200W	210W	280W	380W	570W
Power Supply	AC220V±10%, 50/60Hz(Standard); AC110±10%, 60Hz(Optional)				
Internal Size(mm)	320*300*315	350*350*410	400*400*500	500*500*650	600*600*750
External Size(mm)	650*470*510	510*520*800	580*570*890	680*670*1050	770*780*1150
Package Size(mm)	780*600*680	600*610*850	670*650*940	800*790*1200	890*890*1300
Gross Weight(kg)	45	55	57	90	130

Constant-Temperature Incubator

Features:

- * Large LED display, multiple groups of data to be displayed at a time; function of timing and over-temperature protection.
- * Two-layer toughened-glass observation window.



BJPX-H30/48/64/123II



BJPX-H230II

Technical Parameters:

Model	BJPX-H30II	BJPX-H48II	BJPX-H64II	BJPX-H123II	BJPX-H230II
Capacity	30L	45L	65L	125L	230L
Temp. Range	RT+5~80°C				
Temp. Fluctuation	±0.2°C				
Time Setting	1~9999mins				
Shelves	2 pcs/adjustable				
Consumption	150W	250W	500W	600W	700W
Power Supply	AC220V±10%, 50/60Hz(Standard); AC110±10%, 60Hz(Optional)				
Internal Size(mm)	310*310*310	350*350*350	400*360*450	500*450*550	600*500*750
External Size(mm)	460*510*695	500*550*735	550*550*840	636*680*915	730*670*1220
Package Size(mm)	550*570*765	620*585*800	640*640*905	730*720*1000	900*800*1350
Gross Weight(kg)	51	56	62	71	105

Horizontal Autoclave

Application:

It is applicable for the sterilization of unpacked solid instrument in department of stomatology, ophthalmology, operation room and CSSD.

Features:

- * Sterilizing programs for fabric, instrument, rubber and liquid.
- * Touch screen display of temperature, pressure, time, running status and failure warning.
- * Post-drying function makes the residual humidity of sterilized articles less than 3%.
- * The positive pressure air-exhaust system to exhaust the cold air from chamber.
- * Equipped with printer to print date, time and process parameters.
- * Build-in efficient steam generator, microcomputer temperature control.
- * Perfect four-level authority management system to avoid mis-operation.
- * Double door optional.



Technical Parameters:

Model	BKQ-B100(H)	BKQ-B150(H)	BKQ-B200(H)	BKQ-B300(H)
Capacity	100L	135L	185L	300L
Chamber Size(mm)	φ400*850	φ500*710	φ500*950	φ632*1000
Chamber Material	SUS304			
Max Working Pressure	0.23Mpa			
Working Temp.	115~138°C			
Temp Accuracy	±0.1°C			
Consumption	10KW	11KW		17KW
Power Supply	380V, 50HZ			
External Size(L*W*H) mm	1250*730*1660	1110*750*1742	1350*750*1742	1400*890*1780
Package Size(L*W*H) mm	1500*900*2050	1370*1000*2060	1510*890*2060	1700*1050*2090
Gross Weight(kg)	310	470	540	830

Horizontal Pulse Vacuum Autoclave

Application:

It can be widely used in department of stomatology and ophthalmology, operating room and other medical institutions. It is suitable for all wrapped or unwrapped solid instrument, A-class cavity instrument (dental hand-pieces and endoscopes), implantable instrument, dressing fabric and rubber tubes, etc.

Features:

- * Built-in efficient steam generator, microcomputer temperature control.
- * Equipped with printer to print date, time and process parameters.
- * Perfect four-level authority management system to avoid mis-operation.
- * Sterilization programs for fabric, instrument, rubber, liquid, cavity, B&D test, PCD test and leakage test.
- * Intelligent drying system to guarantee the residual humidity of instrument and dressing no more than 0.2% and 1% respectively.
- * Over-heat auto protection device, dual door safety lock device, over pressure relief valve, short circuit protection, and overpressure protection.
- * LCD displays temperature, pressure, time, running status, failure and warning code.
- * Double door optional.



Technical Parameters:

Model	BKQ-Z100(H)	BKQ-Z150(H)	BKQ-Z200(H)	BKQ-Z300(H)
Capacity	100L	135L	185L	300L
Chamber Size(mm)	φ400*850	φ500*710	φ500*950	φ632*1000
Chamber Material	SUS304			
Max Working Pressure	0.23Mpa			
Vacuum Limit	-0.08MPa			
Working Temp.	115~138°C			
Temp Accuracy	±0.1°C			
Consumption	11KW	11.5KW		18KW
Power Supply	380V, 50Hz			
External Size(L*W*H) mm	1250*730*1660	1110*750*1742	1350*750*1742	1400*890*1780
Package Size(L*W*H) mm	1500*900*2050	1370*1000*2060	1510*890*2060	1700*1050*2090
Gross Weight(kg)	310	470	540	830

Horizontal Cylindrical Pressure Autoclave



Features:

- * Drying function.
- * Automatic sterilization process.
- * Safety valve for over pressure protection.
- * Over-temperature, over-pressure protection device.
- * Interlock function.
- * 304 stainless steel material chamber.
- * Automatically in case of low water level.
- * Water level sensor. The power will be cut-off .
- * Double door optional.

Technical Parameters:

Model	BKQ-H150	BKQ-H200	BKQ-H300	BKQ-H400	BKQ-H500
Capacity	150L	200L	280L	400L	500L
Chamber Size(mm)	φ440*1000	φ515*1000	φ600*1000	φ700*1100	φ700*1300
Working Pressure	0.22MPa				
Working Temp.	134°C				
Temperature Range	105~134°C				
Sterilization Time	0~60 min				
Drying Time	0~60 min				
Temp. Display Accuracy	≤±2°C				
Consumption	9KW		12KW	18KW	
Power Supply	220V/380V, 50/60Hz		380V, 50Hz		
External Size (W*D*H) mm	1400*600*1300	1400*670*1650	1400*770*1780	1430*880*1830	1800*900*1820
Package Size (W*D*H) mm	1550*750*1850	1560*820*1850	1680*920*2100	1600*1050*2100	1850*1050*2100
Gross Weight(kg)	320	350	465	530	580

Hot Air Sterilizer

Application:

Hot air sterilizer is used to sterilize small surgical instrument, glass, petri dishes etc.
This device is suitable for medical and veterinary clinics, hospitals, pharmacies, health care centers, and laboratories.



HAS-T25/HAS-T50/HAS-T105/HAS-T200

HAS-T70

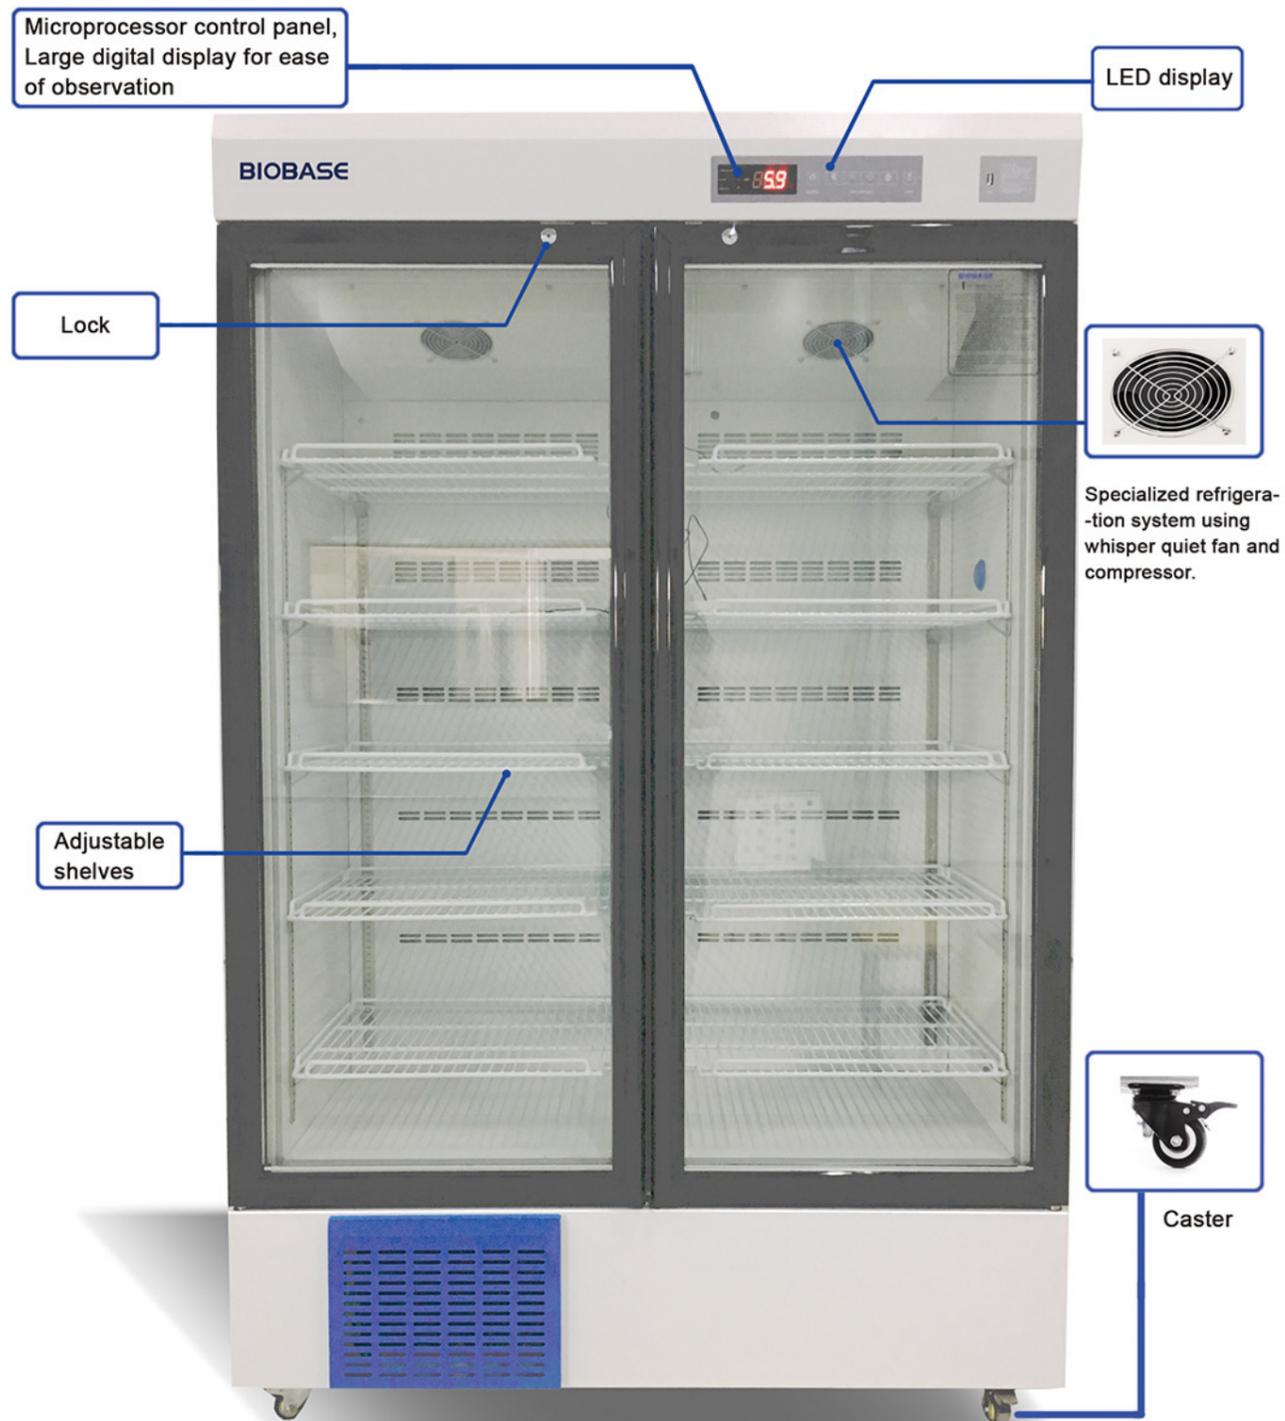
Features:

- * Adjustable sterilization time.
- * Top air outlet with adjustable air volume.
- * Over-temperature alarm.
- * Heating up fast, forced-air convection, fast sterilization.
- * Fan inside, fully sealed inside, no air circulation with external air, temperature rise fast.
- * High precision microprocessor temperature control; 304 stainless steel inner chamber.

Technical Parameters:

Model	HAS-T25	HAS-T50	HAS-T70	HAS-T105	HAS-T200
Capacity	25L	50L	70L	105L	200L
Temp. Range	RT+10~250°C				
Temp. Precision	0.1°C				
Temp. Fluctuation	±0.5°C				
Ambient Temp.	5~40°C				
Timing Range	1~9999min				
Shelves No.	2 pcs				
Consumption	500W	750W	1050W	1500W	2000W
Power Supply	AC110/220V±10%, 50/60Hz				
Internal Size(W*D*H) mm	300*300*270	420*350*350	400*375*470	550*350*520	600*550*570
External Size(W*D*H) mm	590*470*440	710*520*520	540*550*870	840*540*720	890*730*770
Package Size(W*D*H) mm	710*600*550	810*640*600	670*660*1040	950*680*880	1020*890*930
Gross Weight(kg)	45	50	75	80	100

Laboratory Refrigerator(2-8°C)



Laboratory Refrigerator



Technical Parameters

Model	BPR-5V160	BPR-5V250	BPR-5V310	BPR-5V588	BPR-5V1000
External Size(W*D*H) mm	500*550*1300	580*575*1810	620*575*1980	1220*630*1885	1220*860*1885
Capacity	160L	250L	310L	588L	1000L
Temp. Range	2°C~8°C				
Temp. Accuracy	0.1°C				
Control System	Microprocessor Control, Large Screen LED Display				
Alarm	Audible and visual alarm for: High and low temperature, Power failure alarm, Door ajar, Thermostat failure				
Refrigeration Type	Forced air refrigeration system				
Refrigerant	R600a, CFC Free			R134a, CFC Free	
Condenser & Evaporator	Bundy tube condenser				
Defrost	Manual defrost		Auto defrost		
Construction	Structure	Unibody Design & Mono-assembly foaming (Rigid polyurethane insulation material)			Unibody Design & Mono-assembly foaming (Polyurethane cyclopentane insulation material)
	Internal Material	Embossed aluminum sheet			Spraying steel plate
	External Material	Spraying steel plate			
Shelves	4 pc	4pc	5 pc	5 pc	
Door	Glass door with electric heating				
Consumption	136W	170W	180W	560W	
Power Supply	AC220V±10%, 50/60Hz(only for BPR-5V160) ,AC110/220V±10%, 50/60Hz				
Standard Accessories	LED Lamp,uSB port, probe access port(BPR-5V588 & BPR-5V1000)				
Optional Accessory	Temperature recorder, Temperature printer(USB port can not be selected at the same time), probe access port				
Package Size(W*D*H) mm	590*595*1380	670*650*1870	700*650*2030	1340*750*2100	1340*980*2100
Gross Weight	51kg	68kg	84kg	248kg	280kg

BIOBASE

ADD: BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China
TEL: +86-531-81219803 FAX: +86-531-81219804
E-MAIL: export@biobase.cn WEBSITE: www.biobase.cc / www.meihuatrade.com

DECLARATION OF CONFORMITY

Technical file of the company mentioned below has been inspected and audit has been completed successfully

Medical Devices Regulation 2017/745 (EU) has been taken as reference for these processes

Company Name: Biobase Disinfection (Shandong) Co., Ltd.
BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China

Examination Intent: Examination the completeness of the Technical Documentation according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU)

Harmonised Standards: EN 60601-1:2006; EN ISO 13485: 2016; EN ISO 15223-1: 2016

Product(s): Autoclave

Type(s)/Model(s): BKM-Z24B(III), BKM-Z45B(III), BKQ-Z100H

Classification: I (according to the classification rules of the MDR)

Examination Period: July 8, 2021

Date of Expiry: July 7, 2026

Review Result: We, Biobase Disinfection (Shandong) Co., Ltd, declare that during the self-testing and performance evaluation, no Non-compliance according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU) has been detected.

Year of DOC marking: 2021

Signed for and on behalf of

Company: Biobase Disinfection (Shandong) Co., Ltd

RA Specialist: 

Document No: MDR-Z21070807



BIOBASE

ADD: BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China
TEL: +86-531-81219803 FAX: +86-531-81219804
E-MAIL: export@biobase.cn WEBSITE: www.biobase.cc / www.meihuatrade.com

DECLARATION OF CONFORMITY

Technical file of the company mentioned below has been inspected and audit has been completed successfully

Medical Devices Regulation 2017/745 (EU) has been taken as reference for these processes

Company Name: **Biobase Biodustry(Shandong) Co., Ltd.**
BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China

Examination Intent: Examination the completeness of the Technical Documentation according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU)

Harmonised Standards: **EN 60601-1:2006; EN ISO 13485: 2016; EN ISO 15223-1: 2016**

Product(s): **Centrifuge**

Type(s)/Model(s): **BKC-TD6K, BKC-TL5VII, BKC-TD5K-II**

Classification: **I (according to the classification rules of the MDR)**

Examination Period: **July 8, 2021**


Date of Expiry: **July 7, 2026**

Review Result: We, Biobase Biodustry(Shandong) Co., Ltd., declare that during the self-testing and performance evaluation, no Non-compliance according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU) has been detected.

Year of DOC marking: **2021**

Signed for and on behalf of

Company: **Biobase Biodustry(Shandong) Co., Ltd.**

RA Specialist: 

Document No: **MDR-Z21070803**



BIOBASE

ADD: BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China
TEL: +86-531-81219803 FAX: +86-531-81219804
E-MAIL: export@biobase.cn WEBSITE: www.biobase.cc / www.meihuatrade.com

DECLARATION OF CONFORMITY

Technical file of the company mentioned below has been inspected and audit has been completed successfully

Medical Devices Regulation 2017/745 (EU) has been taken as reference for these processes

Company Name: Biobase Disinfection (Shandong) Co., Ltd.
BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China

Examination Intent: Examination the completeness of the Technical Documentation according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU)

Harmonised Standards: EN 60601-1:2006; EN ISO 13485: 2016; EN ISO 15223-1: 2016

Product(s): Hot Air Sterilizer

Type(s)/Model(s): HAS-T25, HAS-T50, HAS-T70, HAS-T105, HAS-T200

Classification: I (according to the classification rules of the MDR)

Examination Period: July 8, 2021

Date of Expiry: July 7, 2026

Review Result: We, Biobase Disinfection (Shandong) Co., Ltd, declare that during the self-testing and performance evaluation, no Non-compliance according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU) has been detected.

Year of DOC marking: 2021

Signed for and on behalf of

Company: Biobase Disinfection (Shandong) Co., Ltd

RA Specialist:  2020.8.14

Document No: MDR-Z21070808



BIOBASE

ADD: BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China
TEL: +86-531-81219803 FAX: +86-531-81219804
E-MAIL: export@biobase.cn WEBSITE: www.biobase.cc / www.mcihuatrade.com

DECLARATION OF CONFORMITY

Technical file of the company mentioned below has been inspected and audit has been completed successfully

Medical Devices Regulation 2017/745 (EU) has been taken as reference for these processes

Company Name: **Biobase Biodustry(Shandong) Co., Ltd.**
BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China

Examination Intent: Examination the completeness of the Technical Documentation according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU)

Harmonised Standards: **EN 60601-1:2006; EN ISO 13485: 2016; EN ISO 15223-1: 2016**

Product(s): **Incubator**

Type(s)/Model(s): **BJPX-H30, BJPX-H80**

Classification: **I (according to the classification rules of the MDR)**

Examination Period: **July 8, 2021**


Date of Expiry: **July 7, 2026**

Review Result: **We, Biobase Biodustry(Shandong) Co., Ltd., declare that during the self-testing and performance evaluation, no Non-compliance according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU) has been detected.**

Year of DOC marking: **2021**

Signed for and on behalf of

Company: **Biobase Biodustry(Shandong) Co., Ltd.**

RA Specialist: 

Document No: **MDR-Z21070805**



BIOBASE

ADD: BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China
TEL: +86-531-81219803 FAX: +86-531-81219804
E-MAIL: export@biobase.cn WEBSITE: www.biobase.cc / www.meihuatrade.com

DECLARATION OF CONFORMITY

Technical file of the company mentioned below has been inspected and audit has been completed successfully

Medical Devices Regulation 2017/745 (EU) has been taken as reference for these processes

Company Name: **Biobase Bioindustry(Shandong) Co., Ltd.**
BIOBASE Headquarters, No. 9 Gangxing Road, Pilot Free Trade Zone of Jinan, Shandong, China

Examination Intent: Examination the completeness of the Technical Documentation according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU)

Harmonised Standards: **EN 60601-1:2006; EN ISO 13485: 2016; EN ISO 15223-1: 2016**

Product(s): **Refrigerator**

Type(s)/Model(s): **BPR-5V160, BPR-5V250, BPR-5V588, BPR-5V650, BPR-5V50(G), BPR-5V100(G)**

Classification: **I (according to the classification rules of the MDR)**

Examination Period: **July 8, 2021**

Date of Expiry: **July 7, 2026**

Review Result: **We, Biobase Bioindustry(Shandong) Co., Ltd., declare that during the self-testing and performance evaluation, no Non-compliance according to the requirements of Annex II excluding section 4 (Module H) of 2017/745 (EU) has been detected.**

Year of DOC marking: **2021**

Signed for and on behalf of

Company: **Biobase Bioindustry(Shandong) Co., Ltd.**

RA Specialist: Zina Su

Document No: **MDR-Z21070802**



QUALITY MANAGEMENT SYSTEM CERTIFICATE

Certification No. : HXC18921Q20254R0M

Awarded to

Biobase Biodustry(Shandong)Co., Ltd.

Organization Code: 9137018179889855X7

Registration Add.: Mingshui Economic Development Zone,Zhangqiu District,Jinan City, Shandong Province
(Biobase Industrial Park in a intersection of East Jingshi Road and Mingbu Road)

Office Add.: Mingshui Economic Development Zone,Zhangqiu District,Jinan City, Shandong Province
(Biobase Industrial Park in a intersection of East Jingshi Road and Mingbu Road)

Production/Service Add.: No.51 Industrial South road,Jinan City, Mingshui Economic Development Zone,
Zhangqiu District,Jinan City(Biobase Industrial Park in a intersection of East Jingshi Road and Mingbu Road),
No.2 Qinghe street, Zhangqiu District, Jinan City,Standard Plant No. 3, Jinshui High-end Equipment
Manufacturing Industrial Park, Pingyin County, Jinan City, Shandong Province

Zip Code: 250200

**The Quality Management System of the above
organization has been assessed and Found to be in accordance with
the requirements of the standard:**

GB/T 19001-2016 / ISO 9001:2015

Scope of this management Certification

**R & D, production and sales of In Vitro Diagnostic Reagents, Biological Safety Cabinets,
Air Purifier, Blood Bank Refrigerator, Medical Incubator, Automatic ELISA Processor,
Hematology Analyzer Diluent, Hematology Analyzer Lyse, Microplate Washer,
Laboratory Refrigerator, Automatic chemistry analyzer, Automatic Chemiluminescence Analyzer,
Automatic Nucleic acid extration system, Disposable Virus Sampling Tube,
Medical centrifuge (within the scope of qualification license)**

First S.A.	Labelling	Second S.A.	Labelling	Third S.A.	Labelling
------------	-----------	-------------	-----------	------------	-----------

The certified organization must accept at least one surveillance audit annually and a qualified mark shall be attached onto the certificate, within validity period of the certificate, then the certificate can be maintained valid.

For more details of this certificate, please login CNCA' s website: www.cnca.gov.cn.

For the validity of the certificate, please scan the QR codes on the right side for accurate information.



Date of Issue:5 Jul. 2021 Date of Supervision:5 Jul. 2021 Valid until:4 Jul. 2024

Room 802, 2nd Building, No. 6 South Street of Gulou, Changping District, Beijing City, China 010-57146599

No. 0002277

MEDICAL DEVICES QUALITY MANAGEMENT SYSTEMS CERTIFICATE

Certification No. : HXC18921YL008R0M

Awarded to

Biobase Biodustry(Shandong)Co., Ltd.

Organization Code: 9137018179889855X7

Registration Add.: Mingshui Economic Development Zone,Zhangqiu District,Jinan City, Shandong Province
(Biobase Industrial Park in a intersection of East Jingshi Road and Mingbu Road)

Office Add.: Mingshui Economic Development Zone,Zhangqiu District,Jinan City, Shandong Province
(Biobase Industrial Park in a intersection of East Jingshi Road and Mingbu Road)

Production/Service Add.: No.51 Industrial South road,Jinan City, Mingshui Economic Development Zone,
Zhangqiu District,Jinan City(Biobase Industrial Park in a intersection of East Jingshi Road and Mingbu Road),
No.2 Qinghe street, Zhangqiu District, Jinan City,Standard Plant No. 3, Jinshui High-end Equipment
Manufacturing Industrial Park, Pingyin County, Jinan City, Shandong Province

Zip Code: 250200

**The Medical Devices Quality Management Systems of the above
Organization has been assessed and Found to be in accordance with
the requirements of the standard:**

ISO 13485:2016

Scope of this management Certification

**R & D, production and sales of In Vitro Diagnostic Reagents, Biological Safety Cabinets,
Air Purifier, Blood Bank Refrigerator, Medical Incubator, Automatic ELISA Processor,
Hematology Analyzer Diluent, Hematology Analyzer Lyse, Microplate Washer,
Laboratory Refrigerator, Automatic chemistry analyzer, Automatic Chemiluminescence Analyzer,
Automatic Nucleic acid extration system, Disposable Virus Sampling Tube,
Medical centrifuge (within the scope of qualification license)**

First S.A.	Labelling	Second S.A.	Labelling	Third S.A.	Labelling
------------	-----------	-------------	-----------	------------	-----------

The certified organization must accept at least one surveillance audit annually and a qualified mark shall be attached onto the certificate, within validity period of the certificate, then the certificate can be maintained valid.

For more details of this certificate, please login CNCA' s website: www.cnca.gov.cn.

For the validity of the certificate, please scan the QR codes on the right side for accurate information.



Date of Issue:5 Jul. 2021 Date of Supervision:5 Jul. 2021 Valid until:4 Jul. 2024

Room 802, 2nd Building, No. 6 South Street of Gulou, Changping District, Beijing City, China 010-57146599