



Benannt durch/Designated by  
Zentralstelle der Länder  
für Gesundheitsschutz  
bei Arzneimitteln und  
Medizinprodukten  
www.zlg.de  
ZLG-BS-245.10.07



Product Service

# EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)  
(List A and B and devices for self-testing)

**No. V1 104507 0003 Rev. 06**

**Manufacturer:**

**ACON Laboratories, Inc.**

5850 Oberlin Drive, #340  
San Diego CA 92121  
USA

**Product Category(ies): Blood glucose measuring systems for self testing  
and self-testing devices for clinical chemistry,  
hematology and pregnancy and ovulation**

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for design, manufacture and final inspection of the respective devices / device families in accordance with IVDD Annex IV. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of List A devices an additional Annex IV (4) certificate is mandatory. All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:V1\\_104507\\_0003\\_Rev.06](http://www.tuvsud.com/ps-cert?q=cert:V1_104507_0003_Rev.06)

**Report no.:** SH22743EXT01

**Valid from:** 2022-05-04

**Valid until:** 2025-05-26

**Date,** 2022-05-04

Christoph Dicks  
Head of Certification/Notified Body



# EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)  
(List A and B and devices for self-testing)

**No. V1 104507 0003 Rev. 06**

## Model(s):

On Call Plus Blood Glucose Monitoring System,  
On Call Plus Blood Glucose Test Strips,  
On Call EZ II Blood Glucose Monitoring System,  
On Call Advanced Blood Glucose Monitoring System,  
On Call Advanced Blood Glucose Test Strips,  
On Call Chosen Blood Glucose Test Strips,  
On Call Vivid Blood Glucose Monitoring System (OGM-101),  
On Call Vivid Blood Glucose Test Strips (OGS-101),  
On Call Sharp Blood Glucose Monitoring System (OGM-121),  
On Call Sharp Blood Glucose Test Strips (OGS-121)  
On Call Plus II Blood Glucose Monitoring System (OGM-171),  
On Call Plus II Blood Glucose Test Strips (OGS-171),  
On Call Extra Blood Glucose Monitoring System (OGM-191),  
On Call Extra Blood Glucose Test Strips (OGS-191),  
On Call GK Dual Blood Glucose & Ketone Monitoring System (OGM-161),  
On Call Blood Ketone Test Strips (OGS-161),  
Urinalysis Reagent Strips (Urine),  
UTI Urinary Tract Infection Test Strips,  
Cholesterol Monitoring System (CCM-111),  
CHOL Total Cholesterol Test Devices (CCS-111),  
TRIG Triglycerides Test Devices (CCS-112),  
HDL High Density Lipoprotein Test Devices (CCS-113),  
3-1 Lipid Panel Test Devices (CCS-114),  
Cholesterol CTRL Control Devices,  
Cholesterol Monitoring System (CCM-101),  
CHOL Total Cholesterol Test Strips (CCS-101),  
PT/INR Monitoring System (CCM-151),  
PT/INR Test Strips (CCS-151),  
Hemoglobin Testing System (CCM-141),  
Hemoglobin Test Strips (CCS-141),  
hCG Pregnancy Rapid Test Cassette (Urine),  
Pregnancy Rapid Test Midstream,  
On Call Extra Mobile Blood Glucose Monitoring System (OGM-281),  
On Call Sure Blood Glucose Monitoring System (OGM-211),  
On Call Sure Sync Blood Glucose Monitoring System (OGM-212),  
On Call Sure Blood Glucose Test Strips (OGS-211),  
GIMA Blood Glucose Monitoring System,  
GIMA Bluetooth Blood Glucose Monitoring System,  
GIMA Blood Glucose Test Strips,  
On Call GU Dual Blood Glucose & Uric Acid Monitoring



# EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)  
(List A and B and devices for self-testing)

**No. V1 104507 0003 Rev. 06**

System (OGM-201),  
On Call Blood Uric Acid Test Strips (OGS-201),  
LH Ovulation Rapid Test Cassette (Urine),  
Ovulation Rapid Test Midstream,  
Ovulation & Pregnancy Test Combo Pack,  
On Call Extra Voice Blood Glucose Monitoring System  
(OGM-291),  
Early Detection Pregnancy Test,  
Digital Pregnancy Test,  
Go-Keto Blood Glucose & Ketone Monitoring System (OGM-  
161),  
Go-Keto Blood Ketone Test Strips (OGS-161),  
Go-Keto Blood Glucose Test Strips,  
On Call Extra GM Blood Glucose Monitoring System(OGM-  
191),  
On Call Extra GM Blood Glucose Test Strips (OGS-191),  
On Call Plus GM Blood Glucose Monitoring System,  
On Call Plus GM Blood Glucose Test Strips,  
Go-Keto Urinalysis Reagent Strips

## Facility(ies):

ACON Laboratories, Inc.  
5850 Oberlin Drive, #340, San Diego CA 92121, USA

ACON Laboratories, Inc.  
10125 Mesa Rim Road, San Diego CA 92121, USA

AZURE Institute, Inc.  
10125 Mesa Rim Road, San Diego CA 92121, USA

Acon Laboratories Inc.  
Guerrero Negro 9942 Parque Industrial Pacifico IV, 22644 Tijuana  
B.C. CP, MEXICO



Product Service

# Certificate

No. Q5 104507 0001 Rev. 03

**Holder of Certificate:** **ACON Laboratories, Inc.**  
 5850 Oberlin Drive, #340  
 San Diego CA 92121  
 USA

**Certification Mark:**



**Scope of Certificate:** **Design and Development, Manufacture and distribution of In Vitro Diagnostic Test Kits and Reagents for the Determination of Infectious Diseases, Clinical Chemistry, Drugs of Abuse, Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose Monitoring System, Lancing Devices and Lancets**

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:Q5 104507 0001 Rev. 03](http://www.tuvsud.com/ps-cert?q=cert:Q5 104507 0001 Rev. 03)

**Report No.:** SH22743A01

**Valid from:** 2022-09-15  
**Valid until:** 2025-09-06

**Date,** 2022-09-15

Christoph Dicks  
 Head of Certification/Notified Body

# Certificate

No. Q5 104507 0001 Rev. 03

## Applied Standard(s):

EN ISO 13485:2016  
Medical devices - Quality management systems -  
Requirements for regulatory purposes  
(ISO 13485:2016)  
DIN EN ISO 13485:2016

## Facility(ies):

**ACON Laboratories, Inc.**  
**5850 Oberlin Drive, #340, San Diego CA 92121, USA**

Address holder for registration only

**ACON Laboratories, Inc.**  
**10125 Mesa Rim Road, San Diego CA 92121, USA**

Manufacture and distribution of  
In Vitro Diagnostic Test Kits and Reagents for the Determination of  
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,  
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose  
Monitoring System, Lancing Devices and Lancets

**ACON Laboratories, Inc.**  
**6865 Flanders Dr., Suite B, San Diego CA 92121, USA**

Storage of  
In Vitro Diagnostic Test Kits and Reagents for the Determination of  
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,  
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose  
Monitoring System, Lancing Devices and Lancets

**AZURE Institute, Inc.**  
**10125 Mesa Rim Road, San Diego CA 92121, USA**

Design and Development of  
In Vitro Diagnostic Test Kits and Reagents for the Determination of  
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,  
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose  
Monitoring System, Lancing Devices and Lancets

**Acon Laboratories Inc.**  
**Guerrero Negro 9942 Parque Industrial Pacifico IV, 22644**  
**Tijuana B.C. CP, MEXICO**

Manufacture of  
blood glucose test strips, antigen rapid test and IgG/IgM antibody  
rapid test for infectious disease.

# Mission® Urinalysis Reagent Strips and Urine Analyzers

Obtain reliable and cost-effective results with *Mission*® Urinalysis Reagent Strips and Urine Analyzers!

- *Accurate*
- *Reliable*
- *Convenient*



**ACON**®

Global Diagnostics for Local Markets™

# Urinalysis Reagent Strips

## Simple and Accurate



- Analytical sensitivity better than or comparable to market leaders
- High quality color chart ensures accurate visual reading

## Flexible

- Compatible for visual and analyzer reading
- More than 30 different combinations available

## Multiple Packaging Options and Long Shelf Life

- Canister Packaging
  - Available in 25, 50, 100 and 150 strips per kit
  - 2 year shelf life for unopened canisters which offers cost savings and convenience for high volume testing
  - 3 month shelf life for strips in opened canisters
- Pouch Packaging *New!*
  - Single-strip Pouch
    - Individually packaged strips with 1, 3, 6 and 20 strips and 1 color chart per kit for OTC or low volume testing
    - Unique packaging maintains 2 year shelf life for all strips in the kit compared to 3 months for remaining strips in an opened canister
  - Multi-strip Pouch
    - Canister Refill Kits with 25 strips/pouch uniquely packaged to save cost for low volume testing and extended shelf life by using the canister for refills

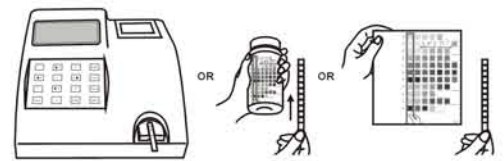

Step 1: Immerse strip into urine

Step 2: Remove excess urine

Step 3: Obtain results by analyzer or visual reading

Catalog No.	No. of Parameters	Type of Strip <sup>♦</sup>		Strips per Canister <sup>◇</sup>	Pouch Packaging <sup>▲</sup>	Reading Method			Analyzer-Read Strips: Standard (S) or Additional (A)	Parameters																
		For Visual Reading	For Analyzer Reading (U120/U500)			Visual	U120	U500		ASC	GLU	BIL	KET	SG	BLO	pH	PRO	URO	NIT	LEU	ALB	CRE				
U031-131	13	13C	NA	100*	✓	✓	NA	NA	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-111	11		11A	100	✓	✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-101	10		10U	100	✓	✓	✓	✓	S		*	*	*	*	*	*	*	*	*	*	*	*	*			
			10A			✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
			10C			✓	✓	✓	S		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
U031-091	9		9U	100	✓	✓	✓	✓	S		*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-081	8		8U	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
			8N			✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
			8S			✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
U031-071	7		7N	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-061	6	6N	6NE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
		6U	6UE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*		
U031-051	5	5B	5BE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
		5N	5NE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*			
		5S	5SE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		5U	5UE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
U031-041	4	4S	4SE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
		4B	4BE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		4K	4KE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		4G	4GE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		4N	4NE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
		4P	4PE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
U031-031	3	3P	3PE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
		3K	3KE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*			
		3G	3GE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		3N	3NE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
U031-021	2	2G	2GE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
		2K	2KE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		2N	2NE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		2B	2BE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		2U	2UE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		2S	2SE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		2C	2CE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
U031-011	1	1B	1BE	100	✓	✓	✓	✓	A		*	*	*	*	*	*	*	*	*	*	*	*	*			
		1P	1PE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*			
		1G	1GE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		1K	1KE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		1R	1RE			✓	✓	✓			*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	

♦Type of Strip:  
 Visual Strip Size  
 1-6 Parameters: 5 mm x 80 mm; 7-11 Parameters: 5 mm x 108 mm;  
 12-13 Parameters: 5 mm x 121 mm  
 U120/U500 Strip Size  
 1-11 Parameters: 5 mm x 108 mm;  
 "E" means extended strip length for 1-6 Parameters

◇ Also available in canisters of 25, 50 and 150 strips  
 \* Not available in canisters of 150 strips  
 ▲ Single-strip Pouch available in 1, 3, 6 and 20 strip kit  
 Canister Refill Kit, with 25 strips per pouch or canister, available in 3-pouch and 1- canister kit, or 4-pouch kit



# U120 Urine Analyzer



## Accurate

- Up to 120 tests/hour in Continuous Test Option
- Capable of reading 1 strip at a time in Single Test Option
- Test modes include Routine, STAT and QC
- Automatic calibration for accurate results and easy operation

## Reliable

- Can read up to 4 Strip combinations with 8, 9, 10, 11 parameters, additional strips with 1-11 parameters available upon request
- Minimal training required

## Convenient Operation

- Saves and recalls the last 2,000 results automatically
- Audible beep signals operator to dip strips in urine
- Can print up to 3 copies per test for convenient reviewing and easy record keeping
- Option to print results on sticker paper for quick and simple record management

## Easy Data Management

- Includes RS232C port for easy data transfer to an external computer or LIS
- Optional Barcode Reader to record patient ID

## Unique Lockout Functions *new!*

- Strip Lockout
  - Prevents using strips of another brand on the U120 Urine Analyzer
  - Requires barcode reader scan or manual entry of the canister code
- User Lockout
  - Eliminates unapproved users from testing
  - Up to 10 lab operators can perform testing, but only the lab administrator can change analyzer settings
- QC Lockout
  - Prevents testing without passing QC
  - QC tests can be performed once every 8 hours, day, week or month
  - Analyzer will alert when to run QC test
  - If QC tests fail, analyzer will switch to STAT mode and list "E" at the end of each test number

## Specifications

Feature	Specifications
Analyzer Type	Manual
Methodology	Reflectance Photometry
Detection	Photosensitive Diode
Throughput	Single Test Option: 60 tests/hour Continuous Test Option: 120 tests/hour
Test Modes	Routine, STAT and QC
Lockout Functions	Strip Lockout: Available Upon Request; User/QC Lockout: Included with option to turn ON/OFF
Memory	Last 2,000 results
Strip Incubation Time	1 Minute
Wavelength of Monochromatic LED	525 nm and 635 nm
Standard Strips	8, 9, 10, 11 Parameters (5 mm x 108 mm)
Additional Strips Available	1-11 Parameters (5 mm x 108 mm); see URS Parameters
Total Combinations Per Analyzer	4 Combinations
Analyzer Ports	Standard RS232C Port for Barcode Reader or Data Transfer USB Port for Data Transfer 25 Pin Parallel Port for External Printer
Capabilities	Internal Thermal Printer (included)      RS232C Barcode Reader (optional) Optional External Printer (not included)      USB or RS232C Data Transfer Cable (optional)
Major Readable Barcodes	Code 128, Code 39, Codabar (NW-7), Interleaved 25, UPC-A, UPC-E, EAN 8, EAN 13
Calibration	Automatic
Available Languages on the Screen	English and additional language(s)
Operating Conditions	0-40°C (32-104°F); ≤ 85% RH
Storage Conditions	-5-50°C (23-122°F); ≤ 90% RH
Power Source	100-240 VAC, 50-60 Hz
Dimensions (L x W x H)	27.2 cm x 26.9 cm x 14.6 cm (10.7" x 10.6" x 5.7")
Display Dimensions (L x W)	10.8 cm x 5.7 cm (4.2" x 2.2")
Weight	2.6 kg (5.7 lbs)

## Ordering Information

Product Name	Catalog No.	Components	Kit Box Dimensions (L x W x H) & Weight	Carton Dimensions (L x W x H) & Weight	Number of Kits/Carton
U120 Urine Analyzer	U111-101 <sup>†</sup>	1 Urine Analyzer 1 Strip holder 2 Printer Paper Rolls	2 Fuses (2.0A) 1 Power Cord 1 Quick Start Guide 1 Instruction Manual	42.0 cm x 41.5 cm x 31 cm; 5.0 kg 16.4" x 16.2" x 12.1"; 176.4 oz	1
U120 Urine Analyzer with Barcode Reader	U111-111 <sup>†</sup>	1 Urine Analyzer 1 Strip holder 2 Printer Paper Rolls 1 Barcode Reader (RS232C)	2 Fuses (2.0A) 1 Power Cord 1 Serial Splitter Cable (RS232C) 1 Quick Start Guide 1 Instruction Manual	44.5 cm x 44.5 cm x 40.0 cm; 5.5 kg 17.5" x 17.5" x 15.7"; 194 oz	1
Barcode Reader	U221-111 <sup>†</sup>	1 Barcode Reader (RS232C)	1 Serial Splitter Cable (RS232C)	23.6 cm x 10.8 cm x 7.8 cm; 0.482 kg 9.3" x 4.3" x 3.1"; 17.0 oz 63.0 cm x 37.0 cm x 30.0 cm; 12.0 kg 24.8" x 14.6" x 11.8"; 423.3 oz	22
Printer Paper Rolls	U121-101	4 Printer Paper Rolls	Thermal Paper (0.06 m x 20 m): 200 results/roll Sticker Paper (0.06 m x 9 m): 100 results/roll	12.0 cm x 12.0 cm x 6.5 cm; 0.36 kg 4.7" x 4.7" x 2.6"; 12.7 oz 63.0 cm x 37.0 cm x 30.0 cm; 21.4 kg 24.8" x 14.6" x 11.8"; 684.3 oz 12.0 cm x 12.0 cm x 6.5 cm; 0.4 kg 4.7" x 4.7" x 2.6"; 14.1 oz 24.8" x 14.6" x 11.8"; 684.3 oz; 754.9 oz	50
U120 Data Transfer Kit	U221-131 <sup>†</sup>	1 Data Transfer Cable (RS232C)	1 Package Insert	16.0 cm x 13.0 cm x 3.5 cm; 0.147 kg 6.3" x 5.1" x 1.4"; 5.2 oz 25.0 cm x 21.0 cm x 15.0 cm; 1.36 kg 9.8" x 8.3" x 5.9"; 48.0 oz	8

✓ CE Marked for sale in the European Community **CE**  
 † Cleared for US 510(k)



# U500 Urine Analyzer



## Accurate and Efficient

- Up to 500 tests/hour for medium/large volume sample testing
- Professional accuracy equivalent to market leader
- Automatic strip detection and alignment for better efficiency
- Test modes include Routine, STAT and QC

## Easy to Operate

- Large touch screen LCD offers simple menu navigation
- Uniquely designed strip platform/waste tray unit for easy one-step cleaning

## Convenient

- Automatic calibration and waste disposal reduce hands-on time
- Can read strips with 8, 9, 10, 11 parameters, additional strips with 1-11 parameters available upon request
- Strip selection of up to 4 combinations for analyzer reading
- Stores up to 2,000 records and automatically flags abnormal results
- Capable of printing results on sticker paper for quick and easy record management

## Data Management Capability

- Includes RS232C port for easy data transfer to an external computer or LIS
- Optional Barcode Reader to record patient ID

## Unique Lockout Functions Coming Soon!

- Strip Lockout
  - Prevents using strips of another brand on the U500 Urine Analyzer
  - Requires barcode reader scan or manual entry of the canister code
- User Lockout
  - Eliminates unapproved users from testing
  - Up to 10 lab operators can perform testing, but only the lab administrator can change analyzer settings
- QC Lockout
  - Prevents testing without passing QC
  - QC tests can be performed once every 8 hours, day, week or month
  - Analyzer will alert when to run QC test
  - If QC tests fail, analyzer will switch to STAT mode and list "E" at the end of each test number

## Specifications

Feature	Specifications
Analyzer Type	Semi-Automatic
Methodology	Reflectance Photometry
Detection	Photosensitive Diode
Throughput	500 tests/hour (Measuring cycle: 7 seconds/test)
Test Modes	Routine, STAT and QC
Lockout Functions	Strip Lockout: Available Upon Request; User/QC Lockout: Included with option to turn ON/OFF
Memory	Last 2,000 Records
Strip Incubation Time	1 Minute
Wavelength	525 and 635 nm
Standard Strips	8, 9, 10, 11 Parameters (5 mm x 108 mm)
Additional Strips Available	1-11 Parameters (5 mm x 108 mm); see URS Parameters
Total Combinations Per Analyzer	4 Combinations
Waste Disposal Capacity	Up to 150 Strips
Analyzer Ports	Standard RS232C Port for Barcode Reader or Data Transfer 25 Pin Parallel Port for External Printer
Capabilities	Internal Thermal Printer (included)      RS232C Barcode Reader (optional) Optional External Printer (not included)      RS232C Data Transfer Cable (optional)
Major Readable Barcodes	Code 128, Code 39, Codabar (NW-7), Interleaved 25, UPC-A, UPC-E, EAN 8, EAN 13
Calibration	Automatic
Available Languages on the Screen	English and additional language(s)
Operating Conditions	0-40°C (32-104°F); ≤85% RH
Storage Conditions	-5-50°C (23-122°F); ≤90% RH
Power Source	100-240 VAC, 50-60 Hz
Dimensions (L x W x H)	36.6 cm x 28.3 cm x 19.5cm (14.4" x 11.1" x 7.7")
Display Dimensions (L x W)	11.5 cm x 9.0 cm (4.5" x 3.5")
Weight	4.0 kg (8.8 lbs)

## Ordering Information

Product Name	Catalog No.	Components	Kit Box Dimensions (L x W x H) & Weight	Carton Dimensions (L x W x H) & Weight	Number of Kits/Carton
U500 Urine Analyzer	U211-101 <sup>✓</sup>	1 Urine Analyzer 1 Strip Platform/Waste Tray 2 Printer Paper Rolls	2 Fuses (2.0A) 1 Power Cord 1 Instruction Manual	51.0 cm x 42.0 cm x 38.5 cm; 7 kg 20.1" x 16.5" x 15.2"; 246.9 oz	1
U500 Urine Analyzer with Barcode Reader	U211-111 <sup>✓</sup>	1 Urine Analyzer 1 Strip Platform/Waste Tray 2 Printer Paper Rolls 1 Barcode Reader (RS232C)	2 Fuses (2.0A) 1 Power Cord 1 Serial Splitter Cable (RS232C) 1 Instruction Manual	55.0 cm x 55.0 cm x 55.0cm; 9.2 kg 21.7" x 21.7" x 21.7"; 324.5 oz	1
Barcode Reader	U221-111 <sup>✓†</sup>	1 Barcode Reader (RS232C)	1 Serial Splitter Cable (RS232C)	23.6 cm x 10.8 cm x 7.8 cm; 0.482 kg 9.3" x 4.3" x 3.1"; 17.0 oz	22
Printer Paper Rolls	U121-101	4 Printer Paper Rolls	Thermal Paper (0.06 m x 20 m): 200 results/roll Sticker Paper (0.06 m x 9 m): 100 results/roll	12.0 cm x 12.0 cm x 6.5 cm; 0.360 kg 4.7" x 4.7" x 2.6"; 12.7oz 63.0 cm x 37.0 cm x 30.0 cm; 19.4 kg 24.8" x 14.6" x 11.8"; 684.3 oz 12.0 cm x 12.0 cm x 6.5 cm; 0.40 kg 4.7" x 4.7" x 2.6"; 14.1oz 63.0 cm x 37.0 cm x 30.0 cm; 21.4 kg 24.8" x 14.6" x 11.8"; 684.3 oz; 754.9 oz	50
U500 Data Transfer Kit	U221-131 <sup>✓</sup>	1 Data Transfer Cable (RS232C)	1 Package Insert	16.0 cm x 13.0 cm x 3.5 cm; 0.147kg 6.3" x 5.1" x 1.4"; 5.2 oz	8

**We also offer other rapid diagnostic and medical products:**

Blood Glucose Monitoring Systems, Immunoassay EIA/ELISA and more.

✓ CE Marked for sale in the European Community **CE**

† Cleared for US 510(k)





**ACON Laboratories, Inc.**

10125 Mesa Rim Road. · San Diego, CA 92121 · USA  
Tel: (858) 875-8000 · Fax: (858) 875-8099 · E-mail: [info@aconlabs.com](mailto:info@aconlabs.com)

November 11<sup>th</sup> 2016

**CERTIFICATION LETTER**

This letter is to certify that, Vitalie Goreacii, employed by Sanmedico SRL located at: Republic of Moldova, city Chisinau, str. Petricani 88/1 of. 10, MD-2059, have received all required training and is enabled and authorized to provide services with installation, commissioning, and maintenance to the products listed below:

Mission® U120 Urine Analyzer  
Mission® U120 Ultra Urine Analyzer  
Mission® U500 Urine Analyzer  
Mission® PT/INR Coagulation Monitoring System  
Mission® Cholesterol Monitoring System  
Mission® Ultra Cholesterol Monitoring System  
Mission® HB Hemoglobin Testing System  
Mission® Plus HB Hemoglobin Testing System  
OnCall® Glucose Meter

For further questions or inquiries regarding this matter, please refer to the contact information below.

Sincerely

A handwritten signature in black ink, appearing to read "Jassy Alvarenga", is written over a red circular stamp.



Jassy Alvarenga  
International Account Manager  
ACON Laboratories, Inc. S.A.

[jalvarenga@aconlabs.com](mailto:jalvarenga@aconlabs.com)

+1 858 875 8085

## Declaration of Conformity

ACON Laboratories, Incorporated  
5850 Oberlin Drive #340  
San Diego, CA 92121, USA

**We, the manufacturer, declare under our sole responsibility that the  
*in vitro* diagnostic device:**


Mission ® U120 Smart Urine Analyzer (U117-101, U117-111)

**classified as Others in the directive 98/79/EC,  
meets all the provisions of the directive 98/79/EC on *in vitro* diagnostic  
medical devices which apply to it**

**The self-declaration is according to Annex III  
(excluding Section 6) of the Directive.**

Authorized Representative:  
Medical Device Safety Service GmbH  
Schiffgraben 41  
30175 Hannover, Germany

Signed this 11<sup>th</sup> day of December, 2019  
in San Diego, CA, USA

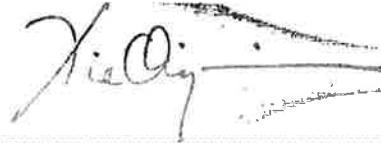

---

Qiyi Xie, MD, MPH  
Senior Staff, Regulatory Affairs & Clinical Affairs  
Acon Laboratories, Inc.



## Declaration of Conformity

ACON Laboratories, Incorporated  
5850 Oberlin Drive #340  
San Diego, CA 92121, USA

**We, the manufacturer, declare under our sole responsibility that the  
*in vitro* diagnostic device:**

*Mission*<sup>®</sup> Urinalysis Reagent Strips (U031-XX1)

**classified as Others in the directive 98/79/EC,**

**meets all the provisions of the directive 98/79/EC on *in vitro* diagnostic  
medical devices which apply to it**

**The self-declaration is according to Annex III  
(excluding Section 6) of the Directive.**

Authorized Representative:  
Medical Device Safety Service GmbH  
Schiffgraben 41  
30175 Hannover, Germany

Signed this 11 day of February, 2020  
in San Diego, CA USA



---

Qiyi Xie, MD, MPH  
Senior Staff, Regulatory Affairs & Clinical Affairs  
Acon Laboratories, Inc.





## STATEMENT

We, ACON Laboratories, Inc., having a registered office at *5850 Oberlin Drive #340, San Diego, CA 92121* authorize SRL Sanmedico having a registered office at *A. Corobceanu street 7A, apt. 9, Chisinău, MD-2012, Moldova*

to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

Date: January 3, 2023

Signature:

A handwritten signature in black ink, appearing to read "Xie", is written over a horizontal line.

Qiyi Xie, Md, MPH  
Sr. Officer, Regulatory & Clinical Affairs  
ACON Laboratories, Inc.  
Ph: 858-875-8011  
Email: [qxie@aconlabs.com](mailto:qxie@aconlabs.com)



## High Accuracy and Reliability

- Automatic calibration before each test
- Up to 120 tests per hour in Continuous Mode
- Reads strips with up to 14 parameters, including
  - Microalbumin/Creatinine/Calcium
- Minimal training required
- Robust construction
- Print up to 3 copies per test for record keeping
- Data Management ready
- Includes RS232C and USB ports for data transfer to an external computer or LIS



Internal Thermal Printer



Large Display Screen



Robust Keyboard

## Strip Combinations for U120 Smart

Catalog Number	Number of Parameters	Type of Strip U120 Smart	Parameter Order (First parameter is closest to strip handle)	Parameter													
				ASC	GLU	BIL	KET	SG	BLO	PH	PRO	URO	NIT	LEU	ALB	CRE	Ca
U031-111	11	11A	Asc/Glu/Bil/Ket/SG/Blo/pH/Pro/Uro/Nit/Leu	*	*	*	*	*	*	*	*	*	*	*			
U031-101	10	10U 10SG	Glu/Bil/Ket/SG/Blo/pH/Pro/Uro/Nit/Leu		*	*	*	*	*	*	*	*	*	*			
U031-091	9	9U	Glu/Bil/Ket/SG/Blo/pH/Pro/Uro/Nit		*	*	*	*	*	*	*	*	*				
U031-081	8	8U	Glu/Bil/Ket/Blo/pH/Pro/Uro/Nit		*	*	*		*	*	*	*					
		8N	Glu/Ket/SG/Blo/pH/Pro/Nit/Leu1		*		*	*	*	*		*	*				
U031-071	7	7N/7OB	Glu/Ket/Pro/pH/Blo/Nit/Leu		*		*		*	*	*		*	*			
U031-061	6	6NE/6OB	Glu/Pro/pH/Blo/Nit/Leu		*				*	*	*		*	*			
U031-051	5	5HE	Blo/pH/Pro/Ket/Glu		*		*		*	*	*						
		5NE/5OB	Glu/Pro/Nit/Blo/Leu		*				*		*		*	*			
U031-041	4	4PE/4NL	Glu/Pro/Nit/Leu		*					*	*		*	*			
		4SE	Glu/SG/pH/Pro		*			*		*	*						
U031-031	3	3PE	Glu/pH/Pro		*					*	*						
		3KE	Glu/Ket/Pro		*		*				*						
U031-021	2	2GE/2GP	Glu/Pro		*						*						
		2CE	ALB/CRE												*	*	

# Specifications

Features	Specifications
<b>Analyzer Type</b>	Semi-automatic
<b>Methodology</b>	Reflectance Photometry
<b>Detection</b>	Photosensitive Diode
<b>Calibration</b>	Automatic
<b>Throughput</b>	Single Test Option: 60 tests/hour , Continuous Test Option: 120 tests/hour
<b>Memory</b>	Last 2,000 results
<b>Strip Incubation Time</b>	1 Minute
<b>Wavelength of Monochromatic LED</b>	525 nm and 635 nm
<b>Strips Available</b>	2-14 parameters (108 mm x 5 mm)
<b>Strip Combinations Per Analyzer</b>	17 Combinations
<b>Analyzer Ports</b>	RS232C Port for Barcode Reader or Data Transfer , USB Port for Data Transfer , 25 Pin Parallel Port for External Printer
<b>Data Entry Capabilities</b>	Operator/Patient ID - Manual Entry and Barcode Reader (Up to 20 characters)
<b>Connection Capabilities</b>	USB or RS232C Data Transfer Cable (optional) , RS232C Barcode Reader (optional) , Optional External Printer (not included)
<b>Available Languages on the Screen</b>	English, French, Italian , Portuguese, Spanish
<b>Operating Conditions</b>	0-40°C (32 - 104°F); <85% RH
<b>Storage Conditions</b>	- 5 - 50°C (23-122°F); <90% RH
<b>Power Source</b>	100 - 240 Volts AC, 50-60 Hz
<b>Dimensions (L x W x H)</b>	27.2 cm x 18 cm x 10.5 cm (10.7" x 7" x 4.1")
<b>Display Dimensions (W x H)</b>	11 cm x 6.5 cm (4.3" x 2.6")
<b>Weight</b>	1.9 kg (4.2 lbs.) without batteries or power supply

CE Marked for sale in the European Community and 510(k) Cleared

## Ordering Information

Product Name	Catalog Number	Components	Carton Dimensions (L x W x H) & Weight	Number of Kits/Carton
<b>U120 Urine Analyzer</b>	U117-101	1 Urine Analyzer 1 Strip Holder 2 Printer Paper Rolls 1 Quick Start Guide	2 Fuses (2.0A) 1 Power Cord 1 Instruction Manual	1
<b>Printer Paper Rolls</b>	U121-101	4 Printer Paper Rolls	<b>Thermal Paper</b> (0.06 m x 20 m): 200 results/roll	50
			<b>Sticker Paper</b> (0.06 m x 9 m): 100 results/roll	



aconlabs.co

ACON Laboratories, Inc.  
10125 Mesa Rim Road, San Diego, CA 92121,  
U.S.A.  
**Tel:** 1.858.875.8000

**GMED certifie que le système de management de la qualité développé par**  
*GMED certifies that the quality management system developed by*

**ATLAS MEDICAL GmbH**  
**Ludwig-Erhard-Ring 3**  
**15827 Blankenfelde-Mahlow GERMANY**

**pour les activités**  
*for the activities*

**Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic in vitro .**

*Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices.*

**réalisées sur le(s) site(s) de**  
*performed on the location(s) of*

**Voir addendum**  
*See addendum*

**est conforme aux exigences des normes internationales**  
*complies with the requirements of the international standards*

**ISO 13485: 2016**

**Début de validité / Effective date October 9th, 2020 (included)**  
**Valable jusqu'au / Expiry date : October 8th, 2023 (included)**  
**Etabli le / Issued on : October 8th, 2020**




Accréditation n°4-0608  
Liste des sites accrédités  
et portée disponible sur  
[www.cofrac.fr](http://www.cofrac.fr)

GMED N° 36655-1

Ce certificat est délivré selon les règles de certification GMED / This certificate is issued according to the rules of GMED certification

Renouvelle le certificat 36655-0



**On behalf of the President**  
**Béatrice LYS**  
**Technical Director**



**Ce certificat couvre les activités et les sites suivants :**  
*This certificate covers the following activities and sites:*

**French version :**

**Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic *in vitro* à usage professionnel et/ ou d'autodiagnostic, dans les domaines du groupage sanguin, de la microbiologie, de la biochimie, de la toxicologie, de l'oncologie, de la cardiologie, de l'histologie, de l'endocrinologie et des maladies infectieuses, dans les techniques d'Agglutination/ ELISA/ Tests rapides/ Colorimétrie/ Disques antibiotiques.**

**English version:**

***Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices for professional use and/or for self-testing, in the field of Immunohematology, Microbiology, Biochemistry, Toxicology, Oncology, Cardiology, Histology, Endocrinology Biosensors and Infectious diseases, in techniques of Agglutination/ ELISA/ Rapid tests/ Colorimetry/Antibiotic disks.***

**ATLAS MEDICAL GmbH  
Ludwig-Erhard-Ring 3  
15827 Blankenfelde-Mahlow  
GERMANY**

French version:

**Siège social, responsable de la mise sur le marché**

*English version:*

*Headquarter, legal manufacturer*

\*\*\*\*\*

**Sahab Industrial Zone Area  
King Abdullah II Industrial City  
Amman 11512  
JORDAN**

French version:

**Conception, fabrication et contrôle final**

*English version:*

*Design, manufacture and final control*

\*\*\*\*\*

**William James House  
Cowley Road,  
Cambridge, CB OWX  
United Kingdom**

French version:

**Contact réglementaire**

*English version:*

*Regulatory Administration*

\*\*\*\*\*

**3 sites / 3 sites**

DocuSigned by:

*Beatrice Lys*  
EF33BDA9BAA04A3...  


**On behalf of the President  
Béatrice LYS  
Technical Director**

Date: 05/Jan/2023

## STATEMENT


We, Atlas Medical having a registered office at Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow, Berlin, Germany assign SRL Sanmedico having a registered office at A. Corobceanu Street 7A, apt.9, Chisinau MD-2012, Moldova, as authorized representative in correspondence with the conditions of directive 98/79/EEC.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

On Behalf of Manufacturer:

General Manager

Haya Amawi

Signature: 

Date: 05.01.2023

**Atlas Medical GmbH**  
Ludwig - Erhard Ring 3  
15827 Blankenfelde - Mahlow  
Tel. (0049) 33708 - 355030

**Atlas Medical:** Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow, Berlin, Germany,  
Tel:+4933708355030

**Regulatory Office:** William James House, Cowley Rd, Cambridge, CB4 0WX, United Kingdom  
Tel: +44 (0) 1223 858 910

**Middle East Site:** P.O Box 204, King Abdullah II Industrial Estate, Amman, 11512, Jordan  
Tel: +962 6 4026468

Declaration Ref No: DC22-0065

## CE Declaration of Conformity

According to Annex III of the IVD Directive 98/79/EC

We,

### Atlas Medical GmbH

Head office: Ludwig-Erhard-Ring 3  
Blankenfelde-Mahlow, Germany.

Tel: +49 - 33708 – 3550 30

Email: [info@atlas-medical.com](mailto:info@atlas-medical.com)

Manufacturing Site: Sahab Free Zone Area, P. O. Box 204, Amman 11512, Jordan.

Tel.: +962 6 4026468

Fax: +962 6 4022588

Email: [info@atlas-medical.com](mailto:info@atlas-medical.com)

Declare our responsibility that the following product:

### See Attached list


- Comply with all essential requirements (Annex I) of the IVD Directive 98/79/EC. This compliance has been properly documented and covers the items listed in Annex I of the IVD Directive.
- This product is produced under Atlas quality system (ISO13485:2016) issued by GMED:  
**Certificate N<sup>o</sup>.**: 36655 rev 1  
**Expiry Date:** October 8<sup>th</sup>.2023
- Comply with the essential requirements of following standards (EN 18113-1, -2,-4:2011, EN ISO 15223:2016 , EN ISO 23640:2015, EN ISO 14971:2019, ISO 2859/1:1999, EN ISO 13612:2002, EN ISO 13641:2002.

And

Intended for In-Vitro Professional use only.

**Manufacturer**  
**Atlas Medical**  
**Ludwig-Erhard-Ring 3**  
**Blankenfelde-Mahlow , Germany.**

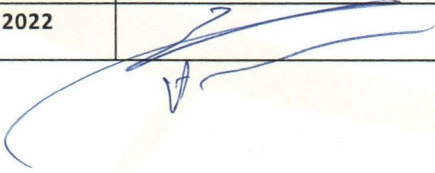

Atlas Medical	Issue date	Date of review	Management approval	MRXDO10F.10 08.02.2011
	May.2022	21.05.2022		

# CE Declaration of Conformity

According to Annex III of the IVD Directive 98/79/EC

Item code	Product Description
8.00.01.0.0100	Atlas CRP Latex Kit with Buffer (100 Tests)
8.00.05.0.0100	Atlas RF Latex kit with Buffer(100 Tests)
8.00.11.0.0050	Atlas SLE Latex kit (50 Tests)
8.00.11.0.0100	Atlas SLE Latex kit (100 Tests)
8.00.12.0.0100	Atlas Staphylococcus Latex Kit (100 Tests)
8.00.17.0.0050	Atlas D-Dimer Latex Kit (50 Tests)
8.00.19.3.0100	Atlas TPHA Kit (100 Tests)
8.00.19.3.0200	Atlas TPHA Kit (200 Tests)
8.00.20.3.2500	Atlas VDRL Kit, 5ml+55ml buffer
8.04.38.0.0020	Atlas Fecal Occult Blood Test (FOB) Test Cassette , 20 Tests/Box
8.04.85.0.0050	Atlas Fecal Occult Blood Test (FOB) Test Strip, 50 Tests/Box
8.04.109.0.0020	Atlas Procalcitonin test (PCT) , 20 Tests/Box
8.16.78.0.0025	Atlas Calprotectin Test Cassette , 25 Tests/Box
8.04.45.0.0001	Atlas Troponin I Test Cassette, Bulk
8.04.45.0.0020	Atlas Troponin I Test Cassette , 20 Tests/Box.
8.04.45.0.0030	Atlas Troponin I Test Cassette , 30 Tests/Box.
8.04.46.0.0001	Atlas Myoglobin Test Cassette, Bulk
8.04.46.0.0020	Atlas Myoglobin Test Cassette , 20 Tests/Box.
8.04.46.0.0030	Atlas Myoglobin Test Cassette , 30 Tests/Box.
8.04.47.0.0001	Atlas CK-MB Test Cassette , Bulk.
8.04.47.0.0020	Atlas CK-MB Test Cassette , 20 Tests/Box.
8.04.47.0.0030	Atlas CK-MB Test Cassette , 30 Tests/Box.
8.04.48.0.0001	Atlas Cardiac Triple Tests Cassette (Troponin I, CK-MB, Myoglobin), Bulk.
8.04.48.0.0020	Atlas Cardiac Triple Tests Cassette (Troponin I, CK-MB, Myoglobin), 20 Tests/Box.
8.04.48.0.0030	Atlas Cardiac Triple Tests Cassette (Troponin I, CK-MB, Myoglobin), 30 Tests/Box.
8.14.19.1.0096	Helicobacter pylori Antigen ELISA, 96 Tests.
8.51.00.0.0096	25-OH VITAMIN D Elisa Kit, 96 Tests.
8.57.00.0.0096	Vitamin B12 Elisa Kit, 96 Tests




## CE Declaration of Conformity

We,  
**Atlas Medical GmbH**  
 Head office: Ludwig-Erhard-Ring 3  
 15827 Blankenfelde-Mahlow Germany  
 Tel: +49(0)33708355030  
 Email: [info@atlas-medical.com](mailto:info@atlas-medical.com)

Middle East Site: Sahab Industrial Zone Area, King Abdullah II Industrial City  
 Amman 11512, Jordan  
 Tel.: +962 6 4026468  
 Fax: +962 6 4022588  
 Email: [info@atlas-medical.com](mailto:info@atlas-medical.com)

Declare our responsibility that the following product:

Product Code	Product Name	Class	GMDN code
8.00.18.0.0005	RPR Carbon Antigen Reagent, 5 ml/vial	General-IVD	32450
8.00.18.2.1000	RPR Carbon Antigen 1000ml/bottle	General-IVD	32450
8.00.18.0.0050	RPR Carbon Antigen Kit, 50 Tests	General-IVD	32450
8.00.18.1.0050	RPR Carbon Antigen Kit, 50 Tests, White Glass Slide.	General-IVD	32450
8.00.18.2.0500	RPR Carbon Antigen Kit, 500 Tests (2ml latex, 2x0.5 ml control) Without card.	General-IVD	32450
8.00.18.3.0500	RPR Carbon Antigen Kit, 500 Tests (10ml latex, 2x0.5 ml control) Without card, stirring sticks.	General-IVD	32450
8.00.18.0.0100	RPR Carbon Antigen Kit, 100 Tests (2ml latex, 2x0.5 ml control)	General-IVD	32450
8.00.18.2.0100	RPR Carbon Antigen Kit, 100 Tests (2ml latex, 2x0.5 ml control +White Glass slide stirring sticks)	General-IVD	32450
8.00.18.0.0025	RPR Carbon Antigen Kit, 25 Tests (0.5ml latex, 2x0.5 ml control)	General-IVD	32450
8.00.18.0.0150	RPR Carbon Antigen Kit, 150 Tests	General-IVD	32450
8.00.18.0.0200	RPR Carbon Antigen Kit, 200 Tests	General-IVD	32450
8.00.18.0.0250	RPR Carbon Antigen Kit, 250 Tests	General-IVD	32450

<b>Atlas Medical</b>	First issue date	Date of review	Management approval Products	MRXDO10F.10 08.02.2011
	September.2021	06.09.2021		

*Amin Al-Habashah*  
*RA Manager*

Declaration Ref No: DC21-0193

8.00.18.0.0500	RPR Carbon Antigen Kit,500 Tests	General-IVD	32450
8.00.18.0.1000	RPR Carbon Antigen Kit, 1000 Tests	General-IVD	32450
8.00.18.4.0500	RPR Carbon Antigen Kit,500 Tests (3x3.4ml reagent,2x1 controls)	General-IVD	32450
8.00.18.5.0500	RPR Carbon Antigen Kit, 500 Tests, (3x3.4ml reagent,2x1 controls)	General-IVD	32450
8.00.18.8.0500	RPR Carbon Antigen 500 Test (10ml reagent) without Control's.	General-IVD	32450
8.00.18.9.0050	RPR Carbon Antigen Kit, (5x10ml Reagent,2x2ml Control) , white glass Slide, Stirring Stick.	General-IVD	32450
8.33.04.0.0001	RPR Positive control	General-IVD	32450
8.33.04.1.0001	RPR Positive control ,Bulk	General-IVD	32450
8.33.04.0.0100	RPR Positive control(100ml/vial)	General-IVD	32450
8.33.04.0.0500	RPR Positive control(500ml/bottle)	General-IVD	32450
8.33.08.0.0001	RPR Negative control	General-IVD	32450

Is produced under Atlas quality system (ISO13485: 2016) supported by GMED certificate:

**Certificate N<sup>o</sup>.: 36655 rev 1**

**Expiry Date: October 8<sup>th</sup>.2023**

and complies with the essential requirements of  
In Vitro Diagnostic Medical Devices Directive 98/79/EC Annex I  
And

**EN ISO 18113-1, -2 :2011, EN ISO 15223:2016**

**EN ISO 14971:2019, EN ISO 23640 :2015 , ISO 2859 :2017,**

**EN 13612:2002, EN 13641:2002 , EN 13975:2003, ISO 13485:2016**

And

Intended for In-Vitro Professional use only.

This Declaration includes the batches produced beyond this day according to the product Lot Log.


#### Manufacturer

**Atlas Medical GmbH**

**Ludwig-Erhard-Ring 3**

**15827 Blankenefelde-Mahlow Germany.**



Atlas Medical	First issue date	Date of review	Management approval	MRXDO10F.10 08.02.2011
	September.2021	06.09.2021		

Anwar Al-Hadad  
RA Manager

# H. pylori Ag Rapid Test Cassette (Feces)



## INTENDED USE

H. pylori Ag Rapid Test Cassette (Feces) is a sandwich lateral flow chromatographic immunoassay for the qualitative detection of H. Pylori antigen in feces. It is for professional *in vitro* diagnostic use only.

## INTRODUCTION

H. Pylori is associated with a variety of gastrointestinal diseases included non-ulcer dyspepsia, duodenal and gastric ulcer and active, chronic gastritis.<sup>1,2</sup> The prevalence of H. pylori infection could exceed 90% in patients with signs and symptoms of gastrointestinal diseases. Recent studies indicate an association of H. Pylori infection with stomach cancer.<sup>3</sup> H. Pylori colonizing in the gastrointestinal system elicits specific antibody responses<sup>4,5,6</sup> which aids in the diagnosis of H. Pylori infection and in monitoring the prognosis of the treatment of H. Pylori related diseases. Antibiotics in combination with bismuth compounds have been shown to be effective in treating active H. Pylori infection. Successful eradication of H. pylori is associated with clinical improvement in patients with gastrointestinal diseases providing a further evidence.<sup>7</sup>

## PRINCIPLE

H. pylori Ag Rapid Test Cassette (Feces) is a lateral flow chromatographic immunoassay based on the principle of the double antibody–sandwich technique. The test cassette consists of: 1) a burgundy colored conjugate pad containing H. Pylori antibodies conjugated with color particles (H. Pylori conjugates). 2) a nitrocellulose membrane strip containing a test band (T band) and a control band (C band). The T band is pre-coated with non-conjugated H. Pylori antibodies.

When an adequate volume of test specimen is dispensed into the sample well of the cassette, the specimen migrates by capillary action across the cassette. The antigen of H. Pylori if present in the specimen will bind to the H. Pylori antibodies conjugates. The immunocomplex is then captured on the membrane by the pre-coated H. Pylori antibodies, forming a burgundy colored T band, indicating a H. Pylori antigen positive test result. To serve as a procedural control, a colored line will always appear in the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred. Otherwise, the test result is invalid and the specimen must be retested with another device.

## PRODUCT CONTENTS

H. pylori Ag Rapid Test Cassette (Feces) containing anti- H. pylori antibodies particles and anti-H. pylori antibodies coated on the membrane.

## MATERIALS SUPPLIED

- 20 Sealed pouches each containing a test cassette and a desiccant
- 20 Specimen collection tubes with extraction buffer, 2.0 mL
- 1 Package insert

## MATERIAL REQUIRED BUT NOT PROVIDED

1. Clock or timer
2. Specimen collection containers.

## STORAGE AND STABILITY

All reagents are ready to use as supplied. Store unused test device unopened at 2°C-30°C. If stored at 2°C-8°C, ensure that the test device is brought to room temperature before opening. The test is not stable out off the expiration date printed on the sealed pouch. Do not freeze the kit or expose the kit over 30°C.

## WARNINGS AND PRECAUTIONS

1. For professional *in vitro* diagnostic use only.
2. Do not use it if the tube/pouch is damaged or broken.
3. Test is for single use only. Do not re- use under any circumstances.
4. Handle all specimens as if they contain infectious agents. Observe established standard procedure for proper disposal of specimens
5. Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assay.
6. Humidity and temperature can adversely affect results

## SPECIMEN COLLECTION

Collect sufficient quantity of feces (1-2 mL or 1-2 g) in a clean, dry specimen collection container to obtain maximum antigens (if present). Best results will be obtained if the assay is performed within 6 hours after collection. Specimen collected may be stored for 3 days at 2-8°C if not tested within 6 hours. For long term storage, specimens should be kept below -20°C.


To process fecal specimens:

• For Solid Specimens:

Unscrew the cap of the specimen collection tube, then randomly stab the specimen collection applicator into the fecal specimen in at least 3 different sites to collect approximately 50 mg of feces (equivalent to 1/4 of a pea). Do not scoop the fecal specimen.

• For Liquid Specimens:


Hold the dropper vertically, aspirate fecal specimens, and then transfer 2 drops (approximately 80 µL) into the specimen collection tube containing the dilution buffer. Screw on and tighten the cap onto the specimen collection tube, then shake the specimen collection tube vigorously to mix the specimen and the dilution buffer. Leave the tube alone for 2 minutes.

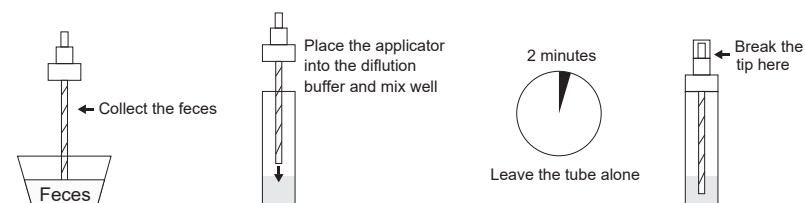

## TEST PROCEDURE

1. Remove the test device from its foil pouch by tearing along the notch and use it as soon as possible.
2. Specimen collection. See also specimen collection.
3. Holding the sample collection device upright, carefully break off the tip of collection device.
4. Squeeze 2 drops (~80 µL) of the sample solution in the sample well of the cassette, as in the illustration.
5. Read the test results in 10 minutes. It is important that the background is clear before the result is read. Do not read results after 10 minutes. To avoid confusion, discard the test device after interpreting the result.

## INTERPRETATION OF RESULTS

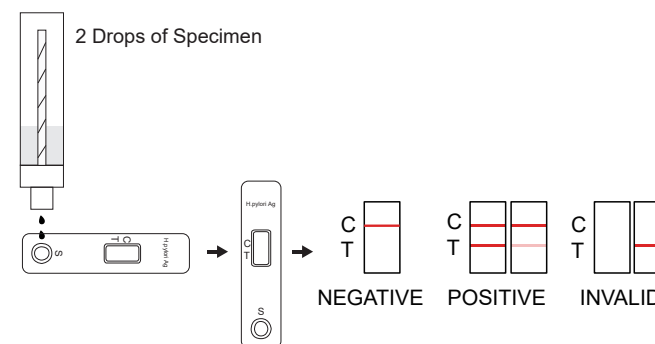

# H. pylori Ag Rapid Test Cassette (Feces)

Positive: Two lines appear. One colored line should be in the control line region (C) and another apparent colored line should be in the test line region (T).

Negative: One colored line appears in the control line region(C). No line appears in the test line region (T).

Invalid: Control line fails to appear.

## QUALITY CONTROL

A procedural control is included in the test. A colored line appearing in the control line region (C) is an internal procedural control. It confirms sufficient specimen volume, adequate membrane wicking and correct procedural technique.

Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

## LIMITATIONS

1. The Assay Procedure and the Assay Result Interpretation must be followed closely when testing the presence of H. Pylori antigen in feces from individual subjects. Failure to follow the procedure may give inaccurate results.

2. H. pylori Ag Rapid Test Cassette (Feces) is limited to the qualitative detection of H. Pylori antigen in feces. The intensity of the test band does not have linear correlation with the antigen titer in the specimen.

3. A negative result for an individual subject indicates absence of detectable H. Pylori antigen. However, a negative test result does not preclude the possibility of exposure to or infection with H. Pylori.

4. A negative result can occur if the quantity of the H. Pylori antigen present in the specimen is below the detection limits of the assay, or the antigen that are detected are not present during the stage of disease in which a sample is collected.

5. The results obtained with this test should only be interpreted in conjunction with other diagnostic procedures and clinical findings.

## PERFORMANCE CHARACTERISTICS

A study was performed with 165 patient feces samples including both symptomatic gastrointestinal disorders and samples from non-symptomatic patients and 100 normal feces samples. Comparison for all subjects with H. pylori Ag Rapid Test Cassette (Feces) and reference ELISA kit is showed in the following table:

Method		EIA		Total Results
H.P Test Cassette	Results	Positive	Negative	
	Positive	163	0	163
	Negative	2	100	102
Total Results		165	100	265

Relative sensitivity: 98.8%

Relative specificity: 100%

Accuracy:98.9%

## REFERENCE

1. Marshall,B.J.et.al. Pyloric Campylobacter infection and gastroduodenal disease. Med. J. Australia.149:439-44, 1985.

2. Marshall,B.J.et.al. Prospective double-blind trial of duodenal ulcer relapse after eradication of Campylobacter pylori. Lancet. Dec.1437-42,1988.

3. Megraud,F.et.al. Seroepidemiology of Campylobacter pylori infection in virious populations J.Clin.Microbiology. 27:1870-3,1989.










4. Soll,A.H. Pathogenesis of peptic ulcer and implications for therapy. New England J. Med.322:909-916,1990.

5. Parsonnet,J.et.al. Helicobacter pylori infection and the risk of gastric carcinoma. New England J.Med. 325:1127-31,1991.

6. Ansong,R. et.al. Evaluation of techniques for isolation, subcultivation and preservation of Helicobacter pylori. J.Clin.Micro. 29:51-53,1991.


7. Pronovost,A.P.et.al. Evaluation of a new immunodiagnostic assay for Helicobacter pylori antibody detection: Correlation with histopathological and microbiological results. J.Clin.Microbiol.32:46-50,1994.

## INDEX OF SYMBOLS

	Consult instructions for use		Tests per kit		Authorized Representative
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2~30°C		Lot Number		Catalog#



Zhejiang Orient Gene Biotech Co.,Ltd  
Address: 3787#, East Yangguang Avenue, Dipu Street,  
Anji 313300, Huzhou, Zhejiang, China.  
TEL: +86-572-5226111 FAX: +86-572-5226222  
Website: www.orientgene.com

 Shanghai International Holding Corp. GmbH (Europe)  
Add: Eiffestrasse 80, 20537 Hamburg, Germany

 GCHP-602a

Revision Date: 2022-03-08  
B20435-03





浙江东方基因生物制品股份有限公司  
Zhejiang Orient Gene Biotech Co., LTD



CE-DOC-OG039  
Version 1.0

# EC Declaration of Conformity

In accordance with Directive 98/79/EC

**Legal Manufacturer:** *Zhejiang Orient Gene Biotech Co., Ltd*

**Legal Manufacturer Address:** *3787#, East Yangguang Avenue, Dipu Street,  
Anji 313300, Huzhou, Zhejiang, China*

Declares, that the products  
Product Name and Model(s)

H. pylori Ag Rapid Test Strip (Feces)	GCHP-601a
H. pylori Ag Rapid Test Cassette (Feces)	GCHP-602a

**Classification:** *Other*  
**Conformity assessment route:** *Annex III (EC DECLARATION OF CONFORMITY)*

We, the Manufacturer, herewith declare with sole responsibility that our product/s mentioned above meet/s the provisions of the Directive 98/79/EC of the European Parliament and of the Council on In-Vitro Diagnostic Medical Devices.

We hereby explicitly appoint

**EC Representative's Name:** Shanghai International Holding Corp. GmbH (Europe)

**EC Representative's Address:** Eiffestrasse 80, 20537 Hamburg, Germany

to act as our European Authorized Representative as defined in the aforementioned Directive.

I, the undersigned, hereby declare that the medical devices specified above conform with the directive 98/79/EC on in vitro diagnostic medical devices and pertinent essential requirements

Date Signed: November 28, 2017

Name of authorized signatory: Joyce Pang  
Position held in the company: Vice-President



# Certificate

No. Q5 092305 0001 Rev. 01

**Holder of Certificate:** **Zhejiang Orient Gene Biotech Co., Ltd.**  
3787#, East Yangguang Avenue, Dipu Street Anji  
313300 Huzhou, Zhejiang  
PEOPLE'S REPUBLIC OF CHINA

**Certification Mark:**



**Scope of Certificate:** **Design and Development, Production and Distribution of In Vitro Diagnostic Reagent and Instrument for the Detection of Drugs of Abuse, Fertility, Infectious Diseases, Oncology, Biochemistry, Cardiac Diseases, Allergic Disease based on Rapid Test, PCR and Liquid Biochip Method.**

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:Q5 092305 0001 Rev. 01](http://www.tuvsud.com/ps-cert?q=cert:Q5_092305_0001_Rev._01)

**Report No.:** SH2198802

**Valid from:** 2022-04-11

**Valid until:** 2024-03-16

**Date,** 2022-04-11



Christoph Dicks

Head of Certification/Notified Body



Product Service

# Certificate

No. Q5 092305 0001 Rev. 01

**Applied Standard(s):** EN ISO 13485:2016  
Medical devices - Quality management systems -  
Requirements for regulatory purposes  
(ISO 13485:2016)  
DIN EN ISO 13485:2016

**Facility(ies):** Zhejiang Orient Gene Biotech Co., Ltd.  
3787#, East Yangguang Avenue, Dipu Street Anji, 313300  
Huzhou, Zhejiang, PEOPLE'S REPUBLIC OF CHINA

See Scope of Certificate



浙江东方基因生物制品股份有限公司  
Zhejiang Orient Gene Biotech Co.,LTD

---

## STATEMENT

We, Zhejiang Orient Gene Biotech Co., Ltd , having a registered office at 3787#, East Yangguang Avenue, Dipu Street Anji 313300, Huzhou, Zhejiang, China assign SRL SANMEDICO having a registered office at A. Corobceanu street 7A, apt. 9, Chişinău MD-2012, Moldova, as non-exclusive authorized representative for Orient Gene Brand product in correspondence with the conditions of directive 98/79/EEC.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

This Statement letter will be valid from Feb.21th,2023 to Feb.20th, 2024.

Zhejiang Orient Gene Biotech Co., Ltd

General Manager:

Date:2023/2/21



---

地址：浙江省湖州市安吉县递铺镇阳光大道东段 3787 号  
Add: 3787#, East Yangguang Avenue, Dipu Street Anji 313300, Huzhou, Zhejiang, China  
电话 Tel:+86-572-5226111 传真 Fax: +86-572-5226222 邮编 P.C.:313300



SYNTESYS S.A.S. DI RINALDO R. & C.

VIA G. GALILEI, 10/3  
35037 Z.I. SELVE DI TEOLO (PD)  
TEL. +39 049 9903866 R.A. FAX +39 049 9903867  
COD. FISCALE P.IVA N.REG.IMP. PADOVA 03573950288  
E-MAIL [INFO@SYNTESYS.IT](mailto:INFO@SYNTESYS.IT) · WEB [WWW.SYNTESYS.IT](http://WWW.SYNTESYS.IT)

DICHIARAZIONE DI CONFORMITA'  
*Conformity declaration*



Il sottoscritto, Rinaldo Ruggero legale rappresentante della ditta:  
*The undersigned, Rinaldo Ruggero legal representative of the company:*

*produttore/manufacturer*

SYNTESYS S.a.s. di Rinaldo R. & C.

*indirizzo/address*

Via G. Galilei, 10/3 35037 Zona Industriale SELVE DI TEOLO (PADOVA) ITALY

ò rappresentante il mandatario autorizzato entro la Unione Europea  
*or representing the authorized mandatary within the European Community*

*Mandatario autorizzato/authorized mandatary*

*indirizzo/address*

Dichiara sotto la propria responsabilità che il prodotto/*declares under his own responsibility that the product:*

*Denominazione/Description*

Padella per ammalati, urinali uomo e donna, speculum vaginali, tamponcini cotonati, tamponi sterili in provetta, tamponi sterili con terreno Amies e Stuart in provetta/ *Bed pan, Urinal's man and woman, Vaginal speculum, Cotton swab, Sterile swab in test tube, Sterile swab with medium Amies or Stuart in test tube*

*Materiale/Material*

Polipropilene, Polietilene, Legno/ *Polypropylene, Polyethylene, Wood*

È conforme alle disposizioni della direttiva 93/42/CE e s.m.i. concernente i dispositivi medici ed al Decreto Legislativo di recepimento con D.lgs. del 24/02/1997 n° 46/97 e soddisfa a tutti i requisiti specificati.

Il dispositivo è stato classificato appartenente alla classe I° secondo i criteri stabiliti in base a quanto previsto dall'Art. 9 ed allegato IX della direttiva sopra citata /*It meets the EC Directive 93/42 about Medical Device, specifications established by the Italian law n 46/97, dated 24<sup>th</sup> February 1997. The device was classified as belonging to the 1<sup>st</sup> class, according to the specifications of the established by the art.9, IX enclosure of the above mentioned directive.*

Dichiara inoltre che la documentazione tecnica di supporto alla presente dichiarazione di conformità è conservata presso gli uffici dell'azienda e sarà posta alla disposizione di chi la richiede/ *declares that all technical documents attached to this conformity statment are filed in our company and can be consulted by any authorized body on demand.*

Data 07.01.2016  
Issued on January 7<sup>th</sup> 2016

SYNTESYS S.A.S.  
Il legale rappresentante  
Rinaldo Ruggero



**SYNTESYS**



SYNTESYS S.A.S. DI RINALDO R. & C.  
VIA G. GALILEI, 10/3  
35037 Z.I. SELVE DI TEOLO (PD)

TEL. +39 049 9903866 R.A. FAX +39 049 9903867

COD. FISCALE P.IVA N.REG.IMP. PADOVA 03573950288  
E-MAIL [INFO@SYNTESYS.IT](mailto:INFO@SYNTESYS.IT) - WEB [WWW.SYNTESYS.IT](http://WWW.SYNTESYS.IT)

**DICHIARAZIONE DI CONFORMITA'**  
*Conformity declaration*



Il sottoscritto, Rinaldo Ruggero legale rappresentante della ditta:  
*The undersigned, Rinaldo Ruggero legal representative of the company:*

*produttore/manufacturer*

**SYNTESYS S.a.s. di Rinaldo Ruggero & C.**  
*indirizzo/address*

**Via G. Galilei, 10/3 35037 Zona Industriale SELVE DI TEOLO (PADOVA) ITALY**

*o rappresentante il mandatario autorizzato entro la Unione Europea or representing the authorized mandatary within the European Community*

*Mandatario autorizzato/authorized mandatary*

*indirizzo/address*

Dichiara sotto la propria responsabilità che il prodotto/*declares under his own responsibility that the product:*

Denominazione degli  
articoli  
prodotti/*Description of  
Manufacturer*

Contenitori per urina, contenitori per feci,  
contenitori universali, Pipette Pasteur, Piastre di  
Petri, Anse Sterili per batteriologia, Aste a "L",  
Puntali Eppendorf gialli e blue, cuvette per  
spettrofotometro, tazzine per campionamento siero,  
bacchette per distacco ed estrazione del coagulo,  
pinzette in polistirolo monouso, provette monouso in  
plastica, tappi alettati per provette diam. 12 mm e  
16mm, provette con granuli ed acceleratore, provette  
sottovuoto per prelievo, Sistema SEDIPLAST,  
Microprovette, Portavetrini, Vetrini precolorati,  
Portaprovette, supporti per microprovette, bottiglie  
per raccolta urine.

*Urine container, faeces container, universal  
container, Pasteur pipette, Petri dishes, Sterile  
loops, Sterile loops open "L", Eppendorf tips yellow  
and blue, cuvettes for spectrophotometer, samples  
cups, Rod to detach clot, disposable forceps,  
Disposable plastic tubes, winged stoppers for tubes  
diam. 12mm & 16mm, Test tube with granules and clot  
activator, vacuum test tube, SEDIPLAST system,  
micro test tubes, Slides Mailer, "TESTSIMPLETS" slide,  
rack for test tubes, rack for micro test tubes,  
Bottles for urine collection.*



**SYNTESYS**



ISO9001:2008  
Cert. N. 6574/0

SYNTESYS S.A.S. DI RINALDO R. & C.  
VIA G. GALILEI, 10/3  
35037 Z.I. SELVE DI TEOLO (PD)  
TEL. +39 049 9903866 R.A. FAX +39 049 9903867  
COD.FISCALE P.IVA N.REG.IMP. PADOVA 03573950288  
E-MAIL [INFO@SYNTESYS.IT](mailto:INFO@SYNTESYS.IT) - WEB [WWW.SYNTESYS.IT](http://WWW.SYNTESYS.IT)

*Materiale/ Material*

**Polipropilene, Polistirolo, Polietilene e  
Polimetilmetacrilato**


***Polypropylene, Polystyrene, Polyethylene and  
Polymethylmetacrylate***

È conforme alle disposizioni della direttiva 98/79/CE concernente i dispositivi medici diagnostici in vitro e recepito in Italia con D.L. del 08/09/2000 n° 332 allegato 1 (requisiti essenziali) ed è fabbricato in accordo ai requisiti di cui all'Allegato III della sopra citata direttiva / *It meets the CE Directive 98/79 CE about in vitro diagnostic device specifications established by the Italian law n. 332, dated 8<sup>th</sup> September 2000. The device is made according to the specifications of the III attached of the above-mentioned directive.*

Dichiara inoltre che la documentazione tecnica di supporto alla presente dichiarazione di conformità è conservata presso gli uffici dell'azienda e sarà posta alla disposizione di chi la richiede/declares that all technical documents attached to this conformity statement are filed in our company and can be consulted by any authorized body on demand.

Data 07/01/2016  
Issued on January 7<sup>th</sup> 2016

**SYNTESYS S.a.s.**  
Il legale rappresentante  
**Rinaldo Ruggero**

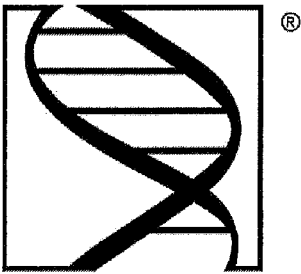

**SYNTESSYS**



Cert. N.7111/2



Cert. N.6574/2



**SYNTESSYS S.R.L. UNIPERSONALE**

VIA G. GALILEI, 10/3 - 35037 Z.I. SELVE DI TEOLO (PD)  
TEL. +39 049 9903866 R.A. FAX +39 049 9903867  
C.F./P.I./N.REG.IMP. PADOVA 03573950288  
REA PD-320123 - CAP.SOC. 20.700,00€  
E-MAIL [INFO@SYNTESSYS.IT](mailto:INFO@SYNTESSYS.IT) - WEB [WWW.SYNTESSYS.IT](http://WWW.SYNTESSYS.IT)  
PEC [POSTA@PEC.SYNTESSYS.IT](mailto:POSTA@PEC.SYNTESSYS.IT)


## AUTHORIZATION LETTER

We, **Syntesys S.R.L.** having a registered office at Via G. Galilei 10/3, 35037 Selve di Teolo - PD - Italy, assign **Sanmedico SRL** having a registered office at A.Corobceanu str., apt. 9, Chişinău MD-2012, Moldova, as authorized representative.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

This letter is valid till 31.12.2021

Teolo, 05.01.2021

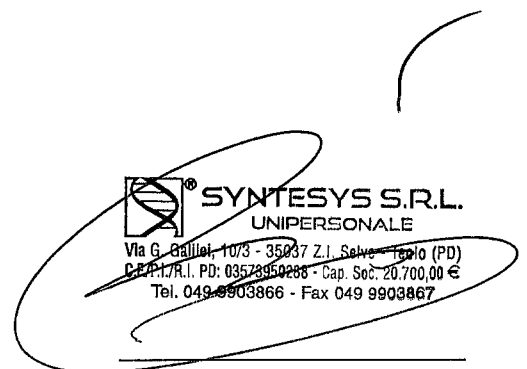

**SYNTESSYS S.R.L.**  
UNIPERSONALE  
Via G. Galilei, 10/3 - 35037 Z.I. Selve di Teolo (PD)  
C.F./P.I./R.I. PD: 03573950288 - Cap. Soc. 20.700,00 €  
Tel. 049.9903866 - Fax 049 9903867

Rinaldo Ruggero  
CEO and Legal Representative  
SYNTESSYS S.R.L.



# Certificate

CISQ/ICIM S.P.A. has issued an IQNet recognized certificate that the organization:

## SYNTESYS S.R.L.

Head Office and Operative Unit

Via G. Galilei, 10/1-2-3 - Zona Industriale - I-35037 Selve di Teolo (PD)

Operative Units

Via G. Galilei, 16/1 - Zona Industriale - I-35037 Selve di Teolo (PD)

Via San Benedetto, 48/A - Zona Industriale - I-35037 Selve di Teolo (PD)

Via G. Galilei, 3 - Zona Industriale - I-35037 Selve di Teolo (PD)

has implemented and maintains a/an

## Quality Management System

for the following scope:

**Trading of products for laboratory analysis. Manufacturing of products for laboratory analysis and sanitary products. Design and production management of sterile swabs for the collection and the preservation of biological samples, also for surgical application, with or without transport medium.**

which fulfils the requirements of the following standard:

## ISO 9001:2015

Issued on: **2022-06-05**

First issued on: **2013-06-05**

Expires on: **2025-06-04**

This attestation is directly linked to the IQNet Partner's original certificate and shall not be used as a stand-alone document.

Registration Number: **IT-83562**



**Alex Stoichitoiu**  
President of IQNET



**Mario Romersi**  
President of CISQ



This attestation is directly linked to the IQNET Member's original certificate and shall not be used as a stand-alone document.

### **IQNET Members\*:**

**AENOR** Spain **AFNOR Certification** France **APCER** Portugal **CCC** Cyprus **CISQ** Italy **CQC** China **CQM** China **CQS** Czech Republic  
**Cro Cert** Croatia **DQS Holding GmbH** Germany **EAGLE Certification Group** USA **FCAV** Brazil **FONDONORMA** Venezuela **ICONTEC**  
Colombia **ICS** Bosnia and Herzegovina **Inspecta Sertifointi Oy** Finland **INTECO** Costa Rica **IRAM** Argentina **JQA** Japan **KFQ** Korea  
**LSQA** Uruguay **MIRTEC** Greece **MSZT** Hungary **Nemko AS** Norway **NSAI** Ireland **NYCE-SIGE** México **PCBC** Poland **Quality Austria**  
Austria **SII** Israel **SIQ** Slovenia **SIRIM QAS International** Malaysia **SQS** Switzerland **SRAC** Romania **TSE** Turkey **YUQS** Serbia

\* The list of IQNET Members is valid at the time of issue of this certificate. Updated information is available under [www.iqnet-certification.com](http://www.iqnet-certification.com)

# Certificate

CISQ/ICIM S.P.A. has issued an IQNet recognized certificate that the organization:

## SYNTESYS S.R.L.

Head Office and Operative Unit

Via G. Galilei, 10/1-2-3 - Zona Industriale - I-35037 Selve di Teolo (PD)

Operative Units

Via G. Galilei, 16/1 - Zona Industriale - I-35037 Selve di Teolo (PD)

Via San Benedetto, 48/A - Zona Industriale - I-35037 Selve di Teolo (PD)

Via G. Galilei, 3 - Zona Industriale - I-35037 Selve di Teolo (PD)

has implemented and maintains a/an

## Quality Management System

for the following scope:

**Trading of products for laboratory analysis. Manufacturing of products for laboratory analysis and sanitary products. Design and production management of sterile swabs for the collection and the preservation of biological samples, also for surgical application, with or without transport medium.**

which fulfils the requirements of the following standard:

## ISO 13485:2016

Issued on: **2022-06-05**

First issued on: **2014-06-21**

Expires on: **2025-06-04**

This attestation is directly linked to the IQNet Partner's original certificate and shall not be used as a stand-alone document.

Registration Number: **IT-93779**



**Alex Stoichitoiu**  
President of IQNET



**Mario Romersi**  
President of CISQ



This attestation is directly linked to the IQNET Member's original certificate and shall not be used as a stand-alone document.

### **IQNET Members\*:**

**AENOR** Spain **AFNOR Certification** France **APCER** Portugal **CCC** Cyprus **CISQ** Italy **CQC** China **CQM** China **CQS** Czech Republic  
**Cro Cert** Croatia **DQS Holding GmbH** Germany **EAGLE Certification Group** USA **FCAV** Brazil **FONDONORMA** Venezuela **ICONTEC**  
Colombia **ICS** Bosnia and Herzegovina **Inspecta Sertifointi Oy** Finland **INTECO** Costa Rica **IRAM** Argentina **JQA** Japan **KFQ** Korea  
**LSQA** Uruguay **MIRTEC** Greece **MSZT** Hungary **Nemko AS** Norway **NSAI** Ireland **NYCE-SIGE** México **PCBC** Poland **Quality Austria**  
Austria **SII** Israel **SIQ** Slovenia **SIRIM QAS International** Malaysia **SQS** Switzerland **SRAC** Romania **TSE** Turkey **YUQS** Serbia

\* The list of IQNET Members is valid at the time of issue of this certificate. Updated information is available under [www.iqnet-certification.com](http://www.iqnet-certification.com)

Date: 23<sup>rd</sup> January 2023**STATEMENT**

We, **HiMedia Laboratories Pvt. Ltd.**, having a registered office at **Plot No.:C40, Road No.:21Y, MIDC, Wagle Industrial Area, Thane (West) - 400 604, Maharashtra, INDIA** assign **SRL SANMEDICO** having a registered office at **A. Corobceanu street 7A, apt. 9, Chişinău MD-2012, Moldova** , as authorized representative in correspondence with the conditions of directive 98/79/EEC.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

For **HIMEDIA LABORATORIES PVT. LTD.**,

**V.M.WARKE.**



**DIRECTOR – SALES & MARKETING**

**REGISTERED OFFICE -**

Plot No. C40, Road No. 21Y, MIDC, Wagle Industrial Area, Thane (West) - 400604, Maharashtra, India.  
Tel: +91-22-6147 1919 / 6116 9797 / 6903 4800 | Fax: +91-22-6147 1920  
Email: info@himedialabs.com | Web: www.himedialabs.com



... expect only quality from us™  
CIN: U85195MH1982PTC028194



THE INTERNATIONAL CERTIFICATION NETWORK

# CERTIFICATE

Quality Austria

has issued an IQNet recognized certificate that the organization:

**HiMedia Laboratories Pvt. Ltd.**

**Plot NO. C40, ROAD - 21Y, WAGLE INDUSTRIAL ESTATE,  
THANE (WEST) - 400604 MAHARASHTRA, INDIA**

for the following scope:

**Design, Development & Testing of Microbiology, Animal Cell Culture,  
Plant Tissue Culture & Molecular Biology products**

EAC: 34

has implemented and maintains a

## QUALITY MANAGEMENT SYSTEM

which fulfils the requirements of the following standard

### ISO 9001:2015

This attestation is directly linked to the IQNet Partner's original certificate and shall not be used as a stand-alone document

Issued on:	2022-02-28
Validity date:	2025-02-27
Quality Austria certified since:	2022-02-28

**Registration Number: AT-27302/0**

**Alex Stoichitoiu**  
President of IQNet

**Mag. Friedrich Khuen-Belasi**  
Authorised Representative  
of Quality Austria



**IQNet Partners\*:**

AENOR Spain AFNOR Certification France APCER Portugal CCC Cyprus CISQ Italy  
CQC China CQM China CQS Czech Republic Cro Cert Croatia DQS Holding GmbH Germany EAGLE Certification Group USA  
FCAV Brazil FONDONORMA Venezuela ICONTEC Colombia Inspecta Sertifointi Oy Finland INTECO Costa Rica  
IRAM Argentina JQA Japan KFQ Korea MIRTEC Greece MSZT Hungary Nemko AS Norway NSAI Ireland  
NYCE-SIGE México PCBC Poland Quality Austria Austria RR Russia SII Israel SIQ Slovenia  
SIRIM QAS International Malaysia SQS Switzerland SRAC Romania TEST St Petersburg Russia TSE Turkey YUQS Serbia

\* The list of IQNet partners is valid at the time of issue of this certificate. Updated information is available under [www.iqnet-certification.com](http://www.iqnet-certification.com)



THE INTERNATIONAL CERTIFICATION NETWORK

# CERTIFICATE

Quality Austria

has issued an IQNet recognized certificate that the organization:

**HiMedia Laboratories Pvt. Ltd.**

**Plot NO. C40, ROAD - 21Y, WAGLE INDUSTRIAL ESTATE,  
THANE (WEST) - 400604 MAHARASHTRA, INDIA**

for the following scope:

**Design, Development & Testing of Biosciences Products for application in Microbiology,  
Animal Cell Culture & Molecular Biology products**

EAC: 34

has implemented and maintains a

## QUALITY MANAGEMENT SYSTEM

which fulfils the requirements of the following standard

### ISO 13485:2016

This attestation is directly linked to the IQNet Partner's original certificate and shall not be used as a stand-alone document

Issued on:	2022-02-28
Validity date:	2025-02-27
Quality Austria certified since:	2022-02-28

**Registration Number: AT-00391/0**

**Alex Stoichitoiu**  
President of IQNet

**Mag. Friedrich Khuen-Belasi**  
Authorised Representative  
of Quality Austria



**IQNet Partners\*:**

AENOR Spain AFNOR Certification France APCER Portugal CCC Cyprus CISQ Italy  
CQC China CQM China CQS Czech Republic Cro Cert Croatia DQS Holding GmbH Germany EAGLE Certification Group USA  
FCAV Brazil FONDONORMA Venezuela ICONTEC Colombia Inspecta Sertifiointi Oy Finland INTECO Costa Rica  
IRAM Argentina JQA Japan KFQ Korea MIRTEC Greece MSZT Hungary Nemko AS Norway NSAI Ireland  
NYCE-SIGE México PCBC Poland Quality Austria Austria RR Russia SII Israel SIQ Slovenia  
SIRIM QAS International Malaysia SQS Switzerland SRAC Romania TEST St Petersburg Russia TSE Turkey YUQS Serbia

\* The list of IQNet partners is valid at the time of issue of this certificate. Updated information is available under [www.iqnet-certification.com](http://www.iqnet-certification.com)