

SuctionPro72™ **Closed Ventilation Suction System**



Reduce Infection. Reduce Patient Stay. Reduce Costs.

PORTEX®

SuctionPro72™



SuctionPro 72™

The Portex® SuctionPro72™ Closed Ventilation Suction System is a single patient use suctioning device for the removal of secretions from the tracheobronchial tree of ventilator dependent adult patients. Intended for 72-hour use.

Key Features

- 3-day recommended duration of use
- Clear pathway evacuation port
- Lockable thumb valve end cap
- Sterile, single patient use
- Clear T piece for visualisation of the pathway
- Soft but strong catheter sleeve
- MDI Adaptor for integrated inhaler capability
- Patient labels now coloured by day for easy identification
- Trac-Wedge™ device to aid in disconnection of the catheter from the patient's endotracheal or tracheostomy tube
- Swivel connector to reduce torque to patient in some packs



Fig. 1



Fig. 3



Fig. 4



Fig. 2

Instructions for Use

To Lavage

Fig. 1 Hold T-piece in one hand and advance catheter approximately 10cm into the airway. Instill saline solution through the irrigation inlet.

To Suction:

Note: Patients may benefit from pre-oxygenation with 100% oxygen.

Fig. 2 Make sure the suction control valve lock is in the 'OPEN' position. Advance the catheter to the desired depth whilst holding the patient end steady. If resistance is met, withdraw the catheter 2-3cm before applying suction.

Fig. 3 Grasp the control valve and apply backwards-sliding pressure on the blue thumb actuator to suction.

Note: Maximum suction is achieved by sliding the actuator fully back.

Withdraw the catheter slowly with suction activated in a straight motion to avoid kinking until blue mark is just fully visible in catheter sleeve.

Fig. 4 Ensure that the catheter tip is out of the breathing path and in-line with the saline port. Begin to clean catheter tip with saline. The saline should be administered through the irrigation inlet whilst vacuum is applied making sure that the tip and area surrounding it is fully flushed with saline. Release control valve actuator and turn the valve lock to the 'CLOSE' position when finished.

Preparation

- Before attaching the system to the patient turn on the suction, make sure the lock is turned to the 'OPEN' position and check the operation of the control valve by sliding back the actuator. Once in the fully back position release and make sure that the device shuts correctly
- Attach ventilator circuit to dual-swivel or Tpiece adaptor
- Attach the dual-swivel or Tpiece adaptor to the tracheal or tracheostomy tube connector
- Attach male connector of the SuctionPro72™ Closed Ventilation Suction System device to suction tubing
- Attach the suction tubing to the male connector of the SuctionPro72™ closed ventilation suction system

smiths medical									
PORTEX									
Respiratory	Endotracheal	Endotracheal	Endotracheal	Endotracheal	Endotracheal	Endotracheal	Endotracheal	Endotracheal	Endotracheal
Intubation	Intubation	Intubation	Intubation	Intubation	Intubation	Intubation	Intubation	Intubation	Intubation
Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy
Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy
Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy
Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy
Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy
Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy
Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy	Tracheostomy

Day Label

SuctionPro72™

Comprehensive product range available in single and dual lumen configurations, with coloured day labels. MDI adaptor in non dual swivel options. Each Portex® SuctionPro72™ suction system offers a wide range of options to enhance patient care outcomes and accommodate clinical practices. Available in a case of 20 units.

IDENTIFICATION MATRIX

	Part No	10 FR	12 FR	14 FR	16 FR	300mm Length	570mm Length	Flex Tube	Coudé Tip	Dual Swivel	MDI adaptor
SINGLE LUMEN	Z110-10	•					•				•
	Z110-12		•				•				•
	Z110-14			•			•				•
	Z110-16				•		•				•
	Z115-10	•				•					•
	Z115-12		•			•					•
	Z115-14			•		•					•
	Z115-16				•	•					•
	Z116-14			•		•		•			•
	Z118-14			•			•	•			•
	Z120-10	•					•		•		•
	Z120-12		•				•		•		•
	Z120-14			•			•		•		•
	Z120-16				•		•		•		•
	Z130-14*			•			•				•
	Z130-16*				•		•				•
	Z135-14*			•		•					•
	Z135-16*				•	•					•
	Z150-10	•					•			•	
	Z150-12		•				•			•	
	Z150-14			•			•			•	
	Z150-16				•		•			•	
	Z155-10	•				•				•	
	Z155-12		•			•				•	
	Z155-14			•		•				•	
	Z155-16				•	•				•	
	Z156-14			•		•		•		•	
	Z160-14			•			•		•	•	
	Z160-16				•		•		•	•	
DOUBLE LUMEN	Z210-12		•				•				•
	Z210-14			•			•				•
	Z210-16				•		•				•
	Z215-12		•			•					•
	Z215-14			•		•					•
	Z216-14			•		•		•			•
	Z250-12		•				•			•	
	Z250-14			•			•			•	
	Z250-16				•		•			•	
	Z255-12		•			•				•	
	Z255-14			•		•				•	
	Z256-14			•		•		•		•	

*not CE marked

PRODUCT(S) DESCRIBED MAY NOT BE LICENSED OR AVAILABLE FOR SALE IN CANADA AND OTHER COUNTRIES

Smiths Medical International Ltd.
Ashford, UK TN25 4BF
Phone: +44 (0) 845 8500445
www.smiths-medical.com

Find your local contact information at: www.smiths-medical.com/customer-support

Smiths Medical is part of the global technology business Smiths Group plc. Please see the Instructions for Use/Operator's Manual for a complete listing of the indications, contraindications, warnings and precautions. Portex, SuctionPro 72 and the Smiths Medical and Portex design marks are registered trademarks of Smiths Medical. The symbol ® indicates the trademark is registered in the U.S. Patent and Trademark Office and certain other countries. All other names and marks mentioned are the trademarks or service marks of their respective owners. ©2013 Smiths Medical. All rights reserved. RE194257GB-082013

CE Rx
0473 ONLY

smiths medical

MHYTCA-1030

Respiratory Care Solutions Improving Quality of Life



Improving quality of life...



The need to rehabilitate patients effectively after respiratory disorders, is of extreme importance, not only to decrease patient recovery time for improved hospital efficiency, but also for the well-being and quality of life of the patient.

Introducing a Pulmonary Rehabilitation Programme (PRP) can help patients with lung disease achieve the highest possible level of functioning. PRPs have been shown to improve quality of life, mitigate symptoms, improve exercise tolerance, and lower the number of hospital admissions.

Two key elements of a PRP are Bronchial Hygiene Therapy (BHT) and Lung Expansion Therapies.

Smiths Medical has developed a comprehensive range of respiratory care products designed for both hospital and home use.

These products help to rehabilitate patients with the aim of improving their physical and social performance. By focusing on the rehabilitation of patients and continued lung training, hospitals can potentially see cost savings due to reduced hospital stays and home rehabilitation.

References:

1. Wiersgalla Susan, RRT, RCP, North Memorial Medical Center, Robbinsdale, MN. Abstract presented at the 48th International Respiratory Congress for the AARC Annual Convention and Exhibition on October 5th, 2002 in Tampa, Florida.
2. Steen HJ, Redmond AOB, O'Neill D, Beattie F. Acta Paediatr Scand. Evaluation of the PEP mask in cystic fibrosis. 1991; 80:51-56.
3. Tyrell JC, Hiller EJ, Martin J. Face mask physiotherapy in cystic fibrosis. Archives of Dis in Child 1986; 61: 598-611.
4. Mahlmeister MJ, Fink JB, Hoffman GL, Fifer LF. "Positive-expiratory-pressure mask therapy: Theoretical and Practical Considerations and a Review of the Literature", Respiratory Care, 1991;36:1218-1230.
5. Guell R. Breath, Home- Based Rehabilitation 2008,5 pg:37

CRITICAL CARE

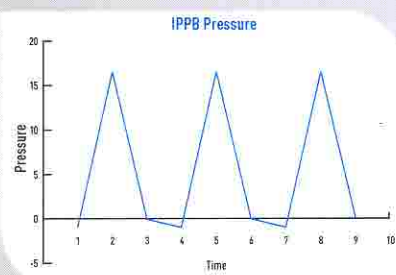
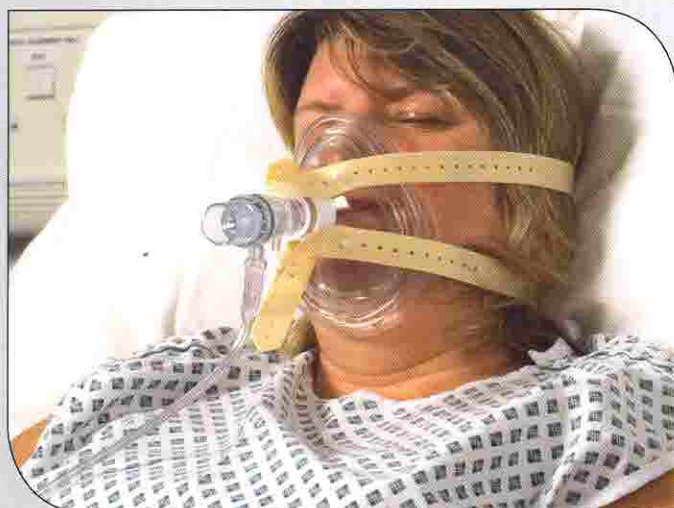


Figure 1

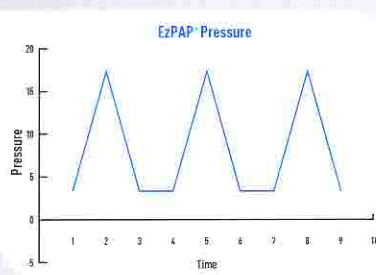
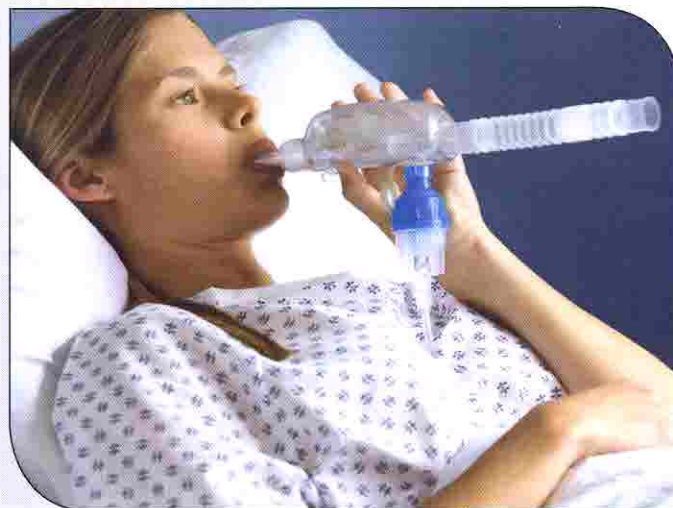


Figure 2

WARD

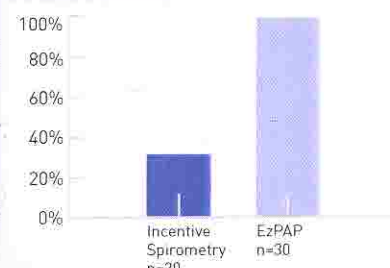


Figure 3
Post-Surgical Atelectasis Improvement
in CABG Patients. $p < .001$

Rehabilitation

For hospitalised patients, the correct rehabilitation can save the hospital both time and money, as well as making the experience more tolerable for the patient.

Many hospitals today, use Intermittent Positive Pressure Breathing (IPPB) to treat and reverse atelectasis as well as being used in re-expanding lung parenchyma. IPPB is a form of assisted ventilation that triggers a positive pressure breath to the patient when the machine senses either effort by the patient, or a negative pressure of an inspiratory breath. Once a certain pressure is reached it then returns to zero. However, IPPB starts with a negative pressure and does not deliver positive expiratory pressure during exhalation. (See figure 1)

EzPAP® is a simple and effective "In-Hospital" method for delivering positive airway pressure throughout the

breathing cycle. Pressure does decrease during inhalation, but it always remains positive, helping to open airways and re-inflate collapsed alveoli. (See figure 2). EzPAP® also provides the additional benefit of Positive Expiratory Pressure therapy during exhalation offering further rehabilitation to the patient. (See figures 4,5 &6)

The combination of therapies offers a safe and effective alternative to IPPB for hospitalised patients. EzPAP® is easy to use and inexpensive in comparison to IPPB. Wiersgella has also demonstrated that EzPAP®, when used post operatively on coronary artery bypass graft patients, shows measurable improvements in atelectasis levels. ¹ (figure 3)

Positive Expiratory Pressure therapy can also be achieved using the acapella® duet from Smiths Medical. The acapella® duet is a vibratory PEP device that

from Hospital...

has a built-in port for aerosolised medication via a small volume nebuliser. Medication such as bronchodilator or mucolytic treatments can be delivered simultaneously with PEP therapy, cutting treatment time to one session, saving time and effort for both clinicians and patients.

Products that encourage PEP therapy are usually well tolerated by most patients and due to the option of self-administering, are an ideal choice for patients who are out of ICU. In contrast to traditional chest physiotherapy (CPT) options, PEP therapy offers effective secretion removal at a low cost. By being independent of daily assistance from clinicians, the compliance level is enhanced and this in turn can also reduce related health-care costs. ^{2,3}

HOME

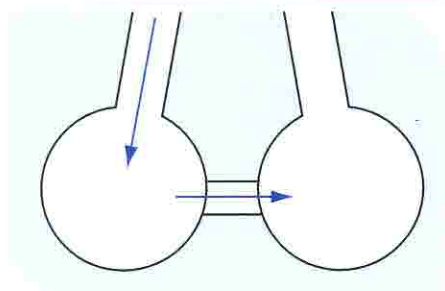
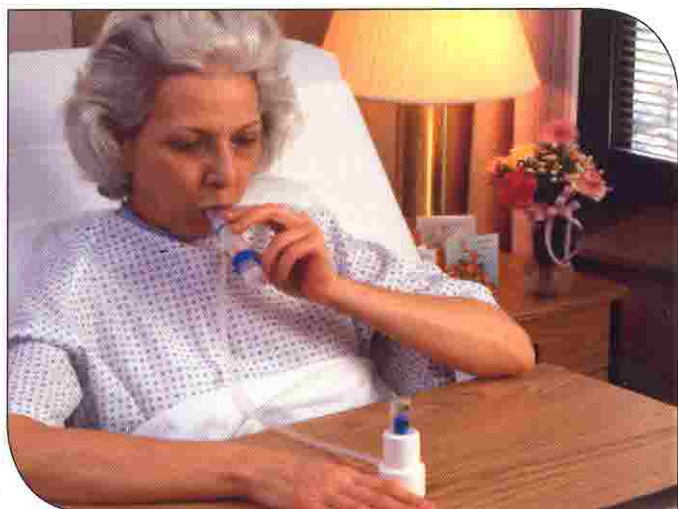


Figure 4
Collateral Ventilation

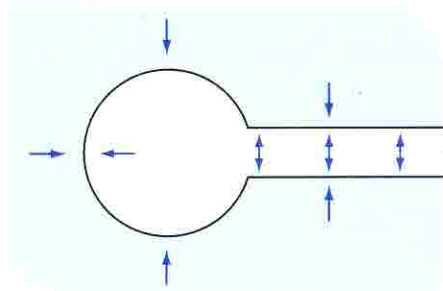


Figure 5 Pursed-lips breathing (or use of a fixed orifice resistor such as a PEP device) creates back pressure that splints the airway open during exhalation.¹⁷

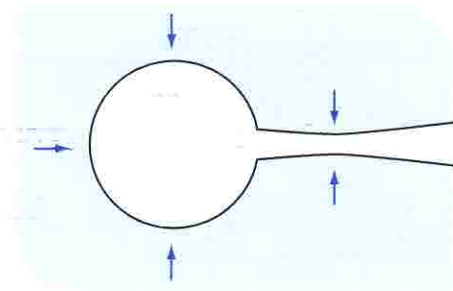


Figure 6 Elevated intrathoracic pressure can compress unstable airways during exhalation.¹⁷

to Home

acapella® duet and acapella® choice, are inexpensive, easy to use standalone options, providing vibratory PEP therapy to remove secretions. They can be used in any position and offer high and low flow rates for the patient. These devices, with the option of a mouthpiece or mask, are a fully versatile product for both patient and hospital.

TheraPEP® is an alternative product offering PEP therapy. This therapy can also be self-administered in half the time of CPT.⁴ TheraPEP® can accommodate virtually any lung capacity and allows inhalation and exhalation without removal from the mouth. With a 22mm ID connector to allow small volume nebulisers or MDI spacers and the option of mouthpiece or mask, this is another great choice for secretion clearance and atelectasis reversal in the hospital setting or at home.

For post-surgical patients, medical devices that help improve their lungs are an important function. Incentive spirometers encourage patients to take slow and deep breaths to expand the lungs. Smiths Medical offers both the Coach® 2 incentive spirometer and the CliniFLO® low-flow incentive spirometer. Coach® 2 combines a one-way valve, highly visible piston and easy to understand graphics indicating correct inspiratory flow rate to help patients perform and monitor their own post-surgical breathing exercises without the need for direct supervision. CliniFLO® is ideal for generic, paediatric or weakened patients due to flow settings as low as 100ml/sec.

Once a patient has been trained to self-administer their chosen therapy in a clinical setting, they are able to continue this therapy at home. acapella® duet, acapella® choice, TheraPEP®, Coach® 2 and CliniFLO® all offer the

versatility to be used in a clinical and/or home setting to provide continued therapy. Each is lightweight, easy to use and transportable. Studies have indicated that home-based rehabilitation programmes not only provide similar benefits to hospital rehabilitation programmes but also can reduce the use of medication and the number of hospitalisations.⁵

Continued lung exercises for patients, whether it is post-surgical in the hospital or at home are key to facilitating patient recovery and therefore an improved quality of life. The respiratory care range from Smiths Medical tailors to each patient's need whilst enabling the clinician to save time and money.


EzPAP®



Features and benefits:

- 22mm OD patient end to accommodate mouthpiece or 3 mask sizes.
- Scalloped ambient air inlet with gaps to resist occlusion.
- Pressure port with detachable cap, allows connection to a gauge for easy monitoring.
- Complete procedural kit.
- Disposable manometer.
- Easy to use, no extensive training.
- Can be used in conjunction with aerosol medication (e.g. nebuliser) via 22mm connection.

acapella® Vibratory PEP Therapy System

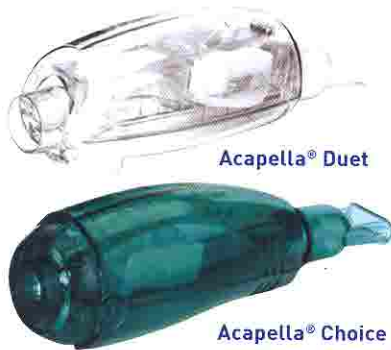

Features and benefits:

- Convenient built-in nebuliser port, standard sized to fit most medication nebulisers (acapella® duet only).
- $\geq 10\text{L/min}$ expiratory flow requirement.
- Streamlined body design offers easy grip (acapella® duet only).
- Adjustable frequency and flow resistance settings.
- Clear colouring aids in visual recognition of cleanliness (acapella® duet only).
- Tethered cap to reduce risk of contamination when in resting position (acapella® duet only).
- Easily disassembled for heat disinfection by boiling, autoclaving and dishwasher (top shelf only)
- Functional in any position – Trendelenburg, standing or sitting.
- Distal 22mm OD fitting allows nebuliser connection via tee adaptor (acapella® choice only).
- One-way inspiratory valve allows inhalation without removal from the mouth.
- Proximal 22mm OD connection allows use with mouthpiece or mask.

TheraPEP®



Features and benefits:

- Six Fixed Orifice Options.
- Built-in durable pressure indicator.
- 22mm OD patient end.
- Inspiratory valve.
- Can accommodate virtually any patient's lung capacity.
- Resists breakage, unlike fragile, costly manometers.
- Provides immediate, visual 360° feedback of prescribed pressure.
- May be used with a mask or mouthpiece, or Nebulizer.
- Allows inhalation and exhalation without removing from mouth

Coach® 2 and CliniFLO®



Features and benefits:

Coach® 2

- Ensures patients inhale, rather than exhale into the unit.
- Easily adjustable for each patient's use.
- Can be seen by patients emerging from the effects of anesthesia.
- Easy to train.
- Stays with the patient for maximum compliance.
- Accommodates patients requiring supplemental oxygen.
- Saves space.
- Colourful deep-sea characters, games, puzzles and stickers.

CliniFLO®

- Can accommodate virtually any patient.
- Reduces the possibility of contamination.
- Provides immediate patient feedback.
- Easy to train.
- Reduces the chance that the setting will be changed inadvertently.

EzPAP®

ORDERING INFORMATION

Product Code	PRODUCT DESCRIPTION	UNITS / CASE
23-0747	EzPAP® System with Mouthpiece	10
23-0757	EzPAP® System with Disposable Manometer and Mouthpiece	10
23-1747	EzPAP® System with Paediatric Mask	1
23-2747	EzPAP® System with Medium Mask	1
23-3747	EzPAP® System with Large Mask	1
23-6000*	EzPAP® Kit: One Pressure Gauge (With Gauge Protector), Three EzPAP® Units (with Mouthpiece), Three Gauge Guards and Ten 22 mm ID Adaptors in a Durable Plastic Box.	1

Each system includes EzPAP® one 7 ft oxygen tube, one pressure port cap, and one of the above

* not CE marked

acapella® Vibratory PEP Therapy System

ORDERING INFORMATION

PART No.	PRODUCT DESCRIPTION	UNITS/CASE
27-9000	acapella® duet kit, includes acapella® duet, mouthpiece, Portex® SVN, oxygen tubing, collapsible flex tubing	10
27-9001	acapella® duet and mouthpiece only	10
007760	Portex® updraft medication nebulizer	50
27-7000	acapella® choice with mouthpiece	10
21-1530	acapella® DH with mouthpiece	10
21-3530	acapella® DH with Paediatric mask	1
21-5530	acapella® DH with medium mask	1
21-7530	acapella® DH with large mask	1
21-1015	acapella® DM with mouthpiece	10
21-3015	acapella® DM with Paediatric mask	1
21-5015	acapella® DM with medium mask	1
21-7015	acapella® DM with large mask	1

ACCESSORIES

Product Code	PRODUCT DESCRIPTION	UNITS/CASE
27-0050	Replacement mouthpiece; fits all acapella® family designs	50

Note: Product is for single patient use only.

For further information please visit:
www.smiths-medical.com/respiratorycare

TheraPEP®

ORDERING INFORMATION

Part No.	PRODUCT DESCRIPTION	UNITS/CASE
20-1112	TheraPEP® System with Mouthpiece	10
20-3112	TheraPEP® System with Paediatric Mask	1
20-5112	TheraPEP® System with Small Mask	1
20-7112	TheraPEP® System with Large Mask	1

ACCESSORIES

Part No.	PRODUCT DESCRIPTION	UNITS/CASE
20-3115	Paediatric Mask	1
20-5115	Small Adult Mask	1
20-7115	Large Adult Mask	1
20-0005	Connector, Straight, 22 mm I. D.	10
20-0010	TheraPEP® Pressure Port	10
20-0022	TheraPEP® Pressure Port, Tubing, Indicator	10
20-0050	TheraPEP® Mouthpiece 22 mm I. D.	50
20-0120	TheraPEP® Pressure Port and Resistor	10
20-1110	TheraPEP® Pressure Port, Resistor and Mouthpiece	10

All TheraPEP® Systems Include: Pressure Port, Resistor, 22 mm ID Straight Connector, Tubing and Pressure Indicator.

Coach® 2 Incentive Spirometers

ORDERING INFORMATION

PART No.	PRODUCT DESCRIPTION	Volume
22-4000	Coach®2 One way valve	4000ml
22-4001	Coach®2	4000ml
22-2500	Coach®2 One way valve	2500ml
22-2501	Coach®2	2500ml
22-2000	Coach®2 Kids One way valve	2000ml

CliniFLO® Low-Flow Incentive Spirometers

ORDERING INFORMATION

PART No.	PRODUCT DESCRIPTION
22-1200	CliniFlo®

PRODUCT(S) DESCRIBED MAY NOT BE LICENSED OR AVAILABLE FOR SALE IN CANADA AND OTHER COUNTRIES

Smiths Medical International Ltd.
Ashford, UK TN25 4BF
Phone: +44 (0) 845 8500445
www.smiths-medical.com

Find your local contact information at: www.smiths-medical.com/customer-support

Smiths Medical is part of the global technology business Smiths Group plc. Please see the Instructions for Use/Operator's Manual for a complete listing of the indications, contraindications, warnings and precautions. Portex, EzPAP, Coach, CliniFLO, acapella, TheraPEP, and the Smiths Medical and Portex design marks are registered trademarks of Smiths Medical. The symbol ® indicates the trademark is registered in the U.S. Patent and Trademark Office and certain other countries. All other names and marks mentioned are the trademarks or service marks of their respective owners. ©2013 Smiths Medical. All rights reserved. RE194286GB-082013

CE Rx
0473 ONLY

smiths medical

MROCCA-0012

Intertek

CT-ISO 9001:2008-UKAS-EN-LT-P-04.jan.12

Intertek

SMITHS MEDICAL CZECH REPUBLIC a.s.

a fost evaluat și înregistrat de AMTAC Certification Services Limited ca fiind conform cerințelor:

EN ISO 13485:2012

Proiectarea, asamblarea, fabricarea, ambalarea si furnizarea de:

Dispozitive și Accesorii pentru Obstetrică și Ginecologie,
 Dispozitive și Accesorii Intervenție Imagistică,
 Dispozitive de Management al Oxigenului și Umidității,
 Dispozitive și Accesorii de Management al Durerii,
 Dispozitive și Accesorii Invasive de Monitorizare a Tensiunii Pacientului,
 Dispozitive Traheotomie,
 Dispozitive de Unică Folosință pentru Injecții,
 Dispozitive Catetere Aspirare,
 Sisteme de Dispozitive de Intubare.

Certificat Număr: 1201-04 B
Data Inițială a Certificării: 10 Ianuarie, 2014
Data Efectivă a Certificatului: 22 Mai 2017
Data Expirării Certificatului: 28 Februarie 2019

Brian Johnson

AMTAC Certification Services Limited, Milton Keynes, UK

Acest Certificat este proprietatea AMTAC Certification Services Ltd



100.3



În emitera acestui certificat, Intertek nu asumă nicio răspundere față de altă Parte în afara de Client, și aceasta, numai în conformitate cu Acordul de Certificare agreat. Validitatea acestui certificat depinde de păstrarea de către organizație a sistemului în conformitate cu cerințele Intertek pentru sisteme de certificare. Validitatea poate fi confirmată prin email la certificates.validation@intertek.com sau prin scanearea codului din dreapta cu un AMTAC Certification Systems Limited este deținută de AMTAC Certification Systems Holdings Limited, care este o succursală juridică integrală de Intertek UK Holdings Limited. AMTAC Certification Systems Limited este un organism acreditat înregistrat la UKAS cu numărul de identificare 001. În emitera acestui certificat, AMTAC nu-și asumă nicio responsabilitate față de nicio parte, altă decât Clientul, și aceasta numai în conformitate cu Termenii și Condițiile agreate. Certificatul rămâne proprietatea Intertek, carea îi trebuie returnat la cerere.

CT-IS 9001:2008-UKAS-EN-17-P-04 ian 12

Subsemnata **MUSUROIA MIRELA**, traducator autorizat de Ministerul Justitiei, certific exactitatea acestei traduceri cu textul înscrisului original în limba engleza, ce a fost vizat de mine.

Traducător autorizat
Nr. 2769/2015



Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Nr. **CE 661325**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Obiect:

Consultati pagina cu obiectul certificatului.

pe baza examinarii noastre a sistemului de asigurare a calitatii conform cerintelor Directivei Consiliului 93/42/CEE, Anexa II excluzand Sectiunea 4. Sistemul de asigurare a calitatii indeplineste cerintele Directivei. Pentru lansarea pe piata a produselor din clasa III este necesar certificatul mentionat in Anexa II, Sectiunea 4.

Pentru si in numele BSI, organ de certificare in acceptiunea sus-mentionatei Directive (Organ de certificare cu numarul 0086):



Stewart Brain, Sef compartiment conformitate si risc

Dispozitive medicale

Prima editie: **2017-06-28**

Data: **2017-06-28**

Data expirarii: **2022-06-27**

...making excellence a habit™

Pagina 1 din 2

Valabilitatea prezentului certificat este conditionata de mentinerea sistemului nde calitate la cerintele Directivei dovedita de organul de certificare care supravegheaza compania. Prezenta aprobare exclude toate produsele proiectate si/sau fabricate de o terta parte on in numele companiei care detine prezentul certificat, cu exceptia unui acord contrar, incheiat cu BSI. Prezentul certificat a fost redactat electronic si este conditionat de respectarea caietului de sarcini.

Informatii si contact: BSI, Kitemark Court, Davy Avenue, Knowlhill, Milton Keynes MK5 8PP. Tel: + 44 345 080 9000 BSI Assurance UK Limited, inregistrata in Anglia sub numarul 7805321 in 389 Chiswick High Road, Londra W4 4AL, UK. A membra a grupului BSI.



Certificat nr.: CE 661325

Obiectul certificatului:

Proiectarea, dezvoltarea si fabricatia produselor sterile:

Sisteme de respiratie, Dispozitive de drenaj, Dispozitive de nutritie, Dispozitive de filtrare pentru Circuite respiratorii, Consumabile pentru perfuzii, Sisteme de intubatie, Dispozitive de prelevare a probelor pentru obstetrica si ginecologie, Dispozitive de gestionare a oxigenului si umiditatii, Accesorii de control al presiunii, Dispozitive de resuscitare, Catetere de absorbtie, Tuburi de traheostomie, Dispozitive de acces vascular

Proiectarea, dezvoltarea si fabricatia de produse nesterile:

Sisteme de respiratie, Sisteme de intubatie, Dispozitive de resuscitare, Supozitoare vaginale, Tuburi de traheostomie, Dispozitive de gestionare a oxigenului si umiditatii



Prima editie: **2017-06-28**

Data: **2017-06-28**

Data expirarii: **2022-06-27**

...making excellence a habit.™

Pagina 2 of 2

Valabilitatea prezentului certificat este conditionata de mentinerea sistemului nde calitate la cerintele Directivei dovedita de organul de certificare care supravegheaza compania. Prezenta aprobare exclude toate produsele proiectate si/sau fabricate de o terta parte on in numele companiei care detine prezentul certificat, cu exceptia unui acord contrar, incheiat cu BSI.
Prezentul certificat a fost redactat electronic si este conditionat de respectarea caietului de sarcini.

Informatii si contact: BSI, Kitemark Court, Davy Avenue, Knowlhill, Milton Keynes MK5 8PP. Tel: + 44 345 080 9000 BSI
Assurance UK Limited, inregistrata in Anglia sub numarul 7805321 in 389 Chiswick High Road, Londra W4 4AL, UK. A
membra a grupului BSI.



Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
 Data: **2017-06-28**
 Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:

Servicii prestate

Brightwake Limited
 Lowmoor Business Park
 Kirkby-in-Ashfield
 Nottinghamshire
 NG17 7JZ
 Marea Britanie

Fabricatie

GaleMed Corporation
 Nr. 87, Li-Gong 2nd Road
 Wu-Jia
 YILAN 268
 Taiwan

Fabricatie

GE Medical
 Pollards Wood
 Nightingales Lane
 Chalfont Saint Giles
 HP8 4SP
 Marea Britanie

Fabricatie

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
Data: **2017-06-28**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:**Servicii prestate**

Koo Medical Equipment (Shanghai)
Co., Ltd
100 Zhongde Road
Dakun Industrial Park
Songjiang, Shanghai 201614
China

Fabricatie

Pentair Filtration Solutions
1350 Hammond Road
St. Paul
Minnesota
55110
USA

Furnizor crucial

Quadrant EPP Belgium N.V.
Industriepark Noord
Robert Tavernierlaan 2
Tielt
8700
Belgia

Fabricatie

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
Data: **2017-06-28**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:

Servicii prestate

Smiths Healthcare Manufacturing
SA de CV
Avenida Calidad Nr.4
Parque, Industrial Internacional
Tijuana
22425
Mexic

Fabricatie

Smiths Healthcare Manufacturing
SA de CV
Carretera Miguel Alemán Km 21.7
Parque Industrial Monterrey
Apodaca
Nuevo León
66603
Mexic

Fabricatie

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
 Data: **2017-06-28**
 Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:

Servicii prestate

Smiths Medical ASD Inc.
 10 Bowman Dr.
 Keene
 New Hampshire
 03431
 USA

Fabricatie

Smiths Medical ASD Inc.
 1265 Grey Fox Road
 St Paul
 Minnesota
 55112
 USA

Fabricatie

Smiths Medical ASD Inc.
 201 West Queen St.,
 Southington
 Connecticut
 06489
 USA

Fabricatie

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
Data: **2017-06-28**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:

Servicii prestate

Smiths Medical ASD Inc.
6250 Shier Rings Road
Dublin
Ohio
43016
USA

Fabricatie

Smiths Medical ASD Inc.
9124 Polk Lane, Suite 101
Olive Branch
Mississippi
38654
USA

Distributie

Smiths Medical Republica Ceha a.s.
Olomoucká 306
753 01 Hranice
Republica Ceha

Fabricatie

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
Data: **2017-06-28**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:

Servicii prestate

Smiths Medical Gary
5700 W 23rd Ave
Gary
Indiana
46406
USA

Fabricatie

Smiths Medical International Ltd
52 Grayhill Rd
Cumbernauld
Glasgow
G68 9HQ
Marea Britanie

Fabricatie

Smiths Medical International
Nijmegen
Bijsterhuizen 22-08
6604 LD Wijchen
Olanda

Distributie

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
Data: **2017-06-28**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:**Servicii prestate**

Smiths Medical Italia Srl
Via della Stazione, 2
Latina Scalo
04100
Italia

Ambalare

Sterigenics Belgium
(Petit-Rechain) SA
Zoning Industriel de Petit-Rechain
Avenue Andre Ernst 21
B-4800 Verviers
Belgium

Sterilizare ETO

Sterigenics UK Limited
Cotes Park Estate
Somercotes
Alfreton
DE55 4NJ
Marea Britanie

Sterilizare ETO

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
 Data: **2017-06-28**
 Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:

Servicii prestate

Sterigenics US, LLC
 344 Bonnie Circle
 Corona
 California
 92880
 USA

Sterilizare cu raze gamma

Sterigenics, LLC
 1700 College Blvd.
 West Memphis
 Arkansas
 72301
 USA

Sterilizare cu raze gamma

Sterilization Services of
 Tennessee, Inc
 2396 Florida Street
 Memphis
 Tennessee 38109
 USA

Sterilizare ETO

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii

Directiva 93/42/CEE privind dispozitivele medicale, Anexa II excluzand Sectiunea 4

Lista subcontractantilor majori

Recunoscuti ca participanti la prestatii aferente produsului certificat prin:

Certificat nr.: **CE 661325**
Data: **2017-06-28**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Subcontractant:

STERIS ISOMEDIX Services, Inc
7685 Saint Andrews Avenue
San Diego
California 92154
USA

Servicii prestate

Sterilizare ETO

UPG
Avenida La Cuspide #1
Parque Industrial Tecnomex
Del. Playas de Tijuana
Tijuana
Baja California
22700
Mexic

Fabricatie

Velcro USA Inc.
95 Sundial Avenue
Manchester
New Hampshire
03103-7206
USA


Furnizor crucial

...making excellence a habit.™

Certificat CE - Sistem Integral de Asigurare a Calitatii – Istoricul certificatului

Certificat nr.: **CE 661325**
Data: **2017-06-28**
Titular: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
Marea Britanie

Data	Numar de referinta	Actiune
Curenta	8603100 8603169	Prima editie. Transferat de alt organ de certificare. Reinnoirea certificatului.

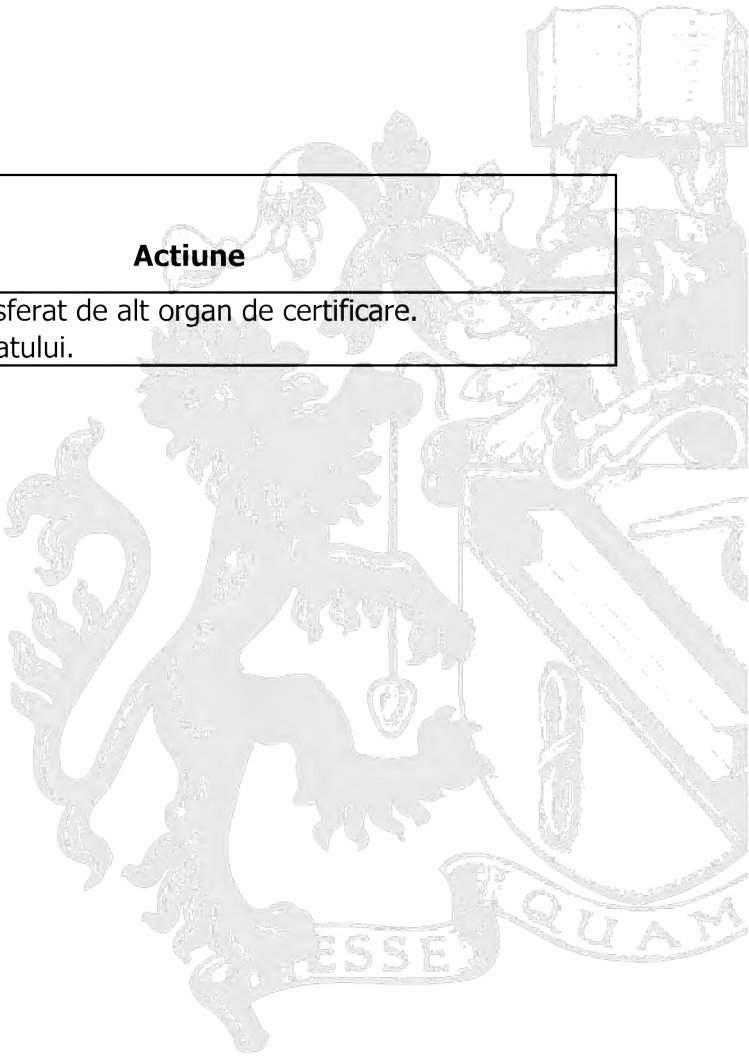

Valabilitatea prezentului certificat este conditionata de mentinerea sistemului nde calitate la cerintele Directivei dovedita de organul de certificare care supravegheaza compania. Prezenta aprobare exclude toate produsele proiectate si/sau fabricate de o terta parte on in numele companiei care detine prezentul certificat, cu exceptia unui acord contrar, incheiat cu BSI.
Prezentul certificat a fost redactat electronic si este conditionat de respectarea caietului de sarcini.

Informatii si contact: BSI, Kitemark Court, Davy Avenue, Knowlhill, Milton Keynes MK5 8PP. Tel: + 44 345 080 9000 BSI Assurance UK Limited, inregistrata in Anglia sub numarul 7805321 in 389 Chiswick High Road, Londra W4 4AL, UK. A membra a grupului BSI.



Subsemnata MUSUROIA MIRELA, traducator autorizat de Ministerul Justitiei, certific exactitatea acestei traducerii cu textul înscrisului original în limba engleza, ce a fost vizat de mine.

Traducător autorizat
Nr. 2769/2015

Certificate of Registration



Intertek

This is to certify that the quality management system of

SMITHS MEDICAL INTERNATIONAL LIMITED

Boundary Road, Hythe, Kent, CT21 6JL, UK

has been assessed and registered by AMTAC Certification Services Limited as conforming to the requirements of:

EN ISO 13485:2012

The quality management system is applicable to:

Design of:

Breathing Systems, Drainage Devices, Feeding Devices,
Filtration Devices, Infusion Disposables, Intubation Systems, Obstetrics and Gynaecology
Devices, Oxygen and Humidity Management Devices, Pressure Monitoring Devices,
Respiratory Mechanics Devices, Resuscitation Devices,
Suction Catheters, Tracheostomy Tubes, Vascular Access Devices, Cardio Thoracic
Catheters and Drapes

Additional Site:

Human Resources and Training, Shipping, Demand Planning, Post Market Surveillance,
Market Intelligence, E-Business, International Customer Services, Business Development,
Registrations, Finance, Wallace Women's Healthcare

Certificate Number:	053-01 B
Initial Certification Date:	20 October 2005
Certificate Effective Date:	23 July 2016
Certificate Expiry Date:	22 July 2019



061



Brian Johnson

AMTAC Certification Services Limited, Milton Keynes, UK

This certificate is the property of AMTAC Certification Services Ltd

In the issuance of this certificate, Intertek assumes no liability to any party other than to the Client, and then only in accordance with the agreed upon Certification Agreement. This certificate's validity is subject to the organization maintaining their system in accordance with Intertek's requirements for systems certification. Validity may be confirmed via email at certificate.validation@intertek.com or by scanning the code to the right with a smartphone. AMTAC Certification Services Limited is owned by AMTAC Certification Services Holdings Limited, which is a wholly owned subsidiary of Intertek UK Holdings Limited. AMTAC Certification Services Limited is an accredited body registered under UKAS with the identification number of 061. In the issuance of this certificate, AMTAC assumes no liability to any party other than to the Client and then only in accordance with the agreed Terms and Conditions.



The certificate remains the property of Intertek, to whom it must be returned upon request.

Intertek



Intertek Intertek Intertek Intertek Intertek

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

No.**CE 661325****Issued To:**


Smiths Medical International Ltd.
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

In respect of:

See certificate scope page.

on the basis of our examination of the quality assurance system under the requirements of Council Directive 93/42/EEC, Annex II excluding section 4. The quality assurance system meets the requirements of the directive. For the placing on the market of class III products an Annex II section 4 certificate is required.

For and on behalf of BSI, a Notified Body for the above Directive (Notified Body Number 0086):



Stewart Brain, Head of Compliance & Risk -
Medical Devices

First Issued: **2017-06-28**

Date: **2017-06-28**

Expiry Date: **2022-06-27**

...making excellence a habit.™

Page 1 of 2

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body. This approval excludes all products designed and/or manufactured by a third party on behalf of the company named on this certificate, unless specifically agreed with BSI.

This certificate was issued electronically and is bound by the conditions of the contract.

Certificate No: CE 661325

Certificate Scope:

The design, development and manufacture of sterile:

Breathing Systems, Drainage Devices, Feeding Devices, Filtration Devices for Breathing Circuits, Infusion Disposables, Intubation Systems, Obstetrics and Gynaecology Sampling Devices, Oxygen and Humidity Management Devices, Pressure Monitoring Accessories, Resuscitation Devices, Suction Catheters, Tracheostomy Tubes, Vascular Access Devices

The design, development and manufacture of non-sterile:

Breathing Systems, Intubation Systems, Resuscitation Devices, Gynecologic Pessaries, Tracheostomy Tubes, Oxygen and Humidity Management Devices

First Issued: **2017-06-28**Date: **2017-06-28**Expiry Date: **2022-06-27**

...making excellence a habit.™

Page 2 of 2

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body. This approval excludes all products designed and/or manufactured by a third party on behalf of the company named on this certificate, unless specifically agreed with BSI.

This certificate was issued electronically and is bound by the conditions of the contract.

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
Date: **2017-06-28**
Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:**Service(s) supplied**

Brightwake Limited
Lowmoor Business Park
Kirkby-in-Ashfield
Nottinghamshire
NG17 7JZ
United Kingdom

Manufacture

GaleMed Corporation
No. 87, Li-Gong 2nd Road
Wu-Jia
YILAN 268
Taiwan

Manufacture

GE Medical
Pollards Wood
Nightingales Lane
Chalfont Saint Giles
HP8 4SP
United Kingdom

Manufacture

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:

Service(s) supplied

Koo Medical Equipment (Shanghai)
 Co., Ltd
 100 Zhongde Road
 Dakun Industrial Park
 Songjiang, Shanghai 201614
 China

Manufacture

Pentair Filtration Solutions
 1350 Hammond Road
 St. Paul
 Minnesota
 55110
 USA

Crucial Supplier

Quadrant EPP Belgium N.V.
 Industriepark Noord
 Robert Tavernierlaan 2
 Tielt
 8700
 Belgium

Manufacture

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:	Service(s) supplied
Smiths Healthcare Manufacturing SA de CV Avenida Calidad No.4 Parque, Industrial Internacional Tijuana 22425 Mexico	Manufacture
Smiths Healthcare Manufacturing SA de CV Carretera Miguel Alemán Km 21.7 Parque Industrial Monterrey Apodaca Nuevo León 66603 Mexico	Manufacture

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:	Service(s) supplied
Smiths Medical ASD Inc. 10 Bowman Dr. Keene New Hampshire 03431 USA	Manufacture
Smiths Medical ASD Inc. 1265 Grey Fox Road St Paul Minnesota 55112 USA	Manufacture
Smiths Medical ASD Inc. 201 West Queen St., Southington Connecticut 06489 USA	Manufacture

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:	Service(s) supplied
Smiths Medical ASD Inc. 6250 Shier Rings Road Dublin Ohio 43016 USA	Manufacture
Smiths Medical ASD Inc. 9124 Polk Lane, Suite 101 Olive Branch Mississippi 38654 USA	Distribution
Smiths Medical Czech Republic a.s. Olomoucká 306 753 01 Hranice Czech Republic	Manufacture

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:	Service(s) supplied
Smiths Medical Gary 5700 W 23rd Ave Gary Indiana 46406 USA	Manufacture
Smiths Medical International Ltd 52 Grayhill Rd Cumbernauld Glasgow G68 9HQ United Kingdom	Manufacture
Smiths Medical International Nijmegen Bijsterhuizen 22-08 6604 LD Wijchen The Netherlands	Distribution

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:	Service(s) supplied
Smiths Medical Italia Srl Via della Stazione, 2 Latina Scalo 04100 Italy	Packaging
Sterigenics Belgium (Petit-Rechain) SA Zoning Industriel de Petit-Rechain Avenue Andre Ernst 21 B-4800 Verviers Belgium	ETO Sterilization
Sterigenics UK Limited Cotes Park Estate Somercotes Alfreton DE55 4NJ United Kingdom	ETO Sterilization

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:	Service(s) supplied
Sterigenics US, LLC 344 Bonnie Circle Corona California 92880 USA	Gamma Sterilization
Sterigenics, LLC 1700 College Blvd. West Memphis Arkansas 72301 USA	Gamma Sterilization
Sterilization Services of Tennessee, Inc 2396 Florida Street Memphis Tennessee 38109 USA	ETO Sterilization

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex II excluding Section 4

List of Significant Subcontractors

Recognised as being involved in services relating to the product covered by:

Certificate No: **CE 661325**
 Date: **2017-06-28**
 Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Subcontractor:	Service(s) supplied
STERIS ISOMEDIX Services, Inc 7685 Saint Andrews Avenue San Diego California 92154 USA	ETO Sterilization
UPG Avenida La Cuspide #1 Parque Industrial Tecnomex Del. Playas de Tijuana Tijuana Baja California 22700 Mexico	Manufacture
Velcro USA Inc. 95 Sundial Avenue Manchester New Hampshire 03103-7206 USA	Crucial Supplier

...making excellence a habit.™

EC Certificate - Full Quality Assurance System

Certificate History

Certificate No: **CE 661325**
Date: **2017-06-28**
Issued To: **Smiths Medical International Ltd.**
Boundary Road
Hythe
Kent
CT21 6JL
United Kingdom

Date	Reference Number	Action
Current	8603100 8603169	First issue. Transferred from another Notified Body. Certificate renewal.

...making excellence a habit.™

Page 1 of 1

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body. This approval excludes all products designed and/or manufactured by a third party on behalf of the company named on this certificate, unless specifically agreed with BSI.

This certificate was issued electronically and is bound by the conditions of the contract.