



## Certificate of Conformity

KIT :

Aflatoxin B1 ELISA Kit **RNM98007**

Release Date

Dec 06<sup>th</sup> 2024

Expiration Date:


Dec 05<sup>th</sup> 2025

Temperature:

25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2. 271	2. 254	2. 246	2. 257	0. 013	0. 566	100%
0.02ppb Calibrator	2. 118	2. 112	2. 121	2. 117	0. 005	0. 216	93. 8%
0.06ppb Calibrator	1. 987	1. 931	1. 960	1. 959	0. 028	1. 429	86. 8%
0.2 ppb Calibrator	1. 483	1. 448	1. 498	1. 476	0. 026	1. 738	65. 4%
0.6 ppb Calibrator	0. 856	0. 877	0. 872	0. 868	0. 011	1. 263	38. 5%
1.5 ppb Calibrator	0. 537	0. 516	0. 509	0. 521	0. 015	2. 799	23. 1%

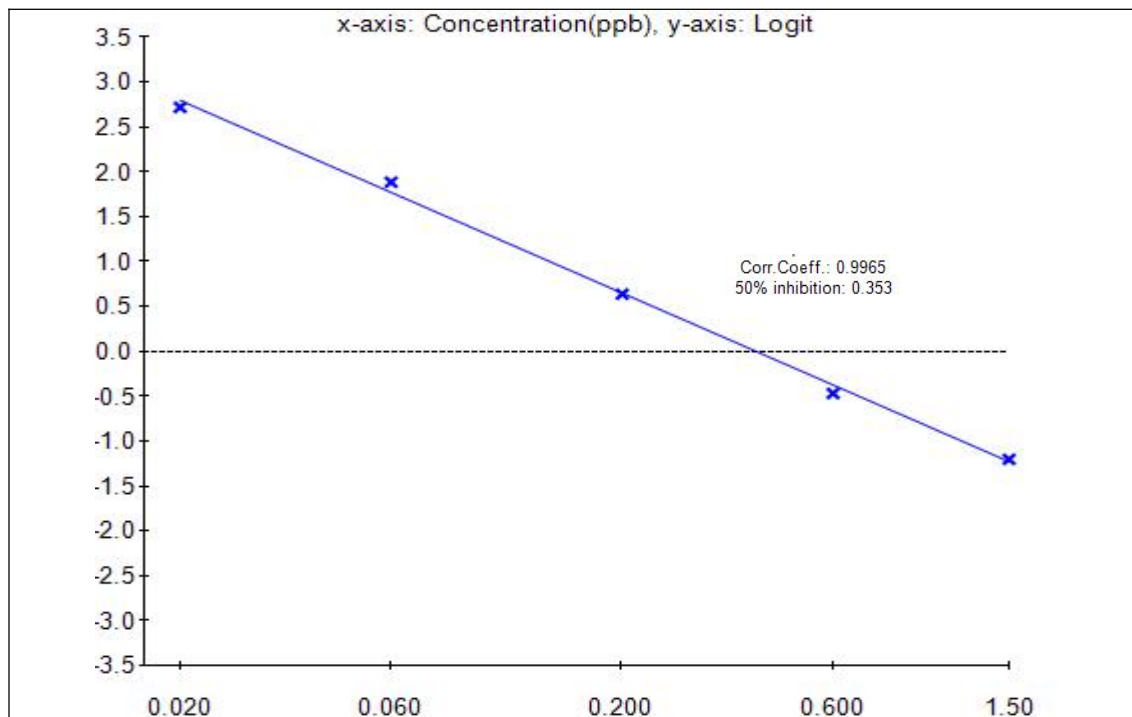

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager

Alexis

Release Date

Dec.06<sup>th</sup> 2024

**REAGEN**