

Revision : 03 / 2022

**Disclaimer :**

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

**Cloxacillin COX 5 mcg****SD075**

Cloxacillin COX 5 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

**Composition**

<b>*Ingredients</b>	<b>Concentration</b>
Cloxacillin	5 mcg/disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

### Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "COX 5" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>S.aureus</i> (25923)	18-30

### Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

### References:

\* Not for Medicinal Use

Revision : 1 / 2012



#### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Amoxycillin AMX 30 mcg

SD076

Amoxycillin AMX 30mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Amoxycillin	30mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.



## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "AMX 30" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E. coli</i> (25922)	19-25
<i>S.aureus</i> (25923)	28-36

## Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)


### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

### Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Netillin (Netilmicin Sulphate)    NET    10 mcg    SD085

Netillin (Netilmicin Sulphate) NET 10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Netillin (Netilmicin Sulphate)	10 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "NET 10" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E. coli</i> (25922)	17-25
<i>S.aureus</i> (25923)	20-29
<i>P.aeruginosa</i> (27853)	13-19

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)


\* Not for Medicinal Use

IVD

In vitro diagnostic medical device


CE

CE Marking




On receipt store at -20°C

Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India

EC REP

CE Partner 4U, Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 02 / 2022

### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

**Nitrofurantoin NIT 100 mcg****SD086**

Nitrofurantoin NIT 100 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

**Composition**

<b>*Ingredients</b>	<b>Concentration</b>
Nitrofurantoin	100 mcg/disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "NIT 100" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E. coli</i> (25922)	17-23
<i>S.aureus</i> (29213)	17-23
<i>E.faecalis</i> (29212)	18-24

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test


For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)


For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For Neisseria spps : G.C.Agar +1% defined growth supplement (M434 + FD025)


\* Not for Medicinal Use



In vitro diagnostic medical device




CE Marking




On receipt store at -20°C

Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India

EC

REP

CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

## Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

**Ofloxacin OF 5 mcg****SD087**

Ofloxacin OF 5 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

**Composition**

*Ingredients	Concentration
Ofloxacin	5 mcg/disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.



### Interpretation:

Use following interpretive criteria for susceptibility categorization\*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Ofloxacin 5 mcg	<i>Enterobacteriaceae</i> , <i>P.aeruginosa</i> , <i>S.pneumoniae</i> , <i>Streptococcus</i> spp. <i>Viridians</i> group, <i>Streptococcus</i> spp. <i>beta haemolytic</i> group	16	13-15	12
	<i>Staphylococcus</i>	18	15-17	14
	<i>Haemophilus influenzae</i> & <i>Haemophilus</i> <i>parainfluenzae</i>	16	-	-
	<i>Neisseria gonorrhoeae</i>	31	25-30	24

### Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "OF 5" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	29-33
<i>S.aureus</i> (25923)	24-28
<i>P.aeruginosa</i> (27853)	17-21

\* = Interpretive criteria & QC ranges as per CLSI standards.

### Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

### References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

\* Not for Medicinal Use





In vitro diagnostic medical device



CE Marking

On receipt store at -20°C



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951  
DB Maam The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 02 / 2022

**Disclaimer :**

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Oxacillin OX 1 mcg

SD088

Oxacillin OX 1 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Oxacillin	1 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

**Interpretation:**

Use following interpretive criteria for susceptibility categorization\*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Oxacillin 1 mcg	<i>Staphylococcus</i>	13	11-12	10
	<i>S.pneumoniae</i>	20	-	-

**Quality Control:**

**Appearance:** Filter paper discs of 6mm diameter with printed "OX 1" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>S.aureus</i> (25923)	18-24

\* = Interpretive criteria & QC ranges as per CLSI standards.

**Storage and Shelf-life:**

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

**References:**

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

**\* Not for Medicinal Use**

In vitro diagnostic medical device



CE Marking



On receipt store at -20°C

Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 02 / 2022

**Disclaimer :**

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.



## Penicillin G P 1 unit

SD089

Penicillin G P 1 unit discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby-Bauer Method

### Composition

Ingredients*	Concentration
Penicillin G	1 unit/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby-Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at  $35 \pm 2^\circ\text{C}$  and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby-Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "P 1" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>S.aureus</i> (29213)	12-18

## Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :


Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

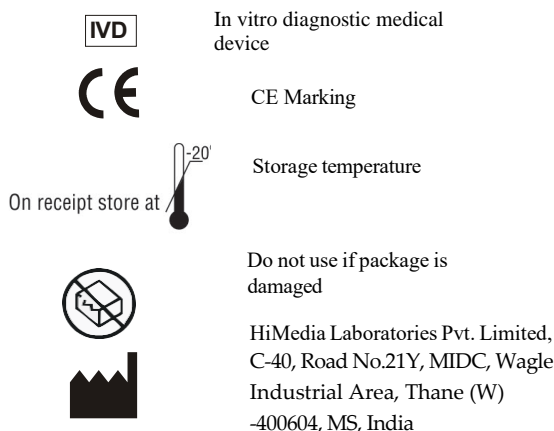

\* Not for Medicinal Use

Disclaimer :

Revision : 02 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Lincomycin L 15 mcg

SD098

Lincomycin L 15 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Lincomycin	15 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "L 15" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>S.aureus</i> (25923)	22-32

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

**\* Not for Medicinal Use**



In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

## Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.



**Ceftriaxone CTR 10 mcg****SD109**

Ceftriaxone CTR 10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby-Bauer Method

**Composition**

<b>*Ingredients</b>	<b>Concentration</b>
Ceftriaxone	10 mcg/disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby-Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "CTR 10" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E. coli</i> (25922)	29-35
<i>S.aureus</i> (25923)	22-28
<i>P.aeruginosa</i> (27853)	17-23

## Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For Neisseria spp : G.C.Agar +1% defined growth supplement (M434 + FD025)

### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



On receipt store at

Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

### Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Amphotericin-B AP 100 units

SD111

Amphotericin-B AP 100 units discs are used for antimicrobial susceptibility testing of fungal cultures

### Composition

*Ingredients	Concentration
Amphotericin-B	100 units/disc

### Susceptibility Test Procedure:

#### Preparation of Inoculum:

1. Inoculum is prepared by picking five distinct colonies of approximately 1mm from 24 hours old culture grown on Sabouraud Dextrose Agar (M063) and incubated at  $35 \pm 2^\circ\text{C}$ . Colonies are suspended in 5ml of sterile 0.85% Saline.
2. Vortex the resulting suspension and adjust the turbidity to yield  $1 \times 10^6$  -  $5 \times 10^6$  cells /ml (i.e. 0.5 McFarland standard).

#### Test Procedure:

1. Prepare plates with Muller Hinton Agar + 2% Glucose + 0.5 mcg/ml Methylene Blue Dye (M1825) for carrying out susceptibility of antifungal discs. The medium in the plates should be sterile and have a depth of about 4 mm.
2. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum (turbidity so adjusted, as to obtain semi confluent growth on the petri plate) and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at  $60^\circ$  angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
3. Apply the discs using aseptic technique. Deposit the discs with centers at least 24 mm apart.
4. Invert the plates and place in an incubator set to  $35 \pm 2^\circ\text{C}$  within 15 minutes after the discs are applied.
5. Examine each plate after 20 - 24 hours of incubation. If plate was satisfactorily streaked the resulting zones of inhibition will be uniformly circular and there will be a semi-confluent lawn of growth. Read at 48 hours only when insufficient growth is observed after 24 hours incubation.

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "AP 100" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Muller Hinton Agar + 2% Glucose + 0.5 mcg/ml Methylene Blue Dye after 24-48 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>C.albicans</i> (90028)*	10-17
<i>C.parapsilosis</i> (22019)*	11-20
<i>C.tropicalis</i> (750)*	8-12
<i>C.krusei</i> (6528)*	9-14
<i>C.albicans</i> (10231)	10-18
<i>S.cerevesiae</i> (9763)	11-18

\* = Q.C. Strains recommended by CLSI

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Method for Antifungal Disk Diffusion Susceptibility Testing of Yeasts; Approved Guidelines-Second edition Vol.29 No.17, August- 2009 CLSI document M44-A2. For more details refer to this volume

**\* Not for Medicinal Use**

Revision : 1 / 2012



### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Ampicillin/Sulbactam A/S 10/10 mcg

SD112

Ampicillin/Sulbactam A/S 10/10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby- Bauer Method

### Composition

Ingredients	Concentration
Ampicillin/Sulbactam	10/10 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby- Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby- Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

**Interpretation:**

Use following interpretive criteria for susceptibility categorization\*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Ampicillin/ Sulbactam 10/10 mcg	<i>Enterobacteriaceae, Acinetobacter</i>	15	12-14	11
	<i>Haemophilus influenzae &amp; Haemophilus parainfluenzae</i>	20	-	19

**Quality Control:**

**Appearance:** Filter paper discs of 6mm diameter with printed "A/S 10/10" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E. coli</i> (25922)	19-24
<i>S. aureus</i> (25923)	29-37
<i>E. coli</i> (35218)	13-19

\* = Interpretive criteria & QC ranges as per CLSI standards & EUCAST standards.

**Storage and Shelf-life:**

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

**References:**

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S. pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C. Agar +1% defined growth supplement (M434 + FD025)

\* **Not for Medicinal Use**



In vitro diagnostic medical device



CE Marking

On receipt store at



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 03 / 2022

**Disclaimer :**



User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.



## Clotrimazole CC 10 mcg

SD115

Clotrimazole CC 10 mcg discs are used for antimicrobial susceptibility testing of fungal cultures

### Composition

*Ingredients	Concentration
Clotrimazole	10 mcg/disc

### Susceptibility Test Procedure:

#### Preparation of Inoculum:

1. Inoculum is prepared by picking five distinct colonies of approximately 1mm from 24 hours old culture grown on Sabouraud Dextrose Agar (M063) and incubated at  $35 \pm 2^\circ\text{C}$ . Colonies are suspended in 5ml of sterile 0.85% Saline.
2. Vortex the resulting suspension and adjust the turbidity to yield  $1 \times 10^6$  -  $5 \times 10^6$  cells /ml (i.e. 0.5 McFarland standard).

#### Test Procedure:

1. Prepare plates with Muller Hinton Agar + 2% Glucose + 0.5 mcg/ml Methylene Blue Dye (M1825) for carrying out susceptibility of antifungal discs. The medium in the plates should be sterile and have a depth of about 4 mm.
2. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum (turbidity so adjusted, as to obtain semi confluent growth on the petri plate) and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at  $60^\circ$  angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
3. Apply the discs using aseptic technique. Deposit the discs with centers at least 24 mm apart.
4. Invert the plates and place in an incubator set to  $35 \pm 2^\circ\text{C}$  within 15 minutes after the discs are applied.
5. Examine each plate after 20 - 24 hours of incubation. If plate was satisfactorily streaked the resulting zones of inhibition will be uniformly circular and there will be a semi-confluent lawn of growth. Read at 48 hours only when insufficient growth is observed after 24 hours incubation.

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "CC 10" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Muller Hinton Agar + 2% Glucose + 0.5 mcg/ml Methylene Blue Dye after 24-48 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>C.albicans</i> (90028)*	18-32
<i>C.parapsilosis</i> (22019)*	16-30
<i>C.tropicalis</i> (750)*	10-20
<i>C.krusei</i> (6528)*	14-24
<i>C.albicans</i> (10231)	12-18
<i>S.cerevesiae</i> (9763)	17-25

\* = Q.C. Strains recommended by CLSI

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Method for Antifungal Disk Diffusion Susceptibility Testing of Yeasts; Approved Guidelines-Second edition Vol.29 No.17, August- 2009 CLSI document M44-A2. For more details refer to this volume

\* Not for Medicinal Use

Revision : 1 / 2012



## Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

**Novobiocin NV 5 mcg****SD121**

Novobiocin NV 5 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby-Bauer Method

**Composition**

<b>*Ingredients</b>	<b>Concentration</b>
Novobiocin	5 mcg/disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby-Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "NV 5" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>S.aureus</i> (25923)	22-31

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

### Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Azithromycin AZM 30 mcg

SD124

Azithromycin AZM 30mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby- Bauer Method

### Composition

*Ingredients	Concentration
Azithromycin	30 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby- Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby- Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "AZM 30" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>S.aureus</i> (25923)	24-30

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For Neisseria spps : G.C.Agar +1% defined growth supplement (M434 + FD025)


### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking


On receipt store at  -20° Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 03 / 2022

### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.





## Roxithromycin RO 30 mcg

## SD126

Roxithromycin RO 30mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Roxithromycin	30mcg /disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.



## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "RO 30" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>S.aureus</i> (25923)	22-30

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, CLSI Vol. 32 No.3, Jan 2012.

\* Not for Medicinal Use

Revision : 1 / 2012



### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

**Vancomycin VA 5 mcg****SD155**

Vancomycin VA 5mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

**Composition**

*Ingredients	Concentration
Vancomycin	5mcg /disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175%barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at  $35 \pm 2^{\circ}\text{C}$  and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "VA 5" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E.faecalis</i> (29212)	15-19
<i>S.pneumoniae</i> (49619)	17-23

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)


**\* Not for Medicinal Use**

IVD

In vitro diagnostic medical device


CE

CE Marking




On receipt store at -20°C

Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India

EC REP

CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 03 / 2022

### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

**Cefaclor CF 30 mcg****SD157**

Cefaclor CF 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method.

**Composition**

<b>*Ingredients</b>	<b>Concentration</b>
Cefaclor	30 mcg/disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Interpretation:

Use following interpretive criteria for susceptibility categorization\*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Cefaclor 30 mcg	<i>Enterobacteriaceae, Staphylococcus</i>	18	15-17	14
	<i>Haemophilus influenzae &amp; Haemophilus parainfluenzae</i>	20	17-19	16

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "CF 30" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	23-27
<i>S.aureus</i> (25923)	27-31

\* = Interpretive criteria & QC ranges as per CLSI standards.

## Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For Neisseria spps : G.C.Agar +1% defined growth supplement (M434 + FD025)


### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

### Disclaimer :

Revision : 02 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Gentamicin GEN 30 mcg

SD170

Gentamicin GEN 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Gentamicin	30 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "GEN 30" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E. faecalis</i> (29212)	12-18

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For Neisseria spps : G.C.Agar +1% defined growth supplement (M434 + FD025)


### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

### Disclaimer :

Revision : 02 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.



## Nitroxoline NO 30 mcg

## SD196

Nitroxoline NO 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Nitroxoline	30 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "NO 30" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E. coli</i> (25922)	18-24

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For Neisseria spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking

On receipt store at -20°C




Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 03 / 2022

### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.



# Technical Data

**Ticarcillin / Clavulanic Acid**

**TCC 75/10 mcg**

**SD201**

Ticarcillin/Clavulanic Acid TCC 75/10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby-Bauer Method

## Composition

### Ingredients

Ticarcillin / Clavulanic Acid

### Concentration

75/10 mcg /disc

## Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby-Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at  $35 \pm 2^\circ\text{C}$  and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

## Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby-Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

**Interpretation:**

Use following interpretive criteria for susceptibility categorization\*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Ticarcillin / Clavulanic Acid 75/10 mcg	<i>Enterobacteriaceae</i> & <i>Acinetobacter</i>	20	15-19	14
	<i>P.aeruginosa</i>	24	16-23	15
	<i>Staphylococcus</i> spp.	23	-	22

**Quality Control:**

**Appearance:** Filter paper discs of 6mm diameter with printed "TCC 75/10" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	24-30
<i>S.aureus</i> (25923)	29-37
<i>P.aeruginosa</i> (27853)	20-28

\* = Interpretive criteria & QC ranges as per CLSI & EUCAST standards.

**Storage and Shelf-life:**

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

**References:**

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

\* Not for Medicinal Use

IVD

In vitro diagnostic medical device



CE Marking

On receipt store at -20°C



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India

EC REP

CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

**Disclaimer :**

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

## Fosfomycin

## FO 200 mcg

## SD205

Fosfomycin FO 200 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby-Bauer Method.

### Composition

Ingredients	Concentration
Fosfomycin	200 mcg/disc
Glucose -6-phosphate	50mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

## Interpretation:

Use following interpretive criteria for susceptibility categorization\*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Fosfomycin 200 mcg	<i>Enterobacterales</i> , <i>Enterococcus spp.</i>	16	13-15	12

## Quality Control:

**Appearance:** Filter paper discs of 6mm diameter with printed "FO 200" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	22-30
<i>S.aureus</i> (25923)	25-33

\* = Interpretive criteria & QC ranges as per CLSI standards.

## Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

## References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)


### \* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 03 / 2022



### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.



## Aztreonam AT 30 mcg

## SD212

Aztreonam AT 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

### Composition

*Ingredients	Concentration
Aztreonam	30 mcg/disc

### Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

### Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

**Interpretation:**

Use following interpretive criteria for susceptibility categorization\*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Aztreonam 30 mcg	<i>Enterobacteriaceae</i>	21	18-20	17
	<i>P.aeruginosa</i>	22	16-21	15
	<i>Haemophilus influenzae</i> & <i>Haemophilus parainfluenzae</i>	26	-	-

**Quality Control:**

**Appearance:** Filter paper discs of 6mm diameter with printed "AT 30" on centre of each side of the disc.

**Cultural response:** Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	28-36
<i>P.aeruginosa</i> (27853)	23-29
<i>E.coli</i> (35218)	31-38
<i>K.pneumoniae</i> (700603)	10-16

\* = Interpretive criteria & QC ranges as per CLSI standards.

**Storage and Shelf-life:**

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

**References:**

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

IVD

In vitro diagnostic medical device



CE Marking

On receipt store at



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,  
C-40, Road No.21Y, MIDC, Wagle  
Industrial Area, Thane (W)  
-400604, MS, India

EC REP

CE Partner 4U ,Esdoornlaan 13, 3951  
DB Maarn The Netherlands,  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Revision : 03 / 2022

**Disclaimer :**

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

**Teicoplanin****TEI 30 mcg****SD213**

Teicoplanin TEI 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

**Composition**

<b>*Ingredients</b>	<b>Concentration</b>
Teicoplanin	30 mcg /disc

**Susceptibility Test Procedure:**

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175%barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

**Principle:**

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.