ACESO laboratories inc.

ACESO Technical File

Multi-Drug Test Specimen: Urine REF: UX4-MDT/UX4-MDTA

Document No.: RA-450

Version: A

Prepared by: Eric Li

Date: 2022.01.17

Reviewed by: Tommy Shen

Date: 2022.01.17

Table of Contents

1 Background 2
1.1 Product Name 2
1.2 Intended Use 2
1.3 Background 5
1.4 Principles 21
1.4.1 Principles (For DOA Tests Excluding Alcohol) 21
1.4.2 Principle (For Alcohol) 21
1.5 Performance and Specification 21
1.6 Composition of Product 25
1.7 Manufacturing Procedure 25
1.8 User 25
1.9 Classification of Product 25
1.10 Product Certification Conformity Assessment Route 25
1.11 Bibliography 25
2 Performance characteristics 28
2.1 Sample correlation 28
2.2 Analytical Sensitivity 34
2.3 Analytical Specificity 55
2.4 Cross Reactivity 133
2.5 Between Day Reproducibility 133
2.6 Between Lot Reproducibility (lot to lot variability) 173
2.7 Accelerated Stability 201
2.8 Precision 421
2.9 Effect of Urinary Specific Gravity 450
2.10 Effect of Urinary pH 495
2.11 Open Pouch Stability 528
Document History Summary 593

1 Background

1.1 Product Name

Multi-Drug Test Dip Card with/without Adulteration.

1.2 Intended Use

The Multi-Drug Test Dip Card with/without Adulteration is a rapid chromatographic immunoassay for the detection of drugs and drug metabolites in urine at the following cut-off concentrations in urine:

Test	Calibrator	Cut-off (ng/mL)
Amphetamine (AMP 1000)	d-Amphetamine	1,000
Amphetamine (AMP 500)	d-Amphetamine	500
Amphetamine (AMP 300)	d-Amphetamine	300
Barbiturates (BAR 300)	Secobarbital	300
Barbiturates (BAR 200)	Secobarbital	200
Benzodiazepines (BZO 500)	Oxazepam	500
Benzodiazepines (BZO 300)	Oxazepam	300
Benzodiazepines (BZO 200)	Oxazepam	200
Benzodiazepines (BZO 100)	Oxazepam	100
Buprenorphine (BUP 10)	Buprenorphine	10
Buprenorphine (BUP 5)	Buprenorphine	5
Cocaine (COC 300)	Benzoylecgonine	300
Cocaine (COC200)	Benzoylecgonine	200
Cocaine (COC 100)	Benzoylecgonine	100
Cocaine (COC 150)	Benzoylecgonine	150
Marijuana (THC 150)	11-nor-Δ9THC-9 COOH	150
Marijuana (THC 50)	11-nor-Δ9THC-9 COOH	50
Marijuana (THC 25)	11-nor-Δ9THC-9 COOH	25
Marijuana (THC 300)	11-nor-Δ9THC-9 COOH	300
Marijuana (THC 200)	11-nor-Δ9THC-9 COOH	200
Marijuana (THC 30)	11-nor-Δ9THC-9 COOH	30
Marijuana (THC 20)	11-nor-Δ9THC-9 COOH	20
Methadone (MTD 300)	Methadone	300
Methadone (MTD 200)	Methadone	200
Methamphetamine (MET 1,000)	d-Methamphetamine	1,000
Methamphetamine (MET 500)	d-Methamphetamine	500
Methamphetamine (MET 300)	d-Methamphetamine	300
Methamphetamine (MET 200)	d-Methamphetamine	200
Methylenedioxymethamphetamine (MDMA 300)	d,l-Methylenedioxymethamphetamine	300
Methylenedioxymethamphetamine (MDMA 500)	d,l-Methylenedioxymethamphetamine	500
Methylenedioxymethamphetamine (MDMA 1000)	d,l-Methylenedioxymethamphetamine	1000
Morphine (MOP 300)	Morphine	300

Morphine (MOP 200)	Morphine	200
Morphine (MOP 100)	Morphine	100
Opiate (OPI 2000)	Morphine	2,000
Methaqualone(MQL)	Methaqualone	300
Phencyclidine (PCP)	Phencyclidine	25
Propoxyphene (PPX)	Propoxyphene	300

Tricyclic Antidepressants (TCA1000)	Nortriptyline	1,000
Tricyclic Antidepressants (TCA500)	Nortriptyline	500
Tramadol (TML 100)	Tramadol	100
Tramadol (TML 200)	Tramadol	200
Tramadol (TML300)	Tramadol	300
Ketamine (KET 1,000)	Ketamine	1,000
Ketamine (KET 500)	Ketamine	500
Ketamine (KET 300)	Ketamine	300
Ketamine (KET 100)	Ketamine	100
Oxycodone (OXY)	Oxycodone	100
Oxycodone (OXY300)	Oxycodone	300
Cotinine(COT 200)	Cotinine	200
Cotinine(COT 100)	Cotinine	100
2-ethylidene-1,5-dimethyl-3,3-diphenylpyrrolidine (EDDP 300)	2-ethylidene-1,5-dimethyl-3,3-diphenyl pyrrolidine	300
2-ethylidene-1,5-dimethyl-3,3-diphenylpyrrolidine (EDDP 100)	2-ethylidene-1,5-dimethyl-3,3-diphenyl pyrrolidine	100
Fentanyl(FYL20)	Norfentanyl	20
Fentanyl(FYL10)	Norfentanyl	10
Synthetic Marijuana(K2 50)	JWH -018, JWH- 073	50
Synthetic Marijuana(K2 30)	JWH -018, JWH- 073	30
Synthetic Marijuana(K2 25)	JWH -018, JWH- 073	25
6-mono-aceto-morphine (6-MAM)	6-mono-aceto-morphine	10
Clonazepam (CLO400)	Clonazepam	400
Clonazepam (CLO150)	Clonazepam	150
Ethyl Glucuronide(ETG500)	Ethyl Glucuronide	500
Ethyl Glucuronide(ETG1000)	Ethyl Glucuronide	1000
ACE (Acetaminophen)	Acetaminophen	5000
LSD 20 (Lysergic Acid Diethylamide)	Lysergic Acid Diethylamide	20
LSD 50 (Lysergic Acid Diethylamide)	Lysergic Acid Diethylamide	50
MDA(3,4-Methylenedioxyamphetamine)	3,4-Methylenedioxyamphetamine	500
MDPV (3, 4-methylenedioxypyrovalerone)	3, 4-methylenedioxypyrovalerone	1000
MPD300(Methylphenidate)	Methylphenidate	300
Zolpidem (ZOL)	Zolpidem	50
Diazepam(DIA300)	Diazepam	300
Diazepam(DIA 200)	Diazepam	200
Mephedrone	Mephedrone	100
Carfentanyl(CFYL500)	Carfentanyl	500
Zopiclone（ZOP 50）	Zopiclone	50
Caffeine(CAF)	Caffeine	1000
Cathine (CAT)	(+)-Norpseudoephedrine	150
Tropicamide(TRO)	Tropicamide	350

7-Aminoclonazepam(7-ACL)	7-Aminoclonazepam	300/200/100
Alprazolam(ALP)	Alprazolam	100
AB-PINACA (ABP)	AB-PINACA	10
α-Pyrrolidinovalerophenone (α-PVP)	α-Pyrrolidinovalerophenone	1,000/500
Cannabinol (CNB)	Cannabinol	500
Meperidine (MPRD)	Meperidine	100
Pregabalin (PGB)	Pregabalin	50,000
Trazodone(TZD)	Trazodone	200
UR-144	UR-144 5-Pentanoic acid	25
Zaleplon(ZAL)	Zaleplon	100
Mescaline (MES)	Mescaline	100
Gabapentin(GAB)	Gabapentin	2,000
Tilidine(TLD)	Nortilidine	50
Quetiapine(QTP)	Quetiapine	1,000
Papaverine(PAP)	Papaverine	500
Kratom(KRA)	Mitragynine	300
Carisoprodol(CAR)	Carisoprodol	2,000
Fluoxetine(FLX)	Fluoxetine	500
Hydromorphone(HMO)	Hydromorphone	250/300
Olanzapine(OZP)	Olanzapine	1000

Configurations of the Multi-Drug Test Dip Card with/without Adulteration come with any combination of the above listed drug analytes with or without S.V.T (Oxidants/PCC, Specific Gravity, pH, Nitrite, Glutaraldehyde, Creatinine and Bleach)**.** This assay provides only a preliminary analytical test result. A more specific alternate chemical method must be used in order to obtain a confirmed analytical result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method. Clinical consideration and professional judgment should be applied to any drug of abuse test result, particularly when preliminary positive results are indicated.

1.3 Background

The Multi-Drug Test Dip Card with/without Adulteration is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes monoclonal antibodies to selectively detect elevated levels of specific drugs in urine.

1.3.1 Amphetamine

Amphetamine is a Schedule II controlled substance available by prescription (Dexedrine®) and is also available on the illicit market. Amphetamines are a class of potent sympathomimetic agents with therapeutic applications. They are chemically related to the human body's natural catecholamines: epinephrine and norepinephrine. Acute higher doses lead to enhanced stimulation of the central nervous system (CNS) and induce euphoria, alertness, reduced appetite, and a sense of increased energy and power. Cardiovascular responses to amphetamines include increased blood pressure and cardiac arrhythmias. More acute responses produce anxiety, paranoia, hallucinations, and psychotic behavior. The effects of Amphetamines generally last 2-4 hours following use and the drug has a half-life of 4-24 hours in the body. About 30% of amphetamines are excreted in the urine in unchanged form, with the remainder as hydroxylated and deaminated derivatives.

1.3.2 Barbiturates

Barbiturates are CNS depressants. They are used therapeutically as sedatives, hypnotics, and anticonvulsants barbiturates are almost always taken orally as capsules or tablets. The effects resemble those of intoxication with alcohol. Chronic use of barbiturates leads to tolerance and physical dependence.

Short-acting barbiturates taken at 400 mg/day for 2-3 months can produce a clinically significant degree of physical dependence. Withdrawal symptoms experienced during periods of drug abstinence can be severe enough to cause death.

Only a small amount (less than 5%) of most barbiturates are excreted unaltered in the urine. The approximate detection time limits for barbiturates are:

Short acting (e.g. Secobarbital)	100 mg PO (oral)	4.5 days
Long acting (e.g. Phenobarbital)	400 mg PO (oral)	7 days

1.3.3 Benzodiazepines

Benzodiazepines are medications that are frequently prescribed for the symptomatic treatment of anxiety and sleep disorders. They produce their effects via specific receptors involving a neurochemical called gamma aminobutyric acid (GABA). Because they are safer and more effective, Benzodiazepines have replaced Barbiturates in the treatment of both anxiety and insomnia. Benzodiazepines are also used as sedatives before some surgical and medical procedures, and for the treatment of seizure disorders and alcohol withdrawal.

Risk of physical dependence increases if Benzodiazepines are taken regularly (e.g., daily) for more than a few months, especially at higher than normal doses. Stopping abruptly can bring on such symptoms as trouble sleeping, gastrointestinal upset, feeling unwell, loss of appetite, sweating, trembling, weakness, anxiety and changes in perception. Only trace amounts (less than 1%) of most Benzodiazepines are excreted unaltered in the urine; most of the concentration in urine is conjugated drug. The detection period for the Benzodiazepines in the urine is 3-7 days.

1.3.4 Buprenorphine

Buprenorphine is a potent analgesic often used in the treatment of opioid addiction. The drug is sold under the trade names Subutex™, Buprenex™, Temgesic™ and Suboxone™, which contain Buprenorphine HCl alone or in combination with Naloxone HCl. Therapeutically, Buprenorphine is used as a substitution treatment for opioid addicts. Substitution treatment is a form of medical care offered to opiate addicts (primarily heroin addicts) based on a similar or identical substance to the drug normally used. In substitution therapy, Buprenorphine is as effective as Methadone but demonstrates a lower level of physical dependence. Concentrations of free Buprenorphine and Norbuprenorphine in urine may be less than 1 ng/ml after therapeutic administration, but can range up to 20 ng/ml in abuse situations. The plasma half life of Buprenorphine is 2-4 hours. While complete elimination of a single dose of the drug can take as long as 6 days, the window of detection for the parent drug in urine is thought to be approximately 3 days.

Substantial abuse of Buprenorphine has also been reported in many countries where various forms of the drug are available. The drug has been diverted from legitimate channels through theft, doctor shopping, and fraudulent prescriptions, and been abused via intravenous, sublingual, intranasal and inhalation routes.

1.3.5 Cocaine

Cocaine is a potent central nervous system stimulant and a local anesthetic. Initially, it brings about extreme energy and restlessness while gradually resulting in tremors, over-sensitivity and spasms. In large amounts, cocaine causes fever, unresponsiveness, difficulty in breathing and unconsciousness. Cocaine is often self-administered by nasal inhalation, intravenous injection and free-base smoking. It is excreted in the urine in a short time primarily as benzoylecgonine. Benzoylecgonine, a major metabolite of cocaine, has a longer biological half-life (5-8 hours) than cocaine (0.5-1.5 hours), and can generally be detected for 24-48 hours after cocaine exposure.

1.3.6 Marijuana

THC (9-petrahydrocannabinol) is the primary active ingredient in cannabis (marijuana). When smoked or orally administered, THC produces euphoric effects. Users have impaired shortperm memory and slowed learning. They may also experience transient episodes of confusion and anxiety. Longperm, relatively heavy use may be associated with behavioral disorders. The peak effect of marijuana administered by smoking occurs in 20-30 minutes and the duration is 90-120 minutes after one cigarette. Elevated levels of urinary metabolites are found within hours of exposure and remain detectable for 3-10 days after smoking. The main metabolite excreted in the urine is 11-nor- 9petrahydrocannabinol-9-carboxylic acid (THC-COOH).

1.3.7 Methadone

Methadone is a narcotic analgesic prescribed for the management of moderate to severe pain and for the treatment of opiate dependence (heroin, Vicodin, Percocet, morphine). The pharmacology of oral methadone is very different from IV methadone. Oral methadone is partially stored in the liver for later use. IV methadone acts more like heroin. In most states you must go to a pain clinic or a methadone maintenance clinic to be prescribed methadone.

Methadone is a long acting pain reliever producing effects that last from twelve to forty-eight hours. Ideally, methadone frees the client from the pressures of obtaining illegal heroin, from the dangers of injection, and from the emotional roller coaster that most opiates produce. Methadone, if taken for long periods and at large doses, can lead to a very long withdrawal period. The withdrawals from methadone are more prolonged and troublesome than those provoked by heroin cessation, yet the substitution and phased removal of methadone is an acceptable method of detoxification for patients and therapists.

1.3.8 Methamphetamine

Methamphetamine is an addictive stimulant drug that strongly activates certain systems in the brain. Methamphetamine is closely related chemically to Amphetamine, but the central nervous system effects of Methamphetamine are greater. Methamphetamine is made in illegal laboratories and has a high potential for abuse and dependence. The drug can be taken orally, injected, or inhaled. Acute higher doses lead to enhanced stimulation of the central nervous system and induce euphoria, alertness, reduced appetite, and a sense of increased energy and power. Cardiovascular responses to Methamphetamine include increased blood pressure and cardiac arrhythmias. More acute responses produce anxiety, paranoia, hallucinations, psychotic behavior, and eventually, depression and exhaustion.

The effects of Methamphetamine generally last 2-4 hours and the drug have a half-life of 9-24 hours in the body. Methamphetamine is excreted in the urine primarily as Amphetamine, and oxidized and deaminated derivatives. However, 10-20% of Methamphetamine is excreted unchanged. Thus, the presence of the parent compound in the urine indicates Methamphetamine use. Methamphetamine is generally detectable in the urine for 3-5 days, depending on urine pH level.

1.3.9 Methylenedioxymethamphetamine

Methylenedioxymethamphetamine (ecstasy) is a designer drug first synthesized in 1914 by a German drug company for the treatment of obesity. Those who take the drug frequently report adverse effects, such as increased muscle tension and sweating. MDMA is not clearly a stimulant, although it has, in common with amphetamine drugs, a capacity to increase blood pressure and heart rate. MDMA does produce some perceptual changes in the form of increased sensitivity to light, difficulty in focusing, and blurred vision in some users. Its mechanism of action is thought to be via release of the neurotransmitter serotonin. MDMA may also release dopamine, although the general opinion is that this is a secondary effect of the drug (Nichols and Oberlender, 1990). The most pervasive effect of MDMA, occurring in virtually all people who took a reasonable dose of the drug, was to produce a clenching of the jaws.

1.3.10 Morphine/Opiate

Morphine/Opiate refers to any drug that is derived from the opium poppy, including the natural products, morphine and codeine, and the semi-synthetic drugs such as heroin. Morphine/Opiate is more general, referring to any drug that acts on the opioid receptor.

Opioid analgesics comprise a large group of substances which control pain by depressing the CNS. Large doses of morphine can produce higher tolerance levels, physiological dependency in users, and may lead to substance abuse. Morphine is excreted unmetabolized, and is also the major metabolic product of codeine and heroin. Morphine is detectable in the urine for several days after an opiate dose.

1.3.11 Phencyclidine

Phencyclidine, also known as PCP or Angel Dust, is a hallucinogen that was first marketed as a surgical anesthetic in the 1950's. It was removed from the market because patients receiving it became delirious

and experienced hallucinations.

PCP is used in powder, capsule, and tablet form. The powder is either snorted or smoked after mixing it with marijuana or vegetable matter. PCP is most commonly administered by inhalation but can be used intravenously, intra-nasally, and orally. After low doses, the user thinks and acts swiftly and experiences mood swings from euphoria to depression. Self-injurious behavior is one of the devastating effects of PCP.

PCP can be found in urine within 4 to 6 hours after use and will remain in urine for 7 to 14 days, depending on factors such as metabolic rate, user's age, weight, activity, and diet.6 PCP is excreted in the urine as an unchanged drug (4% to 19%) and conjugated metabolites (25% to 30%).6

1.3.12 Propoxyphene

Propoxyphene (PPX) is a narcotic analgesic compound bearing structural similarity to methadone. As an analgesic, propoxyphene can be from 50-75% as potent as oral codeine. Darvocet™, one of the most common brand names for the drug, contains 50-100 mg of propoxyphene napsylate and 325-650 mg of acetaminophen. Peak plasma concentrations of propoxyphene are achieved from 1 to **2** hours post dose. In the case of overdose, propoxyphene blood concentrations can reach significantly higher levels.

In humans, propoxyphene is metabolized by N-demethylation to yield norpropoxyphene. Norpropoxyphene has a longer half-life (30 to 36 hours) than parent propoxyphene (6 to 12 hours). The accumulation of norpropoxyphene seen with repeated doses may be largely responsible for resultant toxicity.

2.1.1 Tricyclic Antidepressants

TCA (Tricyclic Antidepressants) are commonly used for the treatment of depressive disorders. TCA overdoses can result in profound CNS depression, cardiotoxicity and anticholinergic effects. TCA overdose is the most common cause of death from prescription drugs. TCAs are taken orally or sometimes by injection. TCAs are metabolized in the liver. Both TCAs and their metabolites are excreted in urine mostly in the form of metabolites for up to ten days.

2.1.2 Tramadol

Tramadol(TML) is a quasi-narcotic analgesic used in the treatment of moderate to severe pain. It is a synthetic analog of codeine, but has a low binding affinity to the mu-opioid receptors. Large doses of tramadol can develop tolerance and physiological dependency and lead to its abuse. Tramadol is extensively metabolized after oral administration. Approximately 30% of the dose is excreted in the urine as unchanged drug, whereas 60% is excreted as metabolites. The major pathways appear to be N- and O- demethylation, glucoronidation or sulfation in the liver.

2.1.3 Ketamine

Ketamine is a dissociative anesthetic developed in 1963 to replace PCP (Phencyclidine). While Ketamine is still used in human anesthesia and veterinary medicine, it is becoming increasingly abused as a street drug. Ketamine is molecularly similar to PCP and thus creates similar effects including numbness, loss of coordination, sense of invulnerability, muscle rigidity, aggressive / violent behavior, slurred or blocked speech, exaggerated sense of strength, and a blank stare. There is depression of respiratory function but not of the central nervous system, and cardiovascular function is maintained. The effects of Ketamine generally last 4-6 hours following use. Ketamine is excreted in the urine as unchanged drug (2.3%) and metabolites (96.8%).

2.1.4 Methaqualone

Methaqualone(Quaalude,Sopor) is a quinazoline derivative that was first synthesized in 1951 and found clinically effective as a sedative and hypnotic in 1956. It soon gained popularity as a drug of abuse and in 1984 was removed from the US market due to extensive misuse. It is occasionally encountered in illicit form, and is also available in Europeon countries in combination with diphenhydramine (Mandrax). Methaqualone is extensively metabolized in vivo principally by hydroxylation at every possible position on the molecule. At least 12 metabolites have been identified in the urine.

1.3.17 Oxycodone

Oxycodone is a semi-synthetic opioid with a structural similarity to codeine. The drug is manufactured by modifying thebaine, an alkaloid found in the opium poppy. Oxycodone, like all opiate agonists, provides pain relief by acting on opioid receptors in the spinal cord, brain, and possibly directly in the affected tissues. Oxycodone is prescribed for the relief of moderate to high pain under the well-known pharmaceutical trade names of OxyContin®, Tylox®, Percodan® and Percocet®. While Tylox®, Percodan® and Percocet® contain only small doses of oxycodone hydrochloride combined with other analgesics such as acetaminophen or aspirin, OxyContin consists solely of oxycodone hydrochloride in a time-release form. Oxycodone is known to metabolize by demethylation into oxymorphone and noroxycodone. In a 24-hour urine, 33-61% of a single, 5 mg oral dose is excreted with the primary constituents being unchanged drug (13-19%), conjugated drug (7-29%) and conjugated oxymorphone (13-14%). The window of detection for Oxycodone in urine is expected to be similar to that of other opioids such as morphine.

1.3.182-ethylidene-1,5-dimethyl-3,3-diphenylpyrrolidine

Methadone is an unusual drug in that its primary urinary metabolites (EDDP and EMDP) are cyclic in structure, making them very difficult to detect using immunoassays targeted to the native compound. Exacerbating this problem, there is a subsection of the population classified as “extensive metabolizers” of methadone. In these individuals, a urine specimen may not contain enough parent methadone to yield a positive drug screen even if the individual is in compliance with their methadone maintenance. EDDP represents a better urine marker for methadone maintenance than unmetabolized methadone.

1.3.19 Cotinine

Cotinine is the first-stage metabolite of nicotine, a toxic alkaloid that produces stimulation of the autonomic ganglia and central nervous system when in humans. Nicotine is a drug to which virtually every member of a tobacco-smoking society is exposed whether through direct contact or second-hand inhalation. In addition to tobacco, nicotine is also commercially available as the active ingredient in smoking replacement therapies such as nicotine gum, transdermal patches and nasal sprays.

In a 24-hour urine, approximately 5% of a nicotine dose is excreted as unchanged drug with 10% as cotinine and 35% as hydroxycotinine; the concentrations of other metabolites are believed to account for less than 5%. While cotinine is thought to be an inactive metabolite, it’s elimination profile is more stable than that of nicotine which is largely urine pH dependent. As a result, cotinine is considered a good biological marker for determining nicotine use. The plasma half-life of nicotine is approximately 60 minutes following inhalation or parenteral administration. Nicotine and cotinine are rapidly eliminated by the kidney; the window of detection for cotinine in urine at a cutoff level of 200 ng/mL is expected to be up to 2-3 days after nicotine use.

1.3.20 Fentanyl

Fentanyl, belongs to powerful narcotics analgesics, and is a μ special opiates receptor stimulant. Fentanyl is one of the varieties that been listed in management of United Nations “Single Convention of narcotic drug in 1961”. Among the opiates agents that under international control, Fentanyl is one of the most commonly used to cure moderate to severe pain. After continuous injection of fentanyl, the sufferer will have the performance of protracted opioid abstinence syndrome, such as ataxia and irritability etc, which presents the addiction after taking fentanyl in a long time. Compared with drug addicts of amphetamine, drug addicts who take fentanyl mainly have got the possibility of higher infection rate of HIV, more dangerous injection behavior and more lifelong medication overdose.

1.3.21 Synthetic Marijuana (K2)

Synthetic Marijuana or K2 a psychoactive herbal and chemical product that, when consumed, mimics the effects of Marijuana. It is best known by the brand names K2 and Spice, both of which have largely become genericized trademarks used to refer to any synthetic Marijuana product. The studies suggest that synthetic marijuana intoxication is associated with acute psychosis, worsening of previously stable psychotic disorders, and also may have the ability to trigger a chronic (longperm) psychotic disorder among vulnerable individuals such as those with a family history of mental illness. Elevated levels of urinary metabolites are found within hours of exposure and remain detectable for 72 hours after

smoking (depending on usage/dosage).
As of March 1, 2011, five cannabinoids, JWH -018, JWH- 073, CP- 47, JWH- 200 and cannabicyclohexanol are now illegal in the US because these substances have the potential to be extremely harmful and, therefore, pose an imminent hazard to the public safety.

1.3.22 6-mono-aceto-morphine

6-Monoacetylmorphine (6-MAM) or 6-acetylmorphine (6-AM) is one of three active metabolites of heroin (diacetylmorphine), the others being morphine and the much less active 3-monoacetylmorphine (3-MAM). 6-MAM is rapidly created from heroin in the body, and then is either metabolized into morphine and excreted in the urine. 6-MAM remains in the urine for no more than 24 hours. The presence of 6-MAM guarantees that heroin was in fact used as recently as within the last day. 6-MAM is naturally found in the brain, but in such small quantities that detection of this compound in urine virtually guarantees that heroin has recently been consumed.

1.3.23 Clonazepam

Clonazepam is a benzodiazepine drug having anxiolytic, anticonvulsant, muscle relaxant, amnestic, sedative, and hypnotic properties. Clonazepam has an intermediate onset of action, with a peak blood level occurring one to four hours after oral administration. Longperm effects of benzodiazepines include tolerance, benzodiazepine dependence, and benzodiazepine withdrawal syndrome, which occurs in one third of patients treated with clonazepam for longer than four weeks. Benzodiazepines such as clonazepam have a fast onset of action, high effectivity rate, and low toxicity in overdose; however, as with most medications, it may have drawbacks due to adverse or paradoxicaleffects.The detection period for the Benzodiazepines in the urine is 3-7 days.

1.3.24 Diazepam

Diazepam (DIA) is a medication of the benzodiazepine family that typically produces a calming effect. It has anticonvulsant properties. Diazepam has no effect on GABA levels and no effect on glutamate decarboxylase activity, but has a slight effect on gamma-amino butyric acid transaminase activity. Diazepam can be administered orally, intravenously intramuscularly (IM), or as a suppository. When administered orally, it is rapidly absorbed and has a fast onset of action. The onset of action is one to five minutes for IV administration and 15–30 minutes for IM administration. The duration of diazepam's peak pharmacological effects is 15 minutes to one hour for both routes of administration. The bioavailability after oral administration is 100% and 90% after rectal administration. Peak plasma levels occur between 30 and 90 minutes after oral administration and between 30 and 60 minutes after intramuscular administration; after rectal administration, peak plasma levels occur after 10 to 45 minutes. Diazepam is highly protein-bound, with 96 to 99% of the absorbed drug being protein-bound. The distribution half-life of diazepam is 2 to 13 minutes. When diazepam is administered IM, absorption is slow, erratic, and incomplete.

1.3.25 Ethyl Glucuronide

Ethyl Glucuronide (ETG) is a metabolite of ethyl alcohol which is formed in the body by glucuronidation following exposure to ethanol, such as by drinking alcoholic beverages. It is used as a biomarker to test for ethanol use and to monitor alcohol abstinence in situations where drinking is prohibited, such as in the military, in professional monitoring programs (health professionals, attorneys, airline pilots in recovery from addictions), in schools, in liver transplant clinics, or in recovering alcoholic patients. ETG can be measured in urine up to approximately 80 hours after ethanol is ingested. ETG is a more accurate indicator of the recent exposure to alcohol than measuring for the presence of ethanol itself.

1.3.26 Acetaminophen

Acetaminophen (ACE) is one of the most commonly used drugs, yet it is also an important cause of serious liver injury. Acetaminophen is the generic name of a drug found in many common brand name over-the-counter (OTC) products, such as Tylenol, and Prescription (Rx) products, such as Vicodin and Percocet. Acetaminophen is an important drug, and its effectiveness in relieving pain and fever is widely known. Unlike other commonly used drugs to reduce pain and fever (e.g., nonsteroidalantinflammatory

drugs (NSAIDs), such as aspirin, ibuprofen, and naproxen), at recommended doses acetaminophen does not cause adverse effects, such as stomach discomfort and bleeding, and acetaminophen is considered safe when used according to the directions on its OTC or Rx labeling. However, taking more than the recommended amount can cause liver damage, ranging from abnormalities in liver function blood tests, to acute liver failure, and even death. Many cases of overdose are caused by patients inadvertently taking more than the recommended dose (i.e., 4 grams a day) of a particular product, or by taking more than one product containing acetaminophen (e.g., an OTC product and an Rx drug containing acetaminophen). The mechanism of liver injury is not related to acetaminophen itself, but to the production of a toxic metabolite. The toxic metabolite binds with liver proteins, which cause cellular injury. The ability of the liver to remove this metabolite before it binds to liver protein influences the extent of liver injury.

1.3.27 Lysergic Acid Diethylamide

Lysergic acid diethylamide (LSD) is a white powder or a clear, colorless liquid. LSD is manufactured from lysergic acid which occurs naturally in the ergot fungus that grows on wheat and rye. It is a Schedule I controlled substance, available in liquid, powder, tablet (microdots), and capsule form. LSD is recreationally used as a hallucinogen for its ability to alter human perception and mood. LSD is primarily used by oral administration, but can be inhaled, injected, and transdermally applied. LSD is a non-selective 5-HT agonist, may exert its hallucinogenic effect by interacting with 5-HT 2Areceptors as a partial agonist and modulating the NMDA receptor-mediated sensory, perceptual, affective and cognitive processes. LSD mimics 5-HT at 5-HT 1A receptors, producing a marked slowing of the firing rate of serotonergic neurons. LSD has a plasma half-life of 2.5-4 hours. Metabolites of LSD include N-desmethyl-LSD, hydroxy-LSD, 2-oxo-LSD, and 2-oxo-3-hydroxy-LSD .These metabolites are all inactive. LSD use can typically be detected in urine for periods of 2-5 days.

1.3.28 3,4-Methylenedioxyamphetamine

3,4-Methylenedioxyamphetamine (MDA), also known as tenamfetamine (INN), or with the street name "Sally" or "Sass" or "Sass-a-frass", is a psychedelic and entactogenic drug of the phenethylamine and amphetamine chemical classes. It is mainly used as a recreational drug, an entheogen, and a tool in use to supplement various types of practices for transcendence, including in meditation, psychonautics, and as an agent in psychedelic psychotherapy. It was first synthesized by
G. Mannish and W. Jacobson in 1910. There are about 20 different synthetic routes described in the literature for its preparation.

1.3.29 3, 4-methylenedioxypyrovalerone

3, 4-methylenedioxypyrovalerone (MDPV) is a psychoactive recreational drug with stimulant properties which acts as a norepinephrine-dopamine reuptake inhibitor (NDRI). It was first developed in the 1960s by a team at BoehringerIngelheim. MDPV remained an obscure stimulant until around 2004 when it was reportedly sold as a designer drug. Products labeled as bath salts containing MDPV were previously sold as recreational drugs in gas stations and convenience stores in the United States, similar to the marketing for Spice and K2 as incense.

MDPV is the 3,4-methylenedioxy ring-substituted analog of the compound pyrovalerone, developed in the 1960s, which has been used for the treatment of chronic fatigue and as an anorectic, but caused problems of abuse and dependence. However, despite its structural similarity, the effects of MDPV bear little resemblance to other methylenedioxyphenylalkylamine derivatives such as 3,4-methylenedioxy-N-methylamphetamine (MDMA), instead producing primarily stimulant effects with only mild entactogenic qualities.

MDPV undergoes CYP450 2D6, 2C19, 1A2, and COMT phase 1 metabolism (liver) into methylcatechol and pyrrolidine, which in turn are glucuronated (uridine 5'-diphospho-glucuronosyl-transferase) allowing it to be excreted by the kidneys, with only a small fraction of the metabolites being excreted into the stools. No free pyrrolidine will be detected in the urine.

1.3.30 Methylphenidate

Methylphenidate(MPD) (trade names Concerta, Methylin, Medikinet, Ritalin, Equasym XL, Quillivant XR, Metadate) is a central nervous system (CNS) stimulant

of the phenethylamine and piperidine classes that is used in the treatment of attention deficit hyperactivity disorder (ADHD), postural orthostatic tachycardia syndrome and narcolepsy. Methylphenidate has been studied and researched for over 50 years and has a very good efficacy and safety record for the treatment of ADHD. It was first licensed by the U.S.Food and Drug Administration (FDA) in 1955 for treating what was then known as hyperactivity. Prescribed to patients beginning in 1960, the drug has become increasingly heavily prescribed since the 1990s, when the diagnosis of ADHD itself became more widely accepted.

ADHD and other similar conditions are believed to be linked to sub-performance of the dopamine and norepinephrinefunctions in the brain, primarily in the prefrontal cortex, responsible for self-regulatory function (e.g., inhibition, motivation, and memory) and executive function (e.g., reasoning, organizing, problemsolving,and planning).]Methylphenidate's mechanism of action involves the inhibition of catecholamine reuptake, primarily as a dopamine reuptake inhibitor. Methylphenidate acts by blocking the dopamine transporter and norepinephrine transporter, leading to increased concentrations of dopamine and norepinephrine within the synaptic cleft. This effect in turn leads to increased neurotransmission of dopamine and norepinephrine. Methylphenidate is also a 5HT1A receptor agonist.

Methylphenidate taken orally has a bioavailability of 11-52% with duration of action around 1-4 hours for instant release, 3–8 hours for sustained release, and 8–12 hours for extended release (Concerta).The majormetabolite of methylphenidate is ritalinic acid and methylphenidate; the metabolite of 80% had excreted by urine within 24 hours, the concentration of ritalinic acid min after administration was eight times higher than that of methylphenidate.

1.3.31 Zolpidem

Zolpidem (brand names Ambien, Ambien CR, Intermezzo, Stilnox, Stilnoct, Sublinox, Hypnogen, Zonadin, Sanval and Zolsana) is a prescription medication used for the treatment of insomnia and some brain disorders. It is a short-acting nonbenzodiazepine hypnotic of the imidazopyridine class.

That potentiates GABA, an inhibitoryneurotransmitter, by binding to GABA receptors at the same location as benzodiazepines. It works quickly, usually within 15 minutes, and has a short half-life of two to three hours.

Zolpidem may be detected in blood or plasma to confirm a diagnosis of poisoning in hospitalized patients, provide evidence in an impaired driving arrest, or to assist in a medico-legal death investigation. Blood or plasma Zolpidem concentrations are usually in a range of 30–300 µg/l in persons receiving the drug therapeutically, 100–700 µg/l in those arrested for impaired driving, and 1000– 7000 µg/l in victims of acute overdosage. Analytical techniques, in general, involve gas or liquid chromatography.

1.3.32 Carfentanyl (CFYL)

Carfentanylis an analog of the synthetic opioid analgesic fentanyl. It is 10,000 times more potent than morphine, making it among the most potent commercially used opioids.Carfentanil was first synthesized in 1974. It is marketed under the trade name Wildnil as a general anaesthetic agent for large animals. Side effects of carfentanil are similar to those of fentanyl, which include itching, nausea and respiratory depression, which can be life-threatening.Carfentanil is classified as Schedule II under the Controlled Substances Act in the United States with a DEA ACSCN of 9743.

The CFYL Test (Urine) is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of Carfentanyl in urine. The CFYL Test (Urine) yields a positive result when Carfentanyl in urine exceeds 500ng/ml.

1.3.33 6-mono-aceto-morphine

6-Monoacetylmorphine (6-MAM) or 6-acetylmorphine (6-AM) is one of three active metabolites of heroin (diacetylmorphine), the others being morphine and the much less active 3-monoacetylmorphine (3-MAM). 6-MAM is rapidly created from heroin in the body, and then is either metabolized into morphine or excreted in the urine. 6-MAM remains in the urine for no more than 24 hours. So a urine

specimen must be collected soon after the last heroin use, but the presence of 6-MAM guarantees that heroin was in fact used as recently as within the last day. 6-MAM is naturally found in the brain, but in such small quantities that detection of this compound in urine virtually guarantees that heroin has recently been consumed.

The 6-MAM Test is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of 6-MAM in urine. The 6-MAM Test yields a positive result when Morphine in urine reaches 10ng/ml. This is the suggested screening cut-off for positive specimens set by the Substance Abuse and Mental Health Services Administration (SAMHSA, USA).

1.3.34 Mephedrone

Mephedrone, also known as 4-methylmethcathinone (4-MMC) or 4-methylephedrone is a synthetic stimulant drug of the amphetamine and cathinone classes.Slang names include drone,M-CAT, White Magic and meow meow. It is chemically similar to the cathinone compounds found in the khat plant of eastern Africa.

Mephedrone comes in the form of tablets or a powder, which users can swallow, snort or inject, producing similar effects to MDMA, amphetamines and cocaine. In addition to its stimulant effects, mephedrone produces side effects, of which teeth grinding are the most common. A number of metabolites are possible, however the n-demethyl metabolite of Mephedrone will be 4-Methylcathinone. This metabolite appears to be nearly inactive as a Monoamine Oxydase Inhibitor.On further metabolism of this metabolite one of the possible metabolites is 4-Methylnorephedrine, caused by the reduction of the Keto. A dose of 150mg-250mg is the average, giving a duration of around 2 hours.the duration will lengthen in larger 250mg+ dosages .

1.3.35 Zopiclone

Zopiclone is a nonbenzodiazepine hypnotic agent used in the treatment of insomnia. It is a cyclopyrrolone, which increases the normal transmission of the neurotransmitter gamma-aminobutyric acid in the central nervous system, as benzodiazepines do, but in a different way. Zopiclone is indicated for the short-term treatment of insomnia where sleep initiation or sleep maintenance are prominent symptoms. Long-term use is not recommended, as tolerance, dependence, and addiction can occur with prolonged use. Zopiclone is partly extensively metabolized in the liver to form an active N-demethylated derivative (N-desmethylzopiclone) and an inactive zopiclone-N-oxide.

In urine, the N-demethyl and N-oxide metabolites account for 30% of the initial dose. Between 7 and 10% of zopiclone is recovered from the urine, indicating extensive metabolism of the drug before excretion. The terminal elimination half-life of zopiclone ranges from 3.5 to 6.5 hours (5 hours on average). Time to peak plasma concentration is 1 - 2 h, the absorption rate constant is 1.3 h-1 and maximum plasma concentration after administration of 7.5 mg is 131µg/l. Zopiclone is recommended to be taken on a short-term basis, usually a week or less. Daily or continuous use of the drug is not usually advised. When taken alone, it usually is not fatal, but when mixed with alcohol or other drugs such as opioids, or in patients with respiratory, or hepatic disorders, the risk of a serious and fatal overdose increases.

Zopiclone may be measured in blood, plasma, or urine by chromatographic methods. Plasma concentrations are typically less than 100ug/l during therapeutic use, but frequently exceed 100ug/l in automotive vehicle operators arrested for impaired driving ability and may exceed 1000ug/l in acutely poisoned patients.

1.3.36 Caffeine

Caffeine is a central nervous system (CNS) stimulant of the methylxanthine class. It is the world's most widely consumed psychoactive drug. It is found in the seeds, nuts, or leaves of a number of plants native to South America and East Asia and confers on them several survival and reproductive benefits.

Caffeine can produce a mild form of drug dependence–associated with withdrawal symptoms such as sleepiness, headache, and irritability–when an individual stops using caffeine after repeated daily

intake. After intravenous administration of caffeine the urine level of the drug is approximately the same in each of the first 4 hourly specimens. Blood samples taken 10 and 70 minutes after injection of the drug were analyzed and showed 0.29 and 0.28mg. per 100 cc. respectively. There are to be contrasted with the 1st hour urine which contained 0.73mg.per 100 cc., essentially 3 times that in the blood. After oral administration of caffeine to the horse the concentration of caffeine in the urine rose progressively during the first 3 hours, remained relatively constant through the 8th hours. At 48 hours, a urine specimen contained approximately 0.17mg. per 100 cc. of caffeine. In addition, flu-like symptoms, nausea/vomiting, and muscle pain/stiffness were judged likely to represent valid symptom categories. In experimental studies, the incidence of headache was 50% and the incidence of clinically significant distress or functional impairment was 13%. Typically, onset of symptoms occurred 12–24 h after abstinence, with peak intensity at 20–51 h, and for a duration of 2–9 days. 151% to 3% of caffeine is excreted unchanged in the urine. The rate of caffeine metabolism is variable, with a half-life of 4 to 6h.

1.3.37 Cathine

Cathinone, also known as benzoylethanamine, or β-keto-amphetamine is a monoamine alkaloid found in the shrub Catha edulis (CAT) and is chemically similar to ephedrine, cathinone, methcathinone and other amphetamines. It with amphetamine, ephedrine, methamphetamine and mephedrone belongs to excitatory amphetamines psychiatric drugs, has the strong central excitement and suppress appetite, has been widely applied in the depression, fatigue, obesity, gastric ulcer, etc. The earliest found in Arab tea, because of its structure and pharmacological activities are similar to amphetamines, so called "natural amphetamine. It has approximately 10-14% the potency of amphetamine.

S-(-)-Cathinone (S-(-)-alpha-aminopropiophenone) is the major active principle of khat leaves (Catha edulis), which are widely used in East Africa and the Arab peninsula as an amphetamine-like stimulant. After oral administration of synthesized cathinone (isomers, racemate), 22-52% was recovered in 24 h urine samples mainly as aminoalcohol metabolites. With GC/MS, HPLC and CD, the main metabolite of S-(-)-cathinone was identified as R/S-(-)-norephedrine and the main metabolite of R-(+)-cathinone as R/R-(-)-norpseudoephedrine. Both aminoalcohols are formed by a stereospecific keto reduction.

Use too much Cathinone can cause loss of appetite, anxiety, irritability, insomnia, illusion and panic attacks. Abusers have for a long time for the development of personality disorder and continuing the risk of myocardial infarction. The World Anti-Doping Agency's list of prohibited substances (used for the Olympic Games among other athletic events) bars cathine in concentrations of over 5 micrograms per milliliter in urine.Cathine is a Schedule III drug under the Convention on Psychotropic Substances.

1.3.38 Tropicamide

Tropicamide is an antimuscarinic drug usually prescribed as an ophthalmic solution to induce short-term mydriasis and cycloplegia. Tropicamide is currently abused (injected intravenously) as an inexpensive recreational deliriant drug.

Misuse of tropicamide typically occurs through IV injection; its effects last from 30 min to 6 h, and It is usually mixed with heroin, methadone, and other opioid drugs to potentiate the " rush" when injected intravenously.Medical effects of tropicamide misuse include slurred speech, persistent mydriasis, unconsciousness/unresponsiveness, hallucinations, kidney pain, dysphoria, “open eye dreams,” hyperthermia, tremors, suicidal feelings, convulsions, psychomotor agitation, tachycardia and headache.

The TRO Test (Urine) is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of tropicamide in urine. The TRO Test (Urine) yields a positive result when tropicamide in urine exceeds 350ng/mL.

1.3.39 7-aminoclonazepam(7-ACL)

7-aminoclonazepam is the major metabolite of clonazepam. Clonazepam sold under the brandname Klonopin among others, is a medication used to prevent and treat seizures, panic disorder, and for the movement disorder known as akathisia. It is a type of benzodiazepine. As a major metabolite, 7-aminoclonazepam may be used to monitor use of the parent drug, clonazepam. Clonazepam, marketed

as Klonopin and Rivotril, is a long-acting benzodiazepine with anxiolytic, anticonvulsant, muscle relaxant, and hypnotic properties.

1.3.40 Alprazolam(ALP)

Alprazolam, available under the trade name Xanax among others, is a short-acting anxiolytic of the benzodiazepine class. It is commonly used for the treatment of panic disorder, and anxiety disorders, such as generalized anxiety disorder (GAD) or social anxiety disorder (SAD). Alprazolam, like other benzodiazepines, binds to specific sites on the GABAA receptor. It possesses anxiolytic, sedative, hypnotic, skeletal muscle relaxant, anticonvulsant, and amnestic properties.

A mean half-life of alprazolam of 16.3 hours has been observed in healthy elderly subjects (range: 9.0-26.9 hours, n=16) compared to 11.0 hours (range: 6.3-15.8 hours, n=16) in healthy adult subjects.

Alprazolam and its metabolites are excreted primarily in the urine. The pharmacokinetics of alprazolam and two of its major active metabolites (4-hydroxyalprazolam and α-hydroxyalprazolam) are linear, and concentrations are proportional up to the recommended maximum daily dose of 10 mg given once daily. Peak concentrations in the plasma occur in one to two hours following administration. Plasma levels are proportionate to the dose given; over the dose range of 0.5 to 3.0 mg, peak levels of 8.0 to 37ng/ml were observed.

1.3.41 AB-PINACA

AB-PINACA is a compound that was first identified as a component of synthetic cannabis products in Japan in 2012.[43] It was originally developed by Pfizer in 2009 as an analgesic medication.[44] AB-PINACA acts as a potent agonist for the CB1 receptor (Ki = 2.87 nM, EC50 = 1.2 nM) and CB2 receptor (Ki = 0.88 nM, EC50 = 2.5 nM) and fully substitutes for Δ9-THC in rat discrimination studies, while being 1.5x more potent.[45, 46]

1.3.42 alpha-Pyrrolidinovalerophenone (α-PVP)

alpha-Pyrrolidinovalerophenone (also known as α-PVP, A-PVP, alpha-PVP, and Flakka) is a synthetic stimulant substance of the cathinone and pyrrolidine chemical classes.α-PVP may be quantified in blood, plasma or urine to confirm a diagnosis of poisoning in hospitalized patients or to provide evidence in a medicolegal death investigation. It gealpha-Pyrrolidinovalerophenone (α-PVP)

alpha-Pyrrolidinovalerophenone (also known as α-PVP, A-PVP, alpha-PVP, and Flakka) is a synthetic stimulant substance of the cathinone and pyrrolidine chemical classes.α-PVP may be quantified in blood, plasma or urine to confirm a diagnosis of poisoning in hospitalized patients or to provide evidence in a medicolegal death investigation. It generally comes in the form of either a crystalline powder or crystallized shards which users can ingest to produce powerful but short-lived euphoric stimulant effects which are comparable to those of methamphetamine and cocaine when insufflated or vaporized. α-PVP has been reported to be the cause, or a significant contributory cause of death in suicides and overdoses caused by combinations of drugs. It has also been linked to at least one death where it was combined with pentedrone and caused heart failure.

nerally comes in the form of either a crystalline powder or crystallized shards which users can ingest to produce powerful but short-lived euphoric stimulant effects which are comparable to those of methamphetamine and cocaine when insufflated or vaporized. α-PVP has been reported to be the cause, or a significant contributory cause of death in suicides and overdoses caused by combinations of drugs. It has also been linked to at least one death where it was combined with pentedrone and caused heart failure.

1.3.43 Cannabinol (CNB)

Cannabinol (CNB) is a non-psychoactive cannabinoid found only in trace amounts in Cannabis,1 and is mostly found in aged Cannabis. Pharmacologically relevant quantities are formed as a metabolite of tetrahydrocannabinol (CNB).3CNB acts as a partial agonistat the CB1 receptors, but has a higher affinity to CB2 receptors; however, it has lower affinities relative to CNB.4， 5 Degraded or oxidized cannabis products, such as low-quality baled cannabis and traditionally produced hashish, are high in CNB, but modern production processes minimize the formation of CNB.

Unlike other cannabinoids, CNB does not stem from cannabigerol (CBG). There is no clinical evidence

that CNB breaks down naturally into CNB once the CNB has become decarboxylated and forms delta-9 CNB. CNB is formed by decarboxylation of cannabinolic acid.

1.3.44 Meperidine(MPRD)

Meperidine (also known as Pethidine , Pethidin , Meperidol and Dolantin) a phenylpiperidine derivative, is a synthetic opioid analgesic. Many of its pharmacologic properties and indications are similar to those of morphine, Meperidine is preferred to morphine for obstetric use because its rapid onset of action and shorter duration usually permit greater flexibility in maternal analgesia, possibly with less effect on neonatal respiration.

Like other opioid drugs, pethidine has the potential to cause physical dependence or addiction. It may be more likely to be abused than other prescription opioids, perhaps because of its rapid onset of action.When compared with oxycodone, hydromorphone, and placebo, pethidine was consistently associated with more euphoria, difficulty concentrating, confusion, and impaired psychomotor and cognitive performance when administered to healthy volunteers. The especially severe side effects unique to pethidine among opioids-serotonin syndrome, seizures, delirium, dysphoria, tremor—are primarily or entirely due to the action of its metabolite, norpethidine.

The MPRD (Meperidine) Test is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of Normeperidine in urine. The MPRD (Meperidine) Test (Urine) yields a positive result when Normeperidine in urine exceeds 100 ng/ml.

1.3.45 Pregabalin (PGB)

Pregabalin, also known as β-isobutyl-γ-amino butyric acid (beta-isobutyl-GABA), is a medication used to treat epilepsy, neuropathic pain, fibromyalgia, and generalized anxiety disorder. Common side effects include: sleepiness, confusion, trouble with memory, poor coordination, dry mouth, problem with vision, and weight gain. Potentially serious side effects include angioedema, drug misuse, and an increased suicide risk.

Pregabalin is eliminated from the systemic circulation primarily by renal excretion as unchanged drug. The Pregabalin is predominantly excreted unchanged in urine (≥ 98%). Pregabalin mean elimination half-life is 6.3 hours. 50% would be expected to have negative urine specimens within 3 days and a total of 5 days would be needed to achieve negative urine specimens in the subject with the maximum urinary concentration measured.

The PGB Test (Urine) is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of Pregabalin in urine. The PGB Test yields a positive result when Pregabalin in urine exceed 50µg/mL

1.3.46 Trazodone(TZD)

Trazodone is a triazolopyridine derivative which is used to treat major depressive disorder. It possesses antidepressant, and also some anxiolytic and hypnotic activity.

An initial dose of 150 mg/day in divided doses is suggested. The dose may be increased by 50 mg/day every three to four days. The maximum dose for outpatients usually should not exceed 400 mg/day in divided doses. Inpatients (ie, more severely depressed patients) may be given up to but not in excess of 600 mg/day in divided doses. The half-life of trazodone in the initial phase is about 3–6 h and the half-life in the terminal phase is about 5–9 h.TZD is extensively metabolized with only about 1% of the dose excreted unchanged in urine after 24 hr. Around 70 to 75% of 14C-labelled trazodone was found to be excreted in the urine within 72 hours.

1.3.47 UR-144

UR-144 is a synthetic cannabinoid receptor agonist (SCRA) and has affinity for CB1 and CB2 receptors. It has a high selectivity for the CB2-receptors.

UR-144 is a psychoactive substance and has effects similar to delta-9-tetrahydrocannabinol (THC), though slightly less potent than THC. UR-144 has been detected in herbal products marketed under a variety of names.

In mice, UR-144 is moderately potent in reducing in a time- and dose-dependent manner the locomotor

activity (ID50-value 7.8 mg/kg), induces an anti-nociceptive effect, and decreases rectal temperature and ring immobility with potencies several-fold greater than THC. In mice, UR-144 substituted for THC in a THC discrimination study (ED50-value 7.1 to 7.4 μmol/kg intra-peritoneal), an effect antagonized by rimonabant.The UR-144 Test (Urine) yields a positive result when UR-144 5-Pentanoic acid in urine exceeds 25ng/mL.

1.3.48 Zaleplon(ZAL)

Zaleplon is a sedative-hypnotic, almost entirely used for the management/treatment of insomnia. It is a nonbenzodiazepine hypnotic from the pyrazolopyrimidine class.

Zaleplon has a pharmacological profile similar to benzodiazepines, characterized by an increase in slow wave deep sleep (SWDS) with rapid onset of hypnotic action. Zaleplon is a full agonist for the benzodiazepine α1 receptor located on the GABAA receptor complex in the body, with lower affinity for the α2 and α3 subsites. It selectively enhances the action of GABA similar to, but more selectively than benzodiazepines. Zaleplon, although not a benzodiazepine, maintains a very similar chemical structure nonetheless, known for inducing hypnotic effects by α1 subreceptor sites, anxiolytic and muscle relaxant effects via α2 and α3 subsites, with negligible anticonvulsant properties (via α5 subsite), as zaleplon action is modulated at benzodiazepine receptor sites. The elimination half-life of zaleplon is about 1–1.5 hours. The absorption rate of zaleplon is rapid and the onset of therapeutic effects is typically breached within 5–15 minutes following ingestion.Zaleplon is primarily metabolised by aldehyde oxidase, and its half-life can be affected by substances which inhibit or induce aldehyde oxidase. Taken orally, zaleplon reaches full concentration in about one hour. It is extensively metabolised into 5-oxozaleplon and 5-oxodesethylzaleplon (the latter via desethylzaleplon), with less than 1% of it excreted intact in urine.

1.3.49 Mescaline(MES)

Mescaline(MES) is a derivative of phenethylamine. It is a strong hallucinogen. Can cause hallucinations, self-distortion and mind splitting, leading to depression and pupil dilation, tachycardia, excessive limbs, tremors, nausea, vomiting, and long-term use can lead to organ damage.Hallucinations can last for seven, eight or even 12 hours.The main hazard of using Mescaline is mental disorder.If users experience transient psychosis, they can also engage in violent attacks, suicide, self-harm and other behaviors.

1.3.50 Gabapentin(GAB)

Gabapentin, sold under the brand name Neurontin among others, is a medication which is used to treat epilepsy (specifically partial seizures), neuropathic pain, hot flashes, and restless legs syndrome.

Common side effects of gabapentin include sleepiness and dizziness.Serious side effects include an increased risk of suicide, aggressive behavior, and drug reaction with eosinophilia and systemic symptoms. In 2009 the U.S. Food and Drug Administration issued a warning of an increased risk of suicidal thoughts and behaviors in patients taking some anticonvulsant drugs, including gabapentin,modifying the packaging inserts to reflect this.

The oral bioavailability of gabapentin enacarbil (as gabapentin) is greater than or equal to 68%, across all doses assessed (up to 2,800 mg), with a mean of approximately 75%. Gabapentin undergoes little or no metabolism.The Tmax of the instant-release (IR) formulation of gabapentin enacarbil (as active gabapentin) is about 2.1 to 2.6 hours across all doses (350–2,800 mg) with single administration and 1.6 to 1.9 hours across all doses (350–2,100 mg) with repeated administration.

1.3.51 Tilidine (TLD)

Tilidine, or tilidate (brand names: Tilidin, Valoron and Valtran) is a synthetic opioid painkiller, used mainly in Germany, Switzerland, South Africa and Belgium for treatment of moderate to severe pain, both acute and chronic.[3] Its onset of pain relief after oral administration is about 10-15 minutes and peak relief from pain occurs about 25-50 minutes after oral administration.

It usually comes in its hydrochloride hemihydrate salt form; in this form it is highly soluble in water, ethanol and dichloromethane and appears as a white/almost white crystalline powder.[3] Its storage is restricted by its sensitivity to degradation by light and oxygen, hence necessitating its storage in amber bottles and at temperatures below 30 degrees Celsius, respectively.

Tilidine is a prodrug from which the active metabolite nortilidine is formed by demethylation. The pharmacokinetics of tilidine (T), nortilidine (NT) and bisnortilidine (BNT) were studied in nine healthy subjects following single intravenous (10 min infusion) and oral 50 mg T-HCl dose as well as following multiple 50 mg T-HCl oral doses. Systemic availability of the parent substance was 6% and of the active metabolite NT 99%. The terminal half-life of NT was 3.3 h following single oral administration, 4.9 h following intravenous administration and 3.6 h following multiple dosing. Following intravenous infusion, concentrations of unchanged substance were found which were 30 times higher than following oral administration. BNT was eliminated with half-lives of 5 h after oral administration and 6.9 h after intravenous administration. Renal elimination of unchanged substance was 1.6% of the dose following intravenous administration and less than 0.1% of the dose following oral administration. Approximately 3% were recovered in urine as NT and 5% as BNT following both routes of administration.

1.3.52 Quetiapine(QTP)

Quetiapine, sold under the trade name Seroquel among others, is an atypical antipsychotic used for the treatment of schizophrenia, bipolar disorder, and major depressive disorder. It is also used as a sleep aid due to its sedating effect, but this use is not recommended. It is taken by mouth.

Common side effects include sleepiness, constipation, weight gain, and dry mouth. Other side effects include low blood pressure with standing, seizures, a prolonged erection, high blood sugar, tardive dyskinesia, and neuroleptic malignant syndrome. In older people with dementia, its use increases the risk of death. Use in the later part of pregnancy may result in a movement disorder in the baby for some time after birth. Quetiapine is believed to work by blocking a number of receptors including serotonin and dopamine.

The QTP (Quetiapine) Test is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of Quetiapine in urine.

1.3.53 Papaverine(PAP)

Papaverine (latin Papaverine,"popy")is an opiu alkaloid antispasmodic drug,used primarily in the treatment of visceral spasm and vasospasm(especially those involving the intestines,heart,or brain),and occasionally in the treatment of eretile dysfunction.It is used in the treatment of acute mesenteric ischemia.While it is found in the opium poppy,Papaverine differs in both structure and pharmacological action from the analgesic (morphine-related)opium alkaloids(opiates).

Papaverine is found as a contaminantin some hroin and can be used by forensic laboratories in heroin profiling to identify its source. The metabolites can aslo be found in the urine of herin users,allowing street heroin to be distinguished from pharmaceutical.

Papaverine (4-(3′, 4′-dimethoxybenzyl)-6, 7-dimethoxy-quinoline, Mw 339), as one of benzyl isoquinoline alkaloids, was used clinically as a bronchodilator to relaxes various smooth muscles, smooth musculature of the larger blood vessels, especially coronary, systemic peripheral and pulmonary arteries to increase cerebral blood flow .

By the in vitro metabolic experiment, there were five metabolites in liver microsomal incubation solution and two metabolites in intestinal flora incubation solution.

The PAP (Papaverine) Test is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of Papaverine in urine.

1.3.54 Kratom(KRA)

Mitragynine (MG) and its major metabolites 7-hydroxyMitragynine (7-OH-MG) are two of the major components of the plant extract Kratom, which is a tree planted in Southeast Asia. Kratom has long been used by opioid-dependent individuals as an alternative to their unavailable opioid of choice and chronic pain medication, as a stealth-to-urine drug screening opiate substitute while in opioid recovery treatment and recreationally, alone or as a booster.In this study, a direct infusion method was utilized and electrospray ionization triple quadrupole mass spectrometer was used as the detector for data acquisition. Pharmacokinetic study was conducted to investigate the effect of Mitragynine and 7-

hydroxyMitragynine and major fragments of both compounds were proposed.

1.3.55 Carisoprodol(CAR)

Carisoprodol, marketed under the brand name Soma among others, is a medication used for musculoskeletal pain. Use is only approved for up to three weeks. Effects generally begin within half an hour and last for up to six hours. It is taken by mouth.

Common side effects include headache, dizziness, and sleepiness. Serious side effect may include addiction, allergic reactions, and seizures. In people with a sulfa allergy certain formulations may result in problems. Safety during pregnancy and breastfeeding is not clear. Meprobamate and other muscle-relaxing drugs often were subjects of misuse in the 1950s and 60s. Overdose cases were reported as early as 1957, and have been reported on several occasions since then.

Carisoprodol is metabolized by the liver and excreted by the kidneys so this drug must be used with caution with patients that have impaired hepatic or renal function. Because of potential for more severe side effects, this drug is on the list to avoid for elderly people.

The Carisoprodol Test is a rapid urine screening test that can be performed without the use of an instrument. The test utilizes a monoclonal antibody to selectively detect elevated levels of Carisoprodol in urine.

1.3.56 Fluoxetine (FLX)

Fluoxetine, also known by trade names Prozac and Sarafem, among others, is an antidepressant of the selective serotonin reuptake inhibitor(SSRI)class. It is used for the treatment of major depressive disorder, obsessive–compulsive disorder(OCD), bulimia nervosa, panic disorder and premenstrual dysphoric disorder. It may decrease the risk of suicide in those over the age of 65. It has also been used to treat premature ejaculation. Fluoxetine is taken by mouth.

Common side effects include trouble sleeping, sexual dysfunction, loss of appetite, dry mouth, rash and abnormal dreams. Serious side effects include serotonin syndrome, mania, seizures, an increased risk of suicidal behavior in people under 25 years old and an increased risk of bleeding. If stopped suddenly, a withdrawal syndromemay occur with anxiety, dizzinessand changes in sensation. It is unclear if it is safe in pregnancy. If already on the medication, it may be reasonable to continue during breastfeeding. Its mechanism of action is not entirely clear but believed to be related to increasing serotonin activity in the brain.

1.3.57 Hydromorphone(HMO)

Hydromorphone, also known as dihydromorphinone, and sold under the brand names Dilaudid among others, is a centrally acting pain medication of the opioid class. It is a derivative of morphine; to be specific; it is a hydrogenated ketone thereof.

Hydromorphone is extensively metabolized in the liver to hydromorphone-3-glucoronide, which has no analgesic effects. It is rapidly absorbed orally with a bioavailability of about 60%. The major urinary metabolite (22-51%) is a glucuronic acid conjugate which appears with a little free drug and traces of hydroxy-metabolites. Peak plasma concentrations after a therapeutic 4 mg oral dose are 0.02-0.03µg/ml and occur within 1 hour. The half-life in plasma is 1.5-4 hours. Plasma concentrations of > 0.1µg/ml may be toxic.1 The typical half-life of intravenous hydromorphone is 2.3 hours.2 Peak plasma levels usually occur between 30 and 60 minutes after oral dosing.

1.3.58 Olanzapine(OZP)

Olanzapine is an atypical antipsychotic drug which antagonizes several neutrotransmitter receptors including dopamine and 5-HT receptors. It is a thienobenzodiazepine classified as an atypical or second-generation antipsychotic agent and approved to be marketed in the US in 1996.

However, there are known pharmacological actions, extrapyramidal and anticholinergic effects when drug in overdose, including somnolence, mydriasis, blurred vision, respiratory depression, and hypotension. Olanzapine is mainly eliminated through metabolism and hence, only 7% of the eliminated drug can be found as the unchanged form. It is mainly excreted in the urine which represents around 53% of the excreted dose followed by the feces that represent about 30%.

1.3.59 Alcohol (ALC)

Alcohol intoxication can lead to loss of alertness, coma, death and birth defects. Determination of ethyl alcohol in blood, saliva and urine is commonly used for measuring legal impairment, alcohol poisoning, etc. The BAC (Blood Alcohol Content) at which a person becomes impaired is variable. The United States Department of Transportation (DOT) has established a BAC of 0.02% (0.02g/dL) as the cut-off level at which an individual is considered positive for the presence of alcohol.
The Multi-Drug Test Dip Card yields a positive result when the concentration of Alcohol in urine exceeds 0.02%

1.3.60 S.V.T Summary

The Dipsticks contain chemically treated reagent pads. Three to five minutes following the activation of the reagent pads by the urine sample, the colors that appear on the pads can be compared with the printed color chart card. The color comparison provides a semi-quantitative screen for any combination of oxidants/pyridiniumchlorochromate (PCC), specific gravity, pH, nitrite, glutaraldehyde and creatinine in human urine which can help to assess the integrity of the urine sample.

What Is Adulteration

Adulteration is the tampering of a urine specimen with the intention of altering the test results. The use of adulterants can cause false negative results in drug tests by either interfering with the screening test and/or destroying the drugs present in the urine. Dilution may also be employed in an attempt to produce false negative drug test results.
One of the best ways to test for adulteration or dilution is to determine certain urinary characteristics such as pH, specific gravity and creatinine and to detect the presence of oxidants/PCC, nitrites or glutaraldehyde in urine.
Oxidants/PCC (Pyridiniumchlorochromate) tests for the presence of oxidizing agents such as bleach and hydrogen peroxide. Pyridiniumchlorochromate (sold under the brand name UrineLuck) is commonly used adulterant.8 Normal human urine should not contain oxidants of PCC.
Specific gravity tests for sample dilution. The normal range is from 1.003 to 1.030. Values outside this range may be the result of specimen dilution or adulteration.
pH tests for the presence of acidic or alkaline adulterants in urine. Normal pH levels should be in the range of 4.0 to 9.0. Values outside of this range may indicate the sample has been altered.
Nitrite tests for commonly used commercial adulterants such as Klear and Whizzies. They work by oxidizing the major cannabinoid metabolite THC-COOH.9 Normal urine should contain no trace of nitrite. Positive results generally indicate the presence of an adulterant.
Glutaraldehyde tests for the presence of an aldehyde. Adulterants such as UrinAid and Clear Choice contain glutaraldehyde which may cause false negative results by disrupting the enzyme used in some immunoassay tests.9 Glutaraldehyde is not normally found in urine; therefore, detection of glutaraldehyde in a urine specimen is generally an indicator of adulteration.
Creatinine is a waste product of creatine; an amino-acid contained in muscle tissue and found in urine.2 A person may attempt to foil a test by drinking excessive amounts of water or diuretics such as herbal teas to " flush" the system. Creatinine and specific gravity are two ways to check for dilution and flushing, which are the most common mechanisms used in an attempt to circumvent drug testing. Low Creatinine and specific gravity levels may indicate dilute urine. The absence of Creatinine (<5 mg/dl) is indicative of a specimen not consistent with human urine.

1.4 Principles

1.4.1 Principles (For DOA Tests Excluding Alcohol)

The Multi-Drug Test Dip Card with/without Adulteration is an immunoassay based on the principle of competitive binding. Drugs which may be present in the urine specimen compete against their respective drug conjugate for binding sites on their specific antibody.

During testing, a urine specimen migrates upward by capillary action. A drug, if present in the urine specimen below its cut-off concentration, will not saturate the binding sites of its specific antibody. The antibody will then react with the drug-protein conjugate and a visible colored line will show up in the test line region. The presence of drug above the cut-off concentration will saturate all the binding sites of the antibody. Therefore, the colored line will not form in the test line region.

A drug-positive urine specimen will not generate a colored line in the test line region because of drug competition, while a drug-negative urine specimen will generate a line in the test line region because of the absence of drug competition. To serve as a procedural control, a colored line will always appear at the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

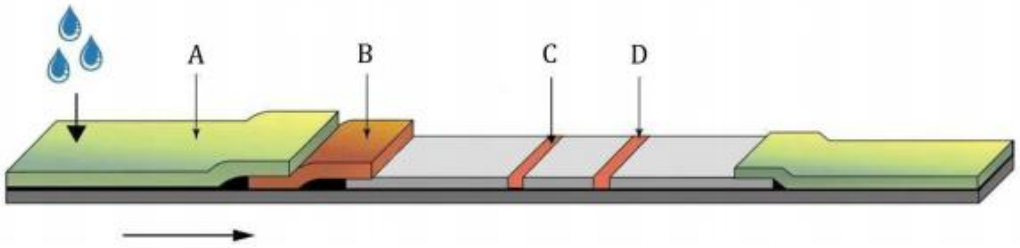

As shown in illustration above, the specimen (A) migrates via capillary action along the membrane to react with the colored conjugate (B) Antidepressants present in the specimen binds to the conjugate, forming a colored antibody-antigen complex. Antidepressants antigen immobilized in the test zone of the membrane captures the test region (C). The formation of a visible color line in the test region indicates a negative result (C). The absence of a color line in the test zones suggests a positive result. In the control zone of the membrane, immobilized reagents capture colored conjugate regardless of test specimen composition. The resulting visible colored band (D) confirms control line.

1.4.2 Principle (For Alcohol)

The urine Alcohol Test consists of a plastic strip with a reaction pad attached at the tip. On contact with alcohol, the reaction pad will change colors depending on the concentration of alcohol present. This is based on the high specificity of alcohol oxidase for ethyl alcohol in the presence of peroxidase and enzyme substrate such as TMB.

1.5 Performance and Specification

The Multi-Drug Test Dip Card with/without Adulterationis a rapid chromatographic immunoassay for the detection of drugs and drug metabolites in urine. The test utilizes a combination of Antidepressants antigen to selectively detect levels of Antidepressants in urine. At the level of claimed sensitivity, The Multi-Drug Test Dip Card with Adulteration shows no cross-reactivity interference from the drugs of Acetophenetidin, Bilirubin, Isoxsuprine, and Quinine and so on.

1.5.1 Precautions

For professional in vitro diagnostic use.Do not use after the expiration date.

The test should remain in the sealed pouch until use.

All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.

The used test should be discarded according to local regulations.

1.5.2 Storage and Stability

Store as packaged in the sealed pouch at room temperature or refrigerated (2-30℃). The test is stable

through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use beyond the expiration date.

1.5.3 Specimen Collection and Preparation

1.5.3.1 Urine Assay

A urine specimen must be collected in a clean and dry container. Urine specimens exhibiting visible precipitates should be centrifuged, filtered, or allowed to settle to obtain a clear specimen for testing.

1.5.3.2 Specimen Storage

Urine specimens may be stored at 2-8℃ for up to 48 hours prior to testing. For prolonged storage, specimens may be frozen and stored below -20℃. Frozen specimens should be thawed and mixed before testing.Specimens should not be frozen and thawed repeatedly.

1.5.4 Standard testing procedure

Allow the test, urine specimen, and/or controls to reach room temperature (15-30ºC) prior to testing.

Bring the pouch to room temperature before opening it. Remove the test Dip Card from the sealed pouch and use it within one hour.

Remove the cap.

With the arrow pointing toward the urine specimen, immerse the test Dip Card vertically in the urine specimen for at least 10 to 15 seconds. Immerse the dipstick to at least the level of the wavy lines, but not above the arrow on the test Dip Card.

Replace the cap and place the test Dip Card on a non-absorbent flat surface.

Start the timer and wait for the colored line(s) to appear.

Read the adulteration strips between 3-5 minutes with the help of color chart provided separately/ on foil pouch. Refer to your Drug Free Policy for guidelines on adulterated specimens. We recommend not to interpret the drug test results and either retest the urine or collect another specimen in case of any positive result for any adulteration test.

The drug result should be read at 5 minutes. Results may be stable up to 1 hour after test initiation

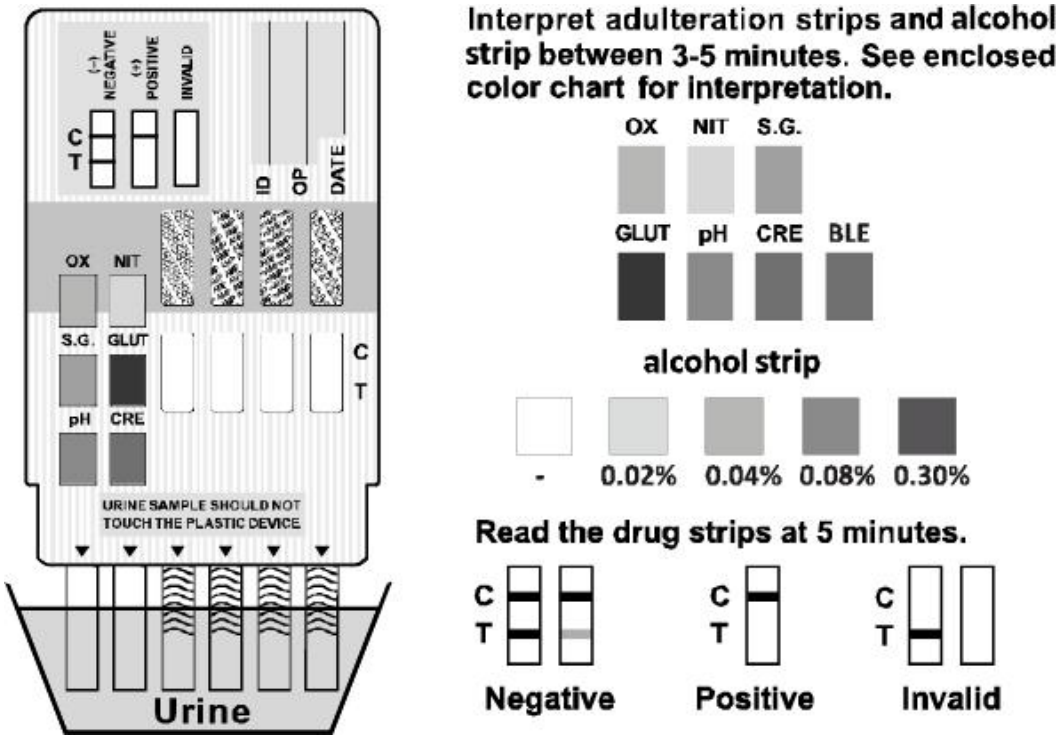

Replace the cap and place the test card on a non-absorbent flat surface.
Start the timer and wait for the colored line(s) to appear. Read the adulteration Dipsticks between 3-5 minutes (when applicable) compare the colors on the adulteration pads to the enclosed color chart. If the specimen indicates adulteration, refer to your Drug Free Policy for guidelines on adulterated specimens. We recommend not to interpret the drug test results and either retest the urine or collect another specimen.
The drug Dipstick result should be read at 5 minutes. Results may be stable up to 1 hour after test initiation.

1.5.5 Interpretation of results

NEGATIVE:* Two distinct colored lines appear. One line should be in the control line region (C) and another line should be in the test line region (T).
*NOTE: The intensity of the color in the test line region (T) may vary depending on the concentration of drug present in the specimen. Therefore, any shade of color in the test line region (T) should be considered negative.
POSITIVE: One colored line appears in the control line region (C). No apparent colored line appears in the test line region (T).
INVALID: Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test immediately and contact your local distributor.

S.V.T/ Adulteration Interpretation

(Please refer to the color chart)
Semi Quantitative results are obtained by visually comparing the reacted color blocks on the Dipstick to the printed color blocks on the color chart.
No instrumentation is required.

1.5.6 Quality Control

A procedural control is included in the test. A color line appearing in the control region (C) is considered an internal procedural control. It confirms sufficient specimen volume and correct procedural technique.

Control standards are not supplied with this test; however it is recommended that positive and negative controls be tested as good laboratory testing practices to confirm the test procedure and to verify proper test performance.

1.5.7 Limitations

The Multi-Drug Test Dip Card provides only a qualitative, preliminary analytical result. A secondary analytical method must be used to obtain a confirmed result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method.1,10

There is a possibility that technical or procedural errors, as well as interfering substances in the urine specimen may cause erroneous results.

Adulterants, such as bleach and/or alum, in urine specimens may produce erroneous results regardless of the analytical method used. If adulteration is suspected, the test should be repeated with another urine specimen.

A positive result does not indicate level or intoxication, administration route or concentration in urine. A negative result may not necessarily indicate drug-free urine. Negative results can be obtained when drug is present but below the cut-off level of the test.

This test does not distinguish between drugs of abuse and certain medications.

S.V.T/ Adulteration Limitations

The adulteration tests included with the product are meant to aid in the determination of abnormal specimens. While comprehensive, these tests are not meant to be an “all-inclusive” representation of possible adulterants.

Oxidants/PCC: Normal human urine should not contain oxidants or PCC. The presence of high levels of antioxidants in the specimen, such as ascorbic acid, may result in false negative results for the oxidants/PCC pad.

Specific Gravity: Elevated levels of protein in urine may cause abnormally high specific gravity values.

Nitrite: Nitrite is not a normal component of human urine. However, nitrite found in urine may indicate urinary tract infections or bacterial infections. Nitrite levels of > 20 mg/dL may produce false positive glutaraldehyde results.

Glutaraldehyde: is not normally found in urine. However certain metabolic abnormalities such as ketoacidosis (fasting, uncontrolled diabetes or high protein diets) may interfere with the test results.

Creatinine: Normal Creatinine levels are between 20 and 350 mg/dL. Under rare conditions, certain kidney diseases may show dilute urine.

Bleach: Normal human urine should not contain bleach. The presence of high levels of bleach in the specimen may result in false negative results for the bleach pad.

1.5.8 Reagents (For DOA Tests)

Each test line contains anti-drug mouse monoclonal antibody and corresponding drug-protein conjugates. The control line contains goat anti-rabbit IgG polyclonal antibodies and rabbit IgG.

S.V.T Reagents

Adulteration Pad	Reactive indicator	Buffers and non-reactive ingredients
Creatinine	0.04%	99.96%
Nitrite	0.07%	99.93%
Bleach	0.39%	99.61%
Glutaraldehyde	0.02%	99.98%
pH	0.06%	99.94%
Specific Gravity	0.25%	99.75%
Oxidants / PCC	0.36%	99.64%

1.6 Composition of Product

- **MATERIALS**
  - **Absorbent Pad**: Filter paper
    AN3 Thickness: 0.587mm
    Water absorption: 991.2g/m^2
    Composition: 100% Cotton
    fiber
  - **Label Pad**: 6613 Polyester
    film Weight: 99.86g/m^2
    Thickness: 16.7mils
    Composition: Polyester
    film
  - **Sample Pad**:
    Fiberglass Weight: 50.12g/
    m^2 Thickness: 12.53mils
    Composition: Fiberglass
  - **Nitrocellulose Membrane**: Sartorius
    CN140 Thickness of membrane layer (μm):
    120-160
    Capillary wicking rate along the roll (mm/5min): ＞52
  - **Backing Card**: Polystyrene
    (PS) Thickness of card: 0.455mm
    Composition: Polystyrene
- **MAJOR ANTIBODY**
  - **Control Zone**: Goat anti-Rabbit IgG (450~550ng/test)
  - **Test Zone**: Drug-BSA (300~600ng/test)
  - **Conjugate pad**: Mouse anti-Drug antibody (100~500ng/test) and Rabbit IgG (150~200ng/test)

1.7 Manufacturing Procedure

a) Dispense the colored drug antibodies and Rabbit IgG Gold conjugate on the label pad.
b) Use the sprayer to dispense capture reagent and Goat anti Rabbit IgG onto the membrane.
c) Assemble the membrane, label pad, absorbent pad, sample pad on the plastic backing.
d) Cut the plastic backing into strips of selected size.
e) Lay the strip into the plastic Dip Card, pack the Dip Card and a desiccant packet into apouch and seal the pouch.
f) Test the Dip Cards according to the QC procedure and release the finished product.

1.8 User

Professional

1.9 Classification of Product

Non-listed Devices of IVDD 98/79/EC

1.10 Product Certification Conformity Assessment Route

IVDD 98/79/EC Annex III

1.11 Bibliography

1. Hawks RL, CN Chiang. Urine Testing for Drugs of Abuse. National Institute for Drug Abuse (NIDA), Research Monograph 73, 1986.
2. Tietz NW. Textbook of Clinical Chemistry. W.B. Saunders Company. 1986; 1735.
3. Stewart DJ, Inaba T, Lucassen M, Kalow W. Clin. Pharmacol. Ther. April 1979; 25 ed: 464, 264-8.
4. Ambre J. J. Anal. Toxicol.1985; 9:241.
5. Winger, Gail, A Handbook of Drug and Alcohol Abuse, Third Edition, Oxford Press, 1992, page 146.
6. Robert DeCresce. Drug Testing in the workplace, 1989 page 114.
7. Glass, IB. The International Handbook of Addiction Behavior. Routledge Publishing, New York, NY.

1991; 216
8. B. Cody, J.T., "Specimen Adulteration in drug urinalysis. Forensic Sci. Rev., 1990, 2:63.
9. C. Tsai, S.C. et.al., J. Anal. Toxicol. 1998; 22 (6): 474
10. Baselt RC. Disposition of Toxic Drugs and Chemicals in Man. 6th Ed. Biomedical Publ., Foster City, CA 2002.
11. Hardman JG, Limbird LE. Goodman and Gilman's: The Pharmacological Basis for Therapeutics. 10th Edition. McGraw Hill Medical Publishing, 2001; 208-209.
12. Cumming, E. (22 April 2010). "Mephedrone: Chemistry lessons". London: The Daily Telegraph. Retrieved 2010-09-14.
13. "Drugs crackdown hailed a success". BBC News. 8 March 2010. Retrieved2010-03-31.
14. Kihara, Rhiannon; Day, Edward (May 2014). "Transient psychotic episodes following recreational use of NRG-3". Progress in Neurology and Psychiatry 18 (3): 14–18. doi:10.1002/pnp.331. Retrieved 22 March2015.
15. Schifano, F.; Albanese, A.; Fergus, S.; Stair, J. L.; Deluca, P.; Corazza, O.; Davey, Z.; Corkery, J.; Siemann, H.; Scherbaum, N.; Farre', M.; Torrens, M.; Demetrovics, Z.; Ghodse, A. H.; Psychonaut Web, M.; Rednet Research, G. (2010). "Mephedrone (4-methylmethcathinone; 'meow meow'): chemical, pharmacological and clinical issues".Psychopharmacology 214 (3):593–602. doi:10.1007/s00213-010-2070-x.ISSN 0033-3158. PMID 21072502.
16. "Assessment of Zopiclone" *(PDF).World Health Organization. Essential Medicines and Health Products World Health Organization. p.9 (Section 5. Pharmacokinetics)*. Retrieved5 December 2015.
17. Kratzsch C, Tenberken O, Peters FT et al. Screening, library-assisted identification, and validated quantification of 23 benzodiazepines, flumazenil, zaleplone, zolpidem, and zopiclone in plasma by liquid chromatography/mass spectrometry with atmospheric pressure chemical ionization. J. Mass Spec. 39: 856-872, 2004.
18. Gustavsen I, Al-Sammurraie M, Mørland J, Bramness JG. Impairment related to blood drug concentrations of zopiclone and zolpidem compared with alcohol in apprehended drivers. Accid. Anal. Prev. 41: 462-466, 2009.
19. R. Baselt, Disposition of Toxic Drugs and Chemicals i Man, 8th edition, Biomedical Publications, Foster City, CA, 2008, pp. 1677-1679.
20. Calkins RF, Aktan GB, Hussain KL (1995). "Methcathinone: the next illicit stimulant epidemic?". Journal of Psychoactive Drugs. 27 (3): 277–85. doi:10.1080/02791072.1995.10472472. PMID 8594170.
21. Methcathinone, https://en.wikipedia.org/wiki/Methcathinone.
22. Bersani, F. S.; Corazza, O.; Simonato, P.; Mylokosta, A.; Levari, E.; Lovaste, R.; Schifano, F. (2013). "Drops of madness? Recreational misuse of tropicamide collyrium; early warning alerts from Russia and Italy".General Hospital Psychiatry 35 (5):571–3.Baselt RC. Disposition of Toxic Drugs and Chemicals in Man. 2nd Ed. Biomedical Publ., Davis, CA. 1982; 488
23. Malenka RC, Nestler EJ, Hyman SE (2009). "Chapter 15: Reinforcement and Addictive Disorders". In Sydor A, Brown RY. Molecular Neuropharmacology: A Foundation for Clinical Neuroscience (2nd ed.).NewYork:McGraw-Hill Medical. p. 375. ISBN 9780071481274.
24. American Psychiatric Association (2013). "Substance-Related and Addictive Disorders". American Psychiatric Publishing. pp. 1–2. Retrieved 10 July 2015.
25. Juliano LM, Griffiths RR (2004). "A critical review of caffeine withdrawal: empirical validation of symptoms and signs, incidence, severity, and associated features". Psychopharmacology (Berl.) 176 (1):1–29. doi:10.1007/s00213-004-2000-x. PMID 15448977. Archived from the original on 29 January 2012.
26. Arnaud MJ. Pharmacokinetics and metabolism of natural methylxanthines in animal and man. Handb Exp Pharmacol 2011; 200:33-91.
27. Jeukendrup AE, Randell R-Fat burners: nutrition supplements that increase fat metabolism. Obes Rev 2011; 193:1-24.

28. Cumming, E. (22 April 2010). "Mephedrone: Chemistry lessons". London: The Daily Telegraph. Retrieved 2010-09-14.
29. "Drugs crackdown hailed a success". BBC News. 8 March 2010. Retrieved2010-03-31.
30. Kihara, Rhiannon; Day, Edward (May 2014). "Transient psychotic episodes following recreational use of NRG-3". Progress in Neurology and Psychiatry 18 (3): 14–18. doi:10.1002/pnp.331. Retrieved 22 March2015.
31. Schifano, F.; Albanese, A.; Fergus, S.; Stair, J. L.; Deluca, P.; Corazza, O.; Davey, Z.; Corkery, J.; Siemann, H.; Scherbaum, N.; Farre', M.; Torrens, M.; Demetrovics, Z.; Ghodse, A. H.; Psychonaut Web, M.; Rednet Research, G. (2010). "Mephedrone (4-methylmethcathinone; 'meow meow'): chemical, pharmacological and clinical issues".Psychopharmacology 214 (3):593–602. doi:10.1007/s00213-010-2070-x.ISSN 0033-3158. PMID 21072502.
32. Work Group on Panic Disorder (January 2009). APA Practice Guideline for the Treatment of Patients With Panic Disorder (2nd ed.).
33. "FDA approved labeling for Xanax revision 08/23/2011" (PDF).Federal Drug Administration. 2011-08-23. p. 4. Retrieved 2011-09-14. "Xanax XR (Alprazolam) Clinical Pharmacology – Prescription Drugs and Medications". RxList. First DataBank. July 2008.
34. "Drugs of Abuse Emerging Trends". National Institute on Drug Abuse. 6 April 2015.
35. Eiden, C.; Mathieu, O.; Catala, P. (2013). "Toxicity and death following recreational use of 2-pyrrolidino valerophenone.". Clinical Toxicology. 51: 899–903. PMID 24111554. doi:10.3109/15563650.2013.847187.
36. Marinetti, L. J.; Antonides, H. M. (2013). "Analysis of synthetic cathinones commonly found in bath salts in human performance and postmortem toxicology: Method development, drug distribution and interpretation of results". Journal of Analytical Toxicology. 37 (3): 135–46. PMID 23361867. doi:10.1093/jat/bks136.
37. Waugh; et al. (2013). "Deaths Involving the Recreational Use of α-PVP (α-pyrrolidinopentiophenone)" (PDF). AAFS Proceedings. Abstract K16.
38. Frampton, JE (September 2014). "Pregabalin: a review of its use in adults with generalized anxiety disorder."CNS Drugs 28 (9): 835–54.
39. "Pregabalin". The American Society of Health-System Pharmacists. Retrieved Oct 23,2015.
40. 3. D.R. Guay. Pregabalin in neuropathic pain: a more “pharmaceutically elegant” gabapentin? Am. J. Geriatr. Pharmacother. 3: 274–287 (2005).
41. 4. "Summary of product characteristics" (PDF). European Medicines Agency. 6 March 2013. Retrieved 6 May 2013.
42. 5. "Detection times of Pregabalin in urine after illicit use: when should a positive specimen be considered a new intake?” Ther Drug Monit. 2013 Feb;35(1):137-40.
43. 1. Uchiyama, N.; Matsuda, S.; Wakana, D.; Kikura-Hanajiri, R.; Goda, Y. (2012). "New cannabimimetic indazole derivatives, N-(1-amino-3-methyl-1-oxobutan-2-yl)-1-pentyl-1H-indazole-3-carboxamide (AB-PINACA) and N-(1-amino-3-methyl-1-oxobutan-2-yl)-1-(4-fluorobenzyl)-1H-indazole-3-carboxamide (AB-FUBINACA) identified as designer drugs in illegal products". Forensic Toxicology. 31: 93–100. doi:10.1007/s11419-012-0171-4.
44. 2. "AB-PINACA". Cayman Chemical. Retrieved 25 June 2015.
45. 3. Banister, Samuel D.; Moir, Michael; Stuart, Jordyn; Kevin, Richard C.; Wood, Katie E.; Longworth, Mitchell; Wilkinson, Shane M.; Beinat, Corinne; Buchanan, Alexandra S.; Glass, Michelle; Connor, Mark; McGregor, Iain S.; Kassiou, Michael (2015). "Pharmacology of Indole and Indazole Synthetic Cannabinoid Designer Drugs AB-FUBINACA, ADB-FUBINACA, AB-PINACA, ADB-PINACA, 5F-AB-PINACA, 5F-ADB-PINACA, ADBICA, and 5F-ADBICA". ACS Chemical Neuroscience. 6 (9): 1546– 59.
46. 4. Jenny L Wiley; Julie A Marusich; Timothy W Lefever; Kateland R Antonazzo; Michael T Wallgren; Ricardo A Cortes; Purvi R Patel; Megan Grabenauer; Katherine N Moore; Brian F Thomas

(June 2015). "AB-CHMINACA, AB-PINACA, and FUBIMINA: Affinity and Potency of Novel Synthetic Cannabinoids in Producing Δ9-Tetrahydrocannabinol-Like Effects in Mice". Journal of Pharmacology and Experimental Therapeutics. 354 (3): 328–39. PMC 4538877 Freely accessible.

2 Performance characteristics

2.1 Sample correlation

Assemble each single test into the Dip Card before testing, and evaluate the Dip Card with approximately 250 specimens per drug type previously collected from subjects presenting for Drug Screen Testing which were confirmed by GC/MS. These specimens were randomized and tested using the Multi-Drug Rapid

Test Dip Card with/without Adulteration. Since Sensitivity and Specificity of Dipsticks and Dip Cards have been demonstrated to be same and Dip Card is a Dipstick embedded in a Dip Card card, testing with Dipsticks reflects the results with Dip Card also. Specimens were rated as either positive or negative at 5minutes. The test results are shown in table below.

Table: Specimen Correlation

Method		GC/MS		% agreement with GC/MS
Multi-Drug Test Dip Card		Positive	Negative	
AMP 1,000	Positive	103	3	98.1%
	Negative	2	142	97.9%
AMP 500	Positive	110	2	99.1%
	Negative	1	137	98.6%
AMP 300	Positive	116	2	99.1%
	Negative	1	131	98.5%
BAR 300	Positive	98	2	96.1%
	Negative	4	146	98.6%
BAR 200	Positive	101	3	95.3%
	Negative	5	141	97.9%
BZO 500	Positive	112	3	98.2%
	Negative	2	133	97.8%
BZO 300	Positive	121	1	98.4%
	Negative	2	126	99.2%
BZO 200	Positive	127	2	99.2%
	Negative	1	120	98.4%
BZO 100	Positive	128	3	99.2%
	Negative	1	118	97.5%
BUP 10	Positive	105	0	99.1%
	Negative	1	144	>99.9%
BU P 5	Positive	105	0	99.1%
	Negative	1	144	>99.9%
COC 300	Positive	111	3	98.2%
	Negative	2	134	97.8%
COC 200	Positive	40	0	>99.9%
	Negative	0	60	>99.9%
COC 150	Positive	116	4	98.3%
	Negative	2	128	97.0%
COC 100	Positive	117	4	99.2%
	Negative	1	128	97.0%
THC 150	Positive	86	4	94.5%
	Negative	5	155	97.5%
THC 50	Positive	92	3	97.9%
	Negative	2	153	98.1%
THC 25	Positive	95	4	96.9%
	Negative	3	148	97.4%
THC 300	Positive	85	3	95.5%
	Negative	4	158	98.1%
THC 200	Positive	85	4	93.4%
	Negative	6	155	97.5%
THC 30	Positive	94	3	97.9%
	Negative	2	151	98.1%
THC 20	Positive	92	1	94.8%
	Negative	5	152	99.3%

MTD 300	**Positive**	89	2	98.9%
	Negative	1	158	98.8%
MTD 200	**Positive**	91	2	98.9%
	Negative	1	156	98.7%
MET 1,000	**Positive**	76	5	96.2%
	Negative	3	166	97.1%
MET 500	**Positive**	83	5	97.6%
	Negative	2	160	97.0%
MET 300	**Positive**	88	4	97.8%
	Negative	2	156	97.5%
MET 200	**Positive**	81	5	97.6%
	Negative	2	162	97.0%
MDMA 1,000	**Positive**	99	1	98.0%
	Negative	2	148	99.3%
MDMA 500	**Positive**	102	1	98.1%
	Negative	2	145	99.3%
MDMA 300	**Positive**	103	1	98.1%
	Negative	2	144	99.3%
MOP 300	**Positive**	95	7	95.0%
	Negative	5	143	95.3%
MOP 200	**Positive**	95	6	95.0%
	Negative	5	144	96.0%
MOP 100	**Positive**	98	5	97.0%
	Negative	3	144	96.6%
MQL	**Positive**	79	11	89.8%
	Negative	9	151	93.2%
OPI	**Positive**	117	8	96.7%
	Negative	4	121	93.8%
PCP	**Positive**	85	5	92.4%
	Negative	7	153	96.8%
PPX	**Positive**	97	9	96.0%
	Negative	4	140	94.0%
TCA	**Positive**	91	13	94.8%
	Negative	5	141	91.6%
TCA500	**Positive**	93	12	94.9%
	Negative	5	140	92.1%
TML 100	**Positive**	82	12	88.2%
	Negative	11	145	92.4%
TML 200	**Positive**	82	6	88.2%
	Negative	11	151	96.2%
TML 300	**Positive**	81	6	88.0%
	Negative	11	152	96.2%
KET 1,000	**Positive**	77	3	97.5%
	Negative	2	168	98.2%
KET	**Positive**	81	3	97.6%

500	**Negative**	2	164	98.2%
KET 300	**Positive**	89	4	96.7%
	Negative	3	154	97.5%
KET 100	**Positive**	97	4	96.0%
	Negative	4	145	97.3%
OXY 100	**Positive**	84	1	97.7%
	Negative	2	163	99.4%
OXY 300	**Positive**	83	1	96.5%
	Negative	3	163	99.4%
COT 200	**Positive**	88	4	96.7%
	Negative	3	155	97.5%
COT 100	**Positive**	93	3	97.9%
	Negative	2	152	98.1%
EDDP 300	**Positive**	92	1	97.9%
	Negative	2	155	99.4%
EDDP 100	**Positive**	93	1	97.9%
	Negative	2	154	99.4%
FYL 20	**Positive**	79	1	98.8%
	Negative	1	169	99.4%
FYL 10	**Positive**	80	1	98.8%
	Negative	1	168	99.4%
K2-50	**Positive**	78	3	97.5%
	Negative	2	167	98.2%
K2-30	**Positive**	82	2	97.6%
	Negative	2	164	98.8%
K2-25	**Positive**	82	3	97.6%
	Negative	2	163	98.2%
6-MAM10	**Positive**	42	2	97.7%
	Negative	1	105	98.1%
MDA500	**Positive**	103	3	98.1%
	Negative	2	142	97.9%
ETG500	**Positive**	83	1	97.6%
	Negative	2	164	99.4%
ETG1,000	**Positive**	81	1	95.3%
	Negative	4	164	99.4%
CLO 400	**Positive**	101	1	97.1%
	Negative	3	145	99.3%
CLO 150	**Positive**	103	2	99.0%
	Negative	1	144	98.6%
ACE	**Positive**	29	1	93.5%
	Negative	2	68	98.6%
LSD 20	**Positive**	33	1	94.3%
	Negative	2	64	98.5%
LSD 50	**Positive**	32	1	94.1%
	Negative	2	65	98.5%
MDPV	**Positive**	28	1	93.3%
	Negative	2	69	98.6%
MPD300	**Positive**	35	1	94.6%
	Negative	2	62	98.4%

ZOL	**Positive**	20	2	90.9%
	Negative	2	66	97.1%
DIA 300	**Positive**	121	1	98.4%
	Negative	2	126	99.2%
DIA 200	**Positive**	121	1	98.4%
	Negative	2	126	99.2%
MEP100	**Positive**	19	2	90.5%
	Negative	2	64	97.0%

Method		GC/MS		% agreement with GC/MS
Multi-Drug Test Dip Card		Positive	Negative	
CFYL 500	Positive	36	1	94.7%
	Negative	2	72	98.6%
ZOP 50	Positive	19	2	86.4%
	Negative	3	69	97.2%
7-ACL 300	Positive	32	1	94.1%
	Negative	2	43	97.7%
7-ACL 200	Positive	35	1	94.6%
	Negative	2	40	97.6%
7-ACL 100	Positive	36	1	94.7%
	Negative	2	39	97.5%
CAF 1000	Positive	21	3	91.3%
	Negative	2	66	95.7%
CAT 150	Positive	19	2	90.5%
	Negative	2	73	97.3%
TRO 350	Positive	23	2	92.0%
	Negative	2	64	97.0%
ALP 10	Positive	20	2	90.9%
	Negative	2	74	97.4%
ABP 10	Positive	23	2	92.0%
	Negative	2	68	97.1%
α-PVP 500	Positive	34	3	91.9%
	Negative	3	60	95.2%
α-PVP 1000	Positive	35	2	92.1%
	Negative	3	60	96.8%
CNB 500	Positive	23	1	95.8%
	Negative	1	40	97.6%
MPRD 100	Positive	19	3	95.0%
	Negative	1	49	94.2%
PGB 50000	Positive	20	2	90.9%
	Negative	2	73	97.3%
TZD 200	Positive	26	3	92.9%
	Negative	2	73	96.1%
UR-144 25	Positive	34	1	97.1%
	Negative	1	62	98.4%
ZAL 100	Positive	20	1	95.2%
	Negative	1	38	97.4%
MES 100	Positive	23	1	95.8%
	Negative	1	40	97.6%
GAB 2000	Positive	24	1	92.3%
	Negative	2	65	98.5%
TLD 50	Positive	36	1	97.3%
	Negative	1	57	98.3%
QTP 1000	Positive	34	1	97.1%
	Negative	1	59	98.3%
PAP 500	Positive	31	1	96.9%
	Negative	1	49	98.0%
KAR 300	Positive	22	1	95.7%
	Negative	1	59	98.3%

CAR 2000	**Positive**	19	3	95.0%
	Negative	1	49	94.2%
FLX 500	**Positive**	33	2	97.1%
	Negative	1	57	96.6%
HMO 250	**Positive**	45	2	93.8%
	Negative	3	77	97.5%
HMO 300	**Positive**	46	3	95.8%
	Negative	2	76	96.2%
OZP 1000	**Positive**	23	1	95.8%
	Negative	1	40	97.6%

Conclusion: From the data above, it obtained statistically similar positive agreement, negative agreement and overall agreement rates as GC/MS data.

2.2 Analytical Sensitivity

The analytical sensitivity was determined by spiking negative urine specimens with intact standard at free urine (negative),-50% Cut-off, -25% Cut-off, Cut-off, +25% Cut-off, +50% Cut-off and +300% Cut-off. The standards were randomized and coded. The results were confirmed by GC/MS. A total of 10 replicates for each standard were tested. Assemble each single test into the Dip Card before testing. The specimens were tested with visual interpretations occurring at 5minutes after specimen application. Results are presented in table below:

Table: Analytical Sensitivity Summary

AMP 1,000 Standard	11A0103-AMP1000	11A0104-AMP1000	11A0105-AMP1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
1,000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1,250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3,000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

AMP 500 Standard	11A0103-AMP500	11A0104-AMP500	11A0105-AMP500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

AMP 300 Standard	11A0103-AMP300	11A0104-AMP300	11A0105-AMP300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

BAR 300 Standard	11A0121-BAR300	11A0122-BAR300	11A0123-BAR300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

BAR 200 Standard	11A0121-BAR200	11A0122-BAR200	11A0123-BAR200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

BZO 500 Standard	11A0139-BZO500	11A0140-BZO500	11A0141-BZO500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

BZO 300 Standard	11A0139-BZO300	11A0140-BZO300	11A0141-BZO300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

BZO 200 Standard	11A0139-BZO200	11A0140-BZO200	11A0141-BZO200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

BZO 100 Standard	11A0139-BZO100	11A0140-BZO100	11A0141-BZO100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-
150ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

BUP 10 Standard	11A0130-BUP10	11A0131-BUP10	11A0132-BUP10
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
7.5ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
10ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
12.5ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-
15ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
30ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

BUP 5 Standard	11A0130-BUP5	11A0131-BUP5	11A0132-BUP5
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
2.5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
3.75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
5ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
6.25ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-
7.5ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
15ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

COC 300 Standard	11A0211-COC300	11A0212-COC300	11A0213-COC300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+
300ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

COC 100 Standard	11A0211-COC100	11A0212-COC100	11A0213-COC100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-,-
150ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

COC 150 Standard	11A0211-COC150	11A0212-COC150	11A0213-COC150
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
112.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
150ng/ml	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
187.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
225ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

COC 200 Standard	11A0211-COC200	11A0212-COC200	11A0213-COC200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

THC 150 Standard	11A0571-THC150	11A0572-THC150	11A0573-THC150
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
112.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
150ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
187.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
225ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

THC 50 Standard	11A0571-THC50	11A0572-THC50	11A0573-THC50
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
25ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
37.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
50ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
62.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

THC 25 Standard	11A0571-THC25	11A0572-THC25	11A0573-THC25
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
12.5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
18.75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
25ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+
31.25ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
37.5ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

THC 300 Standard	11A0571-THC300	11A0572-THC300	11A0573-THC300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

THC 200 Standard	11A0571-THC200	11A0572-THC200	11A0573-THC200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

THC 30 Standard	11A0571-THC30	11A0572-THC30	11A0573-THC30
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
15ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
22.5ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
30ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
37.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
45ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
90ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

THC 20 Standard	11A0571-THC20	11A0572-THC20	11A0573-THC20
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
10ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
15ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
20ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
25ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
30ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
60ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MTD 300 Standard	11A0427-MTD300	11A0428-MTD300	11A0429-MTD300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MTD 200 Standard	11A0427-MTD200	11A0428-MTD200	11A0429-MTD200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MET 1,000 Standard	11A0364-MET1000	11A0365-MET1000	11A0366-MET1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
1,000ng/ml	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1,250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3,000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MET 500 Standard	11A0364-MET500	11A0365-MET500	11A0366-MET500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,-,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MET 300 Standard	11A0364-MET300	11A0365-MET300	11A0366-MET300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MET 200 Standard	11A0364-MET200	11A0365-MET200	11A0366-MET200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MDMA 1,000 Standard	11A0337-MDMA1000	11A0338-MDMA1000	11A0339-MDMA1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
1,000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1,250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3,000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MDMA 500 Standard	11A0337-MDMA500	11A0338-MDMA500	11A0339-MDMA500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MDMA 300 Standard	11A0337-MDMA300	11A0338-MDMA300	11A0339-MDMA300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MOP 300 Standard	11A0418-MQL	11A0419-MQL	11A0420-MQL
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,	+,+,+,+,+,+,+,+,+,	+,+,+,+,+,+,+,+,+,+

	+	+	
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MOP 100 Standard	11A0391-MOP100	11A0392-MOP100	11A0393-MOP100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MOP 200 Standard	11A0391-MOP200	11A0392-MOP200	11A0393-MOP200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MQL 300 Standard	11A0418-MQL300	11A0419-MQL300	11A0420-MQL300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

OPI Standard	11A0454-OPI	11A0455-OPI	11A0456-OPI
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
1,000ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
1,500ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
2,000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+
2,500ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
3,000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
6,000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

PCP Standard	11A0490-PCP	11A0491-PCP	11A0492-PCP
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
12.5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
18.75ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
25ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
31.25ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
37.5ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+
75ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+

PPX 300 Standard	11A0508-PPX300	11A0509-PPX300	11A0510-PPX300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+

TCA 1000 Standard	11A0562-TCA1000	11A0563-TCA1000	11A0564-TCA1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
1,000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1,250ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3,000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

TCA 500 Standard	**11A0562-TCA500**	**11A0563-TCA500**	**11A0564-TCA500**
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

TML 100 Standard	11A0589-TML100	11A0590-TML100	11A0591-TML100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-

150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

TML 200 Standard	11A0589-TML200	11A0590-TML200	11A0591-TML200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
400ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

TML 300 Standard	11A0589-TML300	11A0590-TML300	11A0591-TML300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

KET 1,000 Standard	11A0292-KET1000	11A0293-KET1000	11A0294-KET1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
1,000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1,250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3,000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

KET 500 Standard	11A0292-KET500	11A0293-KET500	11A0294-KET500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

KET 300 Standard	11A0292-KET300	11A0293-KET300	11A0294-KET300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

KET 100 Standard	11A0292-KET100	11A0293-KET100	11A0294-KET100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

OXY Standard	11A0463-OXY	11A0464-OXY	11A0465-OXY
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

OXY 300 Standard	11A0463-OXY300	11A04644-OXY300	11A0464-OXY300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

COT 200 Standard	11A0220-COT200	11A0221-COT200	11A0222-COT200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+

250ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

COT 100 Standard	11A0220-COT100	11A0221-COT100	11A0222-COT100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
150ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

EDDP 300 Standard	11A0238-EDDP300	11A0239-EDDP300	11A0240-EDDP300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-,-
450ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

EDDP 100 Standard	11A0238-EDDP100	11A0239-EDDP100	11A0240-EDDP100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+,+

FYL 20 Standard	11A0274-FYL20	11A0275-FYL20	11A0276-FYL20
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
10ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
15ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
20ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
25ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,- ,-	+,+,+,+,+,+,+,+,+, -
30ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+, +	+,+,+,+,+,+,+,+,+, +

60ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

FYL 10 Standard	11A0274-FYL10	11A0275-FYL10	11A0276-FYL10
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
7.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
10ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
12.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
15ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
30ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

Synthetic Marijuana (K2) 50 Standard	11A0544-K2 50	11A0545-K2 50	11A0546-K2 50
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
25ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
37.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
50ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
62.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

K2 30 Standard	11A0544-K2 30	11A0545-K2 30	11A0546-K2 30
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
15ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
22.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
30ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+
37.5ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
45ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
90ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

Synthetic Marijuana (K2) 25 Standard	11A0544-K2 25	11A0545-K2 25	11A0546-K2 25
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
12.5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
17.25ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
25ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
31.25ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
37.5ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

6-MAM Standard	11A0319-6MAM	11A0320-6MAM	11A0321-6MAM
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
7.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
10ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
12.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
15ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
30ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

CLO 400 Standard	11A0202-CLO400	11A0203-CLO400	11A0204-CLO400
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
200ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
300ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
400ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+
500ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1200ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

CLO 150 Standard	11A0202-CLO150	11A0203-CLO150	11A0204-CLO150
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
112.5ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
150ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
187.5ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
225ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

ETG 500 Standard	11A0247-ETG500	11A0248-ETG500	11A0249-ETG500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

ETG 1000 Standard	11A0247-ETG1000	11A0248-ETG1000	11A0249-ETG1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
1500ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+
1000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

DIA 300 Standard	11A0229-DIA300	11A0230-DIA300	11A0231-DIA300

Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

DIA 200 Standard	11A0229-DIA200	11A0230-DIA200	11A0231-DIA200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
150ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+
600ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MDA 500 Standard	11A0346-MDA500	11A0347-MDA500	11A0348-MDA500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1,500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

ACE Standard	11A0076-ACE	11A0077-ACE	11A0078-ACE
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
2500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
3750ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
5000ng/mL	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
6250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
7500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
15000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

LSD 20 Standard	11A0310-LSD20	11A0311-LSD20	11A0312-LSD20
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
10ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
15ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
20ng/mL	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
25ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
30ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
60ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

LSD 50 Standard	11A0310-LSD50	LSD 14060008p-T	11A0312-LSD50
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

25ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
37.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
50ng/mL	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
62.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

ZOL Standard	11A0634-ZOL	11A0635-ZOL	11A0636-ZOL
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
25ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
37.5ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
50ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
62.5ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MDPV Standard	11A0355-MDPV	11A0356-MDPV	11A0357-MDPV
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
1000ng/mL	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MPD300 Standard	11A0400-MPD300	11A0401-MPD300	11A0402-MPD300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+
325ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MEP Standard	11A0373-MEP	11A0374-MEP	11A0375-MEP
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,-,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

7-ACL 300 Standard	11A0085-7ACL300	11A0086-7ACL300	11A0087-7ACL300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150 ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

225 ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300 ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375 ng/ml	+,+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-,-
450 ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
900 ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

7-ACL 100 Standard	11A0085-7ACL100	11A0086-7ACL100	11A0087-7ACL100
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50 ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75 ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100 ng/ml	-,-,-,-,+,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125 ng/ml	+,+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+,-
150 ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
300 ng/ml	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

7-ACL 200 Standard	11A0085-7ACL200	11A0086-7ACL200	11A0087-7ACL200
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100 ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150 ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
200 ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250 ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
300 ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
600 ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

CFYL Standard	11A0184-CFYL500	11A0185-CFYL500	11A0186-CFYL500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
500ng/mL	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

ZOP Standard	11A0643-ZOP	11A0644-ZOP	11A0645-ZOP
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
25ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
37.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
50ng/ml	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+
62.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

CAF Standard	11A0157-CAF	11A0158-CAF	11A0159-CAF
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
1000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,-,+,+,+,+
1250ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-

1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

CAT Standard	11A0148-CAT	11A0149-CAT	11A0150-CAT
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
112.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
150ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,-,+,+,+,+
187.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
225ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

TRO Standard	11A0598-TRO	11A0599-TRO	11A0600-TRO
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
175ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
262.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
350ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
437.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
525ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1050ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

ALP Standard	11A0094-ALP	11A0095-ALP	11A0096-ALP
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,-,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

AB-PINACA Standard	11A0067-K3 10	11A0068-K3 10	11A0069-K3 10
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
7.5ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
10ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
12.5ng/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
15ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
30ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

α-PVP1000 Standard	11A0112-PVP1000	11A0113-PVP1000	11A0114-PVP1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
1000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

α-PVP500 Standard	11A0112-PVP500	11A0113-PVP500	11A0114-PVP500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

CNB Standard	11A0787-CBN	11A0788-CBN	11A0789-CBN
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
325ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MPRD Standard	11A0409-MPRD	11A0410-MPRD	11A0411-MPRD
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,+,-	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

PGB Standard	11A0499-PGB	11A0500-PGB	11A0501-PGB
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
25ug/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
37.5ug/ml	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,+,+	-,-,-,-,-,-,-,-,-,+
50ug/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
62.5ug/ml	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,-,-	+,+,+,+,+,+,+,+,+,-
75ug/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
150ug/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

TZD Standard	11A0607-TZD	11A0608-TZD	11A0609-TZD
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
100ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,-
200ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
250ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

UR-144 Standard	11A0616-K4	11A0617-K4	11A0618-K4
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
12.5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
18.75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
25ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+

31.25ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
37.5ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

ZAL Standard	11A0625-ZAL	11A0626-ZAL	11A0627-ZAL
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

MES Standard	11A0382-MES	11A0383-MES	11A0384-MES
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
50ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
75ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
100ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+
125ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,-,-
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
300ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

GAB Standard	11A0283-GAB	11A0284-GAB	11A0285-GAB
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
1000ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
1500ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,-
2000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
2500ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

TLD 50 Standard	11A0580-TLD50	11A0581-TLD50	11A0582-TLD50
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
25ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
37.5ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
50ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
62.5ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,-
75ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
150ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

QTP 1000 Standard	11A0517-QTP1000	11A0518-QTP1000	11A0519-QTP1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
1000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
1250ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,-
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

PAP 500 Standard	11A0481-PAP500	11A0482-PAP500	11A0483-PAP500

Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

KRA 300 Standard	11A0301-KRA300	11A0302-KRA300	11A0303-KRA300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
375ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,-
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

CAR 2000 Standard	11A0166-CAR2000	11A0167-CAR2000	11A0168-CAR2000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
1000ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
1500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
2000ng/ml	-,-,-,-,-,-,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
2500ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
6000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

FLX 500 Standard	11A0265-FLX500	11A0266-FLX500	11A0267-FLX500
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
375ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,+
500ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
625ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,-
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

HMO250 Standard	11A1715-HMO250	11A1716-HMO250	11A1717-HMO250
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
125ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
187.5ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,-
250ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+
312.5ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-
375ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
750ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

HMO300 Standard	11A1715-HMO300	11A1716-HMO300	11A1717-HMO300
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
150ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
225ng/ml	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+	-,-,-,-,-,-,-,-,-,+
300ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+

375ng/ml	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,-	+,+,+,+,+,+,+,+,+,+
450ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
900ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

OZP 1000 Standard	11A0472-OZP1000	11A0473-OZP1000	11A0474-OZP1000
Free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
500ng/ml	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
750ng/ml	-,-,-,-,-,-,-,-,+,-	-,-,-,-,-,-,+,-,-,-	-,-,-,-,-,-,-,+,-,-
1000ng/ml	-,-,-,-,-,+,+,+,+,+	-,-,-,-,-,+,+,+,+,+	-,-,-,-,+,+,+,+,+,+
1250ng/ml	+,+,+,+,+,+,+,-,+,+	+,+,+,+,+,+,+,-,+,+	+,+,+,-,+,+,+,-,+,+
1500ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
3000ng/ml	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

Conclusion: The results indicated that each drug in the Multi-Drug Test Dip Card with/without Adulteration could detect above the cut-off concentration.

2.3 Analytical Specificity

The related compounds of each single drug in Dip Card will be spiked in drug-free urine, diluted sequentially to different concentrations and tested until the lowest concentration that has a negative result. The following compounds have negative result at their respective concentrations. And the cutoff concentrations were showed in the tables with "*". The specimens were tested in 5 replicates with visual interpretations occurring at 5 minutes after specimen application. Results are presented in table below.

Table: Interfering Substances

AMP 1,000:

Analytes	Conc. (ng/ml)	11A0103-AMP1000		11A0104-AMP1000		11A0105-AMP1000	
		Negative	Positive	Negative	Positive	Negative	Positive
D,L-Amphetamine sulfate	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
L-Amphetamine	12,500	5	0	5	0	5	0
	*25,000	2	3	2	3	2	3
	37,500	0	5	0	5	0	5
( ) 3,4-Methylenedioxy-amphetamine	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
Phentermine	500	5	0	5	0	5	0
	*1000	2	3	3	2	2	3
	1500	0	5	0	5	0	5
	25,000	5	0	5	0	5	0

Maprotiline	*50,000	4	1	3	2	2	3
	75,000	0	5	0	5	0	5
Methoxyphenamine	3,000	5	0	5	0	5	0
	*6,000	2	3	3	2	2	3
	9,000	0	5	0	5	0	5
D-Amphetamine	500	5	0	5	0	5	0
	*1,000	2	3	3	2	2	3
	1,500	0	5	0	5	0	5

AMP 500:

Analytes	**Conc. (ng/ml)**	**11A0103-AMP500**		**11A0104-AMP500**		**11A0105-AMP500**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
D,L-Amphetamine sulfate	75	5	0	5	0	5	0
	*150	3	2	3	2	2	3
	225	0	5	0	5	0	5
L-Amphetamine	6,250	5	0	5	0	5	0
	*12,500	2	3	2	3	2	3
	18,750	0	5	0	5	0	5
( )3,4-Methylenedioxy-amphetamine	125	5	0	5	0	5	0
	*250	2	3	3	2	2	3
	375	0	5	0	5	0	5
Phentermine	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
Maprotiline	12,500	5	0	5	0	5	0
	*25,000	4	1	3	2	2	3
	37,500	0	5	0	5	0	5
Methoxyphenamine	1,500	5	0	5	0	5	0
	*3,000	2	3	3	2	2	3
	4,500	0	5	0	5	0	5
D-Amphetamine	250	5	0	5	0	5	0
	*500	2	3	2	3	2	3
	750	0	5	0	5	0	5

AMP 300:

	Conc.	**11A0103-AMP300**	**11A0104-AMP300**	**11A0105-AMP300**

Analytes	(ng/ml)	Negative	Positive	Negative	Positive	Negative	Positive
D,L-Amphetamine sulfate	37.5	5	0	5	0	5	0
	*75	3	2	3	2	2	3
	112.5	0	5	0	5	0	5
L-Amphetamine	5,000	5	0	5	0	5	0
	*10,000	2	3	2	3	2	3
	15,000	0	5	0	5	0	5
3,4-Methylenedioxy-amphetamine	75	5	0	5	0	5	0
	*150	2	3	3	2	2	3
	225	0	5	0	5	0	5
Phentermine	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Maprotiline	6,250	5	0	5	0	5	0
	*15,000	4	1	3	2	2	3
	18,750	0	5	0	5	0	5
Methoxyphenamine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
D-Amphetamine	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5

BAR 300:

Analytes	Conc. (ng/ml)	11A0121-BAR300		11A0122-BAR300		11A0123-BAR300	
		Negative	Positive	Negative	Positive	Negative	Positive
Amobarbital	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
5,5-Diphenylhydantoin	4,000	5	0	5	0	5	0
	*8,000	2	3	3	2	2	3
	12,000	0	5	0	5	0	5
Allobarbital	300	5	0	5	0	5	0
	*600	3	2	3	2	2	3

	900	0	5	0	5	0	5
Barbital	4,000	5	0	5	0	5	0
	*8,000	2	3	2	3	2	3
	12,000	0	5	0	5	0	5
Talbutal	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Cyclopentobarbital	15,000	5	0	5	0	5	0
	*30,000	2	3	3	2	2	3
	45,000	0	5	0	5	0	5
Pentobarbital	4,000	5	0	5	0	5	0
	*8,000	2	3	3	2	3	2
	12,000	0	5	0	5	0	5
Alphenol	300	5	0	5	0	5	0
	*600	2	3	3	2	2	3
	900	0	5	0	5	0	5
Aprobarbital	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
Butabarbital	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Butalbital	4,000	5	0	5	0	5	0
	*8,000	2	3	3	2	2	3
	12,000	0	5	0	5	0	5
Butethal	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
Phenobarbital	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Secobarbital	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5

BAR 200:

Analytes	Conc. (ng/ml)	11A0121-BAR200		11A0122-BAR200		11A0123-BAR200	
		Negative	Positive	Negative	Positive	Negative	Positive
Amobarbital	1,500	5	0	5	0	5	0
	*3,000	2	3	3	2	2	3
	4,500	0	5	0	5	0	5
5,5-Diphenylhydantoin	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Allobarbital	200	5	0	5	0	5	0
	*400	1	4	3	2	2	3
	600	0	5	0	5	0	5
Barbital	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Talbutal	75	5	0	5	0	5	0
	*150	2	3	3	2	2	3
	225	0	5	0	5	0	5
Cyclopentobarbital	10,000	5	0	5	0	5	0
	*20,000	2	3	3	2	2	3
	30,000	0	5	0	5	0	5
Pentobarbital	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	3	2
	7,500	0	5	0	5	0	5
Alphenol	200	5	0	5	0	5	0
	*400	2	3	3	2	2	3
	600	0	5	0	5	0	5
Aprobarbital	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Butabarbital	75	5	0	5	0	5	0
	*150	2	3	3	2	2	3
	225	0	5	0	5	0	5
	2,500	5	0	5	0	5	0

Butalbital	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Butethal	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Phenobarbital	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Secobarbital	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5

BUP10:

Analytes	**Conc. (ng/ml)**	**11A0130-BUP10**		**11A0131-BUP10**		**11A0132-BUP10**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Buprenorphine	5	5	0	5	0	5	0
	*10	3	2	3	2	2	3
	15	0	5	0	5	0	5
Buprenorphine 3-D-Glucuron ide	25	5	0	5	0	5	0
	*50	2	3	2	3	2	3
	75	0	5	0	5	0	5
Norbuprenorphine	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5
Norbuprenorphine 3-D-Glucuron ide	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5

BUP 5

Analytes	**Conc. (ng/ml)**	**11A0130-BUP5**		**11A0131-BUP5**		**11A0132-BUP5**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Buprenorphine	2.5	5	0	5	0	5	0
	*5	3	2	3	2	2	3
	7.5	0	5	0	5	0	5
Buprenorphine	12.5	5	0	5	0	5	0
	*25	2	3	2	3	2	3

3-D-Glucuron ide	37.5	0	5	0	5	0	5
Norbuprenorphine	12.5	5	0	5	0	5	0
	*25	3	2	3	2	2	3
	37.5	0	5	0	5	0	5
Norbuprenorphine 3-D-Glucuron ide	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5

BZO 500:

Analytes	Conc. (ng/ml)	11A0139-BZO500		11A0140-BZO500		11A0141-BZO500	
		Negative	Positive	Negative	Positive	Negative	Positive
Alprazolam	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
a-hydroxyalprazolam	1,250	5	0	5	0	5	0
	*2,500	2	3	2	3	3	2
	3,750	0	5	0	5	0	5
Bromazepam	750	5	0	5	0	5	0
	*1,500	2	3	3	2	2	3
	2,250	0	5	0	5	0	5
Chlordiazepoxide	750	5	0	5	0	5	0
	*1,500	3	2	2	3	2	3
	2,250	0	5	0	5	0	5
Clobazam	150	5	0	5	0	5	0
	*300	3	2	2	3	2	3
	450	0	5	0	5	0	5
Clonazepam	400	5	0	5	0	5	0
	*800	3	2	2	3	2	3
	1,200	0	5	0	5	0	5
Clorazepate dipotassium	400	5	0	5	0	5	0
	*800	2	3	2	3	2	3
	1,200	0	5	0	5	0	5
Delorazepam	750	5	0	5	0	5	0
	*1,500	2	3	2	3	2	3

	2,250	0	5	0	5	0	5
Desalkylflurazepam	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
Flunitrazepam	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
( ) Lorazepam	2,500	5	0	5	0	5	0
	*5,000	2	3	2	3	2	3
	7,500	0	5	0	5	0	5
RS-Lorazepam glucuronide	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
Midazolam	5,000	5	0	5	0	5	0
	*10,000	3	2	2	3	2	3
	15,000	0	5	0	5	0	5
Nitrazepam	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Norchlordiazepoxide	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
Nordiazepam	750	5	0	5	0	5	0
	*1,500	3	2	2	3	2	3
	2,250	0	5	0	5	0	5
Oxazepam	250	5	0	5	0	5	0
	*500	2	3	2	3	2	3
	750	0	5	0	5	0	5
Temazepam	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Diazepam	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5

Estazolam	5,000	5	0	5	0	5	0
	*10,000	3	2	3	2	2	3
	15,000	0	5	0	5	0	5
Triazolam	2,500	5	0	5	0	5	0
	*5,000	3	2	3	2	2	3
	7,500	0	5	0	5	0	5

BZO 300:

Analytes	**Conc. (ng/ml)**	**11A0139-BZO300**		**11A0140-BZO300**		**11A0141-BZO300**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Alprazolam	50	5	0	5	0	5	0
	*100	2	3	2	3	2	3
	150	0	5	0	5	0	5
a-hydroxyalprazolam	750	5	0	5	0	5	0
	*1,500	2	3	2	3	3	2
	2,250	0	5	0	5	0	5
Bromazepam	450	5	0	5	0	5	0
	*900	2	3	3	2	2	3
	1,350	0	5	0	5	0	5
Chlordiazepoxide	450	5	0	5	0	5	0
	*900	3	2	2	3	2	3
	1,350	0	5	0	5	0	5
Clobazam	100	5	0	5	0	5	0
	*200	3	2	2	3	2	3
	300	0	5	0	5	0	5
Clonazepam	250	5	0	5	0	5	0
	*500	3	2	2	3	2	3
	750	0	5	0	5	0	5
Clorazepate dipotassium	250	5	0	5	0	5	0
	*500	2	3	2	3	2	3
	750	0	5	0	5	0	5
Delorazepam	450	5	0	5	0	5	0
	*900	2	3	2	3	2	3
	1,350	0	5	0	5	0	5
	100	5	0	5	0	5	0

Desalkylflurazepam	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
Flunitrazepam	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
( ) Lorazepam	1,500	5	0	5	0	5	0
	*3,000	2	3	2	3	2	3
	4,500	0	5	0	5	0	5
RS-Lorazepam glucuronide	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
Midazolam	3,000	5	0	5	0	5	0
	*6,000	3	2	2	3	2	3
	9,000	0	5	0	5	0	5
Nitrazepam	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Norchlordiazepoxide	50	5	0	5	0	5	0
	*100	2	3	2	3	2	3
	150	0	5	0	5	0	5
Nordiazepam	450	5	0	5	0	5	0
	*900	3	2	2	3	2	3
	1,350	0	5	0	5	0	5
Oxazepam	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
Temazepam	50	5	0	5	0	5	0
	*100	2	3	3	2	2	3
	150	0	5	0	5	0	5
Diazepam	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Estazolam	3,000	5	0	5	0	5	0
	*6,000	3	2	3	2	2	3

	9,000	0	5	0	5	0	5
Triazolam	1,500	5	0	5	0	5	0
	*3,000	3	2	3	2	2	3
	4,500	0	5	0	5	0	5

BZO 200:

Analytes	Conc. (ng/ml)	11A0139-BZO200		11A0140-BZO200		11A0141-BZO200	
		Negative	Positive	Negative	Positive	Negative	Positive
Alprazolam	35	5	0	5	0	5	0
	*70	2	3	2	3	2	3
	105	0	5	0	5	0	5
a-hydroxyalprazolam	500	5	0	5	0	5	0
	*1,000	2	3	2	3	3	2
	1,500	0	5	0	5	0	5
Bromazepam	300	5	0	5	0	5	0
	*600	2	3	3	2	2	3
	900	0	5	0	5	0	5
Chlordiazepoxide	300	5	0	5	0	5	0
	*600	3	2	2	3	2	3
	900	0	5	0	5	0	5
Clobazam	60	5	0	5	0	5	0
	*120	3	2	2	3	2	3
	180	0	5	0	5	0	5
Clonazepam	150	5	0	5	0	5	0
	*300	3	2	2	3	2	3
	450	0	5	0	5	0	5
Clorazepate dipotassium	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
Delorazepam	300	5	0	5	0	5	0
	*600	2	3	2	3	2	3
	900	0	5	0	5	0	5
Desalkylflurazepam	60	5	0	5	0	5	0
	*120	2	3	2	3	2	3
	180	0	5	0	5	0	5

Flunitrazepam	60	5	0	5	0	5	0
	*120	2	3	2	3	2	3
	180	0	5	0	5	0	5
( ) Lorazepam	1,000	5	0	5	0	5	0
	*2,000	2	3	2	3	2	3
	3,000	0	5	0	5	0	5
RS-Lorazepam glucuronide	60	5	0	5	0	5	0
	*120	2	3	2	3	2	3
	180	0	5	0	5	0	5
Midazolam	2,000	5	0	5	0	5	0
	*4,000	3	2	2	3	2	3
	6,000	0	5	0	5	0	5
Nitrazepam	60	5	0	5	0	5	0
	*120	2	3	3	2	2	3
	180	0	5	0	5	0	5
Norchlordiazepoxide	35	5	0	5	0	5	0
	*70	2	3	2	3	2	3
	105	0	5	0	5	0	5
Nordiazepam	300	5	0	5	0	5	0
	*600	3	2	2	3	2	3
	900	0	5	0	5	0	5
Oxazepam	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
Temazepam	35	5	0	5	0	5	0
	*70	2	3	3	2	2	3
	105	0	5	0	5	0	5
Diazepam	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Estazolam	2,000	5	0	5	0	5	0
	*4,000	3	2	3	2	2	3
	6,000	0	5	0	5	0	5
	1,000	5	0	5	0	5	0

Triazolam	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5

BZO 100:

Analytes	Conc. (ng/ml)	11A0139-BZO100		11A0140-BZO100		11A0141-BZO100	
		Negative	Positive	Negative	Positive	Negative	Positive
Alprazolam	20	5	0	5	0	5	0
	*40	2	3	2	3	2	3
	60	0	5	0	5	0	5
a-hydroxyalprazolam	250	5	0	5	0	5	0
	*500	2	3	2	3	3	2
	750	0	5	0	5	0	5
Bromazepam	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Chlordiazepoxide	150	5	0	5	0	5	0
	*300	3	2	2	3	2	3
	450	0	5	0	5	0	5
Clobazam	30	5	0	5	0	5	0
	*60	3	2	2	3	2	3
	90	0	5	0	5	0	5
Clonazepam	75	5	0	5	0	5	0
	*150	3	2	2	3	2	3
	225	0	5	0	5	0	5
Clorazepate dipotassium	75	5	0	5	0	5	0
	*150	2	3	2	3	2	3
	225	0	5	0	5	0	5
Delorazepam	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
Desalkylflurazepam	30	5	0	5	0	5	0
	*60	2	3	2	3	2	3
	90	0	5	0	5	0	5
Flunitrazepam	30	5	0	5	0	5	0
	*60	2	3	2	3	2	3

	90	0	5	0	5	0	5
( ) Lorazepam	500	5	0	5	0	5	0
	*1,000	2	3	2	3	2	3
	1,500	0	5	0	5	0	5
RS-Lorazepam glucuronide	30	5	0	5	0	5	0
	*60	2	3	2	3	2	3
	90	0	5	0	5	0	5
Midazolam	1,000	5	0	5	0	5	0
	*2,000	3	2	2	3	2	3
	3,000	0	5	0	5	0	5
Nitrazepam	30	5	0	5	0	5	0
	*60	2	3	3	2	2	3
	90	0	5	0	5	0	5
Norchlordiazepoxide	20	5	0	5	0	5	0
	*40	2	3	2	3	2	3
	60	0	5	0	5	0	5
Nordiazepam	150	5	0	5	0	5	0
	*300	3	2	2	3	2	3
	450	0	5	0	5	0	5
Oxazepam	50	5	0	5	0	5	0
	*100	2	3	2	3	2	3
	150	0	5	0	5	0	5
Temazepam	20	5	0	5	0	5	0
	*40	2	3	3	2	2	3
	60	0	5	0	5	0	5
Diazepam	50	5	0	5	0	5	0
	*100	2	3	3	2	2	3
	150	0	5	0	5	0	5
Estazolam	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
Triazolam	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5

COC 300:

Analytes	Conc. (ng/ml)	11A0211-COC300		11A0212-COC300		11A0213-COC300	
		Negative	Positive	Negative	Positive	Negative	Positive
Benzoylecgonine	150	5	0	5	0	5	0
	*300	1	4	3	2	2	3
	450	0	5	0	5	0	5
Cocaine HCl	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
Cocaethylene	10,000	5	0	5	0	5	0
	*20,000	4	1	1	4	2	3
	30,000	0	5	0	5	0	5
Ecgonine	15,000	5	0	5	0	5	0
	*30,000	3	2	3	2	2	3
	45,000	0	5	0	5	0	5

COC 100:

Analytes	Conc. (ng/ml)	11A0211-COC100		11A0212-COC100		11A0213-COC100	
		Negative	Positive	Negative	Positive	Negative	Positive
Benzoylecgonine	50	5	0	5	0	5	0
	*100	2	3	3	2	2	3
	150	0	5	0	5	0	5
Cocaine HCl	40	5	0	5	0	5	0
	*80	3	2	3	2	2	3
	120	0	5	0	5	0	5
Cocaethylene	3,500	5	0	5	0	5	0
	*7,000	2	3	3	2	2	3
	10,500	0	5	0	5	0	5
Ecgonine	5,000	5	0	5	0	5	0
	*10,000	1	4	3	2	2	3
	15,000	0	5	0	5	0	5

COC 150

Analytes	Conc. (ng/ml)	11A0211-COC150		11A0212-COC150		11A0213-COC150	
		Negative	Positive	Negative	Positive	Negative	Positive
	75	5	0	5	0	5	0

Benzoylecgonine	*150	2	3	4	1	2	3
	225	0	5	0	5	0	5
Cocaine HCl	60	5	0	5	0	5	0
	*120	3	2	3	2	3	2
	180	0	5	0	5	0	5
Cocaethylene	5,000	5	0	5	0	5	0
	*10,000	4	1	3	2	2	3
	15,000	0	5	0	5	0	5
Ecgonine	7,500	5	0	5	0	5	0
	*15,000	3	2	3	2	2	3
	22,500	0	5	0	5	0	5

COC 200

Analytes	**Conc. (ng/ml)**	**11A0211-COC200**		**11A0212-COC200**		**11A0213-COC200**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Benzoylecgonine	100	5	0	5	0	5	0
	*200	1	4	3	2	2	3
	300	0	5	0	5	0	5
Cocaine HCl	67.5	5	0	5	0	5	0
	*135	3	2	3	2	2	3
	202.5	0	5	0	5	0	5
Cocaethylene	6,750	5	0	5	0	5	0
	*13,500	4	1	3	2	2	3
	20,250	0	5	0	5	0	5
Ecgonine	10,500	5	0	5	0	5	0
	*20,000	2	3	3	2	2	3
	30,000	0	5	0	5	0	5

KET 1000:

Analytes	**Conc.**	**11A0292-KET1000**		**11A0293-KET1000**		**11A0294-KET1000**	
	(ng/ml)	**Negative**	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Ketamine	500	5	0	5	0	5	0
	*1,000	2	3	3	2	2	3
	1,500	0	5	0	5	0	5

Benzphetamine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
(+) Chlorpheniramine	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	37,500	0	5	0	5	0	5
Clonidine	50,000	5	0	5	0	5	0
	*100,000	2	3	2	3	2	3
	150,000	0	5	0	5	0	5
Dextromethorpha n	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Disopyramide	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
EDDP	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	3	2
	75,000	0	5	0	5	0	5
Mephentermine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
(1R, 2S) - (-)-Ephedrine	50,000	5	0	5	0	5	0
	*100,000	2	3	3	2	2	3
	150,000	0	5	0	5	0	5
4-Hydroxyphency clidine	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5
Levorphanol	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5
MDE	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5

Tetrahydrozoline	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
d-Methamphetamine	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5
l-Methamphetamine	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5
Methoxyphenamine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
(+)3,4-Methylendioxymethamphetamine (MDMA)	50,000	5	0	5	0	5	0
	*100,000	2	3	3	2	2	3
	150,000	0	5	0	5	0	5
d-Norpropoxyphene	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Pentazocine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Phencyclidine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Promazine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Promethazine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
	25,000	5	0	5	0	5	0

Thioridazine	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5
Meperidine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5

KET 500:

Analytes	Conc. (ng/ml)	11A0292-KET500		11A0293-KET500		11A0294-KET500	
		Negative	Positive	Negative	Positive	Negative	Positive
Ketamine	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
Benzphetamine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
(+) Chlorpheniramine	6,250	5	0	5	0	5	0
	*12,500	3	2	3	2	2	3
	18,750	0	5	0	5	0	5
Clonidine	25,000	5	0	5	0	5	0
	*50,000	2	3	2	3	2	3
	75,000	0	5	0	5	0	5
Dextromethorphan	500	5	0	5	0	5	0
	*1,000	2	3	3	2	2	3
	1,500	0	5	0	5	0	5
Disopyramide	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
EDDP	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	3	2
	37,500	0	5	0	5	0	5
Mephentermine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
(1R, 2S) -	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3

(-)-Ephedrine	75,000	0	5	0	5	0	5
4-Hydroxyphencyclidine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Levorphanol	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
MDE	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Tetrahydrozoline	125	5	0	5	0	5	0
	*250	2	3	3	2	2	3
	325	0	5	0	5	0	5
d-Methamphetamine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
l-Methamphetamine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Methoxyphenamine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
(+)3,4-Methylendioxymethamphetamine (MDMA)	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	3	2
	75,000	0	5	0	5	0	5
d-Norpropoxyphene	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
Pentazocine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
Phencyclidine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5

Promazine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
Promethazine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5
Thioridazine	12,500	5	0	5	0	5	0
	*25,000	2	3	3	2	2	3
	37,500	0	5	0	5	0	5
Meperidine	6,250	5	0	5	0	5	0
	*12,500	2	3	3	2	2	3
	18,750	0	5	0	5	0	5

KET 300:

Analytes	**Conc. (ng/ml)**	**11A0292-KET300**		**11A0293-KET300**		**11A0294-KET300**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Ketamine	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Benzphetamine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5
(+) Chlorpheniramine	3,125	5	0	5	0	5	0
	*6,250	3	2	3	2	2	3
	9,375	0	5	0	5	0	5
Clonidine	15,000	5	0	5	0	5	0
	*30,000	2	3	2	3	2	3
	45,000	0	5	0	5	0	5
Dextromethorphan	300	5	0	5	0	5	0
	*600	2	3	3	2	2	3
	900	0	5	0	5	0	5
Disopyramide	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5
	7,500	5	0	5	0	5	0

EDDP	*15,000	2	3	3	2	3	2
	22,500	0	5	0	5	0	5
Mephentermine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5
(1R, 2S) - (-)-Ephedrine	15,000	5	0	5	0	5	0
	*30,000	2	3	3	2	2	3
	45,000	0	5	0	5	0	5
4-Hydroxyphencyclidine	7,500	5	0	5	0	5	0
	*15,000	2	3	3	2	2	3
	22,500	0	5	0	5	0	5
Levorphanol	7,500	5	0	5	0	5	0
	*15,000	2	3	3	2	2	3
	22,500	0	5	0	5	0	5
MDE	7,500	5	0	5	0	5	0
	*15,000	2	3	3	2	2	3
	22,500	0	5	0	5	0	5
Tetrahydrozoline	75	5	0	5	0	5	0
	*150	2	3	3	2	2	3
	225	0	5	0	5	0	5
d-Methamphetamine	7,500	5	0	5	0	5	0
	*15,000	2	3	3	2	2	3
	22,500	0	5	0	5	0	5
l-Methamphetamine	7,500	5	0	5	0	5	0
	*15,000	2	3	3	2	2	3
	22,500	0	5	0	5	0	5
Methoxyphenamine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5
(+)3,4-Methylendioxymethamphetamine (MDMA)	15,000	5	0	5	0	5	0
	*30,000	3	2	3	2	2	3
	45,000	0	5	0	5	0	5

d-Norpropoxyphene	3,125	5	0	5	0	5	0
	*6,250	2	3	2	3	2	3
	9,375	0	5	0	5	0	5
Pentazocine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5
Phencyclidine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5
Promazine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	3	2
	9,375	0	5	0	5	0	5
Promethazine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5
Thioridazine	7,500	5	0	5	0	5	0
	*15,000	2	3	3	2	2	3
	22,500	0	5	0	5	0	5
Meperidine	3,125	5	0	5	0	5	0
	*6,250	2	3	3	2	2	3
	9,375	0	5	0	5	0	5

KET100

Analytes	Conc. (ng/ml)	11A0292-KET100		11A0293-KET100		11A0294-KET100	
		Negative	Positive	Negative	Positive	Negative	Positive
Ketamine	50	5	0	5	0	5	0
	*100	2	3	3	2	2	3
	150	0	5	0	5	0	5
Benzphetamine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
(+) Chlorpheniramine	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
	5,000	5	0	5	0	5	0

Clonidine	*10,000	2	3	2	3	2	3
	15,000	0	5	0	5	0	5
Dextromethorphan	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Disopyramide	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
EDDP	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	3	2
	7,500	0	5	0	5	0	5
Mephentermine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
(1R, 2S) - (-)-Ephedrine	5,000	5	0	5	0	5	0
	*10,000	2	3	3	2	2	3
	15,000	0	5	0	5	0	5
4-Hydroxyphencyclidine	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Levorphanol	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
MDE	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Tetrahydrozoline	25	5	0	5	0	5	0
	*50	2	3	3	2	2	3
	75	0	5	0	5	0	5
d-Methamphetamin e	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
	2,500	5	0	5	0	5	0

l-Methamphetamine	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Methoxyphenamine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
(+)3,4-Methylendioxymethamphetamine (MDMA)	5,000	5	0	5	0	5	0
	*10,000	2	3	3	2	2	3
	15,000	0	5	0	5	0	5
d-Norpropoxyphene	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Pentazocine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Phencyclidine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Promazine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Promethazine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Thioridazine	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Meperidine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5

MDMA 1000:

Analytes	**Conc. (ng/ml)**	**11A0337-MDMA1000**		**11A0338-MDMA1000**		**11A0339-MDMA1000**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
( )	500	5	0	5	0	5	0

3,4-Methylenedioxymethamphetamine HCl (MDMA)	*1,000	2	3	3	2	2	3
	1,500	0	5	0	5	0	5
( ) 3,4-Methylenedioxyamphetamine HCl (MDA)	3,000	5	0	5	0	5	0
	*6,000	2	3	3	2	2	3
	9,000	0	5	0	5	0	5
3,4-Methylenedioxyethyl-amphetamine (MDE)	300	5	0	5	0	5	0
	*600	1	4	3	2	2	3
	900	0	5	0	5	0	5

MDMA 500:

Analytes	Conc. (ng/ml)	11A0337-MDMA500		11A0338-MDMA500		11A0339-MDMA500	
		Negative	Positive	Negative	Positive	Negative	Positive
( ) 3,4-Methylenedioxymethamphetamine HCl (MDMA)	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
( ) 3,4-Methylenedioxyamphetamine HCl (MDA)	1,500	5	0	5	0	5	0
	*3,000	2	3	3	2	2	3
	4,500	0	5	0	5	0	5
3,4-Methylenedioxyethyl-amphetamine (MDE)	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5

MDMA 300:

Analytes	Conc. (ng/ml)	11A0337-MDMA300		11A0338-MDMA300		11A0339-MDMA300	
		Negative	Positive	Negative	Positive	Negative	Positive
( ) 3,4-Methylenedioxymethamphetamine HCl (MDMA)	150	5	0	5	0	5	0
	*300	3	2	4	1	2	3
	450	0	5	0	5	0	5
( ) 3,4-Methylenedioxyamphetamine HCl (MDA)	900	5	0	5	0	5	0
	*1,800	1	4	3	2	2	3
	2,700	0	5	0	5	0	5
3,4-Methylenedioxyethyl-amphetamine (MDE)	90	5	0	5	0	5	0
	*180	2	3	3	2	2	3
	270	0	5	0	5	0	5

MET 1000:

Analytes	Conc. (ng/ml)	11A0364-MET1000		11A0365-MET1000		11A0366-MET1000	
		Negative	Positive	Negative	Positive	Negative	Positive
-Hydroxymethamphetamine	12,500	5	0	5	0	5	0
	*25,000	2	3	2	3	2	3
	37,500	0	5	0	5	0	5
D-Methamphetamine	500	5	0	5	0	5	0
	*1,000	2	3	3	2	2	3
	1,500	0	5	0	5	0	5
L-Methamphetamine	10,000	5	0	5	0	5	0
	*20,000	2	3	2	3	2	3
	30,000	0	5	0	5	0	5
( )-3,4-Methylened ioxy-methampheta mine	6,250	5	0	5	0	5	0
	*12,500	2	3	2	3	3	2
	18,750	0	5	0	5	0	5
Mephentermine	25,000	5	0	5	0	5	0
	*50,000	3	2	2	3	3	2
	75,000	0	5	0	5	0	5

MET 500:

Analytes	Conc. (ng/ml)	11A0364-MET500		11A0365-MET500		11A0366-MET500	
		Negative	Positive	Negative	Positive	Negative	Positive
-Hydroxymethamphetamine	6,250	5	0	5	0	5	0
	*12,500	2	3	2	3	2	3
	18,750	0	5	0	5	0	5
D-Methamphetamine	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
L-Methamphetamine	5,000	5	0	5	0	5	0
	*10,000	2	3	2	3	2	3
	15,000	0	5	0	5	0	5
( )-3,4-Methylenedi oxy-methamphetam ine	3,125	5	0	5	0	5	0
	*6,250	2	3	2	3	3	2
	9,375	0	5	0	5	0	5
	6,250	5	0	5	0	5	0

Mephentermine	*25,000	3	2	2	3	3	2
	18,750	0	5	0	5	0	5

MET 300:

Analytes	Conc. (ng/ml)	11A0364-MET300		11A0365-MET300		11A0366-MET300	
		Negative	Positive	Negative	Positive	Negative	Positive
-Hydroxymethamphetamine	3,750	5	0	5	0	5	0
	*7,500	2	3	2	3	2	3
	11,250	0	5	0	5	0	5
D-Methamphetamine	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
L-Methamphetamine	3,000	5	0	5	0	5	0
	*6,000	2	3	2	3	2	3
	9,000	0	5	0	5	0	5
( )-3,4-Methylene dioxy-methamphetamine	1,875	5	0	5	0	5	0
	*3,750	2	3	2	3	3	2
	5,625	0	5	0	5	0	5
Mephentermine	7,500	5	0	5	0	5	0
	*15,000	3	2	2	3	3	2
	22,500	0	5	0	5	0	5

MET 200:

Analytes	Conc. (ng/ml)	11A0364-MET200		11A0365-MET200		11A0366-MET200	
		Negative	Positive	Negative	Positive	Negative	Positive
-Hydroxymethamphetamine	2,500	5	0	5	0	5	0
	*5,000	2	3	2	3	2	3
	7,500	0	5	0	5	0	5
D-Methamphetamine	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
L-Methamphetamine	2,000	5	0	5	0	5	0
	*4,000	2	3	2	3	2	3
	6,000	0	5	0	5	0	5
( )-3,4-Methylene dioxy-	1,250	5	0	5	0	5	0
	*2,500	2	3	2	3	3	2

methamphet amine	3,750	0	5	0	5	0	5
Mephentermine	5,000	5	0	5	0	5	0
	*10,000	3	2	2	3	3	2
	15,000	0	5	0	5	0	5

MOP 300:

Analytes	**Conc. (ng/ml)**	**11A0418-MQL**		**11A0419-MQL**		**11A0420-MQL**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Codeine	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Levorphanol	750	5	0	5	0	5	0
	*1,500	2	3	2	3	2	3
	2,250	0	5	0	5	0	5
Morphine-3-β-D-Glucuronide	400	5	0	5	0	5	0
	*800	2	3	3	2	2	3
	1200	0	5	0	5	0	5
Ethylmorphine	3,000	5	0	5	0	5	0
	*6,000	2	3	3	2	2	3
	9,000	0	5	0	5	0	5
Hydrocodone	25,000	5	0	5	0	5	0
	*50,000	4	1	4	1	2	3
	75,000	0	5	0	5	0	5
Hydromorphone	1,500	5	0	5	0	5	0
	*3,000	2	3	3	2	2	3
	4,500	0	5	0	5	0	5
6-Monoacethyl morphine	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Norcodeine	3,000	5	0	5	0	5	0
	*6,000	2	3	3	2	2	3
	9,000	0	5	0	5	0	5
Normorphone	25,000	5	0	5	0	5	0
	*50,000	2	3	1	4	1	4
	75,000	0	5	0	5	0	5

Oxycodone	15,000	5	0	5	0	5	0
	*30,000	2	3	3	2	2	3
	45,000	0	5	0	5	0	5
Oxymorphone	25,000	5	0	5	0	5	0
	*50,000	4	1	4	1	4	1
	75,000	0	5	0	5	0	5
Procaine	7,500	5	0	5	0	5	0
	*15,000	2	3	3	2	2	3
	22,500	0	5	0	5	0	5
Thebaine	3,000	5	0	5	0	5	0
	*6,000	2	3	3	2	2	3
	9,000	0	5	0	5	0	5
Morphine	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5

MOP 100:

Analytes	**Conc. (ng/ml)**	**11A0391-MOP100**		**11A0392-MOP100**		**11A0393-MOP100**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Codeine	40	5	0	5	0	5	0
	*80	3	2	3	2	2	3
	120	0	5	0	5	0	5
Levorphanol	250	5	0	5	0	5	0
	*500	2	3	2	3	2	3
	750	0	5	0	5	0	5
Morphine-3-β-D-Glucuronide	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Ethylmorphine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Hydrocodone	10,000	5	0	5	0	5	0
	*20,000	4	1	4	1	2	3
	30,000	0	5	0	5	0	5
	500	5	0	5	0	5	0

Hydromorphone	*1,000	2	3	3	2	2	3
	1,500	0	5	0	5	0	5
6-Monoacethyl morphine	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Norcodeine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Normorphone	10,000	5	0	5	0	5	0
	*20,000	2	3	1+	4	1	4
	30,000	0	5	0	5	0	5
Oxycodone	5,000	5	0	5	0	5	0
	*10,000	2	3	3	2	2	3
	15,000	0	5	0	5	0	5
Oxymorphone	10,000	5	0	5	0	5	0
	*20,000	4	1	4	1	4	1
	30,000	0	5	0	5	0	5
Procaine	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5
Thebaine	1,000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
Morphine	50	5	0	5	0	5	0
	*100	2	3	3	2	2	3
	150	0	5	0	5	0	5

MOP 200

Analytes	**Conc. (ng/ml)**	**11A0391-MOP200**		**11A0392-MOP200**		**11A0393-MOP200**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Codeine	80	5	0	5	0	5	0
	*160	3	2	3	2	2	3
	240	0	5	0	5	0	5
Levorphanol	500	5	0	5	0	5	0
	*1000	2	3	2	3	2	3

	1500	0	5	0	5	0	5
Morphine-3-β-D-Glucuronide	300	5	0	5	0	5	0
	*600	2	3	3	2	2	3
	900	0	5	0	5	0	5
Ethylmorphine	2,000	5	0	5	0	5	0
	*4,000	2	3	3	2	2	3
	6,000	0	5	0	5	0	5
Hydrocodone	20,000	5	0	5	0	5	0
	*40,000	4	1	4	1	2	3
	60,000	0	5	0	5	0	5
Hydromorphone	1000	5	0	5	0	5	0
	*2,000	2	3	3	2	2	3
	3,000	0	5	0	5	0	5
6-Monoacethyl morphine	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Norcodeine	2,000	5	0	5	0	5	0
	*4,000	2	3	3	2	2	3
	6,000	0	5	0	5	0	5
Normorphone	20,000	5	0	5	0	5	0
	*40,000	2	3	1+	4	1	4
	60,000	0	5	0	5	0	5
Oxycodone	10,000	5	0	5	0	5	0
	*20,000	2	3	3	2	2	3
	30,000	0	5	0	5	0	5
Oxymorphone	20,000	5	0	5	0	5	0
	*40,000	4	1	4	1	4	1
	60,000	0	5	0	5	0	5
Procaine	5,000	5	0	5	0	5	0
	*10,000	2	3	3	2	2	3
	15,000	0	5	0	5	0	5
Thebaine	2,000	5	0	5	0	5	0
	*4,000	2	3	3	2	2	3
	6,000	0	5	0	5	0	5

Morphine	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5

MQL

Analytes	Conc. (ng/ml)	11A0418-MQL		11A0419-MQL		11A0420-MQL	
		Negative	Positive	Negative	Positive	Negative	Positive
Methaqualone	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	600	0	5	0	5	0	5

MTD 300:

Analytes	Conc. (ng/ml)	11A0427-MTD300		11A0428-MTD300		11A0429-MTD300	
		Negative	Positive	Negative	Positive	Negative	Positive
Methadone	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Doxylamine	50,000	5	0	5	0	5	0
	*100,000	2	3	2	3	2	3
	150,000	0	5	0	5	0	5

MTD 200:

Analytes	Conc. (ng/ml)	11A0427-MTD200		11A0428-MTD200		11A0429-MTD200	
		Negative	Positive	Negative	Positive	Negative	Positive
Methadone	100	5	0	5	0	5	0
	*200	3	2	3	2	3	2
	300	0	5	0	5	0	5
Doxylamine	32,500	5	0	5	0	5	0
	*65,000	2	3	2	3	2	3
	97,500	0	5	0	5	0	5

OPI:

Analytes	Conc. (ng/ml)	11A0454-OPI		11A0455-OPI		11A0456-OPI	
		Negative	Positive	Negative	Positive	Negative	Positive
Codeine	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
	1,500	5	0	5	0	5	0

Ethylmorphine	*3,000	2	3	2	3	2	3
	4,500	0	5	0	5	0	5
Hydrocodone	25,000	5	0	5	0	5	0
	*50,000	3	2	3	2	2	3
	75,000	0	5	0	5	0	5
Hydromorpho ne	7,500	5	0	5	0	5	0
	*15,000	2	3	2	3	2	3
	22,500	0	5	0	5	0	5
Levorphanol	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	37,500	0	5	0	5	0	5
6-Monoacetyl morphine	1,500	5	0	5	0	5	0
	*3,000	2	3	2	3	2	3
	4,500	0	5	0	5	0	5
Morphine 3- -D-glucuro nide	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
Morphine	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
Norcodeine	12,500	5	0	5	0	5	0
	*25,000	2	3	2	3	2	3
	37,500	0	5	0	5	0	5
Normorphone	25,000	5	0	5	0	5	0
	*50,000	3	2	3	2	2	3
	75,000	0	5	0	5	0	5
Oxycodone	12,500	5	0	5	0	5	0
	*25,000	2	3	2	3	2	3
	37,500	0	5	0	5	0	5
Oxymorphone	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	37,500	0	5	0	5	0	5
Procaine	25,000	5	0	5	0	5	0
	*50,000	2	3	2	3	2	3

	75,000	0	5	0	5	0	5
Thebaine	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	37,500	0	5	0	5	0	5

PCP:

Analytes	Conc. (ng/ml)	11A0490-PCP		11A0491-PCP		11A0492-PCP	
		Negative	Positive	Negative	Positive	Negative	Positive
Phencyclidine	12.5	5	0	5	0	5	0
	*25	3	2	3	2	3	2
	37.5	0	5	0	5	0	5
4-Hydroxyphencyclidine	6,250	5	0	5	0	5	0
	*12,500	2	3	2	3	2	3
	18,750	0	5	0	5	0	5

PPX:

Analytes	Conc. (ng/ml)	11A0508-PPX300		11A0509-PPX300		11A0510-PPX300	
		Negative	Positive	Negative	Positive	Negative	Positive
D-Propoxyphene	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
D-Norpropoxyphene	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5

THC 150:

Analytes	Conc. (ng/ml)	11A0571-THC150		11A0572-THC150		11A0573-THC150	
		Negative	Positive	Negative	Positive	Negative	Positive
Cannabinol	50,000	5	0	5	0	5	0
	*100,000	3	2	3	2	2	3
	>100,000	0	5	0	5	0	5
11-nor-^{8}THC-9 COOH	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
11-nor-^{9}THC-9 COOH	75	5	0	5	0	5	0
	*150	2	3	2	3	2	3
	225	0	5	0	5	0	5

^{8} THC	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5
^{9} THC	25,000	5	0	5	0	5	0
	*50,000	4	1	3	2	2	3
	75,000	0	5	0	5	0	5

THC 50:

Analytes	**Conc. (ng/ml)**	**11A0571-THC50**		**11A0572-THC50**		**11A0573-THC50**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Cannabinol	17,500	5	0	5	0	5	0
	*35,000	3	2	3	2	2	3
	52,500	0	5	0	5	0	5
11-nor-^{8}THC-9 COOH	15	5	0	5	0	5	0
	*30	3	2	3	2	2	3
	45	0	5	0	5	0	5
11-nor-^{9}THC-9 COOH	25	5	0	5	0	5	0
	*50	2	3	2	3	2	3
	75	0	5	0	5	0	5
^{8} THC	8,500	5	0	5	0	5	0
	*17,000	2	3	3	2	2	3
	25,500	0	5	0	5	0	5
^{9} THC	8,500	5	0	5	0	5	0
	*17,000	4	1	4	1	2	3
	25,500	0	5	0	5	0	5

THC 25:

	Conc.	**11A0571-THC25**	**11A0572-THC25**	**11A0573-THC25**

Analytes	(ng/ml)	Negative	Positive	Negative	Positive	Negative	Positive
Cannabinol	8,750	5	0	5	0	5	0
	*17,500	3	2	3	2	2	3
	26,250	0	5	0	5	0	5
11-nor-^{8}T HC-9 COOH	7.5	5	0	5	0	5	0
	*15	3	2	3	2	2	3
	45	0	5	0	5	0	5
11-nor-^{9} THC-9 COOH	12.5	5	0	5	0	5	0
	*25	2	3	2	3	2	3
	37.5	0	5	0	5	0	5
^{8}THC	4,250	5	0	5	0	5	0
	*8,500	2	3	3	2	2	3
	12,750	0	5	0	5	0	5
^{9}THC	4,250	5	0	5	0	5	0
	*8,500	4	1	4	1	2	3
	12,750	0	5	0	5	0	5

THC 300

Analytes	Conc. (ng/ml)	11A0571-THC300		11A0572-THC300		11A0573-THC300	
		Negative	Positive	Negative	Positive	Negative	Positive
Cannabinol	100,000	5	0	5	0	5	0
	*200,000	3	2	3	2	2	3
	>300,000	0	5	0	5	0	5
11-nor-^{8}-THC-9 COOH	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
11-nor-^{9}-THC-	150	5	0	5	0	5	0

9 COOH	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
^{8}-THC	50,000	5	0	5	0	5	0
	*100,000	2	3	3	2	2	3
	150,000	0	5	0	5	0	5
^{9}-THC	50,000	5	0	5	0	5	0
	*100,000	4	1	3	2	2	3
	150,000	0	5	0	5	0	5

THC 200

Analytes	Conc. (ng/ml)	11A0571-THC200		11A0572-THC200		11A0573-THC200	
		Negative	Positive	Negative	Positive	Negative	Positive
Cannabinol	70,000	5	0	5	0	5	0
	*140,000	3	2	3	2	2	3
	210,000	0	5	0	5	0	5
11-nor-^{8}-THC-9 COOH	60	5	0	5	0	5	0
	*120	3	2	3	2	2	3
	180	0	5	0	5	0	5
11-nor-^{9}-THC-9 COOH	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
^{8}-THC	34,000	5	0	5	0	5	0
	*68,000	2	3	3	2	2	3
	102,000	0	5	0	5	0	5
^{9}-THC	34,000	5	0	5	0	5	0
	*68,000	4	1	3	2	2	3
	102,000	0	5	0	5	0	5

THC30

Analytes	Conc. (ng/ml)	11A0571-THC30		11A0572-THC30		11A0573-THC30	
		Negative	Positive	Negative	Positive	Negative	Positive
Cannabinol	10,000	5	0	5	0	5	0
	*20,000	3	2	3	2	2	3
	>30,000	0	5	0	5	0	5
11-nor-^{8}-THC-9 COOH	10	5	0	5	0	5	0
	*20	3	2	3	2	2	3
	30	0	5	0	5	0	5

11-nor-^{9}-THC-9 COOH	15	5	0	5	0	5	0
	*30	2	3	2	3	2	3
	45	0	5	0	5	0	5
^{8}-THC	5,000	5	0	5	0	5	0
	*10,000	2	3	3	2	2	3
	15,000	0	5	0	5	0	5
^{9}-THC	5,000	5	0	5	0	5	0
	*10,000	4	1	3	2	2	3
	15,000	0	5	0	5	0	5

THC 20

Analytes	Conc. (ng/ml)	11A0571-THC20		11A0572-THC20		11A0573-THC20	
		Negative	Positive	Negative	Positive	Negative	Positive
Cannabinol	7,000	5	0	5	0	5	0
	*14,000	3	2	3	2	2	3
	21,000	0	5	0	5	0	5
11-nor-^{8}-THC-9 COOH	6	5	0	5	0	5	0
	*12	3	2	3	2	2	3
	18	0	5	0	5	0	5
11-nor-^{9}-THC-9 COOH	10	5	0	5	0	5	0
	*20	2	3	2	3	2	3
	30	0	5	0	5	0	5
^{8}-THC	3,400	5	0	5	0	5	0
	*6,800	2	3	3	2	2	3
	10,200	0	5	0	5	0	5
^{9}-THC	3,400	5	0	5	0	5	0
	*6,800	4	1	3	2	2	3
	10,200	0	5	0	5	0	5

TCA:

Analytes	Conc. (ng/ml)	11A0562-TCA1000		11A0563-TCA1000		11A0564-TCA1000	
		Negative	Positive	Negative	Positive	Negative	Positive
Nortriptyline	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5
Nordoxepine	250	5	0	5	0	5	0
	*500	2	3	2	3	2	3

	750	0	5	0	5	0	5
Trimipramine	1,500	5	0	5	0	5	0
	*3,000	3	2	3	2	2	3
	4,500	0	5	0	5	0	5
Amitriptyline	750	5	0	5	0	5	0
	*1,500	2	3	2	3	2	3
	3,000	0	5	0	5	0	5
Promazine	1,500	5	0	5	0	5	0
	*3,000	3	2	3	2	2	3
	4,500	0	5	0	5	0	5
Desipramine	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	400	0	5	0	5	0	5
Cyclobenzaprine	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
Imipramine	200	5	0	5	0	5	0
	*400	2	3	2	3	2	3
	800	0	5	0	5	0	5
Clomipramine	25,000	5	0	5	0	5	0
	*50,000	3	2	3	2	2	3
	100,000	0	5	0	5	0	5
Doxepine	1,000	5	0	5	0	5	0
	*2,000	2	3	2	3	2	3
	3,000	0	5	0	5	0	5
Maprotiline	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
Promethazine	25,000	5	0	5	0	5	0
	*50,000	2	3	2	3	2	3
	100,000	0	5	0	5	0	5
Perphenazine	25,000	5	0	5	0	5	0
	*50,000	3	2	3	2	2	3
	100,000	0	5	0	5	0	5

Dithiaden	5,000	5	0	5	0	5	0
	*10,000	3	2	3	2	3	2
	15,000	0	5	0	5	0	5

TCA 500:

Analytes	**Conc. (ng/ml)**	**11A0562-TCA500**		**11A0563-TCA500**		**11A0564-TCA500**	
		Negative	Positive	Negative	Positive	Negative	Positive
Nortriptyline	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Nordoxepine	125	5	0	5	0	5	0
	*250	2	3	2	3	2	3
	375	0	5	0	5	0	5
Trimipramine	750	5	0	5	0	5	0
	*1,500	3	2	3	2	2	3
	2250	0	5	0	5	0	5
Amitriptyline	375	5	0	5	0	5	0
	*750	2	3	2	3	2	3
	1125	0	5	0	5	0	5
Promazine	750	5	0	5	0	5	0
	*1,500	3	2	3	2	2	3
	2,250	0	5	0	5	0	5
Desipramine	50	5	0	5	0	5	0
	*100	2	3	2	3	2	3
	150	0	5	0	5	0	5
Cyclobenzaprine	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5

Imipramine	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	300	0	5	0	5	0	5
Clomipramine	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	50,000	0	5	0	5	0	5
Doxepine	500	5	0	5	0	5	0
	*1,000	2	3	2	3	2	3
	1,500	0	5	0	5	0	5
Maprotiline	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5
Promethazine	12,500	5	0	5	0	5	0
	*25,000	2	3	2	3	2	3
	50,000	0	5	0	5	0	5
Perphenazine	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	50,000	0	5	0	5	0	5
Dithiaden	2,500	5	0	5	0	5	0
	*5,000	3	2	3	2	3	2
	7,500	0	5	0	5	0	5

TML 100:

Analytes	**Conc. (ng/ml)**	**11A0589-TML100**		**11A0590-TML100**		**11A0591-TML100**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
n-Desmethyl-c is-tramadol	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5

Cis-tramadol	50	5	0	5	0	5	0
	*100	2	3	3	2	2	3
	150	0	5	0	5	0	5
Procyclidine	50,000	5	0	5	0	5	0
	*100,000	2	3	3	2	2	3
	150,000	0	5	0	5	0	5
o-Desmethyl-cis-tramado	5,000	5	0	5	0	5	0
	*10,000	2	3	3	2	2	3
	15,000	0	5	0	5	0	5
Phencyclidine	50,000	5	0	5	0	5	0
	*100,000	2	3	3	2	2	3
	150,000	0	5	0	5	0	5
d,l-O-Desmethyl venlafaxine	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5

TML 200:

Analytes	Conc. (ng/ml)	11A0589-TML200		11A0590-TML200		11A0591-TML200	
		Negative	Positive	Negative	Positive	Negative	Positive
n-Desmethyl-cis-tramadol	200	5	0	5	0	5	0
	*400	2	3	3	2	2	3
	600	0	5	0	5	0	5
Cis-tramadol	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
Procyclidine	100,000	5	0	5	0	5	0
	*200,000	2	3	3	2	2	3
	300,000	0	5	0	5	0	5
o-Desmethyl-cis-tramado	10,000	5	0	5	0	5	0
	*20,000	2	3	3	2	2	3
	30,000	0	5	0	5	0	5
Phencyclidine	100,000	5	0	5	0	5	0
	*200,000	2	3	3	2	2	3

	300,000	0	5	0	5	0	5
d,l-O-Desmethyl venlafaxine	50,000	5	0	5	0	5	0
	*100,000	2	3	3	2	2	3
	150,000	0	5	0	5	0	5

TML300:

Analytes	Conc. (ng/ml)	11A0589-TML300		11A0590-TML300		11A0591-TML300	
		Negative	Positive	Negative	Positive	Negative	Positive
n-Desmethyl-cis-tramadol	300	5	0	5	0	5	0
	*600	2	3	3	2	2	3
	900	0	5	0	5	0	5
Cis-tramadol	150	5	0	5	0	5	0
	*300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Procyclidine	150,000	5	0	5	0	5	0
	*300,000	2	3	3	2	2	3
	450,000	0	5	0	5	0	5
o-Desmethyl-cis-tramado	15,000	5	0	5	0	5	0
	*30,000	2	3	3	2	2	3
	45,000	0	5	0	5	0	5
Phencyclidine	150,000	5	0	5	0	5	0
	*300,000	2	3	3	2	2	3
	450,000	0	5	0	5	0	5
d,l-O-Desmethyl venlafaxine	75,000	5	0	5	0	5	0
	*150,000	2	3	3	2	2	3
	225,000	0	5	0	5	0	5

OXY:

Analytes	Conc. (ng/ml)	11A0463-OXY		11A0445-OXY		11A0465-OXY	
		Negative	Positive	Negative	Positive	Negative	Positive
Oxycodone	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3

	150	0	5	0	5	0	5
Oxymorphone	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	600	0	5	0	5	0	5
Levorphanol	25,000	5	0	5	0	5	0
	*50,000	3	2	3	2	2	3
	100,000	0	5	0	5	0	5
Hydrocodone	12,500	5	0	5	0	5	0
	*25,000	2	3	2	3	2	3
	50,000	0	5	0	5	0	5
Hydromorphone	25,000	5	0	5	0	5	0
	*50,000	3	2	3	2	2	3
	100,000	0	5	0	5	0	5
Naloxone	12,500	5	0	5	0	5	0
	*25,000	2	3	2	3	2	3
	50,000	0	5	0	5	0	5
Naltrexone	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	50,000	0	5	0	5	0	5

Oxy 300:

Analytes	**Conc. (ng/ml)**	**11A0463-OXY300**		**11A0464-OXY300**		**11A0465-OXY300**	
		Negative	Positive	Negative	Positive	Negative	Positive
Oxycodone	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Oxymorphone	450	5	0	5	0	5	0
	*900	2	3	2	3	2	3
	1350	0	5	0	5	0	5
Levorphanol	7,500	5	0	5	0	5	0
	*15,000	3	2	3	2	2	3
	22,500	0	5	0	5	0	5
Hydrocodone	37,500	5	0	5	0	5	0
	*75,000	2	3	2	3	2	3
	112,500	0	5	0	5	0	5

Hydromorphone	75,000	5	0	5	0	5	0
	*150,000	3	2	3	2	2	3
	225,000	0	5	0	5	0	5
Naloxone	37,500	5	0	5	0	5	0
	*75,000	2	3	2	3	2	3
	112,500	0	5	0	5	0	5
Naltrexone	37,500	5	0	5	0	5	0
	*75,000	3	2	3	2	2	3
	112,500	0	5	0	5	0	5

COT 200:

Analytes	Conc. (ng/ml)	11A0220-COT200		11A0221-COT200		11A0222-COT200	
		Negative	Positive	Negative	Positive	Negative	Positive
(-)-Cotinine	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	400	0	5	0	5	0	5
(-)-Nicotine	2,500	5	0	5	0	5	0
	*5,000	2	3	3	2	2	3
	7,500	0	5	0	5	0	5

COT 100:

Analytes	Conc. (ng/ml)	11A0220-COT100		11A0221-COT100		11A0222-COT100	
		Negative	Positive	Negative	Positive	Negative	Positive
(-)-Cotinine	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	200	0	5	0	5	0	5
(-)-Nicotine	1,250	5	0	5	0	5	0
	*2,500	2	3	3	2	2	3
	3,750	0	5	0	5	0	5

EDDP 300:

Analytes	Conc. (ng/ml)	11A0238-EDDP300		11A0239-EDDP300		11A0240-EDDP300	
		Negative	Positive	Negative	Positive	Negative	Positive
2-Ethylidene-1,5-dimet	150	5	0	5	0	5	0
	*300	3	2	2	3	2	3

hyl-3,3-diphenylpyrrolidine (EDDP)	600	0	5	0	5	0	5

EDDP 100:

Analytes	Conc. (ng/ml)	11A0238-EDDP100		11A0239-EDDP100		11A0240-EDDP100	
		Negative	Positive	Negative	Positive	Negative	Positive
2-Ethylidene-1,5-dimethyl-3,3-diphenylpyrrolidine (EDDP)	50	5	0	5	0	5	0
	*100	2	3	2	3	2	3
	200	0	5	0	5	0	5

FYL 20

Analytes	Conc. (ng/ml)	11A0274-FYL20		11A0275-FYL20		11A0276-FYL20	
		Negative	Positive	Negative	Positive	Negative	Positive
Alfentanyl	300,000	5	0	5	0	5	0
	*600,000	3	2	3	2	2	3
	900,000	0	5	0	5	0	5
Fenflurami ne	25,000	5	0	5	0	5	0
	*50,000	3	2	2	3	2	3
	75,000	0	5	0	5	0	5
Norfentanyl	10	5	0	5	0	5	0
	*20	2	3	3	2	2	3
	30	0	5	0	5	0	5
Buspirone	7500	5	0	5	0	5	0
	*15,000	3	2	3	2	2	3
	22,500	0	5	0	5	0	5
Fentanyl	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Sufentanyl	25,000	5	0	5	0	5	0
	*50,000	3	2	3	2	2	3
	75,000	0	5	0	5	0	5

FYL 10

Analytes	Conc. (ng/ml)	11A0274-FYL10		11A0275-FYL10		11A0276-FYL10	
		Negative	Positive	Negative	Positive	Negative	Positive
Alfentanyl	150,000	5	0	5	0	5	0
	*300,000	3	2	3	2	2	3
	450,000	0	5	0	5	0	5
Fenflurami ne	12,500	5	0	5	0	5	0

	*25,000	3	2	2	3	2	3
	37,500	0	5	0	5	0	5
Norfentanyl	5	5	0	5	0	5	0
	*10	2	3	3	2	2	3
	15	0	5	0	5	0	5
Buspirone	4000	5	0	5	0	5	0
	*8,000	3	2	3	2	2	3
	12,000	0	5	0	5	0	5
Fentanyl	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5
Sufentanyl	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	37,500	0	5	0	5	0	5

K2 50

Analytes	**Conc. (ng/ml)**	**11A0544-K2 50**		**11A0545-K2 50**		**11A0546-K2 50**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
JWH-018 5-Pentanoic acid	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5
JWH-073 4-butanoic acid	25	5	0	5	0	5	0
	*50	3	2	2	3	2	3
	75	0	5	0	5	0	5
JWH-018 4-Hydroxypentyl	200	5	0	5	0	5	0
	*400	2	3	3	2	2	3
	800	0	5	0	5	0	5
JWH-018 5-Hydroxypentyl	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
JWH-073 4-Hydroxybutyl	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5

K2 30

	Conc.	**11A0544-K2 30**	**11A0545-K2 30**	**11A0546-K2 30**

Analytes	(ng/ml)	Negative	Positive	Negative	Positive	Negative	Positive
JWH-018 5-Pentanoic acid	15	5	0	5	0	5	0
	*30	3	2	3	2	2	3
	60	0	5	0	5	0	5
JWH-073 4-butanoic acid	15	5	0	5	0	5	0
	*30	3	2	2	3	2	3
	60	0	5	0	5	0	5
JWH-018 4-Hydroxypentyl	125	5	0	5	0	5	0
	*250	2	3	3	2	2	3
	375	0	5	0	5	0	5
JWH-018 5-Hydroxypentyl	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
JWH-073 4-Hydroxybutyl	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5

K2-25

Analytes	Conc. (ng/ml)	11A0544-K2 25		11A0545-K2 25		11A0546-K2 25	
		Negative	Positive	Negative	Positive	Negative	Positive
JWH-018 5-Pentanoic acid metabolite	12.5	5	0	5	0	5	0
	*25	3	2	3	2	2	3
	37.5	0	5	0	5	0	5
JWH-073 4-butanoic acid metabolite	12.5	5	0	5	0	5	0
	*25	2	3	2	3	2	3
	37.5	0	5	0	5	0	5
JWH-0184-Hydroxypentyl metabolite	100	5	0	5	0	5	0
	*200	2	3	3	2	2	3
	300	0	5	0	5	0	5
JWH-018 5-Hydroxypentyl metabolite	125	5	0	5	0	5	0
	*250	2	3	3	2	2	3
	375	0	5	0	5	0	5
JWH-073 4-	125	5	0	5	0	5	0
	*250	4	1	4	1	2	3

Hydroxybuty l metabolite	375	0	5	0	5	0	5

6-MAM

Analytes	Conc. (ng/ml)	MAM14030001-T		MAM14030002-T		MAM14030003-T	
		Negative	Positive	Negative	Positive	Negative	Positive
6-mono-aceto-m orphine	5	5	0	5	0	5	0
	*10	2	3	3	2	2	3
	15	0	5	0	5	0	5
Morphine	5	0	5	0	5	0	5
	2	3	2	3	2	3	2

CLO400

Analytes	Conc. (ng/ml)	11A0202-CLO400		11A0203-CLO400		11A0204-CLO400	
		Negative	Positive	Negative	Positive	Negative	Positive
Clonazepam	200	5	0	5	0	5	0
	*400	3	2	3	2	2	3
	600	0	5	0	5	0	5
Alprazolam	100	5	0	5	0	5	0
	*200	2	3	2	3	2	3
	400	0	5	0	5	0	5
a-hydroxyalprazol am	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	4,000	0	5	0	5	0	5
Bromazepam	500	5	0	5	0	5	0
	*1,000	2	3	2	3	2	3
	1,500	0	5	0	5	0	5
Chlordiazepoxide	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5
Clobazam	125	5	0	5	0	5	0
	*250	2	3	2	3	2	3
	375	0	5	0	5	0	5
Clorazepate	300	5	0	5	0	5	0
	*600	3	2	3	2	2	3

	900	0	5	0	5	0	5
Delorazepam	500	5	0	5	0	5	0
	*1,000	2	3	2	3	2	3
	1,500	0	5	0	5	0	5
Desalkylflurazepam	125	5	0	5	0	5	0
	*250	3	2	3	2	2	3
	375	0	5	0	5	0	5
Diazepam	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
Estazolam	625	5	0	5	0	5	0
	*1250	3	2	3	2	2	3
	1,900	0	5	0	5	0	5
Flunitrazepam	150	5	0	5	0	5	0
	*300	2	3	2	3	2	3
	450	0	5	0	5	0	5
(+-) Lorazepam	625	5	0	5	0	5	0
	*1250	3	2	3	2	2	3
	1,900	0	5	0	5	0	5
RS-Lorazepamglucuronide	125	5	0	5	0	5	0
	*250	3	2	3	2	2	3
	375	0	5	0	5	0	5
Midazolam	2,500	5	0	5	0	5	0
	*5,000	3	2	3	2	2	3
	7,500	0	5	0	5	0	5
Nitrazepam	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	400	0	5	0	5	0	5
Norchlordiazepoxide	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	400	0	5	0	5	0	5
Nordiazepam	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5

Oxazepam	175	5	0	5	0	5	0
	*350	3	2	3	2	2	3
	525	0	5	0	5	0	5
Temazepam	75	5	0	5	0	5	0
	*150	3	2	3	2	2	3
	225	0	5	0	5	0	5
Triazolam	2,500	5	0	5	0	5	0
	*5,000	3	2	3	2	2	3
	7,500	0	5	0	5	0	5

CLO150

Analytes	Conc. (ng/ml)	11A0202-CLO150		11A0203-CLO150		11A0204-CLO150	
		Negative	Positive	Negative	Positive	Negative	Positive
Clonazepam	75	5	0	5	0	5	0
	*150	3	2	3	2	2	3
	225	0	5	0	5	0	5
Alprazolam	37	5	0	5	0	5	0
	*75	2	3	2	3	2	3
	110	0	5	0	5	0	5
a-hydroxyalprazolam	370	5	0	5	0	5	0
	*750	3	2	3	2	2	3
	1,100	0	5	0	5	0	5
Bromazepam	200	5	0	5	0	5	0
	*400	2	3	2	3	2	3
	600	0	5	0	5	0	5
Chlordiazepoxide	200	5	0	5	0	5	0
	*400	3	2	3	2	2	3
	600	0	5	0	5	0	5
Clobazam	50	5	0	5	0	5	0
	*100	2	3	2	3	2	3
	150	0	5	0	5	0	5
Clorazepate	125	5	0	5	0	5	0
	*250	3	2	3	2	2	3
	375	0	5	0	5	0	5
	200	5	0	5	0	5	0

Delorazepam	*400	2	3	2	3	2	3
	600	0	5	0	5	0	5
Desalkylflurazepam	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Diazepam	60	5	0	5	0	5	0
	*120	2	3	2	3	2	3
	180	0	5	0	5	0	5
Estazolam	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Flunitrazepam	60	5	0	5	0	5	0
	*120	2	3	2	3	2	3
	180	0	5	0	5	0	5
(+-) Lorazepam	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
RS-Lorazepamglucuronide	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Midazolam	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
Nitrazepam	40	5	0	5	0	5	0
	*75	3	2	3	2	2	3
	110	0	5	0	5	0	5
Norchlordiazepoxide	40	5	0	5	0	5	0
	*75	3	2	3	2	2	3
	110	0	5	0	5	0	5
Nordiazepam	200	5	0	5	0	5	0
	*400	3	2	3	2	2	3
	600	0	5	0	5	0	5
Oxazepam	65	5	0	5	0	5	0
	*130	3	2	3	2	2	3

	195	0	5	0	5	0	5
Temazepam	30	5	0	5	0	5	0
	*60	3	2	3	2	2	3
	90	0	5	0	5	0	5
Triazolam	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5

ETG 500

Analytes	**Conc. (ng/ml)**	**11A0247-ETG500**		**11A0248-ETG500**		**11A0249-ETG500**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Ethyl- β -D-Glucuronide	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
Propyl β-D-glucuronide	25,000	5	0	5	0	5	0
	*50,000	2	3	3	2	2	3
	75,000	0	5	0	5	0	5
Morphine 3β-glucuronide	50,000	5	0	5	0	5	0
	*100,000	3	2	3	2	2	3
	150,000	0	5	0	5	0	5
Morphine 6β-glucuronide	50,000	5	0	5	0	5	0
	*100,000	3	2	3	2	2	3
	150,000	0	5	0	5	0	5
Glucuronic Acid	50,000	5	0	5	0	5	0
	*100,000	3	2	3	2	2	3
	150,000	0	5	0	5	0	5
Ethanol	50,000	5	0	5	0	5	0
	*>100,000	3	2	3	2	2	3
Methanol	50,000	5	0	5	0	5	0
	*>100,000	3	2	3	2	2	3

ETG1000

Analytes	Conc. (ng/ml)	11A0247-ETG1000		11A0248-ETG1000		11A0249-ETG1000	
		Negative	Positive	Negative	Positive	Negative	Positive
Ethyl- β -D-Glucuronide	500	5	0	5	0	5	0
	*1000	2	3	3	2	2	3
	1500	0	5	0	5	0	5
Propyl β-D-glucuronide	50,000	5	0	5	0	5	0
	*100,000	2	3	3	2	2	3
	*>100,000	0	5	0	5	0	5
Morphine 3β-glucuronide	50,000	5	0	5	0	5	0
	*>100,000	3	2	3	2	2	3
Morphine 6β-glucuronide	50,000	5	0	5	0	5	0
	*>100,000	3	2	3	2	2	3
GlucuronicAcid	50,000	5	0	5	0	5	0
	*>100,000	3	2	3	2	2	3
Ethanol	50,000	5	0	5	0	5	0
	*>100,000	3	2	3	2	2	3
Methanol	50,000	5	0	5	0	5	0
	*>100,000	3	2	3	2	2	3

MDA

Analytes	Conc. (ng/ml)	11A0346-MDA500		11A0347-MDA500		11A0348-MDA500	
		Negative	Positive	Negative	Positive	Negative	Positive
(±) 3,4-Methylenedioxyamphetamine	250	5	0	5	0	5	0
	*500	2	3	3	2	2	3
	750	0	5	0	5	0	5
L-Amphetamine	15,000	5	0	5	0	5	0
	*30,000	2	3	3	2	2	3
	45,000	0	5	0	5	0	5
	1,000	5	0	5	0	5	0

Phentermine	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
Maprotiline	50,000	5	0	5	0	5	0
	*100,000	3	2	3	2	2	3
	150,000	0	5	0	5	0	5
Methoxyphenamine	2, 500	5	0	5	0	5	0
	*5,000	3	2	3	2	2	3
	7,500	0	5	0	5	0	5
D-Amphetamine	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
D,L-Amphetamine sulfate	200	5	0	5	0	5	0
	*400	3	2	3	2	2	3
	600	0	5	0	5	0	5

ACE

Analytes	Conc. (ng/ml)	11A0076-ACE		11A0077-ACE		11A0078-ACE	
		Negative	Positive	Negative	Positive	Negative	Positive
Acetaminophen	2500	5	0	5	0	5	0
	*5000	3	2	3	2	2	3
	7500	0	5	0	5	0	5

LSD20

Analytes	Conc. (ng/ml)	11A0310-LSD20		11A0311-LSD20		11A0312-LSD20	
		Negative	Positive	Negative	Positive	Negative	Positive
Lysergic Acid Diethylamide	10	5	0	5	0	5	0
	*20	3	2	3	2	2	3
	30	0	5	0	5	0	5

LSD50

Analytes	Conc. (ng/ml)	11A0310-LSD50		LSD 14060008p-T		11A0312-LSD50	
		Negative	Positive	Negative	Positive	Negative	Positive
Lysergic Acid Diethylamide	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5

MDPV

Analytes	Conc. (ng/ml)	11A0355-MDPV		11A0356-MDPV		11A0357-MDPV	
		Negative	Positive	Negative	Positive	Negative	Positive
3,4-methylenedioxypyrovalerone	500	5	0	5	0	5	0
	*1000	3	2	3	2	2	3
	1500	0	5	0	5	0	5

MPD300

Analytes	Conc. (ng/ml)	11A0400-MPD300		11A0401-MPD300		11A0402-MPD300	
		Negative	Positive	Negative	Positive	Negative	Positive
Methylphenidate (Ritalin)	150	5	0	5	0	5	0
	*300	2	3	4	1	2	3
	450	0	5	0	5	0	5
Ritalinic Acid	500	5	0	5	0	5	0
	*1000	3	2	3	2	2	3
	1500	0	5	0	5	0	5

ZOL:

Analytes	Conc. (ng/ml)	11A0634-ZOL		11A0635-ZOL		11A0636-ZOL	
		Negative	Positive	Negative	Positive	Negative	Positive
Zolpidem	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5

DIA300:

Analytes	Conc. (ng/ml)	11A0229-DIA300		11A0230-DIA300		11A0231-DIA300	
		Negative	Positive	Negative	Positive	Negative	Positive
Alprazolam	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
a-hydroxyalprazolam	750	5	0	5	0	5	0
	*1,500	3	2	3	2	2	3
	2,250	0	5	0	5	0	5
Bromazepam	450	5	0	5	0	5	0
	*900	3	2	3	2	2	3

	1,350	0	5	0	5	0	5
Chlordiazepoxide	450	5	0	5	0	5	0
	*900	3	2	3	2	2	3
	1,350	0	5	0	5	0	5
Clobazam	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Clonazepam	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Clorazepate	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Delorazepam	450	5	0	5	0	5	0
	*900	3	2	3	2	2	3
	1,350	0	5	0	5	0	5
Desalkylflurazepam	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Diazepam	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	600	0	5	0	5	0	5
Estazolam	3,000	5	0	5	0	5	0
	*6,000	3	2	3	2	2	3
	9,000	0	5	0	5	0	5
Flunitrazepam	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
(+-) Lorazepam	1,500	5	0	5	0	5	0
	*3,000	3	2	3	2	2	3
	4,500	0	5	0	5	0	5
RS-Lorazepamglucuronide	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5

Midazolam	3,000	5	0	5	0	5	0
	*6,000	3	2	3	2	2	3
	9,000	0	5	0	5	0	5
Nitrazepam	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Norchlordiazepoxide	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Nordiazepam	450	5	0	5	0	5	0
	*900	3	2	3	2	2	3
	1,350	0	5	0	5	0	5
Oxazepam	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Temazepam	50	5	0	5	0	5	0

	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Triazolam	1,500	5	0	5	0	5	0
	*3,000	3	2	3	2	2	3
	4,500	0	5	0	5	0	5

DIA 200

Analytes	Conc. (ng/ml)	11A0229-DIA200		11A0230-DIA200		11A0231-DIA200	
		Negative	Positive	Negative	Positive	Negative	Positive
Alprazolam	35	5	0	5	0	5	0
	*70	3	2	3	2	2	3
	105	0	5	0	5	0	5
a-hydroxyalprazolam	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5
Bromazepam	300	5	0	5	0	5	0
	*600	3	2	3	2	2	3
	900	0	5	0	5	0	5
Chlordiazepoxide	300	5	0	5	0	5	0
	*600	3	2	3	2	2	3
	900	0	5	0	5	0	5
Clobazam	60	5	0	5	0	5	0
	*120	3	2	3	2	2	3
	180	0	5	0	5	0	5
Clonazepam	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Clorazepatedipotassium	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Delorazepam	300	5	0	5	0	5	0
	*600	3	2	3	2	2	3
	900	0	5	0	5	0	5
Desalkylfluraze	60	5	0	5	0	5	0

pam	*120	3	2	3	2	2	3
	180	0	5	0	5	0	5
Diazepam	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Estazolam	2,000	5	0	5	0	5	0
	*4,000	3	2	3	2	2	3
	6,000	0	5	0	5	0	5
Flunitrazepam	60	5	0	5	0	5	0
	*120	3	2	3	2	2	3
	180	0	5	0	5	0	5
(+-) Lorazepam	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5
RS-Lorazepam glucuronide	60	5	0	5	0	5	0
	*120	3	2	3	2	2	3
	180	0	5	0	5	0	5
Midazolam	2,000	5	0	5	0	5	0
	*4,000	3	2	3	2	2	3
	6,000	0	5	0	5	0	5
Nitrazepam	60	5	0	5	0	5	0
	*120	3	2	3	2	2	3
	180	0	5	0	5	0	5
Norchlordiazepoxide	35	5	0	5	0	5	0
	*70	3	2	3	2	2	3
	105	0	5	0	5	0	5
Nordiazepam	300	5	0	5	0	5	0
	*600	3	2	3	2	2	3
	900	0	5	0	5	0	5
Oxazepam	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Temazepam	35	5	0	5	0	5	0

	*70	3	2	3	2	2	3
	105	0	5	0	5	0	5
Triazolam	1,000	5	0	5	0	5	0
	*2,000	3	2	3	2	2	3
	3,000	0	5	0	5	0	5

MEP100

Analytes	Conc. (ng/ml)	11A0373-MEP100		11A0374-MEP100		11A0375-MEP100	
		Negative	Positive	Negative	Positive	Negative	Positive
Mephedrone	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
R(+)-Methcathinone HCl	750	5	0	5	0	5	0
	1,500	2	3	3	2	2	3
	2,250	0	5	0	5	0	5
S(-)-MethcathinoneHCl	250	5	0	5	0	5	0
	500	3	2	2	3	2	3
	750	0	5	0	5	0	5
3-Fluoromethcathinone HCl	750	5	0	5	0	5	0
	1,500	3	2	3	2	2	3
	2,250	0	5	0	5	0	5
4-Fluoromethcathinone HCl	150	5	0	5	0	5	0
	300	2	3	3	2	2	3
	450	0	5	0	5	0	5
Methoxyphenamine	50,000	5	0	5	0	5	0
	100,000	3	2	3	2	3	2
	150,000	0	5	0	5	0	5

7-ACL 300

Analytes	Conc. (ng/ml)	11A0085-7ACL300		11A0086-7ACL300		11A0087-7ACL300	
		Negative	Positive	Negative	Positive	Negative	Positive
a-hydroxyalprazo	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5

Bromazepam	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
Chlordiazepoxide	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
Clobazam	4500	5	0	5	0	5	0
	*9000	3	2	3	2	2	3
	13500	0	5	0	5	0	5
Clonazepam	1200	5	0	5	0	5	0
	*2400	3	2	3	2	2	3
	3600	0	5	0	5	0	5
Delorazepam	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
Desalkylflurazep	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
Flunitrazepam	1500	5	0	5	0	5	0
	*3000	3	2	3	2	2	3
	4500	0	5	0	5	0	5
RS-Lorazepam	1350	5	0	5	0	5	0
	*2700	3	2	3	2	2	3
	5400	0	5	0	5	0	5
Norchlordiazepoxide	2250	5	0	5	0	5	0
	*4500	3	2	3	2	2	3
	6750	0	5	0	5	0	5
Nordiazepam	7500	5	0	5	0	5	0
	*15000	3	2	3	2	2	3
	22500	0	5	0	5	0	5
Temazepam	4500	5	0	5	0	5	0
	*9000	3	2	3	2	2	3
	13500	0	5	0	5	0	5
7-	150	5	0	5	0	5	0

Aminoclonazepa	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5

7-ACL 100

Analytes	Conc. (ng/ml)	11A0085-7ACL100		11A0086-7ACL100		11A0087-7ACL100	
		Negative	Positive	Negative	Positive	Negative	Positive
a-hydroxyalprazolam	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5
Bromazepam	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5
Chlordiazepoxide	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5
Clobazam	1500	5	0	5	0	5	0
	*3000	3	2	3	2	2	3
	4500	0	5	0	5	0	5
Clonazepam	400	5	0	5	0	5	0
	*800	3	2	3	2	2	3
	1200	0	5	0	5	0	5
Delorazepam	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5
Desalkylflurazepam	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5
Flunitrazepam	500	5	0	5	0	5	0
	*1000	3	2	3	2	2	3
	1500	0	5	0	5	0	5
RS-Lorazepam	450	5	0	5	0	5	0
	*900	3	2	3	2	2	3
	1350	0	5	0	5	0	5
Norchlordiazepoxi	750	5	0	5	0	5	0

de	*1500	3	2	3	2	2	3
	2250	0	5	0	5	0	5
Nordiazepam	2500	5	0	5	0	5	0
	*5000	3	2	3	2	2	3
	7500	0	5	0	5	0	5
Temazepam	1500	5	0	5	0	5	0
	*3000	3	2	3	2	2	3
	4500	0	5	0	5	0	5
7-Aminoclonazepam	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5

7-ACL 200

Analytes	**Conc. (ng/ml)**	**11A0085-7ACL200**		**11A0086-7ACL200**		**11A0087-7ACL200**	
		Negative	Positive	Negative	Positive	Negative	Positive
a-hydroxyalprazo	2000	5	0	5	0	5	0
	*4000	3	2	3	2	2	3
	6000	0	5	0	5	0	5
Bromazepam	2000	5	0	5	0	5	0
	*4000	3	2	3	2	2	3
	6000	0	5	0	5	0	5
Chlordiazepoxide	2000	5	0	5	0	5	0
	*4000	3	2	3	2	2	3
	6000	0	5	0	5	0	5
Clobazam	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
Clonazepam	800	5	0	5	0	5	0
	*1600	3	2	3	2	2	3
	2400	0	5	0	5	0	5
Delorazepam	2000	5	0	5	0	5	0
	*4000	3	2	3	2	2	3
	6000	0	5	0	5	0	5
Desalkylflurazep	2000	5	0	5	0	5	0

	*4000	3	2	3	2	2	3
	6000	0	5	0	5	0	5
Flunitrazepam	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5
RS-Lorazepam	900	5	0	5	0	5	0
	*1800	3	2	3	2	2	3
	2700	0	5	0	5	0	5
Norchlordiazepoxide	1500	5	0	5	0	5	0
	*3000	3	2	3	2	2	3
	4500	0	5	0	5	0	5
Nordiazepam	5000	5	0	5	0	5	0
	*10000	3	2	3	2	2	3
	15000	0	5	0	5	0	5
Temazepam	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
7-Aminoclonazepa	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5

CFYL

Analytes	Conc. (ng/ml)	11A0184-CFYL500		11A0185-CFYL500		11A0186-CFYL500	
		Negative	Positive	Negative	Positive	Negative	Positive
Carfentanyl	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Fentanyl	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5

ZOP

Analytes	Conc. (ng/ml)	11A0643-ZOP		11A0644-ZOP		11A0645-ZOP	
		Negative	Positive	Negative	Positive	Negative	Positive
Zopiclone-N-oxide	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5
Zopiclone	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5

CAF

Analytes	Conc. (ng/ml)	11A0157-CAF		11A0158-CAF		11A0159-CAF	
		Negative	Positive	Negative	Positive	Negative	Positive
Caffeine	500	5	0	5	0	5	0
	*1000	3	2	3	2	2	3
	1500	0	5	0	5	0	5

CAT

Analytes	Conc. (ng/ml)	11A0148-CAT		11A0149-CAT		11A0150-CAT	
		Negative	Positive	Negative	Positive	Negative	Positive
(+)-Norpseudoephedrine HCl	75	5	0	5	0	5	0
	*150	3	2	3	2	2	3
	225	0	5	0	5	0	5

TRO

Analytes	Conc. (ng/ml)	11A0598-TRO		11A0599-TRO		11A0600-TRO	
		Negative	Positive	Negative	Positive	Negative	Positive
Tropicamide	175	5	0	5	0	5	0

	*350	3	2	3	2	2	3
	525	0	5	0	5	0	5

ALP 100

Analytes	Conc. (ng/ml)	11A0094-ALP		11A0095-ALP		11A0096-ALP	
		Negative	Positive	Negative	Positive	Negative	Positive
Alprazolam	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Benzodiazepines	150	5	0	5	0	5	0
	300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Flunitrazepam	100	5	0	5	0	5	0
	200	3	2	3	2	2	3
	300	0	5	0	5	0	5
a-hydroxyalprazolam	750	5	0	5	0	5	0
	1500	3	2	3	2	2	3
	2250	0	5	0	5	0	5
(±) Lorazepam	1500	5	0	5	0	5	0
	3000	3	2	3	2	2	3
	4500	0	5	0	5	0	5
Bromazepam	450	5	0	5	0	5	0
	900	3	2	3	2	2	3
	1350	0	5	0	5	0	5
RS-Lorazepamglucuronid	100	5	0	5	0	5	0
	200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Chlordiazepoxide	450	5	0	5	0	5	0
	900	3	2	3	2	2	3
	1350	0	5	0	5	0	5
Midazolam	3000	5	0	5	0	5	0
	6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
Clobazam	100	5	0	5	0	5	0

	200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Nitrazepam	100	5	0	5	0	5	0
	200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Clonazepam	250	5	0	5	0	5	0
	500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Norchlordiazepoxide	50	5	0	5	0	5	0
	100	3	2	2	3	2	3
	150	0	5	0	5	0	5
Clorazepatedipotassium	250	5	0	5	0	5	0
	500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Nordiazepam	450	5	0	5	0	5	0
	900	3	2	3	2	2	3
	1350	0	5	0	5	0	5
Delorazepam	450	5	0	5	0	5	0
	900	3	2	2	3	2	3
	1350	0	5	0	5	0	5
Oxazepam	150	5	0	5	0	5	0
	300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Desalkylflurazepam	100	5	0	5	0	5	0
	200	3	2	3	2	2	3
	300	0	5	0	5	0	5
Temazepam	50	5	0	5	0	5	0
	100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Diazepam	150	5	0	5	0	5	0
	300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Triazolam	1500	5	0	5	0	5	0
	3000	3	2	2	3	2	3

	4500	0	5	0	5	0	5
Estazolam	3000	5	0	5	0	5	0
	6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5

ABP10

Analytes	Conc. (ng/ml)	11A0067-K3 10		11A0068-K3 10		11A0069-K3 10	
		Negative	Positive	Negative	Positive	Negative	Positive
AB-PINACA	5	5	0	5	0	5	0
	*10	3	2	3	2	2	3
	15	0	5	0	5	0	5
AB-PINACA 5-Pentanoic	5	5	0	5	0	5	0
	*10	1	4	2	3	2	3
	15	0	5	0	5	0	5
AB-PINACA 5-hydroxypentyl	5	5	0	5	0	5	0
	*10	2	3	2	3	4	1
	15	0	5	0	5	0	5
AB-FUBINACA	5	5	0	5	0	5	0
	*10	4	1	3	2	2	3
	15	0	5	0	5	0	5
AB-PINACA 4-hydroxypentyl	5,000	5	0	5	0	5	0
	*10,000	3	2	2	3	3	2
	15,000	0	5	0	5	0	5
UR-144 5-Pentanoic	2,500	5	0	5	0	5	0
	*5,000	2	3	2	3	2	3
	7,500	0	5	0	5	0	5
UR-144 5-hydroxypentyl	5,000	5	0	5	0	5	0
	*10,000	2	3	3	2	1	4
	15,000	0	5	0	5	0	5
UR-144 4-hydroxypentyl	5,000	5	0	5	0	5	0
	*10,000	4	1	2	3	4	1
	15,000	0	5	0	5	0	5
APINACA 5-hydroxypentyl	5,000	5	0	5	0	5	0
	*10,000	1	4	3	2	1	4

	15,000	0	5	0	5	0	5
ADB-PINACA N-(5-hydroxypentyl)	15	5	0	5	0	5	0
	*30	3	2	3	2	1	4
	45	0	5	0	5	0	5
ADB-PINACA Pentanoic Acid	5	5	0	5	0	5	0
	*10	4	1	3	2	3	2
	15	0	5	0	5	0	5
5-fluoro AB-PINACA N-(4-hydroxypentyl)	15	5	0	5	0	5	0
	*30	2	3	3	2	3	2
	45	0	5	0	5	0	5
5-fluoro AB-PINACA	12.5	5	0	5	0	5	0
	*25	1	4	3	2	1	4
	37.5	0	5	0	5	0	5

APVP1000

Analytes	**Conc. (ng/ml)**	**11A0112-PVP1000**		**11A0113-PVP1000**		**11A0114-PVP1000**	
		Negative	Positive	Negative	Positive	Negative	Positive
alpha-Pyrrolidinovalerophenone	500	5	0	5	0	5	0
	*1,000	3	2	3	2	2	3
	1,500	0	5	0	5	0	5

APVP500

Analytes	**Conc. (ng/ml)**	**11A0112-PVP500**		**11A0113-PVP500**		**11A0114-PVP500**	
		Negative	Positive	Negative	Positive	Negative	Positive
alpha-Pyrrolidinovalerophenone	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5

CNB500

Analytes	**Conc. (ng/ml)**	**11A0787-CBN**		**11A0788-CBN**		**11A0789-CBN**	
		Negative	Positive	Negative	Positive	Negative	Positive
Cannabinol	250	5	0	5	0	5	0
	*500	3	2	3	2	3	2
	750	0	5	0	5	0	5
11-nor-Δ^9 -THC-9	150	5	0	5	0	5	0

COOH	*300	3	2	3	2	3	2
	450	0	5	0	5	0	5
Δ^9 –THC	50,000	5	0	5	0	5	0
	*100,000	3	2	3	2	3	2
	150,000	0	5	0	5	0	5

MPRD100

Analytes	**Conc. (ng/ml)**	**11A0409-MPRD**		**11A0410-MPRD**		**11A0411-MPRD**	
		Negative	Positive	Negative	Positive	Negative	Positive
Normeperidine	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Meperidine	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5

PGB50,000

Analytes	**Conc. (ug/ml)**	**11A0499-PGB**		**11A0500-PGB**		**11A0501-PGB**	
		Negative	Positive	Negative	Positive	Negative	Positive
Pregabalin	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5

TZD200

Analytes	**Conc. (ng/ml)**	**11A0607-TZD**		**11A0608-TZD**		**11A0609-TZD**	
		Negative	**Positive**	**Negative**	**Positive**	**Negative**	**Positive**
Trazodone	100	5	0	5	0	5	0
	*200	3	2	3	2	2	3
	300	0	5	0	5	0	5

UR-144 25

UR-144 Analytes	**Conc. (ng/ml)**	**11A0616-K4**		**11A0617-K4**		**11A0618-K4**	
		Negative	Positive	Negative	Positive	Negative	Positive
UR-144 5-Pentanoic	12.5	5	0	5	0	5	0

acid	*25	3	2	3	2	2	3
	37.5	0	5	0	5	0	5
UR-144 5-Pentanoic acid	5000	5	0	5	0	5	0
	*10000	3	2	3	2	2	3
	15000	0	5	0	5	0	5
UR-144 5-hydroxypentyl	2500	5	0	5	0	5	0
	*5000	3	2	3	2	2	3
	7500	0	5	0	5	0	5
XLR-11 4-hydroxypentyl	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5
5-fluoro AB-Pinaca N-(4-hydroxypentyl)	5000	5	0	5	0	5	0
	*10000	3	2	3	2	2	3
	15000	0	5	0	5	0	5
ADB-PINAC N-(4-hydroxypentyl)	5000	5	0	5	0	5	0
	*>10000	3	2	3	2	2	3
AB-PINACA 4-hydroxypentyl	5000	5	0	5	0	5	0
	*>10000	3	2	3	2	2	3

ZAL100

Analytes	**Conc. (ng/ml)**	**11A0625-ZAL**		**11A0626-ZAL**		**11A0627-ZAL**	
		Negative	Positive	Negative	Positive	Negative	Positive
Zaleplon	50	5	0	5	0	5	0
	*100	3	2	3	2	3	2
	150	0	5	0	5	0	5

MES 100

Analytes	**Conc. (ng/ml)**	**11A0382-MES**		**11A0383-MES**		**11A0384-MES**	
		Negative	Positive	Negative	Positive	Negative	Positive
Mescaline	50	5	0	5	0	5	0
	*100	3	2	3	2	3	2
	150	0	5	0	5	0	5

GAB 2000

Analytes	Conc. (ng/ml)	11A0283-GAB		11A0284-GAB		11A0285-GAB	
		Negative	Positive	Negative	Positive	Negative	Positive
Gabapentin	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5

TLD 50

Analytes	Conc. (ng/ml)	11A0580-TLD50		11A0581-TLD50		11A0582-TLD50	
		Negative	Positive	Negative	Positive	Negative	Positive
Nortilidine	25	5	0	5	0	5	0
	*50	3	2	3	2	2	3
	75	0	5	0	5	0	5
Tilidine	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5

QTP 1000

Analytes	Conc. (ng/ml)	11A0517-QTP1000		11A0518-QTP1000		11A0519-QTP1000	
		Negative	Positive	Negative	Positive	Negative	Positive
Quetiapine	500	5	0	5	0	5	0
	*1000	3	2	3	2	2	3
	1500	0	5	0	5	0	5
NorQuetiazepine	5,000	5	0	5	0	5	0
	*10,000	3	2	3	2	2	3
	15,000	0	5	0	5	0	5

PAP 500

Analytes	Conc. (ng/ml)	11A0481-PAP500		11A0482-PAP500		11A0483-PAP500	
		Negative	Positive	Negative	Positive	Negative	Positive
Papaverine	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5
Diflunisal	500,000	5	0	5	0	5	0

	*1,000,000	3	2	3	2	2	3
Methortrexate	97,500	5	0	5	0	5	0
	*65,000	3	2	3	2	2	3
	32,500	0	5	0	5	0	5
Methedrone	250,000	5	0	5	0	5	0
	*500,000	3	2	3	2	2	3
	750,000	0	5	0	5	0	5
Pragablin	250,000	5	0	5	0	5	0
	*500,000	3	2	3	2	2	3
	750,000	0	5	0	5	0	5
Phenelzine	4,000	5	0	5	0	5	0
	*8,000	3	2	3	2	2	3
	12,000	0	5	0	5	0	5
Quinine	2,000	5	0	5	0	5	0
	*4,000	3	2	3	2	2	3
	6,000	0	5	0	5	0	5

KRA 300

Analytes	**Conc. (ng/ml)**	11A0301-KRA300		11A0302-KRA300		11A0303-KRA300	
		Negative	Positive	Negative	Positive	Negative	Positive
Mitragynine	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
7-hydroxyMitragynine	25,000	5	0	5	0	5	0
	*>50,000	3	2	3	2	2	3

CAR 2000

Analytes	**Conc. (ng/ml)**	**11A0166-CAR2000**		**11A0167-CAR2000**		**11A0168-CAR2000**	
		Negative	Positive	Negative	Positive	Negative	Positive
Carisoprodol	1000	5	0	5	0	5	0
	*2000	3	2	3	2	2	3
	3000	0	5	0	5	0	5

FLX500

Analytes	**Conc.**	**11A0265-FLX500**	**11A0266-FLX500**	**11A0267-FLX500**

	(ng/ml)	Negative	Positive	Negative	Positive	Negative	Positive
Fluoxetine	250	5	0	5	0	5	0
	*500	3	2	3	2	2	3
	750	0	5	0	5	0	5

HMO250

Analytes	Conc. (ng/ml)	11A1715-HMO250		11A1716-HMO250		11A1717-HMO250	
		Negative	Positive	Negative	Positive	Negative	Positive
Hydromorphone	125	5	0	5	0	5	0
	*250	3	2	3	2	2	3
	375	0	5	0	5	0	5
Codeine	30	5	0	5	0	5	0
	*60	3	2	3	2	2	3
	90	0	5	0	5	0	5
Hydrocodone	125	5	0	5	0	5	0
	*250	3	2	3	2	2	3
	375	0	5	0	5	0	5
Levorphanol	500	5	0	5	0	5	0
	*1000	3	2	3	2	2	3
	1500	0	5	0	5	0	5
Normorphine	31,250	5	0	5	0	5	0
	*62,500	3	2	3	2	2	3
	93,750	0	5	0	5	0	5
Oxymorphone	31,250	5	0	5	0	5	0
	*62,500	3	2	3	2	2	3
	93,750	0	5	0	5	0	5
Thebaine	2500	5	0	5	0	5	0
	*5000	3	2	3	2	2	3
	7500	0	5	0	5	0	5
Morphine	50	5	0	5	0	5	0
	*100	3	2	3	2	2	3
	150	0	5	0	5	0	5
Ethylmorphine	30	5	0	5	0	5	0
	*60	3	2	3	2	2	3

	90	0	5	0	5	0	5
Morphine 3-β-D-Glucuronide	62.5	5	0	5	0	5	0
	*125	3	2	3	2	2	3
	187.5	0	5	0	5	0	5
Oxycodone	31,250	5	0	5	0	5	0
	*62,500	3	2	3	2	2	3
	93,750	0	5	0	5	0	5
Norcodeine	7800	5	0	5	0	5	0
	*15,600	3	2	3	2	2	3
	23,400	0	5	0	5	0	5
Nalorphine	12,500	5	0	5	0	5	0
	*25,000	3	2	3	2	2	3
	37,500	0	5	0	5	0	5
Diacetylmorphine (Heroin)	62.5	5	0	5	0	5	0
	*125	3	2	3	2	2	3
	187.5	0	5	0	5	0	5
6-Monoacetylmorphine	30	5	0	5	0	5	0
	*60	3	2	3	2	2	3
	90	0	5	0	5	0	5

HMO300

Analytes	**Conc. (ng/ml)**	**11A1715-HMO300**		**11A1716-HMO300**		**11A1717-HMO300**	
		Negative	Positive	Negative	Positive	Negative	Positive
Hydromorphone	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Codeine	35	5	0	5	0	5	0
	*70	3	2	3	2	2	3
	105	0	5	0	5	0	5
Hydrocodone	150	5	0	5	0	5	0
	*300	3	2	3	2	2	3
	450	0	5	0	5	0	5
Levorphanol	600	5	0	5	0	5	0
	*1200	3	2	3	2	2	3

	1800	0	5	0	5	0	5
Normorphine	37,500	5	0	5	0	5	0
	*75,000	3	2	3	2	2	3
	112,500	0	5	0	5	0	5
Oxymorphone	37,500	5	0	5	0	5	0
	*75,000	3	2	3	2	2	3
	112,500	0	5	0	5	0	5
Thebaine	3000	5	0	5	0	5	0
	*6000	3	2	3	2	2	3
	9000	0	5	0	5	0	5
Morphine	60	5	0	5	0	5	0
	*120	3	2	3	2	2	3
	180	0	5	0	5	0	5
Ethylmorphine	35	5	0	5	0	5	0
	*70	3	2	3	2	2	3
	105	0	5	0	5	0	5
Morphine 3-β-D-Glucuronide	75	5	0	5	0	5	0
	*150	3	2	3	2	2	3
	225	0	5	0	5	0	5
Oxycodone	37,500	5	0	5	0	5	0
	*75,000	3	2	3	2	2	3
	112,500	0	5	0	5	0	5
Norcodeine	9350	5	0	5	0	5	0
	*18,700	3	2	3	2	2	3
	28,050	0	5	0	5	0	5
Nalorphine	15,000	5	0	5	0	5	0
	*30,000	3	2	3	2	2	3
	45,000	0	5	0	5	0	5
Diacetylmorphine (Heroin)	75	5	0	5	0	5	0
	*150	3	2	3	2	2	3
	225	0	5	0	5	0	5
6-Monoacetylmorphine	35	5	0	5	0	5	0
	*70	3	2	3	2	2	3
	105	0	5	0	5	0	5

OZP1000

Analytes	Conc. (ng/ml)	11A0472-OZP1000		11A0473-OZP1000		11A0474-OZP1000	
		Negative	Positive	Negative	Positive	Negative	Positive
Olanzapine	500	5	0	5	0	5	0
	*1000	3	2	3	2	3	2
	1500	0	5	0	5	0	5

Conclusion: The cutoff concentrations of each drug related compounds were showed in the tables with "*".

2.4 Cross Reactivity

A study was conducted to determine the cross-reactivity of the test with compounds in either drug-free urine or drug positive urine containing, Amphetamine, Barbiturates, Benzodiazepines, Buprenorphine, Cocaine, Marijuana, Methadone, Methamphetamine, Methylenedioxymethamphetamine, Morphine, Tramadol, Methaqualone, Ketamine, Phencyclidine, Propoxyphene or Tricyclic Antidepressants. The following compounds show no cross-reactivity when tested with the Multi-Drug Test Dip Card with/without Adulteration at a concentration of 100 µg/mL. Visual interpretations occurred at 5 minutes after specimen application. Results are presented in table below.

Table: Cross Reactivity

Acetophenetidin	Cholesterol	d,l-Isoproterenol	d-Pseudoephedrine
N-Acetylprocainamide	Cortisone	Zomepirac	Quinidine
Acetylsalicylic acid	Creatinine	Ketoprofen	Salicylic acid
Aminopyrine	Deoxycorticosterone	Labetalol	Serotonin
Amoxicillin	Diclofenac	Loperamide	Sulfamethazine
Ampicillin	Digoxin	Meprobamate	Sulindac
l-Ascorbic acid	Diphenhydramine	Isoxsuprine	Tetracycline
Apomorphine	Ethyl-p-aminobenzoate	d,l-Propanolol	Tetrahydrocortisone-3-acetate
Aspartame	β-Estradiol	Nalidixic acid	
Atropine	Estrone-3-sulfate	Naproxen	Tetrahydrocortisone
Benzilic acid	Erythromycin	Niacinamide	Thiamine
Benzoic acid	Fenoprofen	Nifedipine	d,l-Tyrosine
Bilirubin	Furosemide	Norethindrone	Tolbutamide
d,l-Brompheniramine	Gentisic acid	Noscapine	Triamterene
Cannabidiol	Hemoglobin	d,l-Octopamine	Trifluoperazine
Chloral hydrate	Hydralazine	Oxalic acid	Trimethoprim
Chloramphenicol	Hydrochlorothiazide	Oxolinic acid	d,l-Tryptophan
Chlorothiazide	Hydrocortisone	Oxymetazoline	Uric acid
d,l-Chlorpheniramine	o-Hydroxyhippuric acid	Penicillin-G	Verapamil
Chlorpromazine	3-Hydroxytyramine	Prednisone	

Conclusion: The compounds listed in above table show no cross-reactivity when tested at a concentration of 100 g/ml in 5 minutes.

2.5 Between Day Reproducibility

The concentration of all tests in the Dip Card at 0ng/ml, -50%Cut-off, +50%Cut-off specimens were run on ten separate days using the same lot of reagents. The specimens were tested in triplicate in 3 lots of test Dip Card. Results were read visually at 5 minutes after specimen application. Results are presented in table below.

Table: Between Day Results

Day			1	2	3	4	5	6	7	8	9	10
AMP 1,000	0ng/ml	11A0103-AMP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0104-AMP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0105-AMP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0103-AMP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0104-AMP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0105-AMP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1,500ng/ml	11A0103-AMP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0104-AMP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0105-AMP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
AMP 500	0ng/ml	11A0103-AMP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0104-AMP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0105-AMP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0103-AMP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0104-AMP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A0105-AMP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0103-AMP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0104-AMP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0105-AMP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
AMP 300	0ng/ml	11A0103-AMP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0104-AMP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0105-AMP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0103-AMP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0104-AMP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0105-AMP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0103-AMP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0104-AMP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0105-AMP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
BAR 300	0ng/ml	11A0121-BAR300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0122-BAR300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0123-BAR300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0121-BAR300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0122-BAR300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A0123-BAR300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0121-BAR300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0122-BAR300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0123-BAR300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
BAR 200	0ng/ml	11A0121-BAR200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0122-BAR200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0123-BAR200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0121-BAR200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0122-BAR200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0123-BAR200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0121-BAR200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0122-BAR200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0123-BAR200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
BUP10	0ng/ml	11A0130-BUP10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0131-BUP10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0132-BUP10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	5ng/ml	11A0130-BUP10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0131-BUP10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0132-BUP10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	15ng/ml	11A0130-BUP10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0131-BUP10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0132-BUP10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0130-BUP5	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0131-BUP5	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

BUP5		11A0132-BUP5	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	2.5ng/ml	11A0130-BUP5	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0131-BUP5	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0132-BUP5	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	7.5ng/ml	11A0130-BUP5	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0131-BUP5	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0132-BUP5	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
BZO 300	0ng/ml	11A0139-BZO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0139-BZO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0139-BZO300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0140-BZO300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0141-BZO300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
BZO 200	0ng/ml	11A0139-BZO200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0139-BZO200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0139-BZO200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0140-BZO200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0141-BZO200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

BZO 100	0ng/ml	11A0139-BZO100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0139-BZO100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0139-BZO100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0140-BZO100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0141-BZO100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
BZO 500	0ng/ml	11A0139-BZO500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0139-BZO500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0140-BZO500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0141-BZO500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0139-BZO500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0140-BZO500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0141-BZO500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
CO C 300	0ng/ml	11A0211-COC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0213-COC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0211-COC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0213-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		COC300										
	450ng/ml	11A0211-COC300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0212-COC300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0213-COC300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
COC 100	0ng/ml	11A0211-COC100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0213-COC100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0211-COC100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0213-COC100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0211-COC100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0212-COC100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0213-COC100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
COC 150	0ng/ml	11A0211-COC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0213-COC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0211-COC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0213-COC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	225ng/ml	11A0211-COC150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0212-COC150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0213-COC150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0211-COC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

COC 200		11A0213-COC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0211-COC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0212-COC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0213-COC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0211-COC200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0212-COC200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0213-COC200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
KET 1000	0ng/ml	11A0292-KET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0292-KET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/ml	11A0292-KET1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0293-KET1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0294-KET1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
KET 500	0ng/ml	11A0292-KET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0292-KET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0292-KET500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0293-KET500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

		11A0294-KET500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
KET 300	0ng/ml	11A0292-KET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0292-KET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0292-KET300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0293-KET300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0294-KET300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
KET 100	0ng/ml	11A0292-KET100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0292-KET100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0293-KET100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0294-KET100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0292-KET100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0293-KET100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0294-KET100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0337-MDMA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0338-MDMA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0339-MDMA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0337-MDMA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

MDMA 1000	500ng/ml	11A0338-MDMA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0339-MDMA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/ml	11A0337-MDMA1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0338-MDMA1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0339-MDMA1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MDMA 500	0ng/ml	11A0337-MDMA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0338-MDMA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0339-MDMA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0337-MDMA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0338-MDMA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0339-MDMA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0337-MDMA500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0338-MDMA500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0339-MDMA500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MDMA300	0ng/ml	11A0337-MDMA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0338-MDMA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0339-MDMA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0337-MDMA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0338-MDMA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0339-MDMA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

	450ng/ml	11A0337-MDMA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0338-MDMA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0339-MDMA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MET 1000	0ng/ml	11A0364-MET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0366-MET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0364-MET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0366-MET1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/m l	11A0364-MET1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0365-MET1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0366-MET1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MET 500	0ng/ml	11A0364-MET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0366-MET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0364-MET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0366-MET500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0364-MET500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0365-MET500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0366-MET500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0364-MET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

MET 300		11A0366-MET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0364-MET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0366-MET300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0364-MET300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0365-MET300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0366-MET300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MET 200	0ng/ml	11A0364-MET200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0366-MET200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0364-MET200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0365-MET200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0366-MET200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0364-MET200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0365-MET200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0366-MET200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MOP 300	0ng/ml	11A0391-MOP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0392-MOP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0393-MOP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0391-MOP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0392-MOP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A0393-MOP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0391-MOP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0392-MOP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0393-MOP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MOP 100	0ng/ml	11A0391-MOP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0392-MOP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0393-MOP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0391-MOP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0392-MOP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0393-MOP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0391-MOP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0392-MOP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0393-MOP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0391-MOP200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0392-MOP200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0393-MOP200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0391-MOP200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

MOP 200	100ng/ml	11A0392-MOP200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0393-MOP200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0391-MOP200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0392-MOP200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0393-MOP200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MQL	0ng/ml	11A0418-MQL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0419-MQL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0420-MQL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0418-MQL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0419-MQL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0420-MQL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0418-MQL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0419-MQL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0420-MQL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MTD 300	0ng/ml	11A0427-MTD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0428-MTD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0429-MTD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0427-MTD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0428-MTD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A0429-MTD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0427-MTD300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0428-MTD300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0429-MTD300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MTD 200	0ng/ml	11A0427-MTD200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0428-MTD200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0429-MTD200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0427-MTD200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0428-MTD200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0429-MTD200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0427-MTD200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0428-MTD200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0429-MTD200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
OPI	0ng/ml	11A0454-OPI	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0455-OPI	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0456-OPI	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1000ng/ml	11A0454-OPI	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0455-OPI	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0456-OPI	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	3000ng/ml	11A0454-OPI	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

		11A0455-OPI	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0456-OPI	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
PCP	0ng/ml	11A0490-PCP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0491-PCP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0492-PCP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	12.5ng/ml	11A0490-PCP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0491-PCP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0492-PCP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	37.5ng/ml	11A0490-PCP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0491-PCP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0492-PCP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
PPX	0ng/ml	11A0508-PPX300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0509-PPX300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0510-PPX300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0508-PPX300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0509-PPX300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0510-PPX300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0508-PPX300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0509-PPX300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0510-PPX300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
THC 150	0ng/ml	11A0571-THC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0571-THC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		THC150										
	225ng/ml	11A0571-THC150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0572-THC150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0573-THC150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
THC 50	0ng/ml	11A0571-THC50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	25ng/ml	11A0571-THC50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0571-THC50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0572-THC50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0573-THC50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
THC 25	0ng/ml	11A0571-THC25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	12.5ng/ml	11A0571-THC25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	37.5ng/ml	11A0571-THC25	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0572-THC25	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0573-THC25	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0571-THC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

THC 300		11A0573-THC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0571-THC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0571-THC300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0572-THC300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0573-THC300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
THC 200	0ng/ml	11A0571-THC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0571-THC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0571-THC200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0572-THC200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0573-THC200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
THC30	0ng/ml	11A0571-THC30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	15ng/ml	11A0571-THC30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	45ng/ml	11A0571-THC30	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0572-THC30	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

		11A0573-THC30	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
THC 20	0ng/ml	11A0571-THC20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	10ng/ml	11A0571-THC20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0572-THC20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0573-THC20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	30ng/ml	11A0571-THC20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0572-THC20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0573-THC20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
TCA	0ng/ml	11A0562-TCA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0563-TCA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0564-TCA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0562-TCA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0563-TCA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0564-TCA1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/m l	11A0562-TCA1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0563-TCA1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0564-TCA1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
TCA 500	0ng/ml	11A0562-TCA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0563-TCA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0564-TCA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0562-TCA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A0563-TCA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0564-TCA500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0562-TCA500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0563-TCA500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0564-TCA500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
TML 100	0ng/ml	11A0589-TML100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0590-TML100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0591-TML100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0589-TML100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0590-TML100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0591-TML100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0589-TML100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0590-TML100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0591-TML100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
TML 200	0ng/ml	11A0589-TML200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0590-TML200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0591-TML200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0589-TML200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0590-TML200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0591-TML200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0589-TML200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0590-TML200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0591-TML200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

TML 300	0ng/ml	11A0589-TML300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0590-TML300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0591-TML300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0589-TML300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0590-TML300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0591-TML300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0589-TML300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0590-TML300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0591-TML300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
OXY	0ng/ml	11A0463-OXY	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0445-OXY	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0465-OXY	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0463-OXY	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0445-OXY	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0465-OXY	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0463-OXY	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0445-OXY	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0465-OXY	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
OXY 300	0ng/ml	11A0463-OXY300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0464-OXY300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0465-OXY300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0463-OXY300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0464-OXY300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0465-OXY300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0463-OXY300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

		11A0464-OXY300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0465-OXY300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
COT 200	0ng/ml	11A0220-COT200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0221-COT200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0222-COT200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0220-COT200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0221-COT200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0222-COT200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0220-COT200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0221-COT200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0222-COT200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
COT 100	0ng/ml	11A0220-COT100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0221-COT100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0222-COT100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0220-COT100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0221-COT100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0222-COT100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0220-COT100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0221-COT100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0222-COT100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0238-EDDP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0239-EDDP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

EDDP 300		11A0240-EDDP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0238-EDDP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0239-EDDP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0240-EDDP300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0238-EDDP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0239-EDDP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0240-EDDP300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
EDDP 100	0ng/ml	11A0238-EDDP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0239-EDDP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0240-EDDP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0238-EDDP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0239-EDDP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0240-EDDP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0238-EDDP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0239-EDDP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0240-EDDP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0274-FYL20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

FYL20	0ng/ml	11A0275-FYL20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0276-FYL20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	10ng/ml	11A0274-FYL20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0275-FYL20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0276-FYL20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	30ng/ml	11A0274-FYL20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0275-FYL20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0276-FYL20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
FYL10	0ng/ml	11A0274-FYL10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0275-FYL10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0276-FYL10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	5ng/ml	11A0274-FYL10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0275-FYL10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0276-FYL10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	15ng/ml	11A0274-FYL10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0275-FYL10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0276-FYL10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
K250	0ng/ml	11A0544-K250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0545-K250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0546-K250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	25ng/ml	11A0544-K250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0545-K250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0546-K250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

	75ng/ml	11A0544-K2 50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0545-K2 50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0546-K2 50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
K 2 30	0ng/ml	11A0544-K2 30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0545-K2 30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0546-K2 30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	15ng/ml	11A0544-K2 30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0545-K2 30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0546-K2 30	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	45ng/ml	11A0544-K2 30	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0545-K2 30	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0546-K2 30	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
K2-25	0ng/ml	11A0544-K2 25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0545-K2 25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0546-K2 25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	12.5ng/ml	11A0544-K2 25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0545-K2 25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0546-K2 25	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	37.5ng/ml	11A0544-K2 25	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0545-K2 25	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

		11A0546-K225	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
6-MAM10	0ng/ml	11A0319-6MAM10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0320-6MAM10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0321-6MAM10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	5ng/ml	11A0319-6MAM10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0320-6MAM10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0321-6MAM10	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	15ng/ml	11A0319-6MAM10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0320-6MAM10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0321-6MAM10	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
DIA300	0ng/ml	11A0229-DIA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0230-DIA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0231-DIA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0229-DIA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0230-DIA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0231-DIA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450n0g/m l	11A0229-DIA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0230-DIA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0231-DIA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0229-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

DIA 200	0ng/ml	DIA200										
		11A0230-DIA200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0231-DIA200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0229-DIA200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0230-DIA200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0231-DIA200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0229-DIA200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0230-DIA200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0231-DIA200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
CLO 400	0ng/ml	11A0202-CLO400	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0203-CLO400	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0204-CLO400	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	200ng/ml	11A0202-CLO400	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0203-CLO400	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0204-CLO400	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	600ng/ml	11A0202-CLO400	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0203-CLO400	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0204-CLO400	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
CLO 150	0ng/ml	11A0202-CLO150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0203-CLO150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0204-CLO150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0202-CLO150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0203-CLO150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0204-CLO150	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

	225ng/ml	11A0202-CLO150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0203-CLO150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0204-CLO150	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MDA	0ng/ml	11A0346-MDA	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0347-MDA	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0348-MDA	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0346-MDA	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0347-MDA	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0348-MDA	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0346-MDA	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0347-MDA	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0348-MDA	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
ETG 500	0ng/ml	11A0247-ETG500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0248-ETG500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0249-ETG500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0247-ETG500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0248-ETG500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0249-ETG500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0247-ETG500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0248-ETG500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0249-ETG500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
	0ng/ml	11A0247-ETG1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0248-ETG1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

ETG 1000		11A0249-ETG1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0247-ETG1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0248-ETG1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0249-ETG1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/ml	11A0247-ETG1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0248-ETG1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0249-ETG1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
ACE	0ng/ml	11A0076-ACE	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0077-ACE	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0078-ACE	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	2500ng/ml	11A0076-ACE	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0077-ACE	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0078-ACE	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	7500ng/ml	11A0076-ACE	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0077-ACE	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0078-ACE	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
LSD 20	0ng/ml	11A0310-LSD20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0311-LSD20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0312-LSD20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	10ng/ml	11A0310-LSD20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0311-LSD20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0312-LSD20	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	30ng/ml	11A0310-LSD20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0311-LSD20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0312-LSD20	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

LSD 50	0ng/ml	11A0310-LSD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0311-LSD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0312-LSD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	25ng/ml	11A0310-LSD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0311-LSD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0312-LSD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0310-LSD50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0311-LSD50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0312-LSD50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MDPV	0ng/ml	11A0355-MDPV	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0356-MDPV	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0357-MDPV	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0355-MDPV	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0356-MDPV	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0357-MDPV	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/ml	11A0355-MDPV	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0356-MDPV	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0357-MDPV	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MP	0ng/ml	11A0400-MPD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0401-MPD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0402-MPD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0400-MPD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

D 300	150ng/ml	11A0401-MPD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0402-MPD300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0400-MPD300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0401-MPD300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0402-MPD300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
ZOL	0ng/ml	11A0634-ZOL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0635-ZOL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0636-ZOL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	25ng/ml	11A0634-ZOL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0635-ZOL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0636-ZOL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0634-ZOL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0635-ZOL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0636-ZOL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
7-ACL 300	0ng/ml	11A0085-7ACL300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0086-7ACL300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0087-7ACL300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0085-7ACL300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0086-7ACL300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0087-7ACL300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A0085-7ACL300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0086-7ACL300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0087-7ACL300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
7-ACL 100	0ng/ml	11A0085-7ACL100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0086-7ACL100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0087-7ACL100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

	50ng/ml	11A0085-7ACL100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0086-7ACL100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0087-7ACL100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0085-7ACL100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0086-7ACL100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0087-7ACL100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
7-ACL 200	0ng/ml	11A0085-7ACL200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0086-7ACL200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0087-7ACL200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0085-7ACL200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0086-7ACL200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0087-7ACL200	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0085-7ACL200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0086-7ACL200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0087-7ACL200	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
CFYL 500ng/ml	0ng/ml	11A0184-CFYL500500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0185-CFYL500500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0186-CFYL500500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0184-CFYL500500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0185-CFYL500500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0186-CFYL500500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0184-CFYL500500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0185-CFYL500500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

		11A0186-CFYL500500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MEP 100	0ng/ml	11A0373-MEP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0374-MEP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0375-MEP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0373-MEP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0374-MEP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0375-MEP100	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0373-MEP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0374-MEP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0375-MEP100	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
ZOP 50	0ng/ml	11A0643-ZOP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0644-ZOP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0645-ZOP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	25ng/ml	11A0643-ZOP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0644-ZOP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0645-ZOP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0643-ZOP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0644-ZOP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0645-ZOP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
CAF	0ng/ml	11A0157-CAF	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0158-CAF	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0159-CAF	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0157-CAF	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0158-CAF	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0159-CAF	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/m l	11A0157-CAF	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0158-CAF	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0159-CAF	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

CAT 150	0ng/ml	11A0148-CAT	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0149-CAT	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0150-CAT	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75ng/ml	11A0148-CAT	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0149-CAT	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0150-CAT	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	225ng/ml	11A0148-CAT	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0149-CAT	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0150-CAT	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
TRO 350	0ng/ml	11A0598-TRO	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0599-TRO	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0600-TRO	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	175ng/ml	11A0598-TRO	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0599-TRO	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0600-TRO	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	525ng/ml	11A0598-TRO	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0599-TRO	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0600-TRO	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
ALP 100	0ng/ml	11A0094-ALP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0095-ALP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0096-ALP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0094-ALP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0095-ALP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0096-ALP	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0094-ALP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0095-ALP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0096-ALP	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
APVP 1000	0ng/ml	11A0112-PVP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0113-PVP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0114-PVP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0112-PVP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A0113-PVP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0114-PVP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/ml	11A0112-PVP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0113-PVP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0114-PVP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
APVP 500	0ng/ml	11A0112-PVP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0113-PVP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0114-PVP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0112-PVP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0113-PVP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0114-PVP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0112-PVP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0113-PVP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0114-PVP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
CNB 500	0ng/ml	11A0787-CBN	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0788-CBN	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0789-CBN	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0787-CBN	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0788-CBN	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0789-CBN	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0787-CBN	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0788-CBN	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0789-CBN	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MPRB 100	0ng/ml	11A0409-MPRD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0410-MPRD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0411-MPRD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0409-MPRD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0410-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		MPRD										
		11A0411-MPRD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0409-MPRD	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0410-MPRD	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0411-MPRD	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
PGB 50,000	0ng/ml	11A0499-PGB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0500-PGB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0501-PGB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	25,000ng/ml	11A0499-PGB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0500-PGB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0501-PGB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75,000ng/ml	11A0499-PGB	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0500-PGB	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0501-PGB	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
TZD 200	0ng/ml	11A0607-TZD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0608-TZD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0609-TZD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	100ng/ml	11A0607-TZD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0608-TZD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0609-TZD	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	300ng/ml	11A0607-TZD	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0608-TZD	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0609-TZD	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
UR-144 25	0ng/ml	11A0616-K4	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0617-K4	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0618-K4	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	12.5ng/ml	11A0616-K4	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0617-K4	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0618-K4	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	37.5ng/ml	11A0616-K4	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0617-K4	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0618-K4	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
ZAL 100	0ng/ml	11A0625-ZAL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0626-ZAL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A0627-ZAL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0625-ZAL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0626-ZAL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0627-ZAL	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0625-ZAL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0626-ZAL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0627-ZAL	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
MES 100	0ng/ml	11A0382-MES	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0383-MES	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0384-MES	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	50ng/ml	11A0382-MES	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0383-MES	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0384-MES	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0382-MES	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0383-MES	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0384-MES	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
GAB 2000	0ng/ml	11A0283-GAB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0284-GAB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0285-GAB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1000ng/ml	11A0283-GAB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0284-GAB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0285-GAB	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	3000ng/ml	11A0283-GAB	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0284-GAB	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0285-GAB	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
TLD 50	0ng/ml	11A0580-TLD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0581-TLD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0582-TLD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	25 ng/ml	11A0580-TLD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0581-TLD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0582-TLD50	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	75 ng/ml	11A0580-TLD50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0581-TLD50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

		11A0582-TLD50	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
QTP 1000	0ng/ml	11A0517-QTP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0518-QTP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0519-QTP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0517-QTP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0518-QTP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0519-QTP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1500ng/ml	11A0517-QTP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0518-QTP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0519-QTP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
PAP 500	0ng/ml	11A0481-PAP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0482-PAP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0483-PAP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0481-PAP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0482-PAP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0483-PAP500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0481-PAP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0482-PAP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0483-PAP500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
KRA 300	0ng/ml	11A0301-KRA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0302-KRA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0303-KRA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A0301-KRA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0302-KRA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0303-KRA300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

	450ng/ml	11A0301-KRA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0302-KRA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0303-KRA300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
CAR 2000	0ng/ml	11A0166-CAR2000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0167-CAR2000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0168-CAR2000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	1000ng/ml	11A0166-CAR2000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0167-CAR2000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0168-CAR2000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	3000ng/ml	11A0166-CAR2000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0167-CAR2000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0168-CAR2000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
FLX 500	0ng/ml	11A0265-FLX500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0266-FLX500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0267-FLX500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	250ng/ml	11A0265-FLX500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0266-FLX500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0267-FLX500	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	750ng/ml	11A0265-FLX500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0266-FLX500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0267-FLX500	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
HMO 250	0ng/ml	11A1715-HMO250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A1716-HMO250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		11A1717-HMO250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	125ng/ml	11A1715-HMO250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A1716-HMO250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A1717-HMO250	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	375ng/ml	11A1715-HMO250	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A1716-HMO250	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A1717-HMO250	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
HMO 300	0ng/ml	11A1715-HMO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A1716-HMO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A1717-HMO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	150ng/ml	11A1715-HMO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A1716-HMO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A1717-HMO300	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	450ng/ml	11A1715-HMO300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A1716-HMO300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A1717-HMO300	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
OZP1000	0ng/ml	11A0472-OZP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0473-OZP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0474-OZP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
	500ng/ml	11A0472-OZP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0473-OZP1000	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-
		11A0474-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-	-,-,-

		OZP1000										
	1500ng/ml	11A0472-OZP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0473-OZP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+
		11A0474-OZP1000	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+	+,+,+

Conclusion: Test results were consistent over the ten days period.

2.6 Between Lot Reproducibility (lot to lot variability)

Multi-Drug concentration at Drug free urine, -50% Cut-off, and +50% Cut-off urine specimens were run in replicates of ten in three separate lots of products. Results were read visually at 5 after specimen application. The test results are shown in table below.

Table: Between Lot Results

Day			1	2	3	4	5	6	7	8	9	10
AMP 1,000	0ng/ml	11A0103-AMP1000	-	-	-	-	-	-	-	-	-	-
		11A0104-AMP1000	-	-	-	-	-	-	-	-	-	-
		11A0105-AMP1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0103-AMP1000	-	-	-	-	-	-	-	-	-	-
		11A0104-AMP1000	-	-	-	-	-	-	-	-	-	-
		11A0105-AMP1000	-	-	-	-	-	-	-	-	-	-
	1,500ng/ml	11A0103-AMP1000	+	+	+	+	+	+	+	+	+	+
		11A0104-AMP1000	+	+	+	+	+	+	+	+	+	+
		11A0105-AMP1000	+	+	+	+	+	+	+	+	+	+
AMP 500	0ng/ml	11A0103-AMP500	-	-	-	-	-	-	-	-	-	-
		11A0104-AMP500	-	-	-	-	-	-	-	-	-	-
		11A0105-AMP500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0103-AMP500	-	-	-	-	-	-	-	-	-	-
		11A0104-AMP500	-	-	-	-	-	-	-	-	-	-
		11A0105-AMP500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0103-AMP500	+	+	+	+	+	+	+	+	+	+
		11A0104-AMP500	+	+	+	+	+	+	+	+	+	+
		11A0105-AMP500	+	+	+	+	+	+	+	+	+	+

AMP 300	0ng/ml	11A0103-AMP300	-	-	-	-	-	-	-	-	-	-
		11A0104-AMP300	-	-	-	-	-	-	-	-	-	-
		11A0105-AMP300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0103-AMP300	-	-	-	-	-	-	-	-	-	-
		11A0104-AMP300	-	-	-	-	-	-	-	-	-	-
		11A0105-AMP300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0103-AMP300	+	+	+	+	+	+	+	+	+	+
		11A0104-AMP300	+	+	+	+	+	+	+	+	+	+
		11A0105-AMP300	+	+	+	+	+	+	+	+	+	+
BAR 300	0ng/ml	11A0121-BAR300	-	-	-	-	-	-	-	-	-	-
		11A0122-BAR300	-	-	-	-	-	-	-	-	-	-
		11A0123-BAR300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0121-BAR300	-	-	-	-	-	-	-	-	-	-
		11A0122-BAR300	-	-	-	-	-	-	-	-	-	-
		11A0123-BAR300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0121-BAR300	+	+	+	+	+	+	+	+	+	+
		11A0122-BAR300	+	+	+	+	+	+	+	+	+	+
		11A0123-BAR300	+	+	+	+	+	+	+	+	+	+
BAR 200	0ng/ml	11A0121-BAR200	-	-	-	-	-	-	-	-	-	-
		11A0122-BAR200	-	-	-	-	-	-	-	-	-	-
		11A0123-BAR200	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0121-BAR200	-	-	-	-	-	-	-	-	-	-
		11A0122-BAR200	-	-	-	-	-	-	-	-	-	-
		11A0123-BAR200	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0121-BAR200	+	+	+	+	+	+	+	+	+	+
		11A0122-BAR200	+	+	+	+	+	+	+	+	+	+
		11A0123-BAR200	+	+	+	+	+	+	+	+	+	+
BUP 10	0ng/ml	11A0130-BUP10	-	-	-	-	-	-	-	-	-	-
		11A0131-BUP10	-	-	-	-	-	-	-	-	-	-
		11A0132-BUP10	-	-	-	-	-	-	-	-	-	-
	5ng/ml	11A0130-BUP10	-	-	-	-	-	-	-	-	-	-
		11A0131-BUP10	-	-	-	-	-	-	-	-	-	-
		11A0132-BUP10	-	-	-	-	-	-	-	-	-	-
	15ng/ml	11A0130-BUP10	+	+	+	+	+	+	+	+	+	+
		11A0131-BUP10	+	+	+	+	+	+	+	+	+	+
		11A0132-BUP10	+	+	+	+	+	+	+	+	+	+

BUP 5	0ng/ml	11A0130-BUP5	-	-	-	-	-	-	-	-	-	-
		11A0131-BUP5	-	-	-	-	-	-	-	-	-	-
		11A0132-BUP5	-	-	-	-	-	-	-	-	-	-
	2.5ng/ml	11A0130-BUP5	-	-	-	-	-	-	-	-	-	-
		11A0131-BUP5	-	-	-	-	-	-	-	-	-	-
		11A0132-BUP5	-	-	-	-	-	-	-	-	-	-
	7.5ng/ml	11A0130-BUP5	+	+	+	+	+	+	+	+	+	+
		11A0131-BUP5	+	+	+	+	+	+	+	+	+	+
		11A0132-BUP5	+	+	+	+	+	+	+	+	+	+
BZO 300	0ng/ml	11A0139-BZO300	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO300	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0139-BZO300	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO300	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0139-BZO300	+	+	+	+	+	+	+	+	+	+
		11A0140-BZO300	+	+	+	+	+	+	+	+	+	+
		11A0141-BZO300	+	+	+	+	+	+	+	+	+	+
BZO 200	0ng/ml	11A0139-BZO200	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO200	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0139-BZO200	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO200	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0139-BZO200	+	+	+	+	+	+	+	+	+	+
		11A0140-BZO200	+	+	+	+	+	+	+	+	+	+
		11A0141-BZO200	+	+	+	+	+	+	+	+	+	+
BZO 100	0ng/ml	11A0139-BZO100	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO100	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0139-BZO100	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO100	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0139-BZO100	+	+	+	+	+	+	+	+	+	+
		11A0140-BZO100	+	+	+	+	+	+	+	+	+	+
		11A0141-BZO100	+	+	+	+	+	+	+	+	+	+

BZO 500	0ng/ml	11A0139-BZO500	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO500	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0139-BZO500	-	-	-	-	-	-	-	-	-	-
		11A0140-BZO500	-	-	-	-	-	-	-	-	-	-
		11A0141-BZO500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0139-BZO500	+	+	+	+	+	+	+	+	+	+
		11A0140-BZO500	+	+	+	+	+	+	+	+	+	+
		11A0141-BZO500	+	+	+	+	+	+	+	+	+	+
COC 300	0ng/ml	11A0211-COC300	-	-	-	-	-	-	-	-	-	-
		11A0212-COC300	-	-	-	-	-	-	-	-	-	-
		11A0213-COC300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0211-COC300	-	-	-	-	-	-	-	-	-	-
		11A0212-COC300	-	-	-	-	-	-	-	-	-	-
		11A0213-COC300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0211-COC300	+	+	+	+	+	+	+	+	+	+
		11A0212-COC300	+	+	+	+	+	+	+	+	+	+
		11A0213-COC300	+	+	+	+	+	+	+	+	+	+
COC 100	0ng/ml	11A0211-COC100	-	-	-	-	-	-	-	-	-	-
		11A0212-COC100	-	-	-	-	-	-	-	-	-	-
		11A0213-COC100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0211-COC100	-	-	-	-	-	-	-	-	-	-
		11A0212-COC100	-	-	-	-	-	-	-	-	-	-
		11A0213-COC100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0211-COC100	+	+	+	+	+	+	+	+	+	+
		11A0212-COC100	+	+	+	+	+	+	+	+	+	+
		11A0213-COC100	+	+	+	+	+	+	+	+	+	+
COC 150	0ng/ml	11A0211-COC150	-	-	-	-	-	-	-	-	-	-
		11A0212-COC150	-	-	-	-	-	-	-	-	-	-
		11A0213-COC150	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0211-COC150	-	-	-	-	-	-	-	-	-	-
		11A0212-COC150	-	-	-	-	-	-	-	-	-	-
		11A0213-COC150	-	-	-	-	-	-	-	-	-	-
	225ng/ml	11A0211-COC150	+	+	+	+	+	+	+	+	+	+
		11A0212-COC150	+	+	+	+	+	+	+	+	+	+
		11A0213-COC150	+	+	+	+	+	+	+	+	+	+

COC200	0ng/ml	11A0211-COC200	-	-	-	-	-	-	-	-	-	-
		11A0212-COC200	-	-	-	-	-	-	-	-	-	-
		11A0213-COC200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0211-COC200	-	-	-	-	-	-	-	-	-	-
		11A0212-COC200	-	-	-	-	-	-	-	-	-	-
		11A0213-COC200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0211-COC200	+	+	+	+	+	+	+	+	+	+
		11A0212-COC200	+	+	+	+	+	+	+	+	+	+
		11A0213-COC200	+	+	+	+	+	+	+	+	+	+
KET 1000	0ng/ml	11A0292-KET1000	-	-	-	-	-	-	-	-	-	-
		11A0293-KET1000	-	-	-	-	-	-	-	-	-	-
		11A0294-KET1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0292-KET1000	-	-	-	-	-	-	-	-	-	-
		11A0293-KET1000	-	-	-	-	-	-	-	-	-	-
		11A0294-KET1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0292-KET1000	+	+	+	+	+	+	+	+	+	+
		11A0293-KET1000	+	+	+	+	+	+	+	+	+	+
		11A0294-KET1000	+	+	+	+	+	+	+	+	+	+
KET 500	0ng/ml	11A0292-KET500	-	-	-	-	-	-	-	-	-	-
		11A0293-KET500	-	-	-	-	-	-	-	-	-	-
		11A0294-KET500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0292-KET500	-	-	-	-	-	-	-	-	-	-
		11A0293-KET500	-	-	-	-	-	-	-	-	-	-
		11A0294-KET500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0292-KET500	+	+	+	+	+	+	+	+	+	+
		11A0293-KET500	+	+	+	+	+	+	+	+	+	+
		11A0294-KET500	+	+	+	+	+	+	+	+	+	+
KET 300	0ng/ml	11A0292-KET300	-	-	-	-	-	-	-	-	-	-
		11A0293-KET300	-	-	-	-	-	-	-	-	-	-
		11A0294-KET300	-	-	-	-	-	-	-	-	-	-
		11A0292-KET300	-	-	-	-	-	-	-	-	-	-

	150ng/ml	11A0293-KET300	-	-	-	-	-	-	-	-	-	-
		11A0294-KET300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0292-KET300	+	+	+	+	+	+	+	+	+	+
		11A0293-KET300	+	+	+	+	+	+	+	+	+	+
		11A0294-KET300	+	+	+	+	+	+	+	+	+	+
MDMA 1000	0ng/ml	11A0337-MDMA1000	-	-	-	-	-	-	-	-	-	-
		11A0338-MDMA1000	-	-	-	-	-	-	-	-	-	-
		11A0339-MDMA1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0337-MDMA1000	-	-	-	-	-	-	-	-	-	-
		11A0338-MDMA1000	-	-	-	-	-	-	-	-	-	-
		11A0339-MDMA1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0337-MDMA1000	+	+	+	+	+	+	+	+	+	+
		11A0338-MDMA1000	+	+	+	+	+	+	+	+	+	+
		11A0339-MDMA1000	+	+	+	+	+	+	+	+	+	+
MDMA 500	0ng/ml	11A0337-MDMA500	-	-	-	-	-	-	-	-	-	-
		11A0338-MDMA500	-	-	-	-	-	-	-	-	-	-
		11A0339-MDMA500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0337-MDMA500	-	-	-	-	-	-	-	-	-	-
		11A0338-MDMA500	-	-	-	-	-	-	-	-	-	-

		11A0339-MDMA500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0337-MDMA500	+	+	+	+	+	+	+	+	+	+
		11A0338-MDMA500	+	+	+	+	+	+	+	+	+	+
		11A0339-MDMA500	+	+	+	+	+	+	+	+	+	+
MDMA 300	0ng/ml	11A0337-MDMA300	-	-	-	-	-	-	-	-	-	-
		11A0338-MDMA300	-	-	-	-	-	-	-	-	-	-
		11A0339-MDMA300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0337-MDMA300	-	-	-	-	-	-	-	-	-	-
		11A0338-MDMA300	-	-	-	-	-	-	-	-	-	-
		11A0339-MDMA300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0337-MDMA300	+	+	+	+	+	+	+	+	+	+
		11A0338-MDMA300	+	+	+	+	+	+	+	+	+	+
		11A0339-MDMA300	+	+	+	+	+	+	+	+	+	+
MET 1000	0ng/ml	11A0364-MET1000	-	-	-	-	-	-	-	-	-	-
		11A0365-MET1000	-	-	-	-	-	-	-	-	-	-
		11A0366-MET1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0364-MET1000	-	-	-	-	-	-	-	-	-	-
		11A0365-MET1000	-	-	-	-	-	-	-	-	-	-

		11A0366-MET1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0364-MET1000	+	+	+	+	+	+	+	+	+	+
		11A0365-MET1000	+	+	+	+	+	+	+	+	+	+
		11A0366-MET1000	+	+	+	+	+	+	+	+	+	+
MET 500	0ng/ml	11A0364-MET500	-	-	-	-	-	-	-	-	-	-
		11A0365-MET500	-	-	-	-	-	-	-	-	-	-
		11A0366-MET500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0364-MET500	-	-	-	-	-	-	-	-	-	-
		11A0365-MET500	-	-	-	-	-	-	-	-	-	-
		11A0366-MET500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0364-MET500	+	+	+	+	+	+	+	+	+	+
		11A0365-MET500	+	+	+	+	+	+	+	+	+	+
		11A0366-MET500	+	+	+	+	+	+	+	+	+	+
MET 300	0ng/ml	11A0364-MET300	-	-	-	-	-	-	-	-	-	-
		11A0365-MET300	-	-	-	-	-	-	-	-	-	-
		11A0366-MET300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0364-MET300	-	-	-	-	-	-	-	-	-	-
		11A0365-MET300	-	-	-	-	-	-	-	-	-	-
		11A0366-MET300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0364-MET300	+	+	+	+	+	+	+	+	+	+
		11A0365-MET300	+	+	+	+	+	+	+	+	+	+
		11A0366-MET300	+	+	+	+	+	+	+	+	+	+
MET 200	0ng/ml	11A0364-MET200	-	-	-	-	-	-	-	-	-	-
		11A0365-MET200	-	-	-	-	-	-	-	-	-	-
		11A0366-MET200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0364-MET200	-	-	-	-	-	-	-	-	-	-
		11A0365-MET200	-	-	-	-	-	-	-	-	-	-
		11A0366-MET200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0364-MET200	+	+	+	+	+	+	+	+	+	+
		11A0365-MET200	+	+	+	+	+	+	+	+	+	+
		11A0366-MET200	+	+	+	+	+	+	+	+	+	+
	0ng/ml	11A0418-MQL	-	-	-	-	-	-	-	-	-	-
		11A0419-MQL	-	-	-	-	-	-	-	-	-	-
		11A0420-MQL	-	-	-	-	-	-	-	-	-	-

MOP 300	150ng/ml	11A0418-MQL	-	-	-	-	-	-	-	-	-	-
		11A0419-MQL	-	-	-	-	-	-	-	-	-	-
		11A0420-MQL	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0418-MQL	+	+	+	+	+	+	+	+	+	+
		11A0419-MQL	+	+	+	+	+	+	+	+	+	+
		11A0420-MQL	+	+	+	+	+	+	+	+	+	+
MOP 100	0ng/ml	11A0391-MOP100	-	-	-	-	-	-	-	-	-	-
		11A0392-MOP100	-	-	-	-	-	-	-	-	-	-
		11A0393-MOP100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0391-MOP100	-	-	-	-	-	-	-	-	-	-
		11A0392-MOP100	-	-	-	-	-	-	-	-	-	-
		11A0393-MOP100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0391-MOP100	+	+	+	+	+	+	+	+	+	+
		11A0392-MOP100	+	+	+	+	+	+	+	+	+	+
		11A0393-MOP100	+	+	+	+	+	+	+	+	+	+
MOP 200	0ng/ml	11A0391-MOP200	-	-	-	-	-	-	-	-	-	-
		11A0392-MOP200	-	-	-	-	-	-	-	-	-	-
		11A0393-MOP200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0391-MOP200	-	-	-	-	-	-	-	-	-	-
		11A0392-MOP200	-	-	-	-	-	-	-	-	-	-
		11A0393-MOP200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0391-MOP200	+	+	+	+	+	+	+	+	+	+
		11A0392-MOP200	+	+	+	+	+	+	+	+	+	+
		11A0393-MOP200	+	+	+	+	+	+	+	+	+	+
MQL 300	0ng/ml	11A0418-MQL300	-	-	-	-	-	-	-	-	-	-
		11A0419-MQL300	-	-	-	-	-	-	-	-	-	-
		11A0420-MQL300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0418-MQL300	-	-	-	-	-	-	-	-	-	-
		11A0419-MQL300	-	-	-	-	-	-	-	-	-	-
		11A0420-MQL300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0418-MQL300	+	+	+	+	+	+	+	+	+	+
		11A0419-MQL300	+	+	+	+	+	+	+	+	+	+
		11A0420-MQL300	+	+	+	+	+	+	+	+	+	+
	0ng/ml	11A0427-MTD300	-	-	-	-	-	-	-	-	-	-
		11A0428-MTD300	-	-	-	-	-	-	-	-	-	-
		11A0429-MTD300	-	-	-	-	-	-	-	-	-	-

MTD 300	150ng/ml	11A0427-MTD300	-	-	-	-	-	-	-	-	-	-
		11A0428-MTD300	-	-	-	-	-	-	-	-	-	-
		11A0429-MTD300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0427-MTD300	+	+	+	+	+	+	+	+	+	+
		11A0428-MTD300	+	+	+	+	+	+	+	+	+	+
		11A0429-MTD300	+	+	+	+	+	+	+	+	+	+
MTD 200	0ng/ml	11A0427-MTD200	-	-	-	-	-	-	-	-	-	-
		11A0428-MTD200	-	-	-	-	-	-	-	-	-	-
		11A0429-MTD200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0427-MTD200	-	-	-	-	-	-	-	-	-	-
		11A0428-MTD200	-	-	-	-	-	-	-	-	-	-
		11A0429-MTD200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0427-MTD200	+	+	+	+	+	+	+	+	+	+
		11A0428-MTD200	+	+	+	+	+	+	+	+	+	+
		11A0429-MTD200	+	+	+	+	+	+	+	+	+	+
OPI	0ng/ml	11A0454-OPI	-	-	-	-	-	-	-	-	-	-
		11A0455-OPI	-	-	-	-	-	-	-	-	-	-
		11A0456-OPI	-	-	-	-	-	-	-	-	-	-
	1000ng/ml	11A0454-OPI	-	-	-	-	-	-	-	-	-	-
		11A0455-OPI	-	-	-	-	-	-	-	-	-	-
		11A0456-OPI	-	-	-	-	-	-	-	-	-	-
	3000ng/ml	11A0454-OPI	+	+	+	+	+	+	+	+	+	+
		11A0455-OPI	+	+	+	+	+	+	+	+	+	+
		11A0456-OPI	+	+	+	+	+	+	+	+	+	+
PCP	0ng/ml	11A0490-PCP	-	-	-	-	-	-	-	-	-	-
		11A0491-PCP	-	-	-	-	-	-	-	-	-	-
		11A0492-PCP	-	-	-	-	-	-	-	-	-	-
	12.5ng/ml	11A0490-PCP	-	-	-	-	-	-	-	-	-	-
		11A0491-PCP	-	-	-	-	-	-	-	-	-	-
		11A0492-PCP	-	-	-	-	-	-	-	-	-	-
	37.5ng/ml	11A0490-PCP	+	+	+	+	+	+	+	+	+	+
		11A0491-PCP	+	+	+	+	+	+	+	+	+	+
		11A0492-PCP	+	+	+	+	+	+	+	+	+	+
	0ng/ml	11A0508-PPX300	-	-	-	-	-	-	-	-	-	-
		11A0509-PPX300	-	-	-	-	-	-	-	-	-	-
		11A0510-PPX300	-	-	-	-	-	-	-	-	-	-

PPX	150ng/ml	11A0508-PPX300	-	-	-	-	-	-	-	-	-	-
		11A0509-PPX300	-	-	-	-	-	-	-	-	-	-
		11A0510-PPX300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0508-PPX300	+	+	+	+	+	+	+	+	+	+
		11A0509-PPX300	+	+	+	+	+	+	+	+	+	+
		11A0510-PPX300	+	+	+	+	+	+	+	+	+	+
THC 150	0ng/ml	11A0571-THC150	-	-	-	-	-	-	-	-	-	-
		11A0572-THC150	-	-	-	-	-	-	-	-	-	-
		11A0573-THC150	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0571-THC150	-	-	-	-	-	-	-	-	-	-
		11A0572-THC150	-	-	-	-	-	-	-	-	-	-
		11A0573-THC150	-	-	-	-	-	-	-	-	-	-
	225ng/ml	11A0571-THC150	+	+	+	+	+	+	+	+	+	+
		11A0572-THC150	+	+	+	+	+	+	+	+	+	+
		11A0573-THC150	+	+	+	+	+	+	+	+	+	+
THC 50	0ng/ml	11A0571-THC50	-	-	-	-	-	-	-	-	-	-
		11A0572-THC50	-	-	-	-	-	-	-	-	-	-
		11A0573-THC50	-	-	-	-	-	-	-	-	-	-
	25ng/ml	11A0571-THC50	-	-	-	-	-	-	-	-	-	-
		11A0572-THC50	-	-	-	-	-	-	-	-	-	-
		11A0573-THC50	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0571-THC50	+	+	+	+	+	+	+	+	+	+
		11A0572-THC50	+	+	+	+	+	+	+	+	+	+
		11A0573-THC50	+	+	+	+	+	+	+	+	+	+
THC 25	0ng/ml	11A0571-THC25	-	-	-	-	-	-	-	-	-	-
		11A0572-THC25	-	-	-	-	-	-	-	-	-	-
		11A0573-THC25	-	-	-	-	-	-	-	-	-	-
	12.5ng/ml	11A0571-THC25	-	-	-	-	-	-	-	-	-	-
		11A0572-THC25	-	-	-	-	-	-	-	-	-	-
		11A0573-THC25	-	-	-	-	-	-	-	-	-	-
	37.5ng/ml	11A0571-THC25	+	+	+	+	+	+	+	+	+	+
		11A0572-THC25	+	+	+	+	+	+	+	+	+	+
		11A0573-THC25	+	+	+	+	+	+	+	+	+	+
	0ng/ml	11A0571-THC300	-	-	-	-	-	-	-	-	-	-
		11A0572-THC300	-	-	-	-	-	-	-	-	-	-
		11A0573-THC300	-	-	-	-	-	-	-	-	-	-

THC 300	150ng/ml	11A0571-THC300	-	-	-	-	-	-	-	-	-	-
		11A0572-THC300	-	-	-	-	-	-	-	-	-	-
		11A0573-THC300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0571-THC300	+	+	+	+	+	+	+	+	+	+
		11A0572-THC300	+	+	+	+	+	+	+	+	+	+
		11A0573-THC300	+	+	+	+	+	+	+	+	+	+
THC 200	0ng/ml	11A0571-THC200	-	-	-	-	-	-	-	-	-	-
		11A0572-THC200	-	-	-	-	-	-	-	-	-	-
		11A0573-THC200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0571-THC200	-	-	-	-	-	-	-	-	-	-
		11A0572-THC200	-	-	-	-	-	-	-	-	-	-
		11A0573-THC200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0571-THC200	+	+	+	+	+	+	+	+	+	+
		11A0572-THC200	+	+	+	+	+	+	+	+	+	+
		11A0573-THC200	+	+	+	+	+	+	+	+	+	+
THC30	0ng/ml	11A0571-THC30	-	-	-	-	-	-	-	-	-	-
		11A0572-THC30	-	-	-	-	-	-	-	-	-	-
		11A0573-THC30	-	-	-	-	-	-	-	-	-	-
	15ng/ml	11A0571-THC30	-	-	-	-	-	-	-	-	-	-
		11A0572-THC30	-	-	-	-	-	-	-	-	-	-
		11A0573-THC30	-	-	-	-	-	-	-	-	-	-
	45ng/ml	11A0571-THC30	+	+	+	+	+	+	+	+	+	+
		11A0572-THC30	+	+	+	+	+	+	+	+	+	+
		11A0573-THC30	+	+	+	+	+	+	+	+	+	+
THC 20	0ng/ml	11A0571-THC20	-	-	-	-	-	-	-	-	-	-
		11A0572-THC20	-	-	-	-	-	-	-	-	-	-
		11A0573-THC20	-	-	-	-	-	-	-	-	-	-
	10ng/ml	11A0571-THC20	-	-	-	-	-	-	-	-	-	-
		11A0572-THC20	-	-	-	-	-	-	-	-	-	-
		11A0573-THC20	-	-	-	-	-	-	-	-	-	-
	30ng/ml	11A0571-THC20	+	+	+	+	+	+	+	+	+	+
		11A0572-THC20	+	+	+	+	+	+	+	+	+	+
		11A0573-THC20	+	+	+	+	+	+	+	+	+	+
TC A	0ng/ml	11A0562-TCA1000	-	-	-	-	-	-	-	-	-	-
		11A0563-TCA1000	-	-	-	-	-	-	-	-	-	-

		11A0564-TCA1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0562-TCA1000	-	-	-	-	-	-	-	-	-	-
		11A0563-TCA1000	-	-	-	-	-	-	-	-	-	-
		11A0564-TCA1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0562-TCA1000	+	+	+	+	+	+	+	+	+	+
		11A0563-TCA1000	+	+	+	+	+	+	+	+	+	+
		11A0564-TCA1000	+	+	+	+	+	+	+	+	+	+
TCA 500	0ng/ml	11A0562-TCA500	-	-	-	-	-	-	-	-	-	-
		11A0563-TCA500	-	-	-	-	-	-	-	-	-	-
		11A0564-TCA500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0562-TCA500	-	-	-	-	-	-	-	-	-	-
		11A0563-TCA500	-	-	-	-	-	-	-	-	-	-
		11A0564-TCA500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0562-TCA500	+	+	+	+	+	+	+	+	+	+
		11A0563-TCA500	+	+	+	+	+	+	+	+	+	+
		11A0564-TCA500	+	+	+	+	+	+	+	+	+	+
TML100	0ng/ml	11A0589-TML100	-	-	-	-	-	-	-	-	-	-
		11A0590-TML100	-	-	-	-	-	-	-	-	-	-
		11A0591-TML100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0589-TML100	-	-	-	-	-	-	-	-	-	-
		11A0590-TML100	-	-	-	-	-	-	-	-	-	-
		11A0591-TML100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0589-TML100	+	+	+	+	+	+	+	+	+	+
		11A0590-TML100	+	+	+	+	+	+	+	+	+	+
		11A0591-TML100	+	+	+	+	+	+	+	+	+	+
TML200	0ng/ml	11A0589-TML200	-	-	-	-	-	-	-	-	-	-
		11A0590-TML200	-	-	-	-	-	-	-	-	-	-
		11A0591-TML200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0589-TML200	-	-	-	-	-	-	-	-	-	-
		11A0590-TML200	-	-	-	-	-	-	-	-	-	-
		11A0591-TML200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0589-TML200	+	+	+	+	+	+	+	+	+	+
		11A0590-TML200	+	+	+	+	+	+	+	+	+	+

		11A0591-TML200	+	+	+	+	+	+	+	+	+	+
TML300	0ng/ml	11A0589-TML300	-	-	-	-	-	-	-	-	-	-
		11A0590-TML300	-	-	-	-	-	-	-	-	-	-
		11A0591-TML300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0589-TML300	-	-	-	-	-	-	-	-	-	-
		11A0590-TML300	-	-	-	-	-	-	-	-	-	-
		11A0591-TML300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0589-TML300	+	+	+	+	+	+	+	+	+	+
		11A0590-TML300	+	+	+	+	+	+	+	+	+	+
		11A0591-TML300	+	+	+	+	+	+	+	+	+	+
OX Y	0ng/ml	11A0463-OXY	-	-	-	-	-	-	-	-	-	-
		11A0445-OXY	-	-	-	-	-	-	-	-	-	-
		11A0465-OXY	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0463-OXY	-	-	-	-	-	-	-	-	-	-
		11A0445-OXY	-	-	-	-	-	-	-	-	-	-
		11A0465-OXY	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0463-OXY	+	+	+	+	+	+	+	+	+	+
		11A0445-OXY	+	+	+	+	+	+	+	+	+	+
		11A0465-OXY	+	+	+	+	+	+	+	+	+	+
OXY 300	0ng/ml	11A0463-OXY300	-	-	-	-	-	-	-	-	-	-
		11A0464-OXY300	-	-	-	-	-	-	-	-	-	-
		11A0465-OXY300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0463-OXY300	-	-	-	-	-	-	-	-	-	-
		11A0464-OXY300	-	-	-	-	-	-	-	-	-	-
		11A0465-OXY300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0463-OXY300	+	+	+	+	+	+	+	+	+	+
		11A0464-OXY300	+	+	+	+	+	+	+	+	+	+
		11A0465-OXY300	+	+	+	+	+	+	+	+	+	+
CO T 200	0ng/ml	11A0220-COT200	-	-	-	-	-	-	-	-	-	-
		11A0221-COT200	-	-	-	-	-	-	-	-	-	-
		11A0222-COT200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0220-COT200	-	-	-	-	-	-	-	-	-	-
		11A0221-COT200	-	-	-	-	-	-	-	-	-	-
		11A0222-COT200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0220-COT200	+	+	+	+	+	+	+	+	+	+
		11A0221-COT200	+	+	+	+	+	+	+	+	+	+

		11A0222-COT200	+	+	+	+	+	+	+	+	+	+
COT 100	0ng/ml	11A0220-COT100	-	-	-	-	-	-	-	-	-	-
		11A0221-COT100	-	-	-	-	-	-	-	-	-	-
		11A0222-COT100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0220-COT100	-	-	-	-	-	-	-	-	-	-
		11A0221-COT100	-	-	-	-	-	-	-	-	-	-
		11A0222-COT100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0220-COT100	+	+	+	+	+	+	+	+	+	+
		11A0221-COT100	+	+	+	+	+	+	+	+	+	+
		11A0222-COT100	+	+	+	+	+	+	+	+	+	+
EDDP 300	0ng/ml	11A0238-EDDP300	-	-	-	-	-	-	-	-	-	-
		11A0239-EDDP300	-	-	-	-	-	-	-	-	-	-
		11A0240-EDDP300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0238-EDDP300	-	-	-	-	-	-	-	-	-	-
		11A0239-EDDP300	-	-	-	-	-	-	-	-	-	-
		11A0240-EDDP300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0238-EDDP300	+	+	+	+	+	+	+	+	+	+
		11A0239-EDDP300	+	+	+	+	+	+	+	+	+	+
		11A0240-EDDP300	+	+	+	+	+	+	+	+	+	+
EDDP 100	0ng/ml	11A0238-EDDP100	-	-	-	-	-	-	-	-	-	-
		11A0239-EDDP100	-	-	-	-	-	-	-	-	-	-
		11A0240-EDDP100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0238-EDDP100	-	-	-	-	-	-	-	-	-	-

		11A0239-EDDP100	-	-	-	-	-	-	-	-	-	-
		11A0240-EDDP100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0238-EDDP100	+	+	+	+	+	+	+	+	+	+
		11A0239-EDDP100	+	+	+	+	+	+	+	+	+	+
		11A0240-EDDP100	+	+	+	+	+	+	+	+	+	+
FY L 20	0ng/ml	11A0274-FYL20	-	-	-	-	-	-	-	-	-	-
		11A0275-FYL20	-	-	-	-	-	-	-	-	-	-
		11A0276-FYL20	-	-	-	-	-	-	-	-	-	-
	10ng/ml	11A0274-FYL20	-	-	-	-	-	-	-	-	-	-
		11A0275-FYL20	-	-	-	-	-	-	-	-	-	-
		11A0276-FYL20	-	-	-	-	-	-	-	-	-	-
	30ng/ml	11A0274-FYL20	+	+	+	+	+	+	+	+	+	+
		11A0275-FYL20	+	+	+	+	+	+	+	+	+	+
		11A0276-FYL20	+	+	+	+	+	+	+	+	+	+
FY L 10	0ng/ml	11A0274-FYL10	-	-	-	-	-	-	-	-	-	-
		11A0275-FYL10	-	-	-	-	-	-	-	-	-	-
		11A0276-FYL10	-	-	-	-	-	-	-	-	-	-
	5ng/ml	11A0274-FYL10	-	-	-	-	-	-	-	-	-	-
		11A0275-FYL10	-	-	-	-	-	-	-	-	-	-
		11A0276-FYL10	-	-	-	-	-	-	-	-	-	-
	15ng/ml	11A0274-FYL10	+	+	+	+	+	+	+	+	+	+
		11A0275-FYL10	+	+	+	+	+	+	+	+	+	+
		11A0276-FYL10	+	+	+	+	+	+	+	+	+	+
K 2 50	0ng/ml	11A0544-K2 50	-	-	-	-	-	-	-	-	-	-
		11A0545-K2 50	-	-	-	-	-	-	-	-	-	-
		11A0546-K2 50	-	-	-	-	-	-	-	-	-	-
	25ng/ml	11A0544-K2 50	-	-	-	-	-	-	-	-	-	-
		11A0545-K2 50	-	-	-	-	-	-	-	-	-	-
		11A0546-K2 50	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0544-K2 50	+	+	+	+	+	+	+	+	+	+
		11A0545-K2 50	+	+	+	+	+	+	+	+	+	+
		11A0546-K2 50	+	+	+	+	+	+	+	+	+	+
K 2 30	0ng/ml	11A0544-K2 30	-	-	-	-	-	-	-	-	-	-
		11A0545-K2 30	-	-	-	-	-	-	-	-	-	-
		11A0546-K2 30	-	-	-	-	-	-	-	-	-	-
		11A0544-K2 30	-	-	-	-	-	-	-	-	-	-

	15ng/ml	11A0545-K2 30	-	-	-	-	-	-	-	-	-	-
		11A0546-K2 30	-	-	-	-	-	-	-	-	-	-
	45ng/ml	11A0544-K2 30	+	+	+	+	+	+	+	+	+	+
		11A0545-K2 30	+	+	+	+	+	+	+	+	+	+
		11A0546-K2 30	+	+	+	+	+	+	+	+	+	+
K 2 25	0ng/ml	11A0544-K2 25	-	-	-	-	-	-	-	-	-	-
		11A0545-K2 25	-	-	-	-	-	-	-	-	-	-
		11A0546-K2 25	-	-	-	-	-	-	-	-	-	-
	12.5ng/ml	11A0544-K2 25	-	-	-	-	-	-	-	-	-	-
		11A0545-K2 25	-	-	-	-	-	-	-	-	-	-
		11A0546-K2 25	-	-	-	-	-	-	-	-	-	-
	37.5ng/ml	11A0544-K2 25	+	+	+	+	+	+	+	+	+	+
		11A0545-K2 25	+	+	+	+	+	+	+	+	+	+
		11A0546-K2 25	+	+	+	+	+	+	+	+	+	+
6-MAM 10	0ng/ml	11A0319-6MAM	-	-	-	-	-	-	-	-	-	-
		11A0320-6MAM	-	-	-	-	-	-	-	-	-	-
		11A0321-6MAM	-	-	-	-	-	-	-	-	-	-
	5ng/ml	11A0319-6MAM	-	-	-	-	-	-	-	-	-	-
		11A0320-6MAM	-	-	-	-	-	-	-	-	-	-
		11A0321-6MAM	-	-	-	-	-	-	-	-	-	-
	15ng/ml	11A0319-6MAM	+	+	+	+	+	+	+	+	+	+
		11A0320-6MAM	+	+	+	+	+	+	+	+	+	+
		11A0321-6MAM	+	+	+	+	+	+	+	+	+	+
DI A 300	0ng/ml	11A0229-DIA300	-	-	-	-	-	-	-	-	-	-
		11A0230-DIA300	-	-	-	-	-	-	-	-	-	-
		11A0231-DIA300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0229-DIA300	-	-	-	-	-	-	-	-	-	-
		11A0230-DIA300	-	-	-	-	-	-	-	-	-	-
		11A0231-DIA300	-	-	-	-	-	-	-	-	-	-
	450n0g/ml	11A0229-DIA300	+	+	+	+	+	+	+	+	+	+
		11A0230-DIA300	+	+	+	+	+	+	+	+	+	+
		11A0231-DIA300	+	+	+	+	+	+	+	+	+	+
DI A 200	0ng/ml	11A0229-DIA200	-	-	-	-	-	-	-	-	-	-
		11A0230-DIA200	-	-	-	-	-	-	-	-	-	-
		11A0231-DIA200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0229-DIA200	-	-	-	-	-	-	-	-	-	-

		11A0230-DIA200	-	-	-	-	-	-	-	-	-	-
		11A0231-DIA200	-	-	-	-	-	-	-	-	-	-
	300n0g/ml	11A0229-DIA200	+	+	+	+	+	+	+	+	+	+
		11A0230-DIA200	+	+	+	+	+	+	+	+	+	+
		11A0231-DIA200	+	+	+	+	+	+	+	+	+	+
CLO 400	0ng/ml	11A0202-CLO400	-	-	-	-	-	-	-	-	-	-
		11A0203-CLO400	-	-	-	-	-	-	-	-	-	-
		11A0204-CLO400	-	-	-	-	-	-	-	-	-	-
	200ng/ml	11A0202-CLO400	-	-	-	-	-	-	-	-	-	-
		11A0203-CLO400	-	-	-	-	-	-	-	-	-	-
		11A0204-CLO400	-	-	-	-	-	-	-	-	-	-
	600ng/ml	11A0202-CLO400	+	+	+	+	+	+	+	+	+	+
		11A0203-CLO400	+	+	+	+	+	+	+	+	+	+
		11A0204-CLO400	+	+	+	+	+	+	+	+	+	+
CLO 150	0ng/ml	11A0202-CLO150	-	-	-	-	-	-	-	-	-	-
		11A0203-CLO150	-	-	-	-	-	-	-	-	-	-
		11A0204-CLO150	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0202-CLO150	-	-	-	-	-	-	-	-	-	-
		11A0203-CLO150	-	-	-	-	-	-	-	-	-	-
		11A0204-CLO150	-	-	-	-	-	-	-	-	-	-
	225ng/ml	11A0202-CLO150	+	+	+	+	+	+	+	+	+	+
		11A0203-CLO150	+	+	+	+	+	+	+	+	+	+
		11A0204-CLO150	+	+	+	+	+	+	+	+	+	+
MDA	0ng/ml	11A0346-MDA500	-	-	-	-	-	-	-	-	-	-
		11A0347-MDA500	-	-	-	-	-	-	-	-	-	-
		11A0348-MDA500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0346-MDA500	-	-	-	-	-	-	-	-	-	-
		11A0347-MDA500	-	-	-	-	-	-	-	-	-	-
		11A0348-MDA500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0346-MDA500	+	+	+	+	+	+	+	+	+	+
		11A0347-MDA500	+	+	+	+	+	+	+	+	+	+
		11A0348-MDA500	+	+	+	+	+	+	+	+	+	+
ET G 500	0ng/ml	11A0247-ETG500	-	-	-	-	-	-	-	-	-	-
		11A0248-ETG500	-	-	-	-	-	-	-	-	-	-
		11A0249-ETG500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0247-ETG500	-	-	-	-	-	-	-	-	-	-

		11A0248-ETG500	-	-	-	-	-	-	-	-	-	-
		11A0249-ETG500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0247-ETG500	+	+	+	+	+	+	+	+	+	+
		11A0248-ETG500	+	+	+	+	+	+	+	+	+	+
		11A0249-ETG500	+	+	+	+	+	+	+	+	+	+
ET G 1000	0ng/ml	11A0247-ETG1000	-	-	-	-	-	-	-	-	-	-
		11A0248-ETG1000	-	-	-	-	-	-	-	-	-	-
		11A0249-ETG1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0247-ETG1000	-	-	-	-	-	-	-	-	-	-
		11A0248-ETG1000	-	-	-	-	-	-	-	-	-	-
		11A0249-ETG1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0247-ETG1000	+	+	+	+	+	+	+	+	+	+
		11A0248-ETG1000	+	+	+	+	+	+	+	+	+	+
		11A0249-ETG1000	+	+	+	+	+	+	+	+	+	+
ACE	0ng/ml	11A0076-ACE	-	-	-	-	-	-	-	-	-	-
		11A0077-ACE	-	-	-	-	-	-	-	-	-	-
		11A0078-ACE	-	-	-	-	-	-	-	-	-	-
	2500ng/ml	11A0076-ACE	-	-	-	-	-	-	-	-	-	-
		11A0077-ACE	-	-	-	-	-	-	-	-	-	-
		11A0078-ACE	-	-	-	-	-	-	-	-	-	-
	7500ng/ml	11A0076-ACE	+	+	+	+	+	+	+	+	+	+
		11A0077-ACE	+	+	+	+	+	+	+	+	+	+
		11A0078-ACE	+	+	+	+	+	+	+	+	+	+
LSD 20	0ng/ml	11A0310-LSD20	-	-	-	-	-	-	-	-	-	-
		11A0311-LSD20	-	-	-	-	-	-	-	-	-	-
		11A0312-LSD20	-	-	-	-	-	-	-	-	-	-
	10ng/ml	11A0310-LSD20	-	-	-	-	-	-	-	-	-	-
		11A0311-LSD20	-	-	-	-	-	-	-	-	-	-
		11A0312-LSD20	-	-	-	-	-	-	-	-	-	-
	30ng/ml	11A0310-LSD20	+	+	+	+	+	+	+	+	+	+
		11A0311-LSD20	+	+	+	+	+	+	+	+	+	+
		11A0312-LSD20	+	+	+	+	+	+	+	+	+	+

LSD 50	0ng/ml	11A0310-LSD50	-	-	-	-	-	-	-	-	-	-
		11A0311-LSD50	-	-	-	-	-	-	-	-	-	-
		11A0312-LSD50	-	-	-	-	-	-	-	-	-	-

	25ng/ml	11A0310-LSD50	-	-	-	-	-	-	-	-	-	-
		11A0311-LSD50	-	-	-	-	-	-	-	-	-	-
		11A0312-LSD50	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0310-LSD50	+	+	+	+	+	+	+	+	+	+
		11A0311-LSD50	+	+	+	+	+	+	+	+	+	+
		11A0312-LSD50	+	+	+	+	+	+	+	+	+	+
MDPV	0ng/ml	11A0355-MDPV	-	-	-	-	-	-	-	-	-	-
		11A0356-MDPV	-	-	-	-	-	-	-	-	-	-
		11A0357-MDPV	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0355-MDPV	-	-	-	-	-	-	-	-	-	-
		11A0356-MDPV	-	-	-	-	-	-	-	-	-	-
		11A0357-MDPV	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0355-MDPV	+	+	+	+	+	+	+	+	+	+
		11A0356-MDPV	+	+	+	+	+	+	+	+	+	+
		11A0357-MDPV	+	+	+	+	+	+	+	+	+	+
MP D 300	0ng/ml	11A0400-MPD300	-	-	-	-	-	-	-	-	-	-
		11A0401-MPD300	-	-	-	-	-	-	-	-	-	-
		11A0402-MPD300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0400-MPD300	-	-	-	-	-	-	-	-	-	-
		11A0401-MPD300	-	-	-	-	-	-	-	-	-	-
		11A0402-MPD300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0400-MPD300	+	+	+	+	+	+	+	+	+	+
		11A0401-MPD300	+	+	+	+	+	+	+	+	+	+
		11A0402-MPD300	+	+	+	+	+	+	+	+	+	+
7-ACL 300	0ng/ml	11A0085-7ACL300	-	-	-	-	-	-	-	-	-	-
		11A0086-7ACL300	-	-	-	-	-	-	-	-	-	-
		11A0087-7ACL300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0085-7ACL300	-	-	-	-	-	-	-	-	-	-
		11A0086-7ACL300	-	-	-	-	-	-	-	-	-	-
		11A0087-7ACL300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0085-7ACL300	+	+	+	+	+	+	+	+	+	+
		11A0086-7ACL300	+	+	+	+	+	+	+	+	+	+
		11A0087-7ACL300	+	+	+	+	+	+	+	+	+	+
7-ACL	0ng/ml	11A0085-7ACL100	-	-	-	-	-	-	-	-	-	-

100		11A0086-7ACL100	-	-	-	-	-	-	-	-	-	-
		11A0087-7ACL100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0085-7ACL100	-	-	-	-	-	-	-	-	-	-
		11A0086-7ACL100	-	-	-	-	-	-	-	-	-	-
		11A0087-7ACL100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0085-7ACL100	+	+	+	+	+	+	+	+	+	+
		11A0086-7ACL100	+	+	+	+	+	+	+	+	+	+
		11A0087-7ACL100	+	+	+	+	+	+	+	+	+	+
7-ACL 200	0ng/ml	11A0085-7ACL200	-	-	-	-	-	-	-	-	-	-
		11A0086-7ACL200	-	-	-	-	-	-	-	-	-	-
		11A0087-7ACL200	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0085-7ACL200	-	-	-	-	-	-	-	-	-	-
		11A0086-7ACL200	-	-	-	-	-	-	-	-	-	-
		11A0087-7ACL200	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0085-7ACL200	+	+	+	+	+	+	+	+	+	+
		11A0086-7ACL200	+	+	+	+	+	+	+	+	+	+
		11A0087-7ACL200	+	+	+	+	+	+	+	+	+	+
ZOL	0ng/ml	11A0634-ZOL	-	-	-	-	-	-	-	-	-	-
		11A0635-ZOL	-	-	-	-	-	-	-	-	-	-
		11A0636-ZOL	-	-	-	-	-	-	-	-	-	-
	25ng/ml	11A0634-ZOL	-	-	-	-	-	-	-	-	-	-
		11A0635-ZOL	-	-	-	-	-	-	-	-	-	-
		11A0636-ZOL	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0634-ZOL	+	+	+	+	+	+	+	+	+	+
		11A0635-ZOL	+	+	+	+	+	+	+	+	+	+
		11A0636-ZOL	+	+	+	+	+	+	+	+	+	+
CFYL	0ng/ml	11A0184-CFYL500	-	-	-	-	-	-	-	-	-	-

500		11A0185-CFYL500	-	-	-	-	-	-	-	-	-	-
		11A0186-CFYL500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0184-CFYL500	-	-	-	-	-	-	-	-	-	-
		11A0185-CFYL500	-	-	-	-	-	-	-	-	-	-
		11A0186-CFYL500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0184-CFYL500	+	+	+	+	+	+	+	+	+	+
		11A0185-CFYL500	+	+	+	+	+	+	+	+	+	+
		11A0186-CFYL500	+	+	+	+	+	+	+	+	+	+
MEP 100	0ng/ml	11A0373-MEP100	-	-	-	-	-	-	-	-	-	-
		11A0374-MEP100	-	-	-	-	-	-	-	-	-	-
		11A0375-MEP100	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0373-MEP100	-	-	-	-	-	-	-	-	-	-
		11A0374-MEP100	-	-	-	-	-	-	-	-	-	-
		11A0375-MEP100	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0373-MEP100	+	+	+	+	+	+	+	+	+	+
		11A0374-MEP100	+	+	+	+	+	+	+	+	+	+
		11A0375-MEP100	+	+	+	+	+	+	+	+	+	+
ZOP 50	0ng/ml	11A0643-ZOP	-	-	-	-	-	-	-	-	-	-
		11A0644-ZOP	-	-	-	-	-	-	-	-	-	-
		11A0645-ZOP	-	-	-	-	-	-	-	-	-	-
	25ng/ml	11A0643-ZOP	-	-	-	-	-	-	-	-	-	-
		11A0644-ZOP	-	-	-	-	-	-	-	-	-	-
		11A0645-ZOP	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0643-ZOP	+	+	+	+	+	+	+	+	+	+
		11A0644-ZOP	+	+	+	+	+	+	+	+	+	+
		11A0645-ZOP	+	+	+	+	+	+	+	+	+	+
CAF	0ng/ml	11A0157-CAF	-	-	-	-	-	-	-	-	-	-

		11A0158-CAF	-	-	-	-	-	-	-	-	-	-
		11A0159-CAF	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0157-CAF	-	-	-	-	-	-	-	-	-	-
		11A0158-CAF	-	-	-	-	-	-	-	-	-	-
		11A0159-CAF	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0157-CAF	+	+	+	+	+	+	+	+	+	+
		11A0158-CAF	+	+	+	+	+	+	+	+	+	+
		11A0159-CAF	+	+	+	+	+	+	+	+	+	+
CAT	0ng/ml	11A0148-CAT	-	-	-	-	-	-	-	-	-	-
		11A0149-CAT	-	-	-	-	-	-	-	-	-	-
		11A0150-CAT	-	-	-	-	-	-	-	-	-	-
	75ng/ml	11A0148-CAT	-	-	-	-	-	-	-	-	-	-
		11A0149-CAT	-	-	-	-	-	-	-	-	-	-
		11A0150-CAT	-	-	-	-	-	-	-	-	-	-
	225ng/ml	11A0148-CAT	+	+	+	+	+	+	+	+	+	+
		11A0149-CAT	+	+	+	+	+	+	+	+	+	+
		11A0150-CAT	+	+	+	+	+	+	+	+	+	+
TRO	0ng/ml	11A0598-TRO	-	-	-	-	-	-	-	-	-	-
		11A0599-TRO	-	-	-	-	-	-	-	-	-	-
		11A0600-TRO	-	-	-	-	-	-	-	-	-	-
	175ng/ml	11A0598-TRO	-	-	-	-	-	-	-	-	-	-
		11A0599-TRO	-	-	-	-	-	-	-	-	-	-
		11A0600-TRO	-	-	-	-	-	-	-	-	-	-
	525ng/ml	11A0598-TRO	+	+	+	+	+	+	+	+	+	+
		11A0599-TRO	+	+	+	+	+	+	+	+	+	+
		11A0600-TRO	+	+	+	+	+	+	+	+	+	+
ALP 100	0ng/ml	11A0094-ALP	-	-	-	-	-	-	-	-	-	-
		11A0095-ALP	-	-	-	-	-	-	-	-	-	-
		11A0096-ALP	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0094-ALP	-	-	-	-	-	-	-	-	-	-
		11A0095-ALP	-	-	-	-	-	-	-	-	-	-
		11A0096-ALP	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0094-ALP	+	+	+	+	+	+	+	+	+	+
		11A0095-ALP	+	+	+	+	+	+	+	+	+	+
		11A0096-ALP	+	+	+	+	+	+	+	+	+	+
APVP	0ng/ml	11A0112-PVP1000	-	-	-	-	-	-	-	-	-	-

1000		11A0113-PVP1000	-	-	-	-	-	-	-	-	-	-
		11A0114-PVP1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0112-PVP1000	-	-	-	-	-	-	-	-	-	-
		11A0113-PVP1000	-	-	-	-	-	-	-	-	-	-
		11A0114-PVP1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0112-PVP1000	+	+	+	+	+	+	+	+	+	+
		11A0113-PVP1000	+	+	+	+	+	+	+	+	+	+
		11A0114-PVP1000	+	+	+	+	+	+	+	+	+	+
APVP 500	0ng/ml	11A0112-PVP500	-	-	-	-	-	-	-	-	-	-
		11A0113-PVP500	-	-	-	-	-	-	-	-	-	-
		11A0114-PVP500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0112-PVP500	-	-	-	-	-	-	-	-	-	-
		11A0113-PVP500	-	-	-	-	-	-	-	-	-	-
		11A0114-PVP500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0112-PVP500	+	+	+	+	+	+	+	+	+	+
		11A0113-PVP500	+	+	+	+	+	+	+	+	+	+
		11A0114-PVP500	+	+	+	+	+	+	+	+	+	+
CNB 500	0ng/ml	11A0787-CBN	-	-	-	-	-	-	-	-	-	-
		11A0788-CBN	-	-	-	-	-	-	-	-	-	-
		11A0789-CBN	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0787-CBN	-	-	-	-	-	-	-	-	-	-
		11A0788-CBN	-	-	-	-	-	-	-	-	-	-
		11A0789-CBN	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0787-CBN	+	+	+	+	+	+	+	+	+	+
		11A0788-CBN	+	+	+	+	+	+	+	+	+	+
		11A0789-CBN	+	+	+	+	+	+	+	+	+	+
MPRB 100	0ng/ml	11A0409-MPRD	-	-	-	-	-	-	-	-	-	-
		11A0410-MPRD	-	-	-	-	-	-	-	-	-	-
		11A0411-MPRD	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0409-MPRD	-	-	-	-	-	-	-	-	-	-
		11A0410-MPRD	-	-	-	-	-	-	-	-	-	-
		11A0411-MPRD	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0409-MPRD	+	+	+	+	+	+	+	+	+	+
		11A0410-MPRD	+	+	+	+	+	+	+	+	+	+
		11A0411-MPRD	+	+	+	+	+	+	+	+	+	+
PGB 50,000	0ng/ml	11A0499-PGB	-	-	-	-	-	-	-	-	-	-
		11A0500-PGB	-	-	-	-	-	-	-	-	-	-
		11A0501-PGB	-	-	-	-	-	-	-	-	-	-

	25,000ng/ml	11A0499-PGB	-	-	-	-	-	-	-	-	-	-
		11A0500-PGB	-	-	-	-	-	-	-	-	-	-
		11A0501-PGB	-	-	-	-	-	-	-	-	-	-
	75,000ng/ml	11A0499-PGB	+	+	+	+	+	+	+	+	+	+
		11A0500-PGB	+	+	+	+	+	+	+	+	+	+
		11A0501-PGB	+	+	+	+	+	+	+	+	+	+
TZD 200	0ng/ml	11A0607-TZD	-	-	-	-	-	-	-	-	-	-
		11A0608-TZD	-	-	-	-	-	-	-	-	-	-
		11A0609-TZD	-	-	-	-	-	-	-	-	-	-
	100ng/ml	11A0607-TZD	-	-	-	-	-	-	-	-	-	-
		11A0608-TZD	-	-	-	-	-	-	-	-	-	-
		11A0609-TZD	-	-	-	-	-	-	-	-	-	-
	300ng/ml	11A0607-TZD	+	+	+	+	+	+	+	+	+	+
		11A0608-TZD	+	+	+	+	+	+	+	+	+	+
		11A0609-TZD	+	+	+	+	+	+	+	+	+	+
UR-144 25	0ng/ml	11A0616-K4	-	-	-	-	-	-	-	-	-	-
		11A0617-K4	-	-	-	-	-	-	-	-	-	-
		11A0618-K4	-	-	-	-	-	-	-	-	-	-
	12.5ng/ml	11A0616-K4	-	-	-	-	-	-	-	-	-	-
		11A0617-K4	-	-	-	-	-	-	-	-	-	-
		11A0618-K4	-	-	-	-	-	-	-	-	-	-
	37.5ng/ml	11A0616-K4	+	+	+	+	+	+	+	+	+	+
		11A0617-K4	+	+	+	+	+	+	+	+	+	+
		11A0618-K4	+	+	+	+	+	+	+	+	+	+
ZAL 100	0ng/ml	11A0625-ZAL	-	-	-	-	-	-	-	-	-	-
		11A0626-ZAL	-	-	-	-	-	-	-	-	-	-
		11A0627-ZAL	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0625-ZAL	-	-	-	-	-	-	-	-	-	-
		11A0626-ZAL	-	-	-	-	-	-	-	-	-	-
		11A0627-ZAL	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0625-ZAL	+	+	+	+	+	+	+	+	+	+
		11A0626-ZAL	+	+	+	+	+	+	+	+	+	+
		11A0627-ZAL	+	+	+	+	+	+	+	+	+	+
MES 100	0ng/ml	11A0382-MES	-	-	-	-	-	-	-	-	-	-
		11A0383-MES	-	-	-	-	-	-	-	-	-	-
		11A0384-MES	-	-	-	-	-	-	-	-	-	-
	50ng/ml	11A0382-MES	-	-	-	-	-	-	-	-	-	-
		11A0383-MES	-	-	-	-	-	-	-	-	-	-

		11A0384-MES	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0382-MES	+	+	+	+	+	+	+	+	+	+
		11A0383-MES	+	+	+	+	+	+	+	+	+	+
		11A0384-MES	+	+	+	+	+	+	+	+	+	+
GAB 2000	0ng/ml	11A0283-GAB	-	-	-	-	-	-	-	-	-	-
		11A0284-GAB	-	-	-	-	-	-	-	-	-	-
		11A0285-GAB	-	-	-	-	-	-	-	-	-	-
	1000ng/ml	11A0283-GAB	-	-	-	-	-	-	-	-	-	-
		11A0284-GAB	-	-	-	-	-	-	-	-	-	-
		11A0285-GAB	-	-	-	-	-	-	-	-	-	-
	3000ng/ml	11A0283-GAB	+	+	+	+	+	+	+	+	+	+
		11A0284-GAB	+	+	+	+	+	+	+	+	+	+
		11A0285-GAB	+	+	+	+	+	+	+	+	+	+
TLD 50	0ng/ml	11A0580-TLD50	-	-	-	-	-	-	-	-	-	-
		11A0581-TLD50	-	-	-	-	-	-	-	-	-	-
		11A0582-TLD50	-	-	-	-	-	-	-	-	-	-
	25 ng/ml	11A0580-TLD50	-	-	-	-	-	-	-	-	-	-
		11A0581-TLD50	-	-	-	-	-	-	-	-	-	-
		11A0582-TLD50	-	-	-	-	-	-	-	-	-	-
	75 ng/ml	11A0580-TLD50	+	+	+	+	+	+	+	+	+	+
		11A0581-TLD50	+	+	+	+	+	+	+	+	+	+
		11A0582-TLD50	+	+	+	+	+	+	+	+	+	+
QTP 1000	0ng/ml	11A0517-QTP1000	-	-	-	-	-	-	-	-	-	-
		11A0518-QTP1000	-	-	-	-	-	-	-	-	-	-
		11A0519-QTP1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0517-QTP1000	-	-	-	-	-	-	-	-	-	-
		11A0518-QTP1000	-	-	-	-	-	-	-	-	-	-
		11A0519-QTP1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0517-QTP1000	+	+	+	+	+	+	+	+	+	+
		11A0518-QTP1000	+	+	+	+	+	+	+	+	+	+
		11A0519-QTP1000	+	+	+	+	+	+	+	+	+	+
PAP 500	0ng/ml	11A0481-PAP500	-	-	-	-	-	-	-	-	-	-
		11A0482-PAP500	-	-	-	-	-	-	-	-	-	-
		11A0483-PAP500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0481-PAP500	-	-	-	-	-	-	-	-	-	-
		11A0482-PAP500	-	-	-	-	-	-	-	-	-	-
		11A0483-PAP500	-	-	-	-	-	-	-	-	-	-
		11A0481-PAP500	+	+	+	+	+	+	+	+	+	+

	750ng/ml	11A0482-PAP500	+	+	+	+	+	+	+	+	+	+
		11A0483-PAP500	+	+	+	+	+	+	+	+	+	+
KRA 300	0ng/ml	11A0301-KRA300	-	-	-	-	-	-	-	-	-	-
		11A0302-KRA300	-	-	-	-	-	-	-	-	-	-
		11A0303-KRA300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A0301-KRA300	-	-	-	-	-	-	-	-	-	-
		11A0302-KRA300	-	-	-	-	-	-	-	-	-	-
		11A0303-KRA300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A0301-KRA300	+	+	+	+	+	+	+	+	+	+
		11A0302-KRA300	+	+	+	+	+	+	+	+	+	+
		11A0303-KRA300	+	+	+	+	+	+	+	+	+	+
CAR 2000	0ng/ml	11A0166-CAR2000	-	-	-	-	-	-	-	-	-	-
		11A0167-CAR2000	-	-	-	-	-	-	-	-	-	-
		11A0168-CAR2000	-	-	-	-	-	-	-	-	-	-
	1000ng/ml	11A0166-CAR2000	-	-	-	-	-	-	-	-	-	-
		11A0167-CAR2000	-	-	-	-	-	-	-	-	-	-
		11A0168-CAR2000	-	-	-	-	-	-	-	-	-	-
	2000ng/ml	11A0166-CAR2000	+	+	+	+	+	+	+	+	+	+
		11A0167-CAR2000	+	+	+	+	+	+	+	+	+	+
		11A0168-CAR2000	+	+	+	+	+	+	+	+	+	+
FLX 500	0ng/ml	11A0265-FLX500	-	-	-	-	-	-	-	-	-	-
		11A0266-FLX500	-	-	-	-	-	-	-	-	-	-
		11A0267-FLX500	-	-	-	-	-	-	-	-	-	-
	250ng/ml	11A0265-FLX500	-	-	-	-	-	-	-	-	-	-
		11A0266-FLX500	-	-	-	-	-	-	-	-	-	-
		11A0267-FLX500	-	-	-	-	-	-	-	-	-	-
	750ng/ml	11A0265-FLX500	+	+	+	+	+	+	+	+	+	+
		11A0266-FLX500	+	+	+	+	+	+	+	+	+	+
		11A0267-FLX500	+	+	+	+	+	+	+	+	+	+
HMO 250	0ng/ml	11A1715-HMO250	-	-	-	-	-	-	-	-	-	-
		11A1716-HMO250	-	-	-	-	-	-	-	-	-	-
		11A1717-HMO250	-	-	-	-	-	-	-	-	-	-
	125ng/ml	11A1715-HMO250	-	-	-	-	-	-	-	-	-	-
		11A1716-HMO250	-	-	-	-	-	-	-	-	-	-
		11A1717-HMO250	-	-	-	-	-	-	-	-	-	-
	375ng/ml	11A1715-HMO250	+	+	+	+	+	+	+	+	+	+
		11A1716-HMO250	+	+	+	+	+	+	+	+	+	+
		11A1717-HMO250	+	+	+	+	+	+	+	+	+	+

HMO 300	0ng/ml	11A1715-HMO300	-	-	-	-	-	-	-	-	-	-
		11A1716-HMO300	-	-	-	-	-	-	-	-	-	-
		11A1717-HMO300	-	-	-	-	-	-	-	-	-	-
	150ng/ml	11A1715-HMO300	-	-	-	-	-	-	-	-	-	-
		11A1716-HMO300	-	-	-	-	-	-	-	-	-	-
		11A1717-HMO300	-	-	-	-	-	-	-	-	-	-
	450ng/ml	11A1715-HMO300	+	+	+	+	+	+	+	+	+	+
		11A1716-HMO300	+	+	+	+	+	+	+	+	+	+
		11A1717-HMO300	+	+	+	+	+	+	+	+	+	+
OZP1000	0ng/ml	11A0472-OZP1000	-	-	-	-	-	-	-	-	-	-
		11A0473-OZP1000	-	-	-	-	-	-	-	-	-	-
		11A0474-OZP1000	-	-	-	-	-	-	-	-	-	-
	500ng/ml	11A0472-OZP1000	-	-	-	-	-	-	-	-	-	-
		11A0473-OZP1000	-	-	-	-	-	-	-	-	-	-
		11A0474-OZP1000	-	-	-	-	-	-	-	-	-	-
	1500ng/ml	11A0472-OZP1000	+	+	+	+	+	+	+	+	+	+
		11A0473-OZP1000	+	+	+	+	+	+	+	+	+	+
		11A0474-OZP1000	+	+	+	+	+	+	+	+	+	+

Conclusion: Test results were consistent among the three lots of each test in Multi-Drug Test Dip Card with/without Adulteration.

2.7 Accelerated Stability

Accelerated Stability of The Multi-Drug Test Dip Card with/without Adulteration was evaluated using samples from three different batches; each batch will assembled in 10 in 1 Dip Card. These were placed in an incubator with the temperature calibrated at 45℃ and 55℃, and relative humidity (RH) calibrated at 60%. A series of stability tests were performed at 7, 14, 21, 28, 35, 42, 56, 77, 84 days. Tests were assayed using each test concentration at drug free urine, -50% Cut-off and +50% Cut-off urine specimens. Testing at each specific time interval consisted of triplicates for each specimen. The tests were performed according to the package insert. Results are presented in tables below.

Table: Timeline for Accelerate Stability Study

Day / Temp.	0 day	7 days	14 days	21 days	28 days	35 days	42 days	56 days	77 days	84 days
45℃	√	√	√	√	√	√	√	√	√	√
55℃	√	√	√	√	√	√	√	X	X	X

Table: Accelerated Stability Summary

Accelerated Stability Study Results at 45℃			
			Batch No.

Product	Day	Specimen	11A0103-AMP1000	11A0104-AMP1000	11A0105-AMP1000
AMP 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0103-AMP1000	11A0104-AMP1000	11A0105-AMP1000
	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

AMP 1000		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0103-AMP500	11A0104-AMP500	11A0105-AMP500
AMP 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0103-AMP500	11A0104-AMP500	11A0105-AMP500
AMP 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0103-AMP300	11A0104-AMP300	11A0105-AMP300
	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

AMP 300	7	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0103-AMP300	11A0104-AMP300	11A0105-AMP300
AMP 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	28	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0121-BAR300	11A0122-BAR300	11A0123-BAR300
BAR 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0121-BAR300	11A0122-BAR300	11A0123-BAR300
BAR 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0121-BAR200	11A0122-BAR200	11A0123-BAR200
	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

BAR 200		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0121-BAR200	11A0122-BAR200	11A0123-BAR200
BAR 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0130-BUP10	11A0131-BUP10	11A0132-BUP10
BUP 10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0130-BUP10	11A0131-BUP10	11A0132-BUP10
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

BUP 10	0	+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0130-BUP10	11A0131-BUP10	11A0132-BUP10
BUP 10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0130-BUP10	11A0131-BUP10	11A0132-BUP10
BUP 10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO500	11A0140-BZO500	11A0141-BZO500
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

BZO 500	0	-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO500	11A0140-BZO500	11A0141-BZO500
	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

BZO 500	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO300	11A0140-BZO300	11A0141-BZO300
BZO 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO300	11A0140-BZO300	11A0141-BZO300
BZO 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO200	11A0140-BZO200	11A0141-BZO200
BZO 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO200	11A0140-BZO200	11A0141-BZO200
BZO 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	21	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO100	11A0140-BZO100	11A0141-BZO100
BZO 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0139-BZO100	11A0140-BZO100	11A0141-BZO100
BZO 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0211-COC300	11A0212-COC300	11A0213-COC300
COC 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0211-COC300	11A0212-COC300	11A0213-COC300
COC 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.

			11A0211-COC150	11A0212-COC150	11A0213-COC150
COC 150	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0211-COC150	11A0212-COC150	11A0213-COC150
COC 150	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0211-COC100	11A0212-COC100	11A0213-COC100
COC 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	77	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0211-COC100	11A0212-COC100	11A0213-COC100
COC 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0211-COC200	11A0212-COC200	11A0213-COC200
COC 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0211-COC200	11A0212-COC200	11A0213-COC200
COC 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0292-KET1000	11A0293-KET1000	11A0294-KET1000
KET 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0292-KET1000	11A0293-KET1000	11A0294-KET1000
KET 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

			+	+	+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0292-KET500	11A0293-KET500	11A0294-KET500
KET 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0292-KET500	11A0293-KET500	11A0294-KET500
KET 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0292-KET300	11A0293-KET300	11A0294-KET300
KET 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0292-KET300	11A0293-KET300	11A0294-KET300
KET 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0292-KET100	11A0293-KET100	11A0294-KET100
KET 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,	+,+,+,+,+,+,+,+,+,
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0292-KET100	11A0293-KET100	11A0294-KET100
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

KET 100	0	+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0337-MDMA500	11A0338-MDMA500	11A0339-MDMA500
MDMA 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0337-MDMA500	11A0338-MDMA500	11A0339-MDMA500
MDMA 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0337-MDMA1000	11A0338-MDMA1000	11A0339-MDMA1000
MDMA 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	7	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0337-MDMA1000	11A0338-MDMA1000	11A0339-MDMA1000
MDMA 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	35	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0337-MDMA300	11A0338-MDMA300	11A0339-MDMA300
MDMA 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0337-MDMA300	11A0338-MDMA300	11A0339-MDMA300
MDM	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

A 300		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0364-MET1000	11A0365-MET1000	11A0366-MET1000
MET 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0364-MET1000	11A0365-MET1000	11A0366-MET1000
MET 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0364-MET500	11A0365-MET500	11A0366-MET500
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

MET 500	0	+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0364-MET500	11A0365-MET500	11A0366-MET500
MET 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	28	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0364-MET300	11A0365-MET300	11A0366-MET300
MET 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
			Batch No.		

Product	Day	Specimen	11A0364-MET300	11A0365-MET300	11A0366-MET300

MET 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0364-MET200	11A0365-MET200	11A0366-MET200
MET 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	35	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0364-MET200	11A0365-MET200	11A0366-MET200
MET 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃			
			Batch No.

Product	Day	Specimen	11A0391-MOP 300	11A0392-MOP300	11A0393-MOP300
MOP 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0391-MOP 300	11A0392-MOP300	11A0393-MOP300
	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

MOP 300	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0391-MOP100	11A0392-MOP100	11A0393-MOP100
MOP 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0391-MOP100	11A0392-MOP100	11A0393-MOP100
MOP 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0391-MOP200	11A0392-MOP200	11A0393-MOP200
MOP 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0391-MOP200	11A0392-MOP200	11A0393-MOP200
MOP 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0418-MQL	11A0419-MQL	11A0420-MQL
MQL	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	21	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0418-MQL	11A0419-MQL	11A0420-MQL
MQL	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0427-MTD300	11A0428-MTD300	11A0429-MTD300
MTD 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0427-MTD300	11A0428-MTD300	11A0429-MTD300
MTD 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	7	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0427-MTD200	11A0428-MTD200	11A0429-MTD200
MTD 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0427-MTD200	11A0428-MTD200	11A0429-MTD200
MTD 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0454-OPI	11A0455-OPI	11A0456-OPI
OPI	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0454-OPI	11A0455-OPI	11A0456-OPI
OPI	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			PCP14030001p-T	11A0491-PCP	11A0492-PCP
PCP	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			PCP14030001p-T	11A0491-PCP	11A0492-PCP
PCP	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			PPX14030001p-T	11A0509-PPX300	11A0510-PPX300
PPX	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			PPX14030001p-T	11A0509-PPX300	11A0510-PPX300
PPX	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			THC14030001p-T	11A0572-THC150	11A0573-THC150
THC 150	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			THC14030001p-T	11A0572-THC150	11A0573-THC150
THC 150	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			THC14030007p-T	11A0572-THC50	11A0573-THC50
THC 50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			THC14030007p-T	11A0572-THC50	11A0573-THC50
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

THC 50	0	+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			THC14030013p-T	11A0572-THC25	11A0573-THC25
THC 25	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			THC14030013p-T	11A0572-THC25	11A0573-THC25
THC 25	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			THC14030019p - T	11A0572-THC300	11A0573-THC300
THC 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			THC14030019p-T	11A0572-THC300	11A0573-THC300
THC 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	35	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			THC14030025p-T	11A0572-THC200	11A0573-THC200
THC 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			THC14030025p-T	11A0572-THC200	11A0573-THC200

THC 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			THC14030031p-T	11A0572-THC30	11A0573-THC30
THC 30	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			THC14030031p - T	11A0572-THC30	11A0573-THC30
THC 30	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			THC14030037p-T	11A0572-THC20	11A0573-THC20
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

THC 20	0	+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			THC14030037p-T	11A0572-THC20	11A0573-THC20
THC 20	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	21	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			TCA14030001p-T	11A0563-TCA1000	11A0564-TCA1000
TCA	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
			Batch No.		

Product	Day	Specimen	TCA14030001p-T	11A0563-TCA1000	11A0564-TCA1000
TCA	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0562-TCA500	11A0563-TCA500	11A0564-TCA500
TCA500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0562-TCA500	11A0563-TCA500	11A0564-TCA500
TCA500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			TML14030001p-T	TML14030002p-T	11A0591-TML100
TML 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			TML14030001p-T	TML14030002p-T	11A0591-TML100

TML 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			TML14030007p - T	TML14030008p - T	11A0591-TML200
TML 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			TML14030007p-T	TML14030008p-T	11A0591-TML200
TML 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			TML14030013p-T	TML14030014p-T	11A0591-TML300

TM L 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			TML14030007p-T	TML14030008p-T	11A0591-TML200
TML 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			OXY14030001p - T	11A0445-OXY	11A0465-OXY
OXY	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			OXY14030001p-T	11A0445-OXY	11A0465-OXY
OXY	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0463-OXY300	11A0464-OXY300	11A0465-OXY300
OXY300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0463-OXY300	11A0464-OXY300	11A0465-OXY300
OXY300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

			Batch No.

Product	Day	Specimen	COT14030001p-T	11A0221-COT200	11A0222-COT200
COT 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			COT14030001p-T	11A0221-COT200	11A0222-COT200
COT 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.

			COT14030007p-T	11A0221-COT100	11A0222-COT100
COT 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			COT14030007p-T	11A0221-COT100	11A0222-COT100
COT 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			EDDP14030001p-T	EDDP14030002p-T	11A0240-EDDP300
EDDP 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	77	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			EDDP14030001p-T	EDDP14030002p-T	EDDP14030003p-T
EDDP 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			EDDP14030007p-T	EDDP14030008p-T	11A0240-EDDP100
EDDP 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			EDDP14030007p-T	EDDP14030008p-T	EDDP14030009p-T
EDDP100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0274-FYL20	11A0275-FYL20	11A0276-FYL20
FYL20	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0274-FYL20	11A0275-FYL20	11A0276-FYL20
FYL20	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0274-FYL10	11A0275-FYL10	11A0276-FYL10
FYL10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0274-FYL10	11A0275-FYL10	11A0276-FYL10
FYL10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0544-K2 50	11A0545-K2 50	11A0546-K2 50
K250	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0544-K2 50	11A0545-K2 50	11A0546-K2 50
K 2 50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			SMA14030007p-T	SMA14030008p-T	SMA14030009p-T
K 2 30	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			SMA14030007p-T	SMA14030008p-T	SMA14030009p-T
K 2	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

30	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			SMA14030013p-T	SMA14030014p-T	SMA14030015p-T
K 2 30	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			SMA14030013p-T	SMA14030014p-T	SMA14030015p-T
K 2 30	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			MAM14030001p-T	MAM14030002p-T	MAM14030003p-T
6-MAM 10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			MAM14030001p-T	MAM14030002p-T	MAM14030003p-T
6-MAM 10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0229-DIA300	11A0230-DIA300	11A0231-DIA300
DIA 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0229-DIA300	11A0230-DIA300	11A0231-DIA300
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

DIA 300	0	+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0229-DIA200	11A0230-DIA200	11A0231-DIA200
DIA 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0229-DIA200	11A0230-DIA200	11A0231-DIA200
DIA 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			CLO14030001p - T	11A0203-CLO400	11A0204-CLO400
CLO 400	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			CLO14030001p-T	11A0203-CLO400	11A0204-CLO400
CLO 400	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	42	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			CLO14030007p-T	11A0203-CLO150	11A0204-CLO150
CLO 150	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			CLO14030007p-T	11A0203-CLO150	11A0204-CLO150
CLO	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

150			+	+	
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			MDA14030001p-T	11A0347-MDA	11A0348-MDA
MDA	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	56	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			MDA14030001p-T	11A0347-MDA	11A0348-MDA
MDA	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			ETG14030001p-T	11A0248-ETG500	11A0249-ETG500
ETG500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			ETG14030001p-T	11A0248-ETG500	11A0249-ETG500
ETG500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			ETG14030007p-T	11A0248-ETG1000	11A0249-ETG1000
ETG1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			ETG14030007p - T	11A0248-ETG1000	11A0249-ETG1000
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

ETG1000	0	+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			ACE14060001p-T	11A0077-ACE	11A0078-ACE
ACE	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	56	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			ACE14060001p-T	11A0077-ACE	11A0078-ACE
ACE	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0310-LSD20	11A0311-LSD20	11A0312-LSD20
LSD20	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	7	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0310-LSD20	11A0311-LSD20	11A0312-LSD20
LSD20	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0310-LSD50	11A0311-LSD50	11A0312-LSD50
LSD50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0310-LSD50	11A0311-LSD50	11A0312-LSD50
LSD50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+

			+	+	
	7	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0355-MDPV	11A0356-MDPV	11A0357-MDPV
MDPV	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0355-MDPV	11A0356-MDPV	11A0357-MDPV
MDPV	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0400-MPD300	11A0401-MPD300	11A0402-MPD300
MPD 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	7	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0400-MPD300	11A0401-MPD300	11A0402-MPD300
MPD 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	35	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0634-ZOL	11A0635-ZOL	11A0636-ZOL
ZOL	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0634-ZOL	11A0635-ZOL	11A0636-ZOL
ZOL	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0085-7ACL300	11A0086-7ACL300	11A0087-7ACL300
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

7-ACL300	0	+50% Cut-off	+,+,+,+,+,+,+,+,+, +, +	+,+,+,+,+,+,+,+,+,+ , +	+,+,+,+,+,+,+,+,+, +
	7	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0085-7ACL300	11A0086-7ACL300	11A0087-7ACL300
7-ACL 300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	28	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0085-7ACL100	11A0086-7ACL100	11A0087-7ACL100
7-ACL100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
			Batch No.		

Product	Day	Specimen	11A0085-7ACL100	11A0086-7ACL100	11A0087-7ACL100

7-ACL 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0085-7ACL200	11A0086-7ACL200	11A0087-7ACL200
7-ACL200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0085-7ACL200	11A0086-7ACL200	11A0087-7ACL200
7-ACL 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0184-CFYL500	**11A0185-CFYL500**	**11A0186-CFYL500**
		Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-

CFY L 500	0	-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+

	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0184-CFYL500	**11A0185-CFYL500**	**11A0186-CFYL500**
CFYL500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	28	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0373-MEP100	11A0374-MEP100	11A0375-MEP100
MEP100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
			Batch No.		

Product	Day	Specimen	11A0373-MEP100	11A0374-MEP100	11A0375-MEP100

MEP 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0643-ZOP50	11A0644-ZOP50	11A0645-ZOP50
ZOP 50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	35	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0643-ZOP50	11A0644-ZOP50	11A0645-ZOP50
ZOP 50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0157-CAF1000	11A0158-CAF1000	11A0159-CAF1000
CAF1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0157-CAF1000	11A0158-CAF1000	11A0159-CAF1000
CAF1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0148-CAT	11A0149-CAT	11A0150-CAT
CAT150	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
		Drug free urine	-,-,-	-,-,-	-,-,-

	21	-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0148-CAT	11A0149-CAT	11A0150-CAT
CAT150	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.

			TRO15050001p-T	TRO15050001p-T	TRO15050003p-T
TRO350	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0598-TRO350	11A0599-TRO350	11A0600-TRO350
TRO350	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0094-ALP	11A0095-ALP	11A0096-ALP
ALP 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0094-ALP	11A0095-ALP	11A0096-ALP
ALP 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0067-K3 10	11A0068-K3 10	11A0069-K3 10
ABP 10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0067-K3 10	11A0068-K3 10	11A0069-K3 10
ABP 10	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0112-PVP1000	11A0113-PVP1000	11A0114-PVP1000
APVP 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0112-PVP1000	11A0113-PVP1000	11A0114-PVP1000
APVP 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0112-PVP500	11A0113-PVP500	11A0114-PVP500
APVP 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0112-PVP500	11A0113-PVP500	11A0114-PVP500
APVP 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0787-CBN	11A0788-CBN	11A0789-CBN
CNB 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0787-CBN	11A0788-CBN	11A0789-CBN
CNB 500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0409-MPRD	11A0410-MPRD	11A0411-MPRD
MPRD 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0409-MPRD	11A0410-MPRD	11A0411-MPRD
MPRD 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0499-PGB	11A0500-PGB	11A0501-PGB
PGB 50,000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0499-PGB	11A0500-PGB	11A0501-PGB
PGB 50,000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0607-TZD	11A0608-TZD	11A0609-TZD
TZD 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0607-TZD	11A0608-TZD	11A0609-TZD
TZD 200	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0616-K4	11A0617-K4	11A0618-K4
UR-144 25	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0616-K4	11A0617-K4	11A0618-K4
UR-144 25	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0625-ZAL	11A0626-ZAL	11A0627-ZAL
ZAL 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	Day	Specimen	Batch No.		
			11A0625-ZAL	11A0626-ZAL	11A0627-ZAL
ZAL 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0382-MES	11A0383-MES	11A0384-MES
MES 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0382-MES	11A0383-MES	11A0384-MES
MES 100	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0283-GAB	11A0284-GAB	11A0285-GAB
GAB 2000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0283-GAB	11A0284-GAB	11A0285-GAB
GAB 2000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0580-TLD50	11A0581-TLD50	11A0582-TLD50
TLD 50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		

			11A0580-TLD50	11A0581-TLD50	11A0582-TLD50
TLD 50	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0517-QTP1000	11A0518-QTP1000	11A0519-QTP1000
QTP 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0517-QTP1000	11A0518-QTP1000	11A0519-QTP1000
QTP 1000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0481-PAP500	11A0482-PAP500	11A0483-PAP500
PAP500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-

		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Product	**Day**	**Specimen**	**Batch No.**		
			11A0481-PAP500	11A0482-PAP500	11A0483-PAP500
PAP500	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0301-KRA300	11A0302-KRA300	11A0303-KRA300
KRA300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0301-KRA300	11A0302-KRA300	11A0303-KRA300
KRA300	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-

		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Product	Day	Specimen	Batch No.		
			11A0166-CAR2000	11A0167-CAR2000	11A0168-CAR2000
CAR2000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	56	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	77	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	84	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0166-CAR2000	11A0167-CAR2000	11A0168-CAR2000
CAR2000	0	Drug free urine	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50% Cut-off	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50% Cut-off	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	14	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	21	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	28	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	35	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+
	42	Drug free urine	-,-,-	-,-,-	-,-,-
		-50% Cut-off	-,-,-	-,-,-	-,-,-
		+50% Cut-off	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃																
Product	**Day**	**Specimen**	**Batch No.**													
			11A0265-FLX500					11A0266-FLX500					11A0267-FLX500			
FLX	0	Negative	-	-	-	-	-	-	-	-	-	-	-	-	-	-
			-	-	-	-	-	-	-	-	-	-	-	-	-	-
		-50%cutoff	-	-	-	-	-	-	-	-	-	-	-	-	-	-
			-	-	-	-	-	-	-	-	-	-	-	-	-	-
		+50%cutoff	+	+	+	+	+	+	+	+	+	+	+	+	+	+
			+	+	+	+	+	+	+	+	+	+	+	+	+	+
	7	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	14	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	21	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	28	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	35	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					

	42	Negative	-	-	-	-	-	-	-	-	-
		-50%cutoff	-	-	-	-	-	-	-	-	-
		+50%cutoff	+	+	+	+	+	+	+	+	+
	56	Negative	-	-	-	-	-	-	-	-	-
		-50%cutoff	-	-	-	-	-	-	-	-	-
		+50%cutoff	+	+	+	+	+	+	+	+	+
	77	Negative	-	-	-	-	-	-	-	-	-
		-50%cutoff	-	-	-	-	-	-	-	-	-
		+50%cutoff	+	+	+	+	+	+	+	+	+
	84	Negative	-	-	-	-	-	-	-	-	-
		-50%cutoff	-	-	-	-	-	-	-	-	-
		+50%cutoff	+	+	+	+	+	+	+	+	+

	Accelerated Stability Study Results at 55℃															
	Day	**Specimen**	**Batch No.**													
			11A0265-FLX500					11A0266-FLX500					11A0267-FLX500			
FLX	0	Negative	-	-	-	-	-	-	-	-	-	-	-	-	-	-
			-	-	-	-	-	-	-	-	-	-	-	-	-	-
		-50%cutoff	-	-	-	-	-	-	-	-	-	-	-	-	-	-
			-	-	-	-	-	-	-	-	-	-	-	-	-	-
		+50%cutoff	+	+	+	+	+	+	+	+	+	+	+	+	+	+
			+	+	+	+	+	+	+	+	+	+	+	+	+	+
	7	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	14	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	21	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	28	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	35	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					
	42	Negative	-	-	-	-	-	-	-	-	-					
		-50%cutoff	-	-	-	-	-	-	-	-	-					
		+50%cutoff	+	+	+	+	+	+	+	+	+					

Accelerated Stability Study Results at 45℃				
Day	**Specimen**	**Batch No.**		
		11A1715-HMO250	11A1716-HMO250	11A1717-HMO250
0	Negative	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-
	-50%cutoff	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-
	+50%cutoff	+,+,+,+,+	+,+,+,+,+	+,+,+,+,+
7	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
14	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-

	+50%cutoff	+,+,+	+,+,+	+,+,+
21	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
28	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
35	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
42	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
56	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
77	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
84	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Day	Specimen	Batch No.		
		11A1715-HMO250	11A1716-HMO250	11A1717-HMO250
0	Negative	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-
	-50%cutoff	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-
	+50%cutoff	+,+,+,+,+	+,+,+,+,+	+,+,+,+,+
7	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
14	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
21	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
28	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
35	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
42	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃

Day	Specimen	Batch No.		
		11A1715-HMO300	11A1716-HMO300	11A1717-HMO300
0	Negative	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-

	-50%cutoff	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-
	+50%cutoff	+,+,+,+,+	+,+,+,+,+	+,+,+,+,+
7	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
14	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
21	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
28	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
35	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
42	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
56	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
77	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
84	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 55℃

Day	Specimen	Batch No.		
		11A1715-HMO300	11A1716-HMO300	11A1717-HMO300
0	Negative	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-
	-50%cutoff	-,-,-,-,-	-,-,-,-,-	-,-,-,-,-
	+50%cutoff	+,+,+,+,+	+,+,+,+,+	+,+,+,+,+
7	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
14	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
21	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
28	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
35	Negative	-,-,-	-,-,-	-,-,-
	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+
42	Negative	-,-,-	-,-,-	-,-,-

	-50%cutoff	-,-,-	-,-,-	-,-,-
	+50%cutoff	+,+,+	+,+,+	+,+,+

Accelerated Stability Study Results at 45℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0472-OZP1000	**11A0473-OZP1000**	**11A0474-OZP1000**
OZP1000	**0**	**Negative**	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50%cutoff	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50%cutoff	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	14	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	21	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	28	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	35	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	42	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	56	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	77	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	91	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	105	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	112	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	119	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	126	**Negative**	-,-,-	-,-,-	-,-,-

		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	133	Negative	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
Accelerated Stability Study Results at 55℃					
Product	**Day**	**Specimen**	**Batch No.**		
			11A0472-OZP1000	**11A0473-OZP1000**	**11A0474-OZP1000**
OZP1000	**0**	**Negative**	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		-50%cutoff	-,-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-	-,-,-,-,-,-,-,-,-,-
		+50%cutoff	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+	+,+,+,+,+,+,+,+,+,+
	7	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	14	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	21	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	28	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	35	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	42	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	46	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	49	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	56	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+
	60	**Negative**	-,-,-	-,-,-	-,-,-
		-50%cutoff	-,-,-	-,-,-	-,-,-
		+50%cutoff	+,+,+	+,+,+	+,+,+

Conclusion: Multi-Drug Test Dip Card with/without Adulteration is stable at 45℃ for 84 days or 55℃ for 42 days. These data were plotted on an Arrhenius Plot and the shelf life of this product was determined to be at least 24 months from the data of manufacture.

2.8 Precision

A study was conducted at three hospitals by untrained operators using three different lots of product which assemble in Dip Card to demonstrate the within run, between run and between operator precision. An identical Dip Card of coded specimens, containing drug free urine, -50% Cut-off, -25%Cut-off, +25% Cut-off and +50% Cut-off to each site.

Results:

AMP

1,000

Amphetamine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	8	2	9	1
1,250	10	1	9	2	8	2	8
1,500	10	0	10	0	10	0	10

AMP 500

Amphetamine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	9	1	9	1	9	1
625	10	2	8	1	9	2	8
750	10	0	10	0	10	0	10

AMP 300

Amphetamine	n	Site A		Site B		Site C	
conc. (ng/mL)	per	-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	8	2	8	2	8	2
375	10	2	8	2	8	2	8
450	10	0	10	0	10	0	10

BAR 300

Secobarbital conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	8	2	9	1
375	10	2	8	1	9	2	8
450	10	0	10	0	10	0	10

BAR 200

Secobarbital conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	9	1	9	1	9	1
250	10	1	9	1	9	1	9
300	10	0	10	0	10	0	10

BZO 500

Oxazepam conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	8	2	9	1	8	2
625	10	1	9	2	8	1	9
750	10	0	10	0	10	0	10

BZO 300

Oxazepam conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

BZO 200

Oxazepam conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	9	1	8	2	9	1
250	10	1	9	1	9	2	8
300	10	0	10	0	10	0	10

BZO 100

Oxazepam conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	8	2	7	3
125	10	1	9	1	9	2	8
150	10	0	10	0	10	0	10

BUP10

Buprenorphine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
5	10	10	0	10	0	10	0
7.5	10	9	1	9	1	8	2
12.5	10	1	9	1	9	1	9
15	10	0	10	0	10	0	10

BUP5

Buprenorphine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
2.5	10	10	0	10	0	10	0
3.75	10	9	1	9	1	8	2
6.25	10	1	9	1	9	1	9
7.5	10	0	10	0	10	0	10

COC 300

Benzoylecgonine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

COC 100

Benzoylecgonine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	9	1	9	1
125	10	2	8	2	8	2	8
150	10	0	10	0	10	0	10

COC150

Cocaine Concentration	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
75	10	10	0	10	0	10	0
112.5	10	9	1	9	1	9	1
187.5	10	2	8	2	8	2	8
225	10	0	10	0	10	0	10

COC200

Cocaine Concentration	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	9	1	9	1	9	1
250	10	1	9	1	9	1	9
300	10	0	10	0	10	0	10

THC300

11-nor- 9-COOH conc (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	8	2	9	1	9	1
375	10	2	8	3	7	1	9
450	10	0	10	0	10	0	10

THC200

11-nor- 9-COOH conc (ng/mL)	N per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	9	1	9	1	9	1
250	10	2	8	1	9	1	9
300	10	0	10	0	10	0	10

THC150

11-nor- 9-COOH conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
75	10	10	0	10	0	10	0
112.5	10	9	1	9	1	9	1
187.5	10	2	8	1	9	1	9
225	10	0	10	0	10	0	10

THC50

11-nor- 9-	n	Site A	Site B	Site C

COOH conc. (ng/mL)	per	-	+	-	+	-	+

0	10	10	0	10	0	10	0
25	10	10	0	10	0	10	0
37.5	10	9	1	8	2	9	1
62.5	10	1	9	1	9	2	8
75	10	0	10	0	10	0	10

THC25

11-nor- 9-COOH conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
12.5	10	10	0	10	0	10	0
18.75	10	8	2	8	2	8	2
31.25	10	1	9	1	9	2	8
37.5	10	0	10	0	10	0	10

THC30

THC Concentration (ng/mL)	**n per Site**	**Site A**		**Site B**		**Site C**	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
15	10	10	0	10	0	10	0
22.5	10	9	1	9	1	9	1
37.5	10	2	8	2	8	1	9
45	10	0	10	0	10	0	10

MTD300

Methadone conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

THC20

THC Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	1	0
10	10	10	0	10	0	1	0
15	10	8	2	8	2	8	2

25	10	1	9	1	9	2	8
30	10	0	10	0	10	0	10

MTD200

Methadone conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	8	2	8	2	8	2
250	10	1	9	1	9	2	8
300	10	0	10	0	10	0	10

MET1, 000

Methamphetamine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	9	1	9	1
1,250	10	1	9	2	8	1	9
1,500	10	0	10	0	10	0	10

MET 500

Methamphetamine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	9	1	9	1	9	1
625	10	1	9	1	9	1	9
750	10	0	10	0	10	0	10

MET 300

Methamphetamine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

MET 200

Methamphetamine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0

100	10	10	0	10	0	10	0
150	10	9	1	9	1	9	1
250	10	1	9	1	9	2	8
300	10	0	10	0	10	0	10

MDMA1, 000

Methylenedioxy methamphetamine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	9	1	8	2
1,250	10	1	9	1	9	1	9
1,500	10	0	10	0	10	0	10

MDMA 500

Methylenedioxymetham phetamine	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	1	0	10	0	10	0
250	10	1	0	10	0	10	0

375	10	8	2	9	1	9	1
625	10	1	9	1	9	1	9
750	10	0	10	0	1	0	10

MDMA 300

Methylenedioxymethamphetamine	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	1	0	10	0	10	0
150	10	1	0	10	0	10	0
225	10	8	2	9	1	7	3
375	10	2	8	1	9	1	9
450	10	0	10	0	1	0	10

MOP 300

Morphine conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

MOP 100

Morphine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	9	1	9	1
125	10	1	9	1	9	1	9
150	10	0	10	0	10	0	10

MOP 200

Morphine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	7	3	9	1	9	1
250	10	1	9	2	8	1	9
300	10	0	10	0	10	0	10

MQL 300

Methaqualone conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0

150	10	10	0	10	0	10	0

225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

OPI 2,000

Morphine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
1,000	10	10	0	10	0	10	0
1,500	10	9	1	9	1	9	1
2,500	10	1	9	1	9	1	9
3,000	10	0	10	0	10	0	10

PCP

Phencyclidine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
12.5	10	10	0	10	0	10	0
18.75	10	8	2	9	1	9	1
31.25	10	1	9	1	9	1	9
37.5	10	0	10	0	10	0	10

PPX

Propoxyphene conc. (ng/mL)	n per	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	8	2	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

TCA

Nortriptyline conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	8	2	8	2
1,250	10	1	9	1	9	1	9

1,500	10	0	10	0	10	0	10

TCA500

Nortriptyline conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	7	3	9	1	8	2
625	10	2	8	1	9	1	9
750	10	0	10	0	10	0	10

TML100

Tramadol conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	9	1	8	2
125	10	1	9	1	9	2	8
150	10	0	10	0	10	0	10

TML200

Tramadol conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	9	1	9	1	8	2
250	10	1	9	1	9	2	8
300	10	0	10	0	10	0	10

TML300

Tramadol conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	8	2
375	10	1	9	1	9	2	8
450	10	0	10	0	10	0	10

KET1, 000

Ketamine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	8	2	9	1
1,250	10	1	9	1	9	2	8
1,500	10	0	10	0	10	0	10

KET500

Ketamine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	9	1	9	1	8	2
625	10	1	9	1	9	2	8
750	10	0	10	0	10	0	10

KET300

Ketamine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

KET100

Ketamine conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	9	1	9	1
125	10	1	9	1	9	2	8
150	10	0	10	0	10	0	10

OXY100

Oxycodone Concentration (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0

50	10	10	0	10	0	10	0
75	10	9	1	9	1	9	1
125	10	1	9	1	9	1	9
150	10	0	10	0	10	0	10

OXY300

Oxycodone Concentration (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

COT 200

Cotinine Concentration (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	9	1	9	1	9	1
250	10	1	9	1	9	2	8
300	10	0	10	0	10	0	10

COT 100

Cotinine Concentration (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	9	1	9	1
125	10	1	9	1	9	1	9
150	10	0	10	0	10	0	10

EDDP 300

EDDP Concentration (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	2	8	1	9
450	10	0	10	0	10	0	10

EDDP 100

EDDP Concentration (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	9	1	9	1
125	10	1	9	1	9	1	9

150	10	0	10	0	10	0	10

FYL 20

FYL Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	10
10	10	10	0	10	10	10	10
15	10	9	1	9	1	9	1
25	10	1	9	1	9	1	9
30	10	0	10	0	10	10	0

FYL 10

FYL Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
5	10	10	0	10	0	10	0
7.5	10	9	1	9	1	9	1
12.5	10	1	9	1	9	1	9
15	10	0	10	0	10	0	10

K2 50

K2 Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
25	10	10	0	10	0	10	0
37.5	10	8	2	8	2	9	1
67.5	10	1	9	2	8	2	8
75	10	0	10	0	10	0	10

K2 30

K2 Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
15	10	10	0	10	0	10	0
22.5	10	8	2	9	1	9	1
37.5	10	1	9	1	9	1	9
45	10	0	10	0	10	0	10

K2 25

K2 Concentration (ng/mL)	**n per Site**	**Site A**		**Site B**		**Site C**	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
12.5	10	10	0	10	0	10	0
17.25	10	7	3	8	2	8	2

31.25	10	1	9	1	9	2	8
37.5	10	0	10	0	10	0	10

6-MAM

6-MAM conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
5	10	10	0	10	0	10	0
7.5	10	9	1	9	1	9	1
12.5	10	1	9	1	9	1	9
15	10	0	10	0	10	0	10

CLO 400

Clonazepam conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
200	10	10	0	10	0	10	0
300	10	9	1	8	2	9	1
500	10	1	9	2	8	1	9
600	10	0	10	0	10	0	10

CLO 150

Clonazepam conc. (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
75	10	10	0	10	0	10	0
112	10	9	1	8	2	9	1
187	10	1	9	2	8	1	9
225	10	0	10	0	10	0	10

MDA

MDA Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0

375	10	9	1	9	1	9	1
625	10	1	9	1	9	1	9
750	10	0	10	0	10	0	10

DIA300

DIA Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

DIA200

DIA Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	9	1	9	1	9	1
250	10	1	9	1	9	1	9
300	10	0	10	0	10	0	10

ETG500

ETG Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	8	2	8	2	9	1
625	10	1	9	2	8	2	8
750	10	0	10	0	10	0	10

ETG1000

ETG Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	8	2	8	2	9	1
1250	10	1	9	2	8	2	8
1500	10	0	10	0	10	0	10

ACE

ACE Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
2500	10	10	0	10	0	10	0
3750	10	9	1	9	1	8	2
6250	10	1	9	1	9	1	9
7500	10	0	10	0	10	0	10

LSD 20

LSD Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
10	10	10	0	10	0	10	0
15	10	9	1	9	1	9	1
25	10	1	9	1	9	1	9
30	10	0	10	0	10	0	10

LSD 50

LSD Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0

25	10	10	0	10	0	10	0
37.5	10	9	1	9	1	9	1
62.5	10	1	9	1	9	1	9
75	10	0	10	0	10	0	10

MDPV

MDPV Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	9	1	8	2
1250	10	1	9	1	9	1	9
1500	10	0	10	0	10	0	10

MPD300

MPD Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	8	2	9	1
375	10	1	9	2	8	1	9
450	10	0	10	0	10	0	10

ZOL

ZOL Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
25	10	9	1	10	0	10	0
75	10	0	10	1	9	0	10

7-ACL300

7-ACL Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	8	2	9	1	9	1
375	10	2	8	2	8	3	7
450	10	0	10	0	10	0	10

7-ACL200

7-ACL Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	8	2	9	1	8	2
250	10	2	8	2	8	2	8
300	10	0	10	0	10	0	10

7-ACL100

7-ACL Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	7	3	7	3	9	1
125	10	2	8	1	9	2	8
150	10	0	10	0	10	0	10

CFYL

CFYL Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0

250	10	10	0	10	0	10	0
375	10	7	3	9	1	8	2
625	10	2	8	1	9	2	8
750	10	0	10	0	10	0	10

MEP

MEP Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	7	3	9	1	8	2
625	10	2	8	1	9	2	8
750	10	0	10	0	10	0	10

ZOP

Zopiclone Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
25	10	10	0	10	0	10	0
37.5	10	9	1	8	2	9	1
62.5	10	2	8	2	8	2	8
75	10	0	10	0	10	0	10

CAF

Caffeine Concentration (ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	**10**	**10**	**0**	**10**	**0**	**10**	**0**
500	**10**	**10**	**0**	**10**	**0**	**10**	**0**
750	**10**	**9**	**1**	**8**	**2**	**9**	**1**
1250	**10**	**2**	**8**	**2**	**8**	**2**	**8**
1500	**10**	**0**	**10**	**0**	**10**	**0**	**10**

CAT

(+)-Norpseudoephedrine HCl Concentration(ng/mL)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
75	10	10	0	10	0	10	0
112.5	10	9	1	8	2	9	1
187.5	10	2	8	2	8	2	8
225	10	0	10	0	10	0	10

TRO

Tropicamide Concentration (ng/ml)	n per site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
175	10	10	0	10	0	10	0
262.5	10	8	2	8	2	8	2
437.5	10	2	8	2	8	2	8
525	10	0	10	0	10	0	10

ALP

ALP Concentration (ng/ml)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0

50	10	10	0	10	0	10	0
75	10	9	1	8	2	9	1
125	10	2	8	2	8	2	8
150	10	0	10	0	10	0	10

ABP

AB-PINACA Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
5	10	10	0	10	0	10	0
7.5	10	8	2	8	2	9	1
12.5	10	2	8	3	7	1	9
15	10	0	10	0	10	0	10

APVP1000

α-PVP Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	8	2	9	1	9	1
1,250	10	2	8	3	7	1	9
1,500	10	0	10	0	10	0	10

APVP500

α-PVP Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	8	2	8	2	9	1
625	10	2	8	2	8	1	9

750	10	0	10	0	10	0	10

CNB

CNB Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	9	1	9	1	9	1
625	10	2	8	1	9	1	9
750	10	0	10	0	10	0	10

MPRD

Normeperidine Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	8	2	9	1	9	1
125	10	2	8	3	7	1	9
150	10	0	10	0	10	0	10

PGB

PGB Concentration (ug/ml)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
25	10	10	0	10	0	10	0
37.5	10	8	2	8	2	8	2
62.5	10	2	8	2	8	2	8
75	10	0	10	0	10	0	10

TZD

TZD Concentration (ng/ml)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+

0	10	10	0	10	0	10	0
100	10	10	0	10	0	10	0
150	10	8	2	8	2	8	2
250	10	1	9	2	8	2	8
300	10	0	10	0	10	0	10

UR-144

UR-144 5-Pentanoic Concentration (ng/ml)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
12.5	10	10	0	10	0	10	0
18.75	10	9	1	8	2	9	1
31.25	10	1	9	2	8	2	8
62.5	10	0	10	0	10	0	10

ZAL

ZAL Concentration (ng/ml)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	10	0	10	0	10	0
125	10	2	8	1	9	1	9
150	10	0	10	0	10	0	10

MES

MES Concentration (ng/ml)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
50	10	10	0	10	0	10	0
75	10	9	1	9	1	9	1

125	10	2	8	1	9	1	9
150	10	0	10	0	10	0	10

GAB

GAB Concentration (ng/ml)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
1000	10	10	0	10	0	10	0
1500	10	9	1	9	1	8	2
2500	10	2	8	2	8	2	8
3000	10	0	10	0	10	0	10

QTP 1000

QTP Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	9	1	9	1
1250	10	1	9	1	9	1	9
1500	10	0	10	0	10	0	10

PAP 500

PAP Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	8	2	9	1	9	1
625	10	2	8	2	8	2	8
750	10	0	10	0	10	0	10

KRA 300

KRA Concentration (ng/mL)	n per Site	Site A	Site B	Site C

		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	2	8
450	10	0	10	0	10	0	10

CAR 2000

CAR Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
1000	10	10	0	10	0	10	0
1500	10	9	1	9	1	8	2
2500	10	2	8	2	8	2	8
3000	10	0	10	0	10	0	10

FLX 500

Fluoxetine Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
250	10	10	0	10	0	10	0
375	10	9	1	9	1	9	1
625	10	2	8	2	8	2	8
750	10	0	10	0	10	0	10

HMO 250

HMO Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
125	10	10	0	10	0	10	0

187.5	10	8	2	8	2	8	2
312.5	10	2	8	2	8	2	8
375	10	0	10	0	10	0	10

HMO300

HMO Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	8	2	9	1	8	2
375	10	2	8	2	8	2	8
450	10	0	10	0	10	0	10

OZP1000

OZP Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
500	10	10	0	10	0	10	0
750	10	9	1	9	1	9	1
1250	10	2	8	1	9	1	9
1500	10	0	10	0	10	0	10

Conclusion: Specimens determined to be negative, -50% cutoff, -25% cutoff, +25% cutoff and +50%cutoff values demonstrate high precision for Multi-Drug Test Dip Card with/without Adulteration.

2.9 Effect of Urinary Specific Gravity

The urine specific gravity was measured with Clinical Refractometer. Five urine samples with the specific gravity at each following range were used for the study: (1) Specific gravity >1.025. (2) Specific gravity 1.015 – 1.025. (3) Specific gravity < 1.015. Each urine sample was aliquoted to three parts: (1) Drug free urine (2) Urine samples were spiked with each drug which contained in the Dip Cardto-50% Cut-off; (3) Urine samples were spiked with each drug which contained in the Dip Card to+50% Cut-off. The each drug test is assembled in the 10 in 1 Dip Card. The Multi-Drug Test Dip Card with/without Adulteration will test in duplicates with above urine samples Read the result at 5 minutes after sample application.

Results:

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
AMP 1000	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
AMP 500	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+

AMP 300	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
BAR 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
BAR 200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+

	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
BUP 10	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
BUP 5	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+

BZO 500	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
BZO 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
BZO 200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+

	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
BZO 100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
COC 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
COC 100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
COC 200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+

	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
COC 150	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
KET 1000	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+

	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
KET 500	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
KET 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
KET 100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+

	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MDMA 1000	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MDMA 500	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+

	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MDMA 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MET 1000	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MET 500	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MET 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+

MET 200	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MOP 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+

	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MOP 200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+
Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MOP 100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+

	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MQL	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MTD 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MTD 200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+

	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
OPI 2000	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
PCP	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+

	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
PPX	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
THC300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
THC 200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
THC 150	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
THC 50	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+

	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
THC 25	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
THC 30	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+

	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
THC 20	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
TCA	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
TCA500	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+

	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
TML100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
TML200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+

	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
TML300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
OXY100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+

	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
OXY300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
COT 200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
COT 100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
EDDP 300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
EDDP 100	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
FYL 20	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+

	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
FYL 10	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
K2 50	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+

	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
K2 30	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
K2 25	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
6-MAM	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+

	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
CLO400	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
CLO150	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+

	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
DIA300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
DIA200	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MDA	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ETG500	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ETG1000	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+

	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ACE	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
LSD20	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+

	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
LSD50	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MDPV	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MPD300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ZOL	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
	1	1.007	2	-	-	-	-	+	+
	2	1.023	2	-	-	-	-	+	+
	3	1.025	2	-	-	-	-	+	+
	4	1.004	2	-	-	-	-	+	+
	5	1.014	2	-	-	-	-	+	+
	6	1.013	2	-	-	-	-	+	+

7-ACL300	7	1.017	2	-	-	-	-	+	+
	8	1.019	2	-	-	-	-	+	+
	9	1.020	2	-	-	-	-	+	+
	10	1.019	2	-	-	-	-	+	+
	11	1.030	2	-	-	-	-	+	+
	12	1.008	2	-	-	-	-	+	+
	13	1.031	2	-	-	-	-	+	+
	14	1.030	2	-	-	-	-	+	+
	15	1.023	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
7-ACL200	1	1.007	2	-	-	-	-	+	+
	2	1.023	2	-	-	-	-	+	+
	3	1.025	2	-	-	-	-	+	+
	4	1.004	2	-	-	-	-	+	+
	5	1.014	2	-	-	-	-	+	+
	6	1.013	2	-	-	-	-	+	+
	7	1.017	2	-	-	-	-	+	+
	8	1.019	2	-	-	-	-	+	+
	9	1.020	2	-	-	-	-	+	+
	10	1.019	2	-	-	-	-	+	+
	11	1.030	2	-	-	-	-	+	+

	12	1.008	2	-	-	-	-	+	+
	13	1.031	2	-	-	-	-	+	+
	14	1.030	2	-	-	-	-	+	+
	15	1.023	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
7-ACL100	1	1.007	2	-	-	-	-	+	+
	2	1.023	2	-	-	-	-	+	+
	3	1.025	2	-	-	-	-	+	+
	4	1.004	2	-	-	-	-	+	+
	5	1.014	2	-	-	-	-	+	+
	6	1.013	2	-	-	-	-	+	+
	7	1.017	2	-	-	-	-	+	+
	8	1.019	2	-	-	-	-	+	+
	9	1.020	2	-	-	-	-	+	+
	10	1.019	2	-	-	-	-	+	+
	11	1.030	2	-	-	-	-	+	+
	12	1.008	2	-	-	-	-	+	+
	13	1.031	2	-	-	-	-	+	+
	14	1.030	2	-	-	-	-	+	+
	15	1.023	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
CFYL	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MEP	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ZOP	1	1.008	2	-	-	-	-	+	+
	2	1.013	2	-	-	-	-	+	+
	3	1.014	2	-	-	-	-	+	+
	4	1.003	2	-	-	-	-	+	+
	5	1.015	2	-	-	-	-	+	+
	6	1.019	2	-	-	-	-	+	+
	7	1.018	2	-	-	-	-	+	+
	8	1.022	2	-	-	-	-	+	+
	9	1.020	2	-	-	-	-	+	+
	10	1.024	2	-	-	-	-	+	+
	11	1.026	2	-	-	-	-	+	+
	12	1.029	2	-	-	-	-	+	+
	13	1.035	2	-	-	-	-	+	+
	14	1.027	2	-	-	-	-	+	+
	15	1.028	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
CAF	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
CAT	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+

	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
TRO	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

ALP

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ALP	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

ABP

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ABP	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+

	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

APVP1000

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
APVP	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

APVP500

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
APVP	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+

	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

CNB

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
CNB	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

MPRD

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MPRD	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

PGB

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
PGB	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+

	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

TZD

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
TZD	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

UR-144

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
UR-144	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

ZAL

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
ZAL	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

MES

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
MES	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

GAB

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
GAB	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+

	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
QTP 1000	1	1.018	2	-	-	-	-	+	+
	2	1.012	2	-	-	-	-	+	+
	3	1.008	2	-	-	-	-	+	+
	4	1.006	2	-	-	-	-	+	+
	5	1.022	2	-	-	-	-	+	+
	6	1.024	2	-	-	-	-	+	+
	7	1.017	2	-	-	-	-	+	+
	8	1.028	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.035	2	-	-	-	-	+	+
	11	1.031	2	-	-	-	-	+	+
	12	1.043	2	-	-	-	-	+	+
	13	1.037	2	-	-	-	-	+	+
	14	1.040	2	-	-	-	-	+	+
	15	1.033	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
PAP 500	1	1.018	2	-	-	-	-	+	+
	2	1.012	2	-	-	-	-	+	+
	3	1.008	2	-	-	-	-	+	+
	4	1.006	2	-	-	-	-	+	+
	5	1.022	2	-	-	-	-	+	+
	6	1.024	2	-	-	-	-	+	+
	7	1.017	2	-	-	-	-	+	+
	8	1.028	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.035	2	-	-	-	-	+	+
	11	1.031	2	-	-	-	-	+	+
	12	1.043	2	-	-	-	-	+	+
	13	1.037	2	-	-	-	-	+	+
	14	1.040	2	-	-	-	-	+	+
	15	1.033	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine	-50% Cut-off	+50% Cut-off

KRA 300	1	1.018	2	-	-	-	-	+	+
	2	1.012	2	-	-	-	-	+	+
	3	1.008	2	-	-	-	-	+	+
	4	1.006	2	-	-	-	-	+	+
	5	1.022	2	-	-	-	-	+	+
	6	1.024	2	-	-	-	-	+	+
	7	1.017	2	-	-	-	-	+	+
	8	1.028	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.035	2	-	-	-	-	+	+
	11	1.031	2	-	-	-	-	+	+
	12	1.043	2	-	-	-	-	+	+
	13	1.037	2	-	-	-	-	+	+
	14	1.040	2	-	-	-	-	+	+
	15	1.033	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
CAR 2000	1	1.018	2	-	-	-	-	+	+
	2	1.012	2	-	-	-	-	+	+
	3	1.008	2	-	-	-	-	+	+
	4	1.006	2	-	-	-	-	+	+
	5	1.022	2	-	-	-	-	+	+
	6	1.024	2	-	-	-	-	+	+
	7	1.017	2	-	-	-	-	+	+
	8	1.028	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.035	2	-	-	-	-	+	+
	11	1.031	2	-	-	-	-	+	+
	12	1.043	2	-	-	-	-	+	+
	13	1.037	2	-	-	-	-	+	+
	14	1.040	2	-	-	-	-	+	+
	15	1.033	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
FLX	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+

	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
HMO250	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	Urine ID	Urine Specific Gravity	N*	Drug free urine		-50% Cut-off		+50% Cut-off	
HMO300	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+
	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Product	**Urine ID**	**Urine Specific Gravity**	**N***	**Negative**		**OZP 500ng/ml**		**OZP 1500ng/ml**	
OZP1000	1	1.010	2	-	-	-	-	+	+
	2	1.011	2	-	-	-	-	+	+

	3	1.007	2	-	-	-	-	+	+
	4	1.005	2	-	-	-	-	+	+
	5	1.012	2	-	-	-	-	+	+
	6	1.014	2	-	-	-	-	+	+
	7	1.015	2	-	-	-	-	+	+
	8	1.018	2	-	-	-	-	+	+
	9	1.017	2	-	-	-	-	+	+
	10	1.025	2	-	-	-	-	+	+
	11	1.036	2	-	-	-	-	+	+
	12	1.045	2	-	-	-	-	+	+
	13	1.036	2	-	-	-	-	+	+
	14	1.041	2	-	-	-	-	+	+
	15	1.043	2	-	-	-	-	+	+

Conclusion: The results demonstrate that varying ranges of urinary specific gravity do not affect the test results.

2.10 Effect of Urinary pH

Approximately 150 ml of negative urine pool were allocated into 5 test tubes. The pH of the urine was adjusted within the range of 5 to 9 in 1 pH unit increments using NaOH or HCl. Each pH-adjusted urine was split into three glass containers (10ml/container): Multi-Drug Test Dip Card with/without Adulteration was added to two aliquots to bring the final sample concentration of -50% cut-off and +50% cut-off respectively. Each pH-adjusted urine was tested in duplicate and read 5 and 10 minutes after sample application.

Results:

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
AMP 1000 Lot#: 11A0103-AMP1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
AMP 500 Lot#: 11A0103-AMP500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+

	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
AMP 300 Lot#: 11A0103-AMP300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+

	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
BAR 300 Lot#: 11A0121-BAR300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
BAR 200 Lot#: 11A0121-BAR200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
BUP 10 Lot#: 11A0130-BUP10	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine	-50% cutoff	+50% cutoff

		5min	10min	5min	10min	5min	10min
BUP 5 Lot#: 11A0130-BUP5	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
BZO 500 Lot#:11A0139- BZO500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
BZO 300 Lot#:11A0139- BZO300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
BZO 200 Lot#:11A0139- BZO200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+

	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
BZO 100 Lot#:11A0139-BZO100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
COC 300 Lot#:11A0211-COC300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
COC 100 Lot#:11A0211-COC100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
COC 150 Lot#:11A0211-COC150	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
COC 200 Lot#:11A0211-COC200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
KET 1000 Lot#:11A0292-KET1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
KET 500 Lot#:11A0292-KET500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+

	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
KET 300 Lot#:11A0292-KET300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
KET 100 Lot#:11A0292-KET100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MDMA 1000 LOT#: 11A0337-MDMA1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MDMA 500 LOT#: 11A0337-MDMA500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MDMA 300 LOT#: 11A0337-MDMA300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MET 1000 LOT#: 11A0364-MET1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MET 500 LOT#:	5	-	-	-	-	+	+
	5	-	-	-	-	+	+

11A0364-MET500	6	-	-	-	-	+	+

	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MET 300 LOT#:11A0364-MET300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MET 200 LOT#:11A0364-MET200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MOP 300 LOT#: 11A0391-MOP300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MOP 100 LOT#: 11A0391-MOP100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+

	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MOP 200 LOT#: 11A0391-MOP200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MQL LOT#:11A0418-MQL	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MTD 300 LOT#:11A0427-MTD300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MTD 200 LOT#:11A0427-MTD200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+

	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
OPI LOT#:11A0454-OPI	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
PCP LOT# : 11A0490-PCP	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
PPX LOT#:11A0508-PPX	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+

	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
THC 150 LOT#:11A0571-THC150	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
THC 50 LOT#:11A0571-THC50	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
THC 25 LOT#:11A0571-THC25	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
THC 300	5	-	-	-	-	+	+

LOT#:11A0571-THC300	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
THC 200 LOT#:11A0571-THC200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
THC 30 LOT#:11A0571-THC30	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
THC 20 LOT#:11A0571-THC20	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+

	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
TCA LOT#:11A0562-TCA	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
TCA LOT#:11A0562-TCA500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
TML 100 LOT#:11A0589-TML100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine	-50% cutoff	+50% cutoff

		5min	10min	5min	10min	5min	10min
TML 200 LOT#:11A0589-TML200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
TML300 LOT#:11A0589-TML300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine	-50% cutoff	+50% cutoff

		5min	10min	5min	10min	5min	10min
OXY100 LOT#:11A0463-OXY100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
OXY300 LOT#:11A0463-OXY300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
COT 200 LOT#:11A0220-COT200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
COT 100 LOT#:11A0220-	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+

COT100	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
EDDP300 LOT#:11A0238-EDDP300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+

	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
EDDP 100 LOT#:11A0238-EDDP100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
FYL 20 LOT#:11A0274-FYL10	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
FYL 10 LOT#:11A0274-FYL10	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
K2 50 LOT#:11A0544-K2 50	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
K2 30 LOT#:11A0544-K2 30	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
K2 25 LOT#:11A0544-K2 25	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
6-MAM LOT#:11A0319-6MAM	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+

	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
CLO 400 LOT#:11A0 202-CLO400	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
CLO 150 LOT#:11A0 202-CLO150	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
DIA300 LOT#:11A0 229-DIA300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
DIA 200 LOT#:11A0229-DIA200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MDA LOT#:11A0346-MDA	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ETG500 LOT#:11A0247-ETG500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ETG1000 LOT#:11A0247-ETG1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+

	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ACE LOT#:11A0076-ACE	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
LSD 20 LOT#:11A0310-LSD20	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
LSD 50 LOT#:11A0310-LSD50	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+

	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MDPV LOT#:11A0355-MDPV	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MPD300 LOT#:11A0400-MPD	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ZOL LOT#:11A0634-ZOL	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+

7-ACL300 LOT#:11A0085-7ACL300	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
7-ACL100 LOT#:11A0085-7ACL100	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
7-ACL200 LOT#:11A0085-7ACL200	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+

	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
CFYL LOT#:11A0184-CFYL	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MEP LOT#:11A0373-MEP	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ZOP LOT#:11A0643-ZOP	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
CAF LOT#:11A0157-CAF	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
CAT LOT#:11A0148-CAT	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
TRO LOT#:11A0598-TRO	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+

	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ALP LOT#:11A0094-ALP	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ABP LOT#:11A0067-K310	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
APVP1000 LOT#:11A0112-PVP1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min

APVP500 LOT#:11A0112-PVP500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
CNB LOT#:11A0787-CBN	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MPRD LOT#:11A0409-MPRD	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
PGB LOT#:11A0499-PGB	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+

	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
TZD LOT#:11A0607-TZD	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
UR-144 LOT#:11A0616-K4	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
ZAL LOT#:11A0625-ZAL	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
MES LOT#:11A0382-MES	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+

	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
GAB LOT#:11A0283-GAB	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+
Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
QTP 1000 LOT#: 11A0517-QTP1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
PAP 500 LOT#: 11A0481-PAP500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min

KRA 300 LOT#: 11A0301-KRA300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
CAR 2000 LOT#: 11A0166-CAR2000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
FLX 500 LOT#:11A0265-FLX500	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
HMO 250 LOT#:11A1715-HMO250	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+

	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
HMO 300 LOT#:11A1715-HMO300	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Product	pH	Negative urine		-50% cutoff		+50% cutoff	
		5min	10min	5min	10min	5min	10min
OZP 1000 LOT#:11A0472-OZP1000	5	-	-	-	-	+	+
	5	-	-	-	-	+	+
	6	-	-	-	-	+	+
	6	-	-	-	-	+	+
	7	-	-	-	-	+	+
	7	-	-	-	-	+	+
	8	-	-	-	-	+	+
	8	-	-	-	-	+	+
	9	-	-	-	-	+	+
	9	-	-	-	-	+	+

Conclusion: The results demonstrate that varying ranges of pH from 5-9 do not interfere with the performance of the Multi-Drug Test Dip Card.

2.11 Open Pouch Stability

Drug standards including negative urine, the -50% cutoff, + 50% cutoff and 300% cutoff were run in triplicate using the Multi-Drug Tests which were opened pouch after 10 minutes, 20 minutes, 30 minutes, 1 hour, 1.5 hours and 2 hours at room temperature. One lot test (Lot 1 for each) was used. All results were read as positive or negative at 5 and 10 minutes after sample application. Read the results by ACESO gold color card at 5 minutes after sample application, T line <=3.5 regard as positive, T line >=4 regard as negative.

AMP1000 Lot: 11A0103-AMP1000

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

20 minutes	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

AMP500 Lot: 11A0103-AMP500

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+

2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

AMP300 Lot: 11A0103-AMP300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

BAR300 Lot: 11A0121-BAR300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

BAR200 Lot: 11A0121-BAR200

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

2 hours	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+

BZO500 Lot: 11A0139-BZO500

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+

BZO300 Lot: 11A0139-BZO300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+

30 minutes	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+

BZO200 Lot: 11A0139-BZO200

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+

	5	-	-	-	-	-	-	+	+

BZO100 Lot: 11A0139-BZO100

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	+	+

BUP10 Lot: 11A0130-BUP10

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

BUP5 Lot: 11A0130-BUP5

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

COC300 Lot: 11A0211-COC300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

COC100 Lot: 11A0211-COC100

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

COC150 Lot: 11A0211-COC150

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	-	+
	5	-	-	-	-	-	-	-	-

COC200 Lot: 11A0211-COC200

Time after	**N**	**Negative urine**	**–50% cutoff**	**+ 50% cutoff**	**300% cutoff**

opened pouch		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

THC150 Lot: 11A0571-THC150

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

1 hour	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

THC50 Lot: 11A0571-THC50

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+/-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

THC25 Lot: 11A0571-THC25

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
	1	-	-	-	-	+	+	+	+

10 minutes	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+/-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

THC300 Lot: 11A0571-THC300

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

THC200 Lot: 11A0571-THC200

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

THC30 Lot: 11A0571-THC30

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

THC20 Lot: 11A0571-THC20

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+

1.5 hours	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

MTD300 Lot: 11A0427-MTD300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	-

MTD200 Lot: 11A0427-MTD200

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

MET1000 Lot: 11A0364-MET1000

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

MET500 Lot: 11A0364-MET500

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

MET300 Lot: 11A0364-MET300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

20 minutes	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	-

MET200 Lot: 11A0364-MET200

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+

2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	-

MDMA1000 Lot: 11A0337-MDMA1000

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

MDMA500 Lot: 11A0337-MDMA500

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

MDMA300 Lot: 11A0337-MDMA300

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

MOP300 Lot: 11A0418-MQL

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

MOP100 Lot: 11A0391-MOP200

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+

30 minutes	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

MOP200 Lot: 11A0391-MOP100

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+

	5	-	-	-	-	-	-	-	+

MQL300 Lot: 11A0418-MQL300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

OPI2000 Lot: 11A0454-OPI

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

PCP25 Lot: 11A0490-PCP

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+/-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

PPX300 Lot: 11A0508-PPX300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

TCA1000 Lot: 11A0562-TCA1000

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

TCA500 Lot: 11A0562-TCA500

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

TML100 Lot: 11A0589-TML100

Time after	**N**	**Negative urine**	**–50% cutoff**	**+ 50% cutoff**	**300% cutoff**

opened pouch		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

TML200 Lot: 11A0589-TML200

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

1 hour	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

TML300 Lot: 11A0589-TML300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+/-	+	+
	5	-	-	-	-	-	-	-	+

KET1000 Lot: 11A0292-KET1000

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
	1	-	-	-	-	+	+	+	+

10 minutes	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

KET500 Lot: 11A0292-KET500

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

KET300 Lot: 11A0292-KET300

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

KET100 Lot: 11A0292-KET100

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

OXY100 Lot: 11A0463-OXY

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+

1.5 hours	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+/-	-	-	+

OXY300 Lot: 11A0463-OXY300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+

COT200 Lot: 11A0220-COT200

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

COT100 Lot: 11A0220-COT100

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	-	+	+
	5	-	-	-	-	-	-	-	+

EDDP300 Lot: 11A0238-EDDP300

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

EDDP100 Lot: 11A0238-EDDP100

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	+	-	+

FYL20 Lot: 11A0274-FYL20

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	+	+	+
	5	-	-	-	-	-	-	-	+

FYL10 Lot: 11A0274-FYL10

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	+	+	+
	5	-	-	-	-	-	-	-	+

K2-50 Lot: 11A0544-K2 50

Time after	**N**	**Negative urine**	**–50% cutoff**	**+ 50% cutoff**	**300% cutoff**

opened pouch		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

K2-30 Lot: 11A0544-K2 30

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

1 hour	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	+/-	+	+
	5	-	-	-	-	-	-	-	+

K2 25 Lot: 11A0544-K2 25

Time after opened pouch	N	Negative urine		K2 –50% cutoff		K2 + 50% cutoff		K2 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	+	+	-	+	+
	4	-	-	-	+	+	-	+	+
	5	-	-	-	+	+	-	+	+
2 hours	1	-	-	-	+	+	-	+	+
	2	-	-	-	+	+	-	+	+
	3	-	-	-	+	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	+	+	+	+

6-MAM Lot: 11A0319-6MAM

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
	1	-	-	-	-	+	+	+	+

10 minutes	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	+	+	+
	5	-	-	-	-	-	-	-	+

CLO400 Lot: 11A0202-CLO400

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	+	+	+
	5	-	-	-	-	-	-	-	+

CLO150 Lot: 11A0202-CLO150

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

ETG500 Lot: 11A0247-ETG500

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	+	+	+
	5	-	-	-	-	-	-	-	+

ETG1000 Lot: 11A0247-ETG1000

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+

1.5 hours	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

DIA300 Lot: 11A0229-DIA300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

DIA200 Lot: 11A0229-DIA200

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

MDA500 Lot: 11A0346-MDA500

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

ACE50000 Lot: 11A0076-ACE

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+/-	+	+	+
	5	-	-	-	-	-	-	-	+

CAT500 Lot: 11A0148-CAT

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

20 minutes	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	-	+

LSD20 Lot: 11A0310-LSD20

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+

2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

LSD50 Lot: 11A0310-LSD50

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

ZOL50 Lot: 11A0634-ZOL

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	+	+	+
	5	-	-	-	-	-	-	-	+

MDPV1000 Lot: 11A0355-MDPV

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

MPD300 Lot: 11A0400-MPD300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

FLX500 Lot: 11A0265-FLX500

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+

30 minutes	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	-	+	+
2 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	-	+

ABP10 Lot: 11A0067-K3 10

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+

CFYL500 Lot: 11A0184-CFYL500

Time after opened pouch	N	Negative urine		CFYL –50% cutoff		CFYL + 50% cutoff		CFYL 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	+	+	+	+	+	+
	3	-	-	+	+	+	+	+	+
	4	-	-	+	+	+	+	+	+
	5	-	-	+	+	+	+	+	+
2 hours	1	-	-	+	+	+	+	+	+
	2	-	-	+	+	+	+	+	+
	3	-	-	+	+	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

α-PVP 1000 Lot: 11A0112-PVP1000

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

30 minutes	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

α-PVP 500 Lot: 11A0112-PVP1000

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

7-ACL300 LOT#:11A0085-7ACL300

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

7-ACL200 LOT#:11A0085-7ACL200

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

7-ACL100 LOT#:11A0085-7ACL100

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+

	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

CNB 500 LOT#:11A0787-CBN

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

MPRD 100 LOT#: 11A0409-MPRD

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+

	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

TZD 200 LOT#: 11A0607-TZD

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+

1 hour	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

ZAL 100 LOT#: 11A0625-ZAL

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

UR-144 25 LOT#: 11A0616-K4

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

MES 100 LOT#: 11A0382-MES

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

GAB 2000 LOT#: 11A0283-GAB

Time after opened pouch	**N**	**Negative urine**		**–50% cutoff**		**+ 50% cutoff**		**300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

TLD 50 LOT#:11A0580-TLD50

Time after opened pouch	N	Negative urine		–50% cutoff		+ 50% cutoff		300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

QTP1000 LOT#: 11A0517-QTP1000

Time after opened pouch	N	Negative urine		Quetiapine –50% cutoff		Quetiapine + 50% cutoff		Quetiapine 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+

	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

PAR 500 LOT#: 11A0481-PAP500

Time after opened pouch	**N**	**Negative urine**		**Papaverine –50% cutoff**		**Papaverine + 50% cutoff**		**Papaverine 300% cutoff**	
		5min	**10min**	**5min**	**10min**	**5min**	**10min**	**5min**	**10min**
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+

1.5 hours	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

KRA300 LOT#:11A0301-KRA300

Time after opened pouch	N	Negative urine		Mitragynine –50% cutoff		Mitragynine + 50% cutoff		Mitragynine 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

CAR2000 Lot1#: 11A0166-CAR2000

Time after opened pouch	N	Negative urine		Carisoprodol –50% cutoff		Carisoprodol + 50% cutoff		Carisoprodol 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

HMO250 Lot1#: 11A1715-HMO250

Time after opened pouch	N	Negative urine		HMO –50% cutoff		HMO + 50% cutoff		HMO 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+

	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	+	+	+	+

HMO300 Lot1#: 11A1715-HMO300

Time after opened pouch	N	Negative urine		HMO –50% cutoff		HMO + 50% cutoff		HMO 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
20 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	-	-	+	+
	5	-	-	-	-	+	+	+	+

OZP1000 Lot1#: 11A0472-OZP1000

Time after opened pouch	N	Negative urine		OZP –50% cutoff		OZP + 50% cutoff		OZP 300% cutoff	
		5min	10min	5min	10min	5min	10min	5min	10min
10 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
	1	-	-	-	-	+	+	+	+

20 minutes	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
30 minutes	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1 hour	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	+	+	+	+
	3	-	-	-	-	+	+	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+
1.5 hours	1	-	-	-	-	+	+	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	-	-	+	+
2 hours	1	-	-	-	-	-	-	+	+
	2	-	-	-	-	-	-	+	+
	3	-	-	-	-	-	-	+	+
	4	-	-	-	-	+	+	+	+
	5	-	-	-	-	+	+	+	+

Conclusion: The products were stable at 1 hour after the pouch was opened.

Document History Summary

Version No.	Date	Description	Remark
A	2022.01.17	Initial version	N/A