
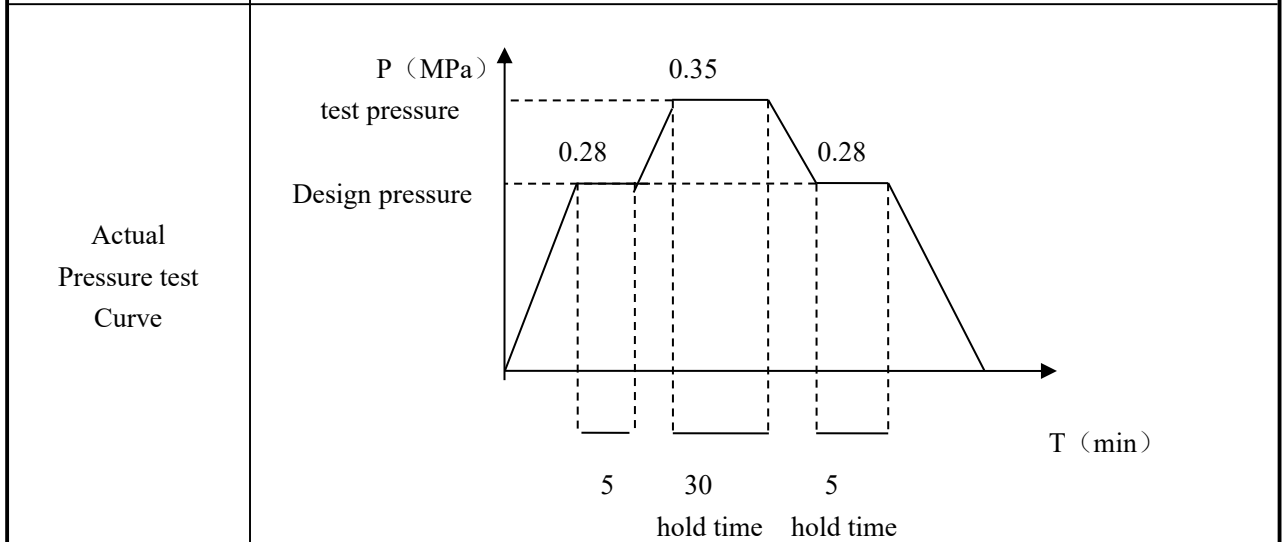


Hydraulic test report

Pressure testing site	Disinfection Tank of Vertical Autoclave	Test date	2026.2.27	Product number	BKQ-Z100I
Accuracy level of pressure gauge	1.6	Pressure gauge range	0-1MPa	Validity period of pressure gauge	2026.3.16
Pressure gauge number	241010018	Pressure gauge dial diameter (mm)	100	Test medium	W
Chlorine ion content (mg/L)	18.6	ambient temperature (°C)	12	Medium temperature(°C)	10

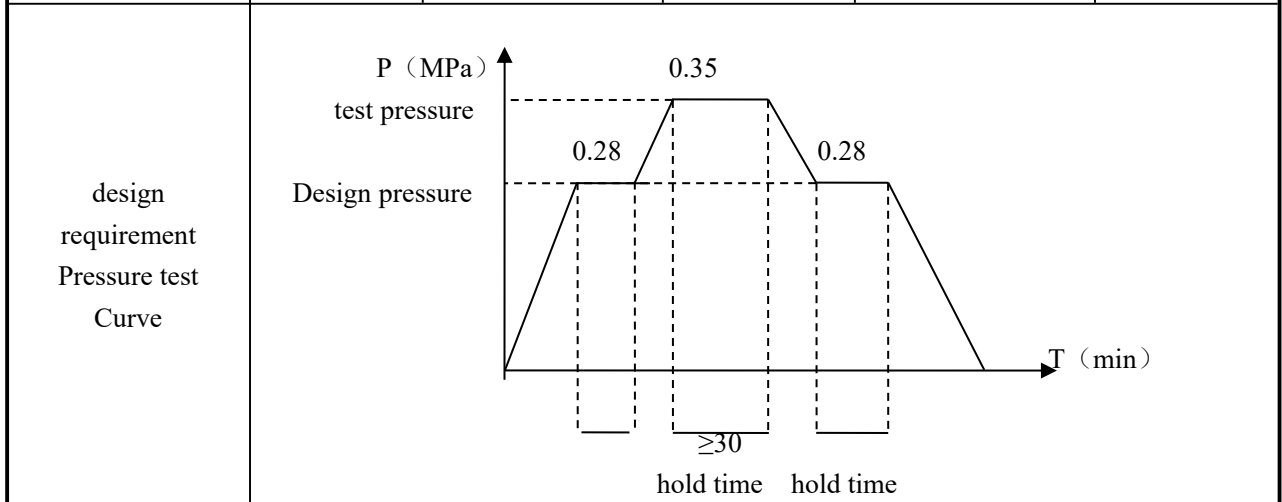

Conclusion:

This product has undergone a 0.35MPa test and shows no leakage; No visible abnormal deformation; No abnormal sound; The experimental conclusion is qualified.

Operator:
Time:

Inspector:

Inspection and Test Responsible Person: